

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\
 Data File : PD066323.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2021 19:05
 Operator : AR\AJ
 Sample : M4126-02
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AA1

Manual Integrations
 APPROVED

mohammad
 10/20/2021 2:48:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 01:33:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 19 10:18:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.980	82010062	1207.1E6	40.163	135.453 #
27)	SA Decachlor...	8.163	9.024	94014016	90227781	69.149	19.000m#
Target Compounds							
10)	B trans-Chl...	5.363	6.072	10171164	220.2E6	3.711m	24.357m#
11)	B cis-Chlor...	5.421	6.146	12113017	74770535	4.516m	8.435 #
12)	B 4,4'-DDE	5.589	6.303	6408488	64967676	2.558m	8.176m#
14)	MA Endrin	5.972	6.666	5432615	21480665	2.285	4.058 #
15)	B Endosulfa...	6.257	6.900	9131587	26797139	4.065m	3.760

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\
Data File : PD066323.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2021 19:05
Operator : AR\AJ
Sample : M4126-02
Misc :
ALS Vial : 47 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 01:33:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 19 10:18:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

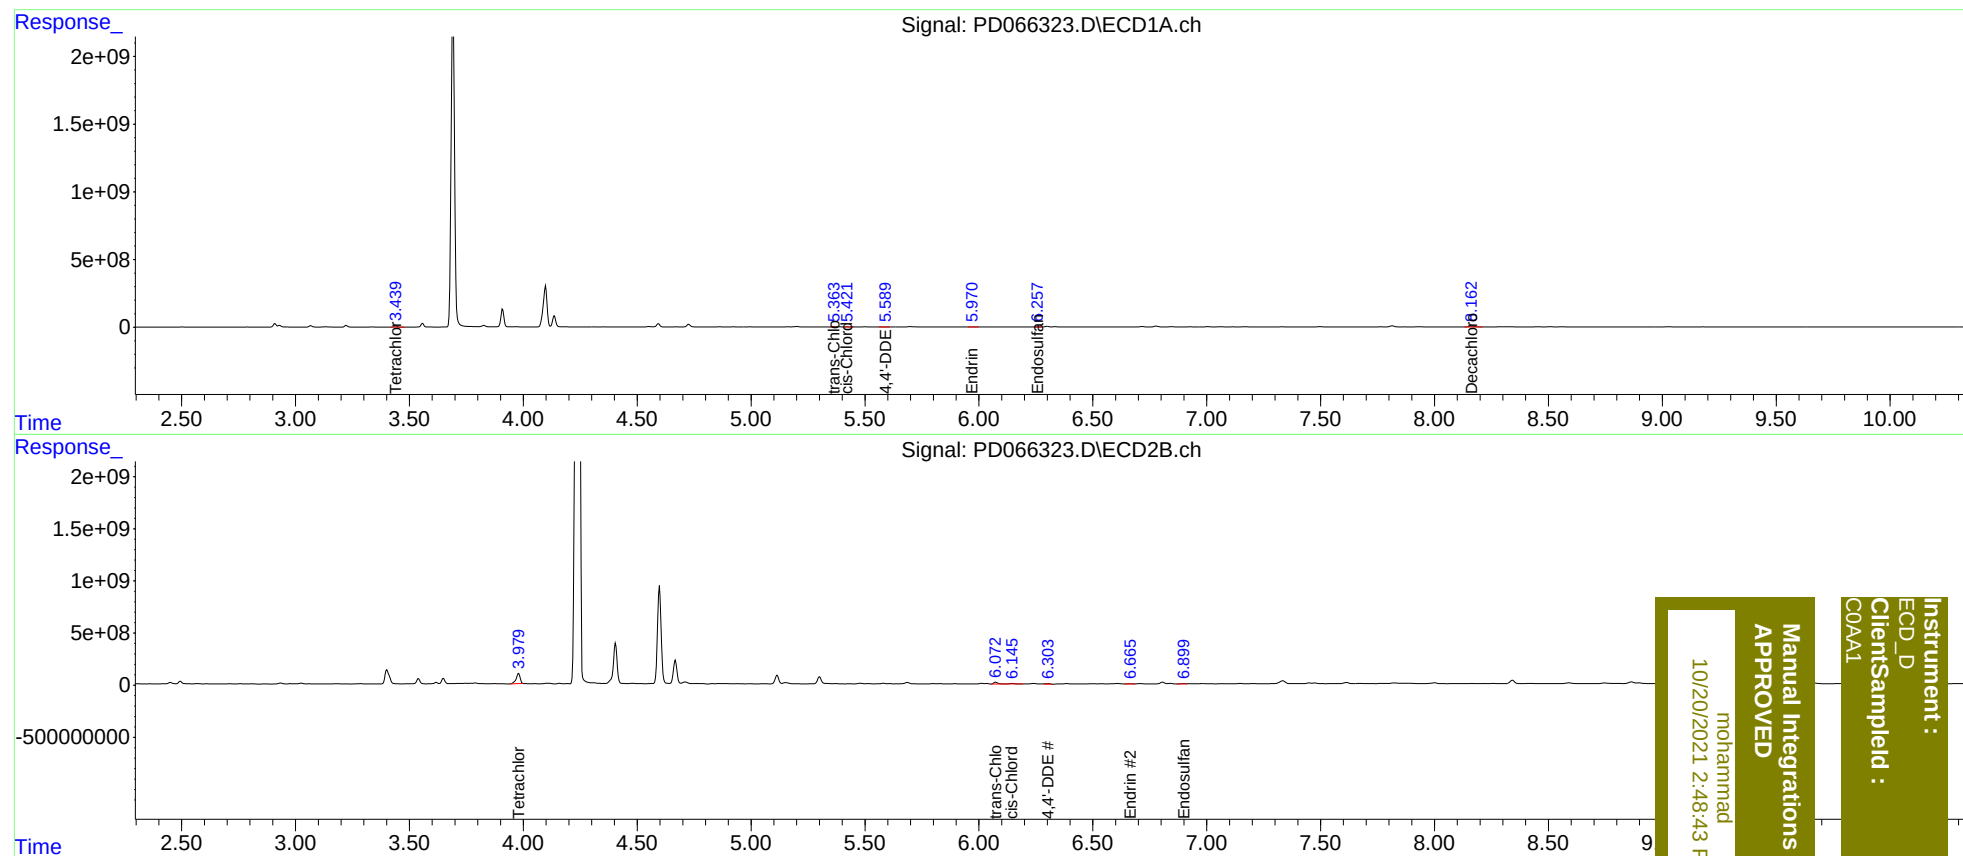

Manual Integrations
APPROVED

10/20/2021 2:48:43 PM
mohammad

Instrument :
ECD_D
Client Sampled :
C0AA1