

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\
 Data File : PD066325.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2021 20:04
 Operator : AR\AJ
 Sample : M4126-04
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AA4

Manual Integrations
 APPROVED

mohammad
 10/20/2021 2:48:56 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 03:34:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 19 10:18:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.440	3.979	3353.5E6	19993.9E6	1642.310	2243.615 #
2) SA Decachlor...	8.176	8.993	1917.3E6	328.5E6	1410.246m	69.168m#
Target Compounds						
10) B trans-Chl...	5.378	6.073	90719840	429.5E6	33.100m	47.501m#
11) B cis-Chlor...	5.419	6.144	31080422	101.2E6	11.588m	11.411m
12) B 4,4'-DDE	5.578	6.302	17582452	117.6E6	7.019m	14.803m#
17) MA 4,4'-DDT	6.333	7.099	39608569	60309128	19.905m	9.196 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\
Data File : PD066325.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2021 20:04
Operator : AR\AJ
Sample : M4126-04
Misc :
ALS Vial : 49 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 03:34:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 19 10:18:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

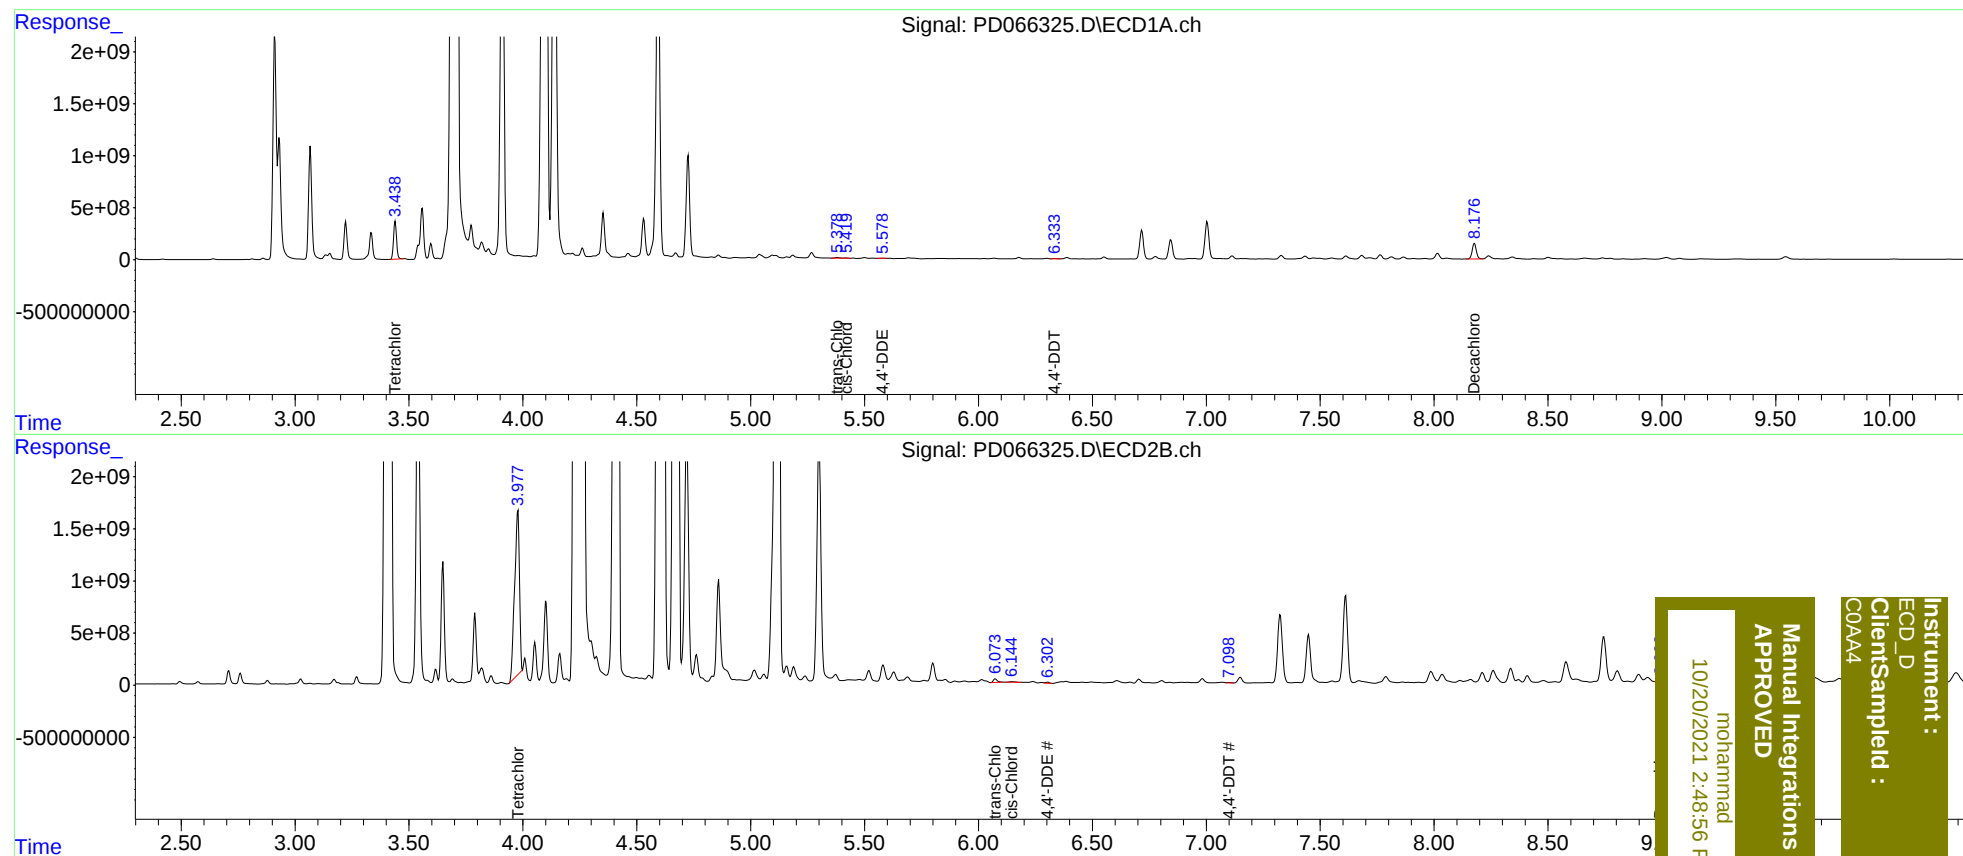

Manual Integrations
APPROVED

10/20/2021 2:48:56 PM
mohammad

Instrument :
ECD_D
Client Sampled :
C0AA4