

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\
 Data File : PD066329.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2021 21:58
 Operator : AR\AJ
 Sample : M4126-21MS
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AD1MS

Manual Integrations
 APPROVED

mohammad
 10/20/2021 2:49:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 03:50:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 19 10:18:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	3.971	2649.8E6	54924.4E6	1297.716	6163.326m#
27)	SA Decachlor...	8.179	8.995	1313.7E6	1353.9E6	966.263m	285.089m#
Target Compounds							
2)	A alpha-BHC	3.901	4.391f	46719.1E6	63852.1E6	14974.542m	5495.621m#
3)	MA gamma-BHC...	4.138	4.667	13039.5E6	21070.2E6	4224.152m	1908.964m#
4)	MA Heptachlor	4.461	5.113f	1882.3E6	21587.9E6	642.974m	2133.391m#
5)	MB Aldrin	4.726f	5.479f	13527.3E6	2912.4E6	4398.706m	288.846m#
6)	B beta-BHC	4.408	4.830	246.1E6	628.6E6	184.817m	120.738m#
7)	B delta-BHC	4.592	5.019	5505.2E6	5899.0E6	1908.225m	609.597m#
8)	B Heptachlo...	5.130	5.830	1425.9E6	4021.5E6	526.887	500.807m
9)	A Endosulfan I	5.477	6.200	197.9E6	445.0E6	78.287	52.773 #
10)	B trans-Chl...	5.384	6.074	1888.2E6	2523.0E6	688.901m	279.059m#
11)	B cis-Chlor...	5.425	6.160	1055.4E6	1748.5E6	393.508m	197.242 #
12)	B 4,4'-DDE	5.588	6.304	1104.0E6	3783.8E6	440.758m	476.161m
13)	MA Dieldrin	5.710	6.454	2782.4E6	809.1E6	1035.931m	95.720 #
14)	MA Endrin	5.965	6.664	1103.6E6	6009.1E6	464.201m	1135.318m#
15)	B Endosulfa...	6.230	6.874	1751.8E6	1658.0E6	779.895	232.650 #
16)	A 4,4'-DDD	6.100	6.799	148.2E6	1661.9E6	71.365	249.061m#
17)	MA 4,4'-DDT	6.342	7.055f	6160.0E6	14851.2E6	3095.619	2264.491 #
18)	B Endrin al...	6.425	6.984	698.8E6	1368.8E6	446.158m	258.223m#
19)	B Endosulfa...	6.621	7.236	510.1E6	1997.2E6	257.087m	302.858m
20)	A Methoxychlor	6.884	7.558	663.7E6	1651.5E6	640.077m	508.520
21)	B Endrin ke...	7.113	7.687	997.3E6	2700.8E6	431.874m	376.564m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\
Data File : PD066329.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2021 21:58
Operator : AR\AJ
Sample : M4126-21MS
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 03:50:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 19 10:18:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

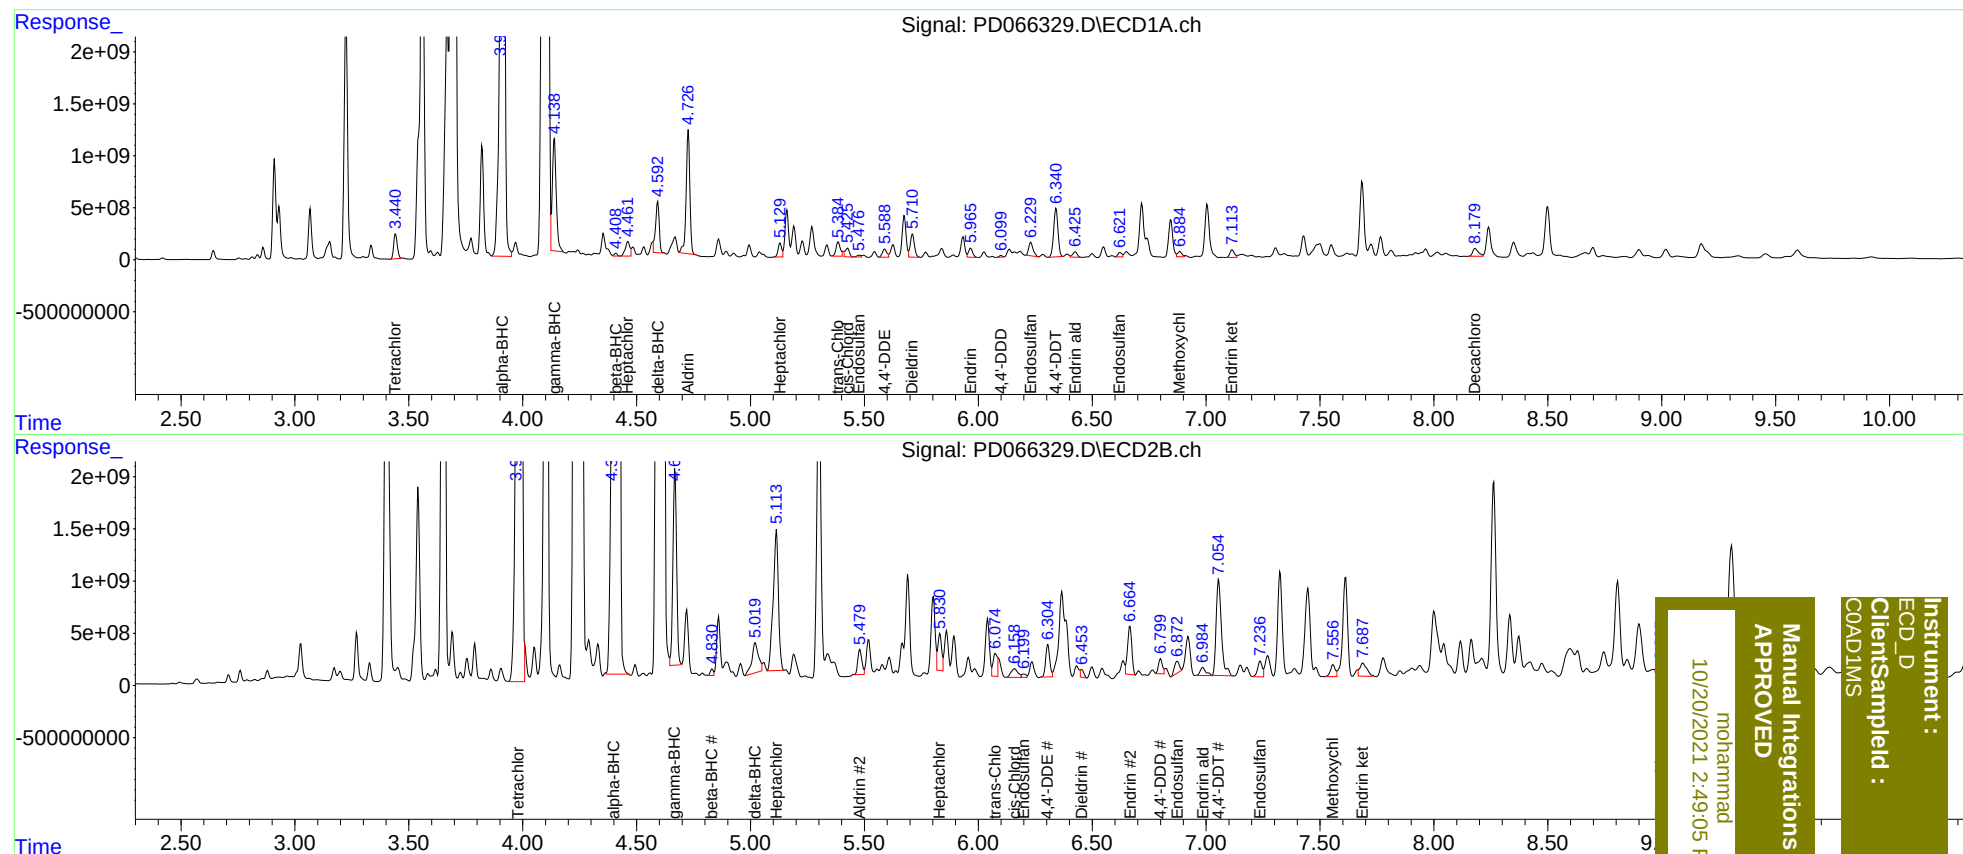

Instrument :
ECD_D
ClientSample :
COADIMS

Manual Integrations
APPROVED
mohammad
10/20/2021 2:49:05 PM