

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\
 Data File : PD066330.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2021 22:12
 Operator : AR\AJ
 Sample : M4126-22MSD
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleID :
 C0AD1MSD

Manual Integrations
 APPROVED

mohammad
 10/20/2021 2:49:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 04:06:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 19 10:18:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	3.968	3099.0E6	57081.4E6	1517.710	6405.375m#
27)	SA Decachlor...	8.180	8.997	1604.6E6	1603.7E6	1180.185m	337.690m#
Target Compounds							
2)	A alpha-BHC	3.902	4.388f	48335.4E6	65530.2E6	15492.601m	5640.047m#
3)	MA gamma-BHC...	4.138	4.668	14814.9E6	23616.6E6	4799.272m	2139.668m#
4)	MA Heptachlor	4.461	5.113f	2167.8E6	24596.4E6	740.496m	2430.710m#
5)	MB Aldrin	4.726f	5.479f	15725.4E6	3584.3E6	5113.457m	355.480m#
6)	B beta-BHC	4.408	4.830	275.4E6	655.3E6	206.841m	125.852m#
7)	B delta-BHC	4.592	5.021	6470.8E6	6257.4E6	2242.915m	646.631 #
8)	B Heptachlo...	5.130	5.831	1670.8E6	4054.6E6	617.387	504.932m
9)	A Endosulfan I	5.477	6.202	223.5E6	491.3E6	88.423	58.261 #
10)	B trans-Chl...	5.386	6.074	2125.5E6	3554.7E6	775.512	393.177m#
11)	B cis-Chlor...	5.427	6.160	1146.7E6	2001.0E6	427.558	225.720 #
12)	B 4,4'-DDE	5.588	6.306	1158.5E6	3522.7E6	462.494m	443.308
13)	MA Dieldrin	5.710	6.452	3171.7E6	1040.6E6	1180.881m	123.102m#
14)	MA Endrin	5.965	6.664	1290.4E6	7151.1E6	542.780m	1351.082m#
15)	B Endosulfa...	6.231	6.874	2031.3E6	1834.9E6	904.325	257.484 #
16)	A 4,4'-DDD	6.101	6.799	164.4E6	2130.9E6	79.148	319.360m#
17)	MA 4,4'-DDT	6.342	7.095	7114.8E6	801.9E6	3575.445	122.270 #
18)	B Endrin al...	6.427	6.985	576.6E6	1273.2E6	368.141	240.182m#
19)	B Endosulfa...	6.621	7.237	582.7E6	2178.4E6	293.664m	330.333m
20)	A Methoxychlor	6.885	7.558	548.6E6	1781.8E6	529.061m	548.638
21)	B Endrin ke...	7.114	7.687	1161.8E6	2668.7E6	503.072m	372.095m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\
Data File : PD066330.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2021 22:12
Operator : AR\AJ
Sample : M4126-22MSD
Misc :
ALS Vial : 54 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 04:06:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 19 10:18:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

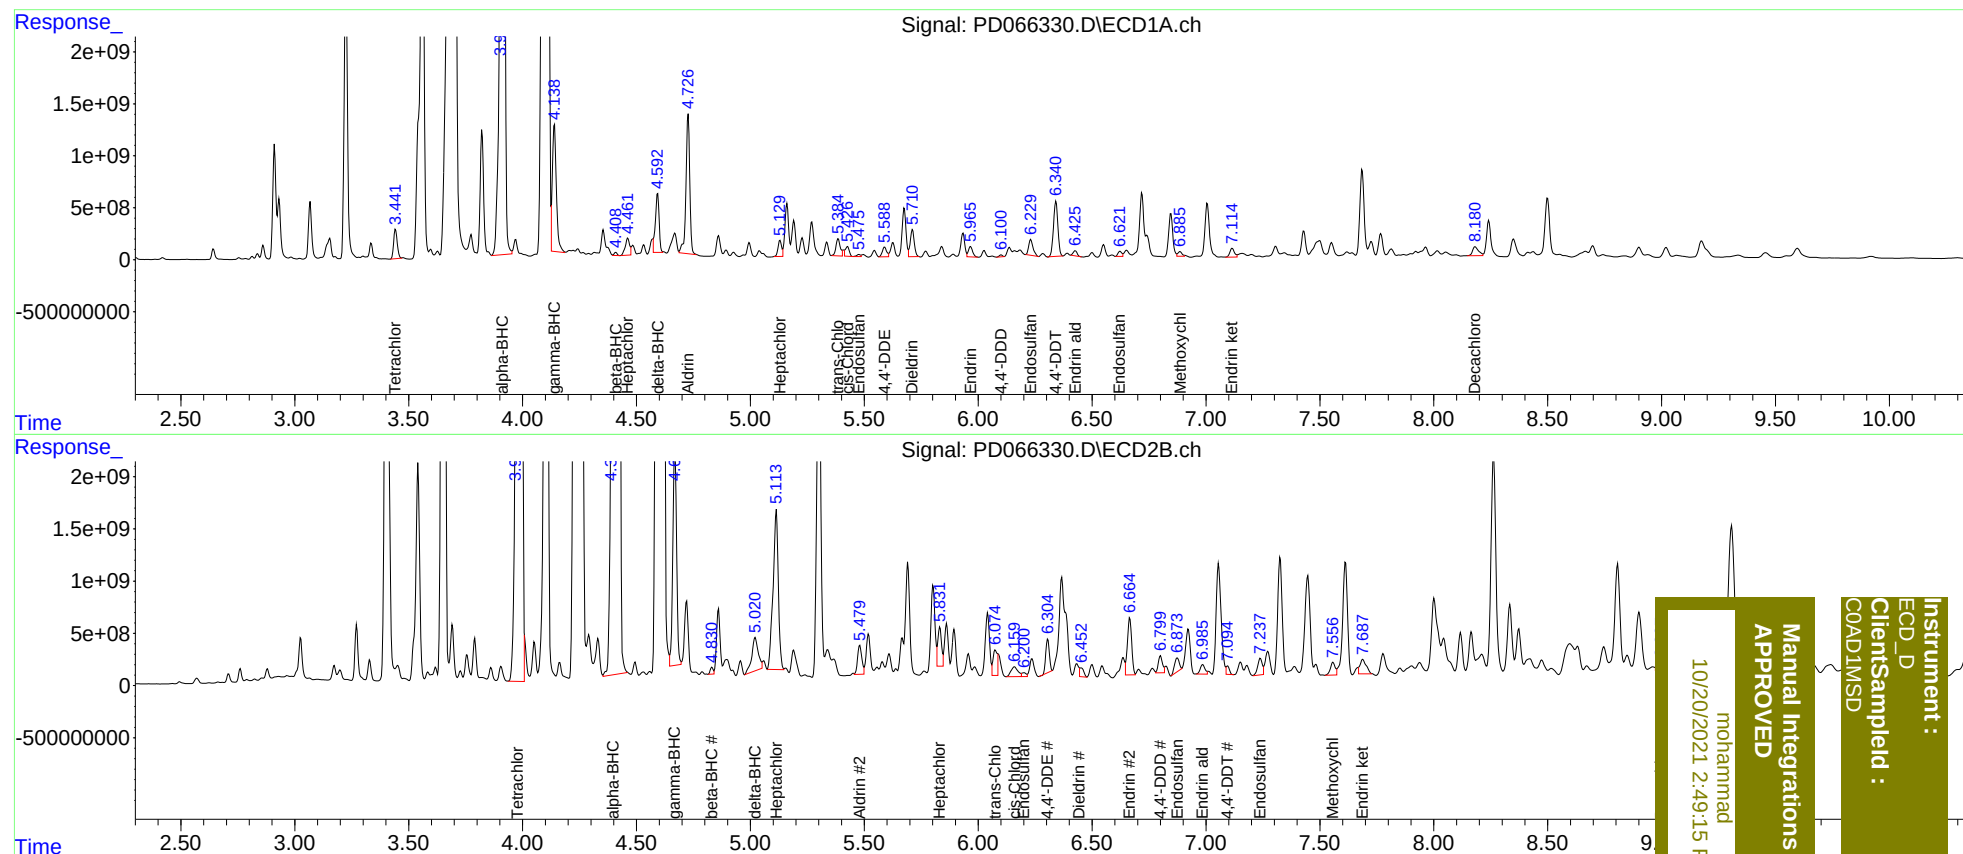

Instrument :
ECD_D
Client Sample :
C04D1MSD

Manual Integrations
APPROVED
mohammad
10/20/2021 2:49:15 PM