

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\
 Data File : PD066318.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2021 17:57
 Operator : AR\AJ
 Sample : M4126-06
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AA6

Manual Integrations
 APPROVED

mohammad
 10/20/2021 2:48:33 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 12:33:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 19 10:18:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.978	101.3E6	1006.0E6	49.599	112.893 #
2)	SA Decachlor...	8.173	9.021	49756821	90483802	36.597	19.054m#
Target Compounds							
11)	B cis-Chlor...	5.424	6.147	5465832	25884651	2.038m	2.920 #
12)	B 4,4'-DDE	5.586	6.304	5362544	45774048	2.141m	5.760 #
14)	MA Endrin	5.970	6.665	5089693	29039595	2.141	5.487 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\
Data File : PD066318.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2021 17:57
Operator : AR\AJ
Sample : M4126-06
Misc :
ALS Vial : 42 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 12:33:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 19 10:18:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

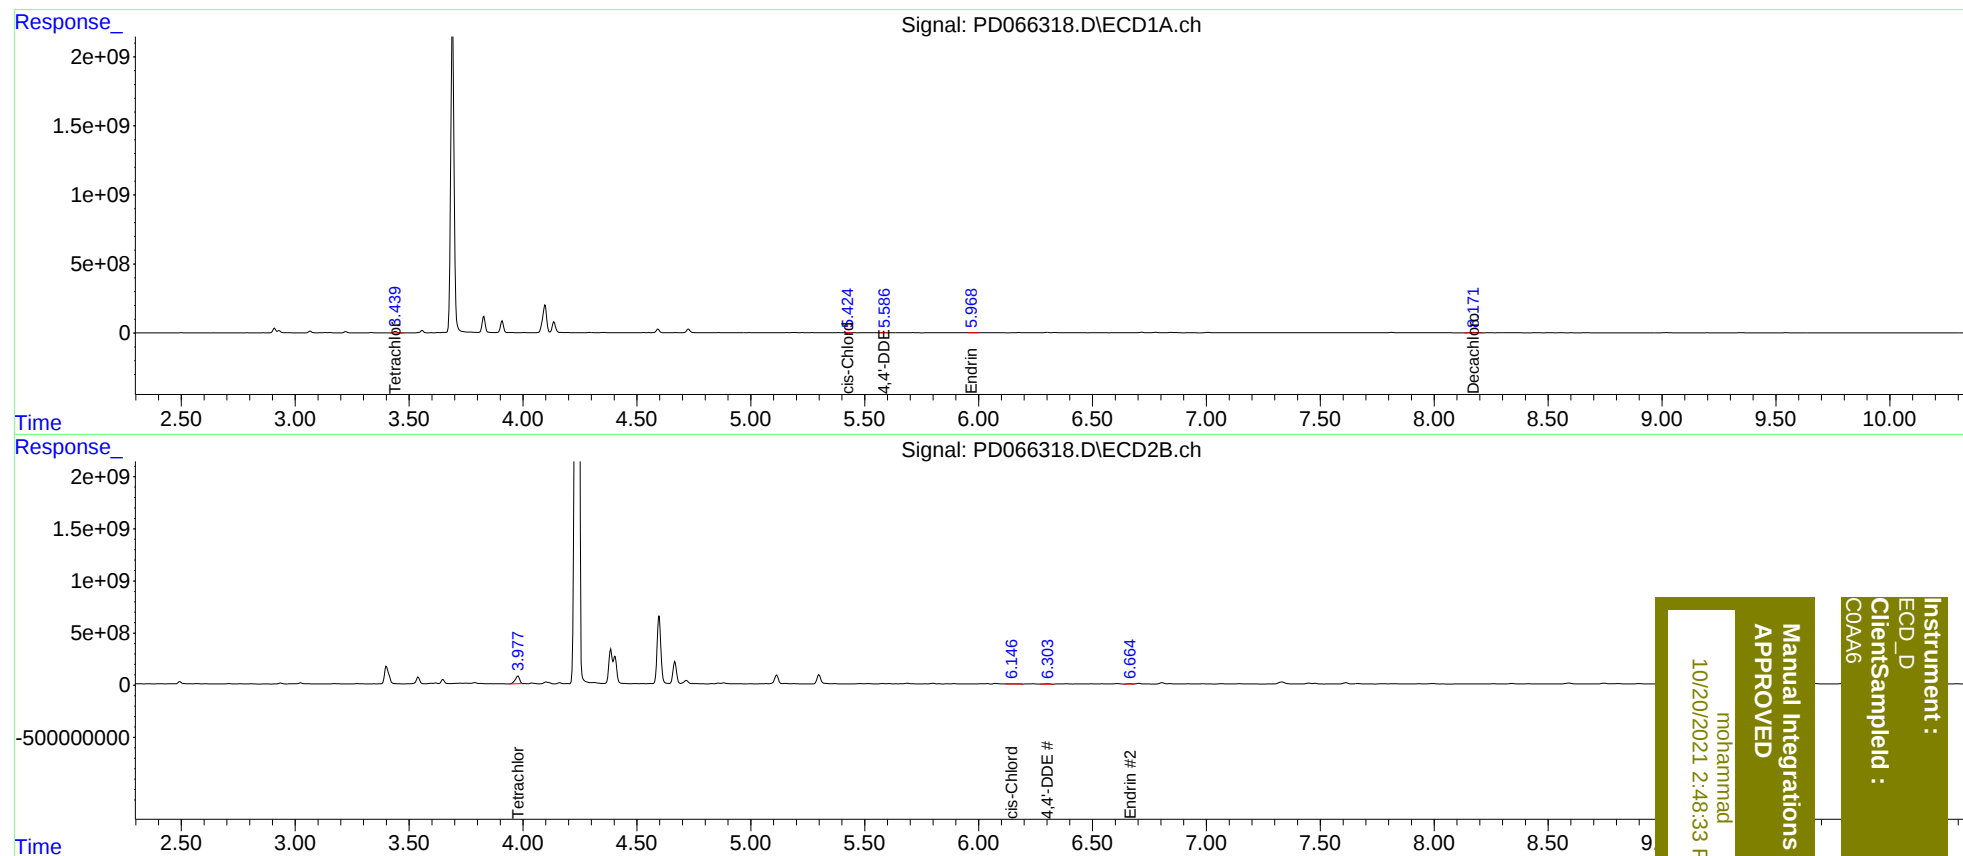

Manual Integrations
APPROVED

mohammad
10/20/2021 2:48:33 PM


Instrument :
ECD_D
Client Sampled :
C0A06

File :Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\PD066318.D
Operator : AR\AJ
Acquired : 16 Oct 2021 17:57 using AcqMethod ECD_D.M
Instrument : ECD_D
Sample Name: M4126-06
Misc Info :
Vial Number: 42

Instrument :
ECD_D
ClientSampleId :
C0AA6

Manual Integrations
APPROVED

mohammad
10/20/2021 2:48:33 PM

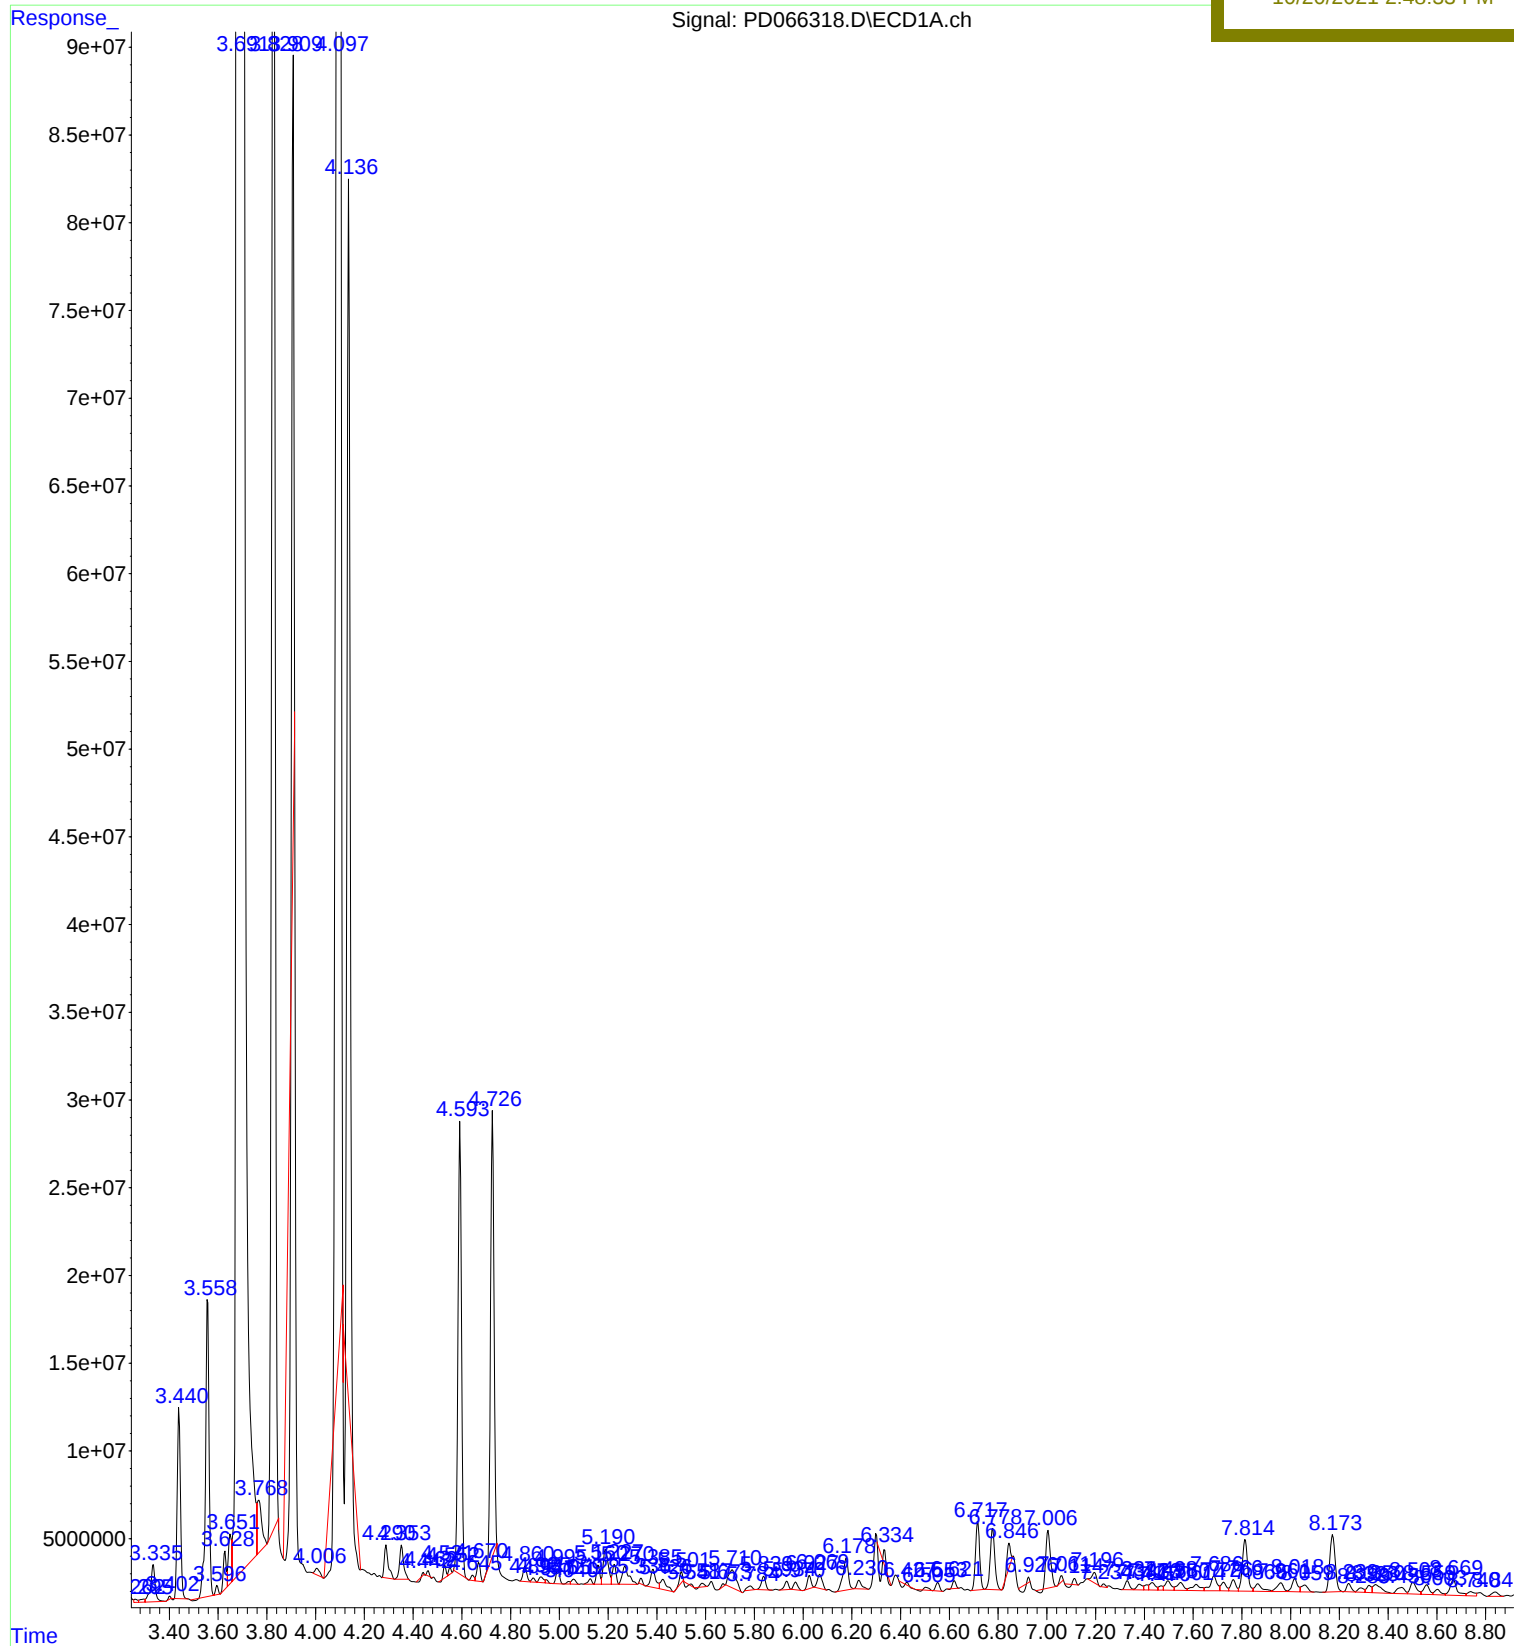

File :Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\PD066318.D
Operator : AR\AJ
Acquired : 16 Oct 2021 17:57 using AcqMethod ECD_D.M
Instrument : ECD_D
Sample Name: M4126-06
Misc Info :
Vial Number: 42

Instrument :
ECD_D
ClientSampleId :
C0AA6

Manual Integrations
APPROVED

mohammad
10/20/2021 2:48:33 PM

