

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\
 Data File : PD066321.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2021 18:38
 Operator : AR\AJ
 Sample : M4126-09
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AA9

Manual Integrations
 APPROVED

mohammad
 10/20/2021 2:48:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 12:47:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 19 10:18:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.970	27173563	110.4E6	13.308	12.391
2)	SA Decachlor...	8.167	9.021	23495399	101.7E6	17.281m	21.407m
Target Compounds							
12)	B 4,4'-DDE	5.584	6.305	6379666	34697179	2.547m	4.366 #
15)	B Endosulfa...	6.249	6.872	2436605	23934273	1.085m	3.359 #
16)	A 4,4'-DDD	6.105	6.800	5824279	50698243	2.805	7.598 #
17)	MA 4,4'-DDT	6.335	7.096	10325370	21221660	5.189m	3.236 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\
Data File : PD066321.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2021 18:38
Operator : AR\AJ
Sample : M4126-09
Misc :
ALS Vial : 45 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 12:47:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 19 10:18:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

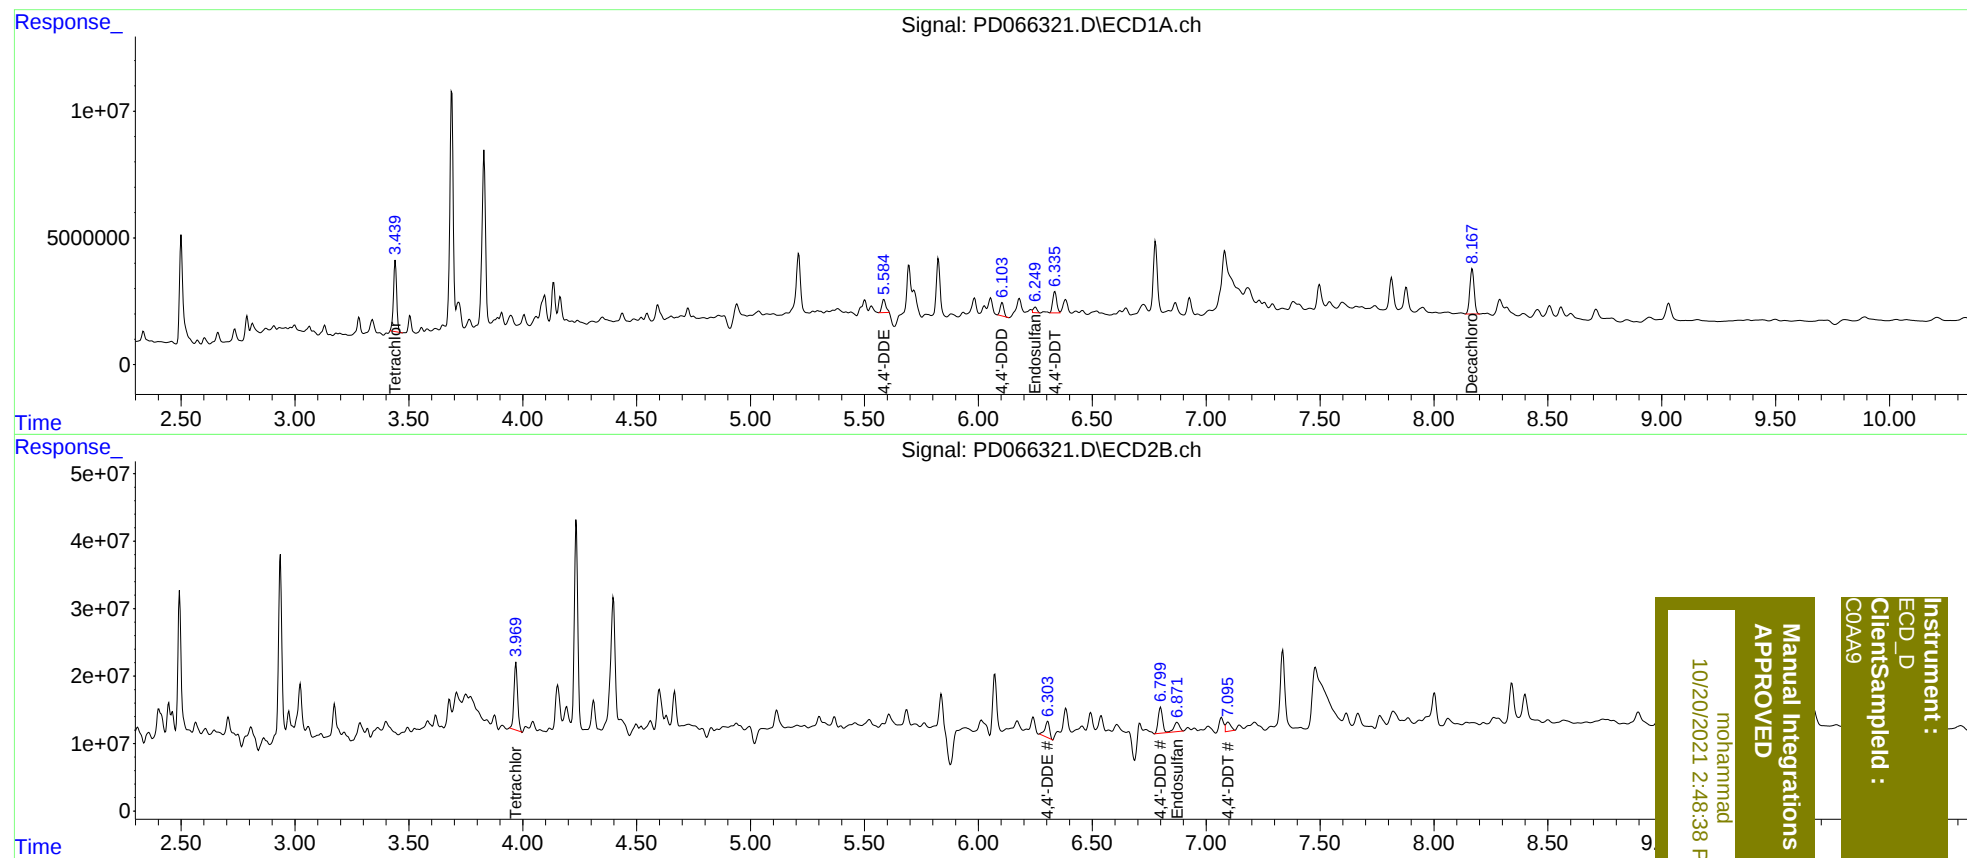

Manual Integrations
APPROVED

10/20/2021 2:48:38 PM
mohammad

Instrument :
ECD_D
ClientSampled :
COAA9