

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\
 Data File : PD066322.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2021 18:52
 Operator : AR\AJ
 Sample : M4126-10
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AB0

Manual Integrations
 APPROVED

mohammad
 10/20/2021 2:48:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 12:52:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 19 10:18:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.972	29319646	146.7E6	14.359	16.457
27)	SA Decachlor...	8.167	9.022	30634434	118.7E6	22.532m	24.994m
Target Compounds							
11)	B cis-Chlor...	5.422	6.145	1812127	12468461	0.676m	1.407m#
12)	B 4,4'-DDE	5.584	6.304	10018775	47056567	4.000m	5.922m#
16)	A 4,4'-DDD	6.105	6.801	8411721	76416357	4.051	11.452 #
17)	MA 4,4'-DDT	6.335	7.095	14852436	23399005	7.464m	3.568 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\
Data File : PD066322.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2021 18:52
Operator : AR\AJ
Sample : M4126-10
Misc :
ALS Vial : 46 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 12:52:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 19 10:18:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

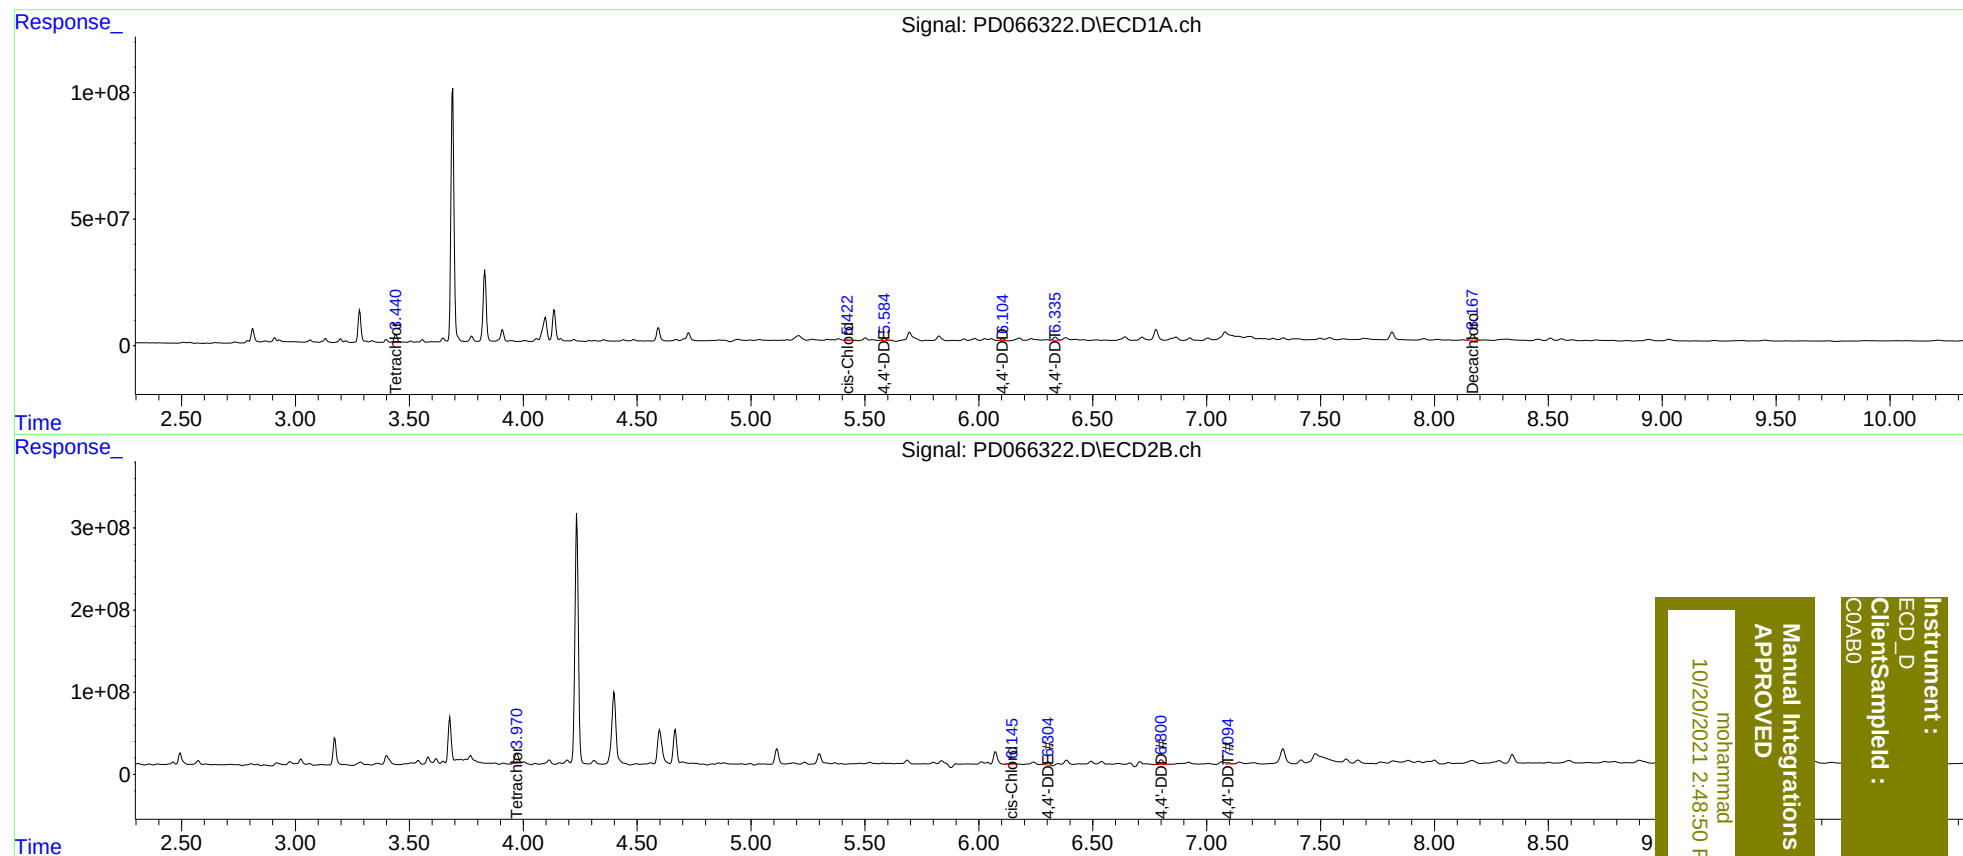


File : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\PD066322.D
Operator : AR\AJ
Acquired : 16 Oct 2021 18:52 using AcqMethod ECD_D.M
Instrument : ECD_D
Sample Name: M4126-10
Misc Info :
Vial Number: 46

Instrument :
ECD_D
ClientSampleId :
C0AB0

Manual Integrations
APPROVED

mohammad
10/20/2021 2:48:50 PM

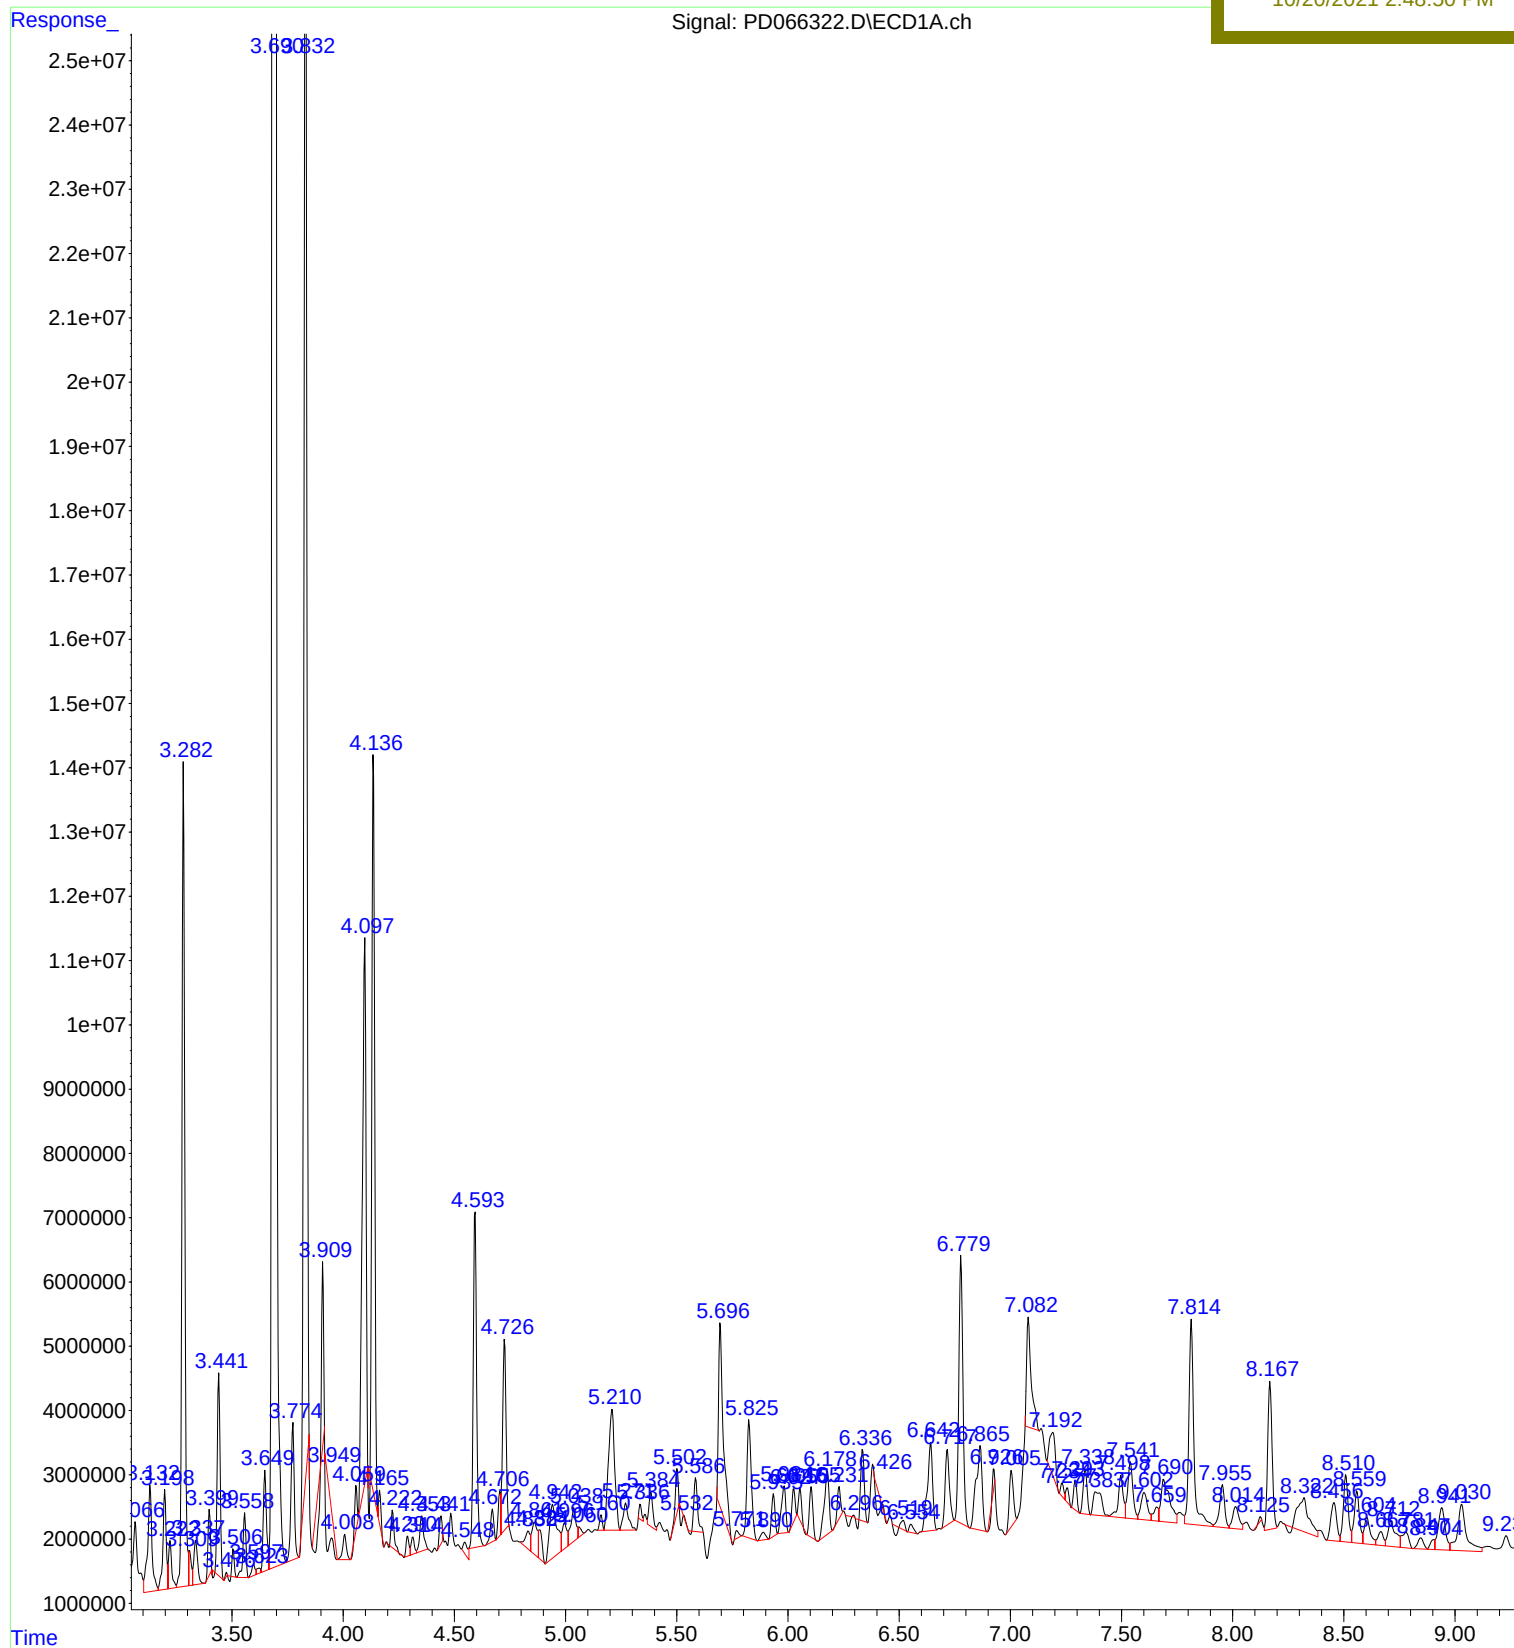

File : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\PD066322.D
Operator : AR\AJ
Acquired : 16 Oct 2021 18:52 using AcqMethod ECD_D.M
Instrument : ECD_D
Sample Name: M4126-10
Misc Info :
Vial Number: 46

Instrument :
ECD_D
ClientSampleId :
C0AB0

Manual Integrations
APPROVED

mohammad
10/20/2021 2:48:50 PM

