

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\
 Data File : PD066327.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2021 21:02
 Operator : AR\AJ
 Sample : M4126-14
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AB4

Manual Integrations
 APPROVED

mohammad
 10/20/2021 2:49:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 03:44:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 19 10:18:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.979	3439.7E6	19608.4E6	1684.565	2200.351 #
2)	SA Decachlor...	8.175	8.995	2920.4E6	201.0E6	2147.984m	42.336m#
Target Compounds							
11)	B cis-Chlor...	5.421	6.147	41035897	113.4E6	15.300	12.795
12)	B 4,4'-DDE	5.579	6.303	23472533	118.2E6	9.371m	14.872m#
17)	MA 4,4'-DDT	6.332	7.098	44453930	50842388	22.340m	7.752 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\
Data File : PD066327.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2021 21:02
Operator : AR\AJ
Sample : M4126-14
Misc :
ALS Vial : 51 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 03:44:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 19 10:18:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

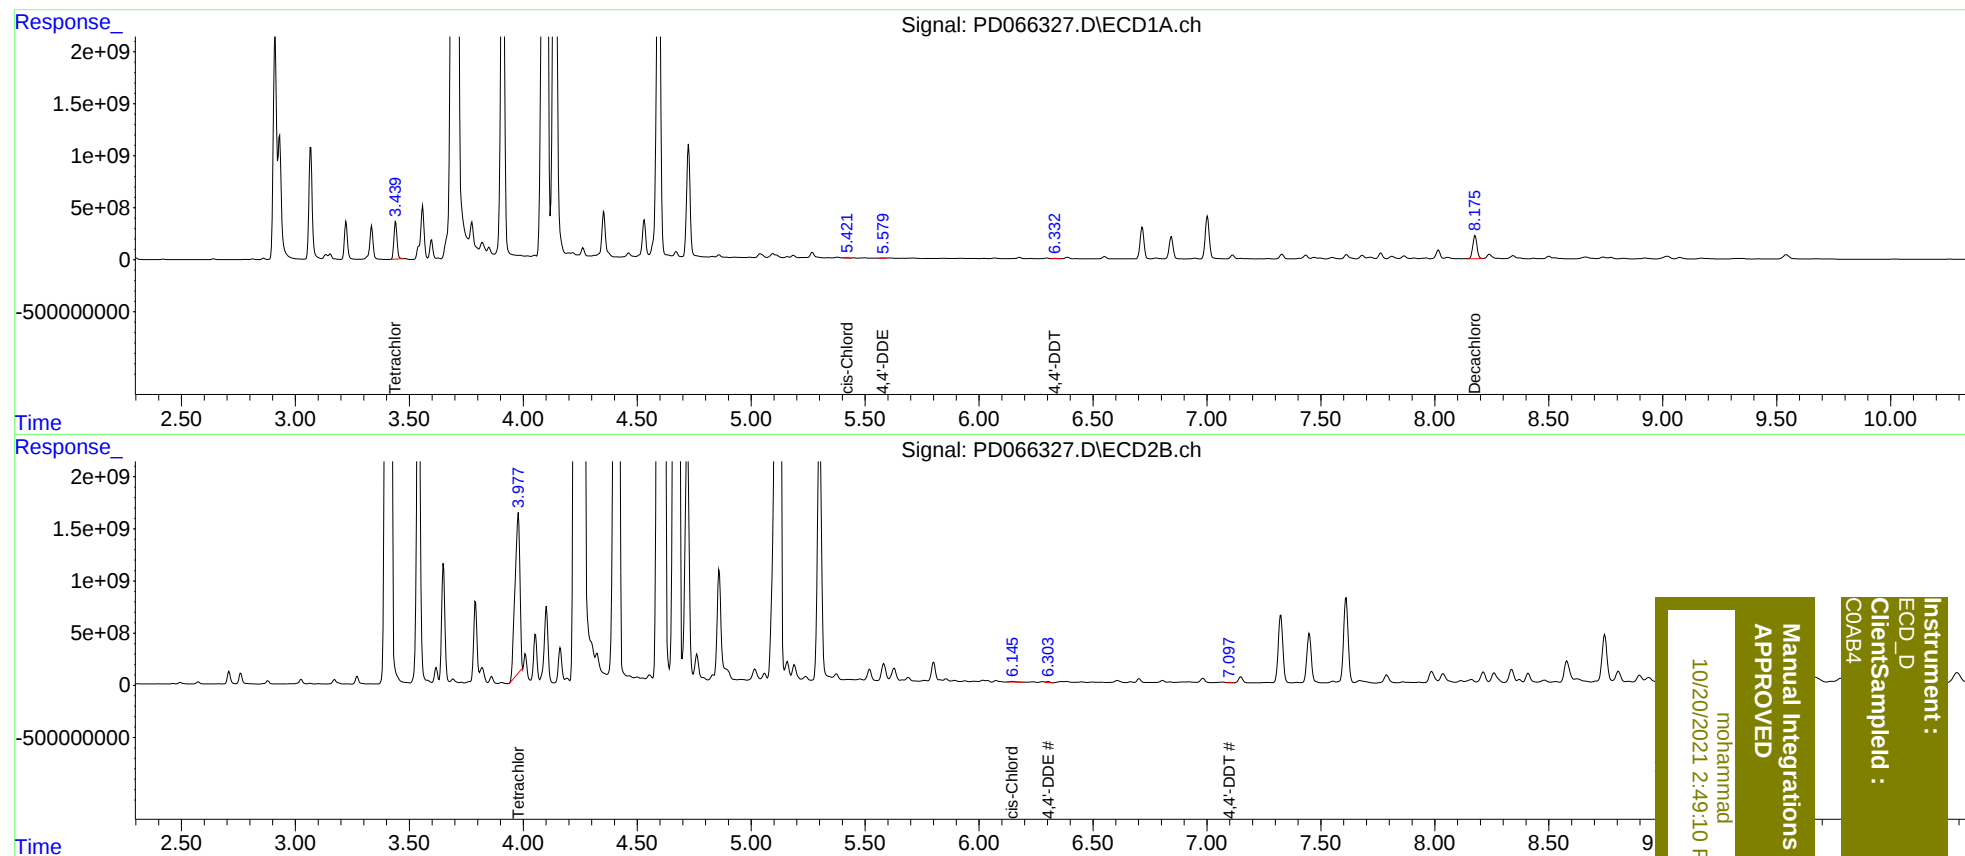

Manual Integrations
APPROVED

mohammad
10/20/2021 2:49:10 PM


Instrument :
ECD_D
ClientSampled :
C0AB4

File : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\PD066327.D
Operator : AR\AJ
Acquired : 16 Oct 2021 21:02 using AcqMethod ECD_D.M
Instrument : ECD_D
Sample Name: M4126-14
Misc Info :
Vial Number: 51

Instrument :
ECD_D
ClientSampleId :
C0AB4

Manual Integrations
APPROVED

mohammad
10/20/2021 2:49:10 PM

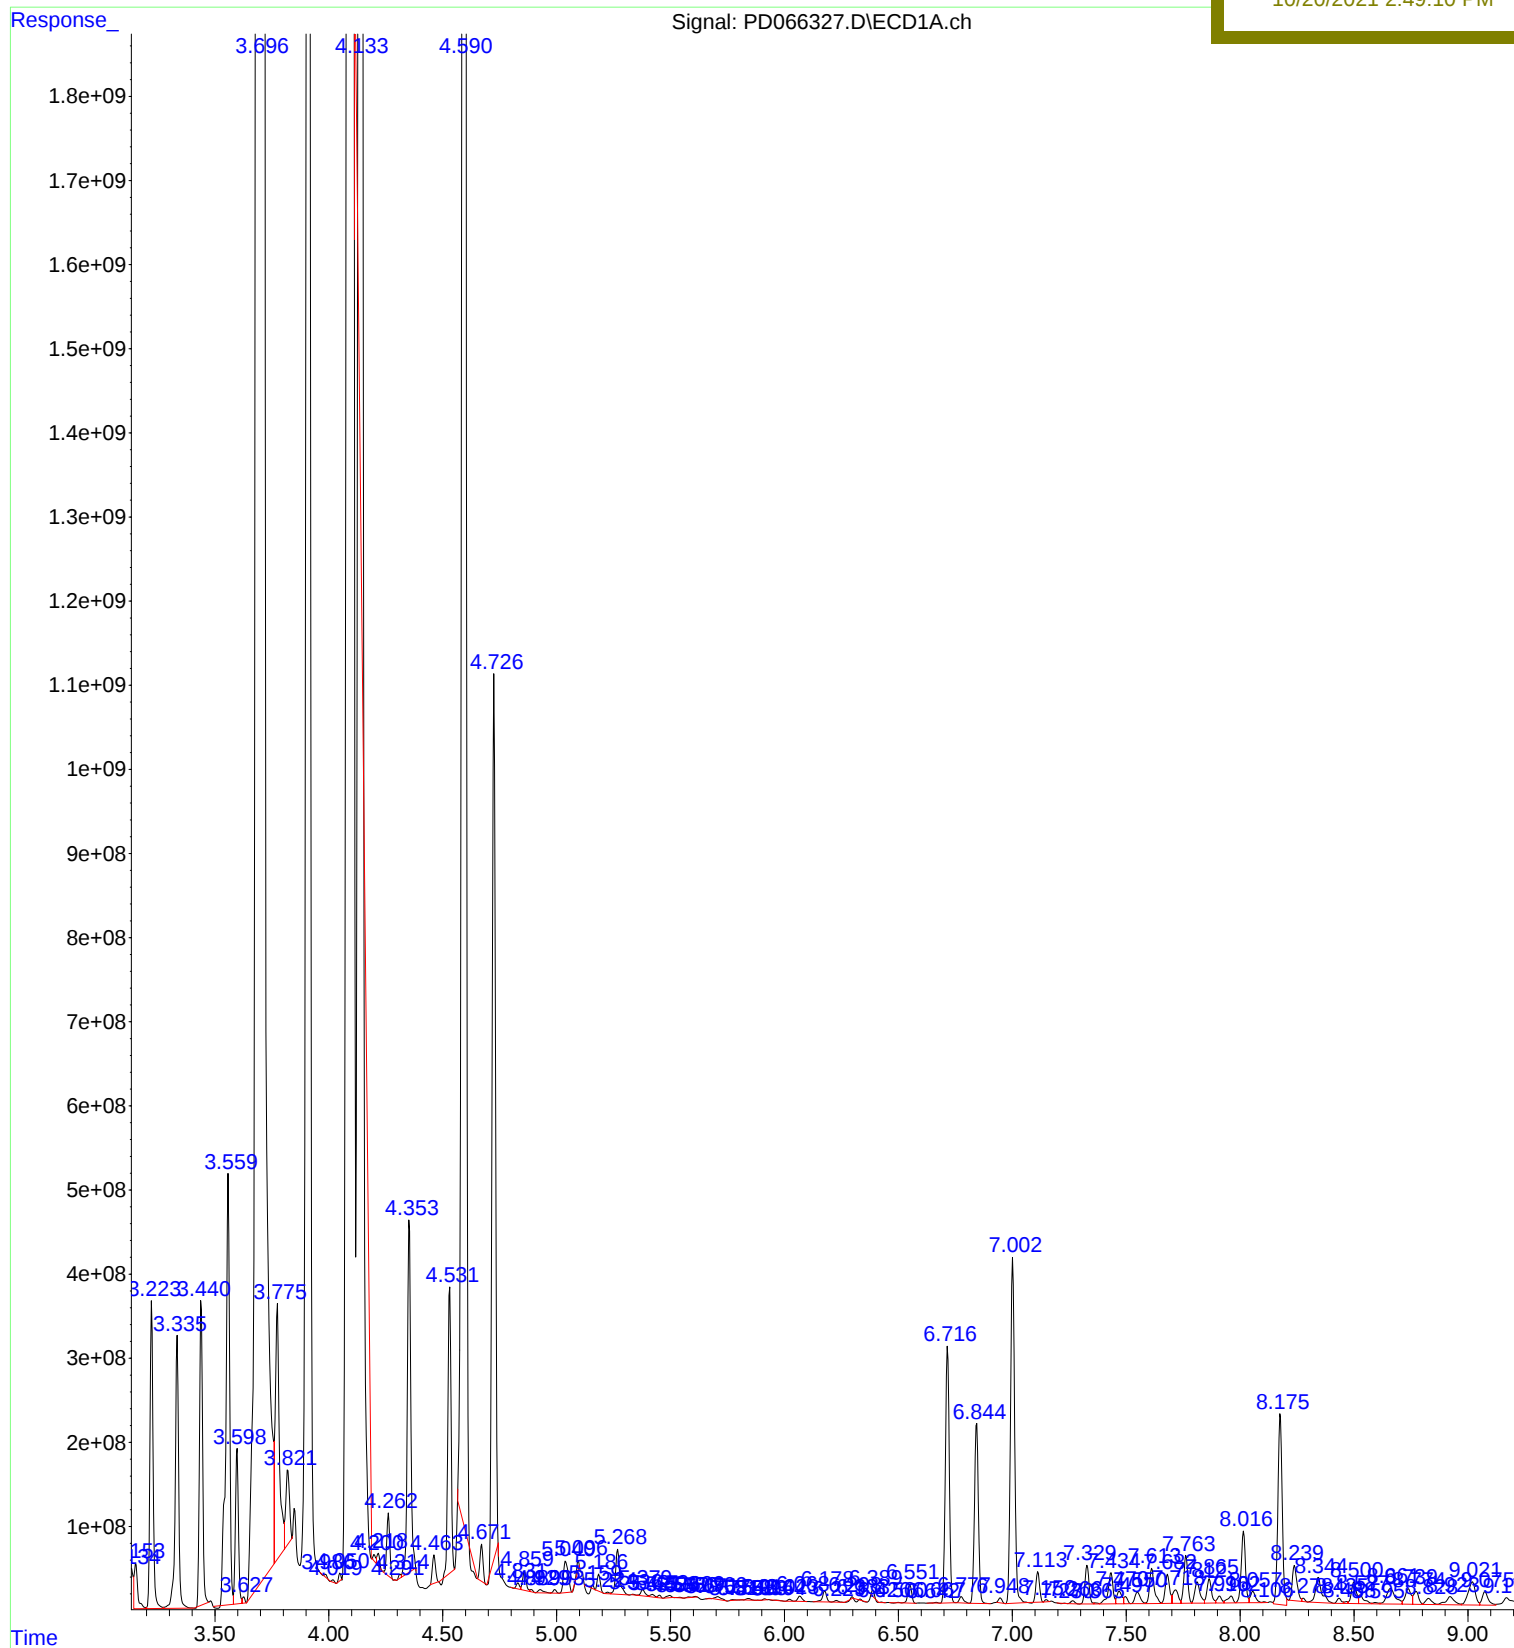

File :Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101621\PD066327.D
Operator : AR\AJ
Acquired : 16 Oct 2021 21:02 using AcqMethod ECD_D.M
Instrument : ECD_D
Sample Name: M4126-14
Misc Info :
Vial Number: 51

Instrument :
ECD_D
ClientSampleId :
C0AB4

Manual Integrations
APPROVED

mohammad
10/20/2021 2:49:10 PM

