

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101623\
 Data File : PD078895.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2023 01:17
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 05:15:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101623CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 05:13:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.806	7816539	11069502	20.000	20.000
27)	SA Decachlor...	9.119	7.957	21287141	25684140	40.000	40.000
Target Compounds							
2)	A alpha-BHC	4.026	3.310	12272294	15548458	20.000	20.000
3)	MA gamma-BHC...	4.360	3.640	11984537	14807397	20.000	20.000
4)	MA Heptachlor	4.953	3.983	13281205	14827690	20.000	20.000
9)	A Endosulfan I	6.110	5.137	11221734	12724256	20.000	20.000
13)	MA Dieldrin	6.386	5.402	22429486	27311433	40.000	40.000
14)	MA Endrin	6.616	5.677	18688875	24057240	40.000	40.000
16)	A 4,4'-DDD	6.746	5.825	16602017	21147824	40.000	40.000
17)	MA 4,4'-DDT	7.062	6.076	17845264	21125322	40.000	40.000
20)	A Methoxychlor	7.536	6.652	50445740	64329185	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101623\
Data File : PD078895.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2023 01:17
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 05:15:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101623CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 05:13:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

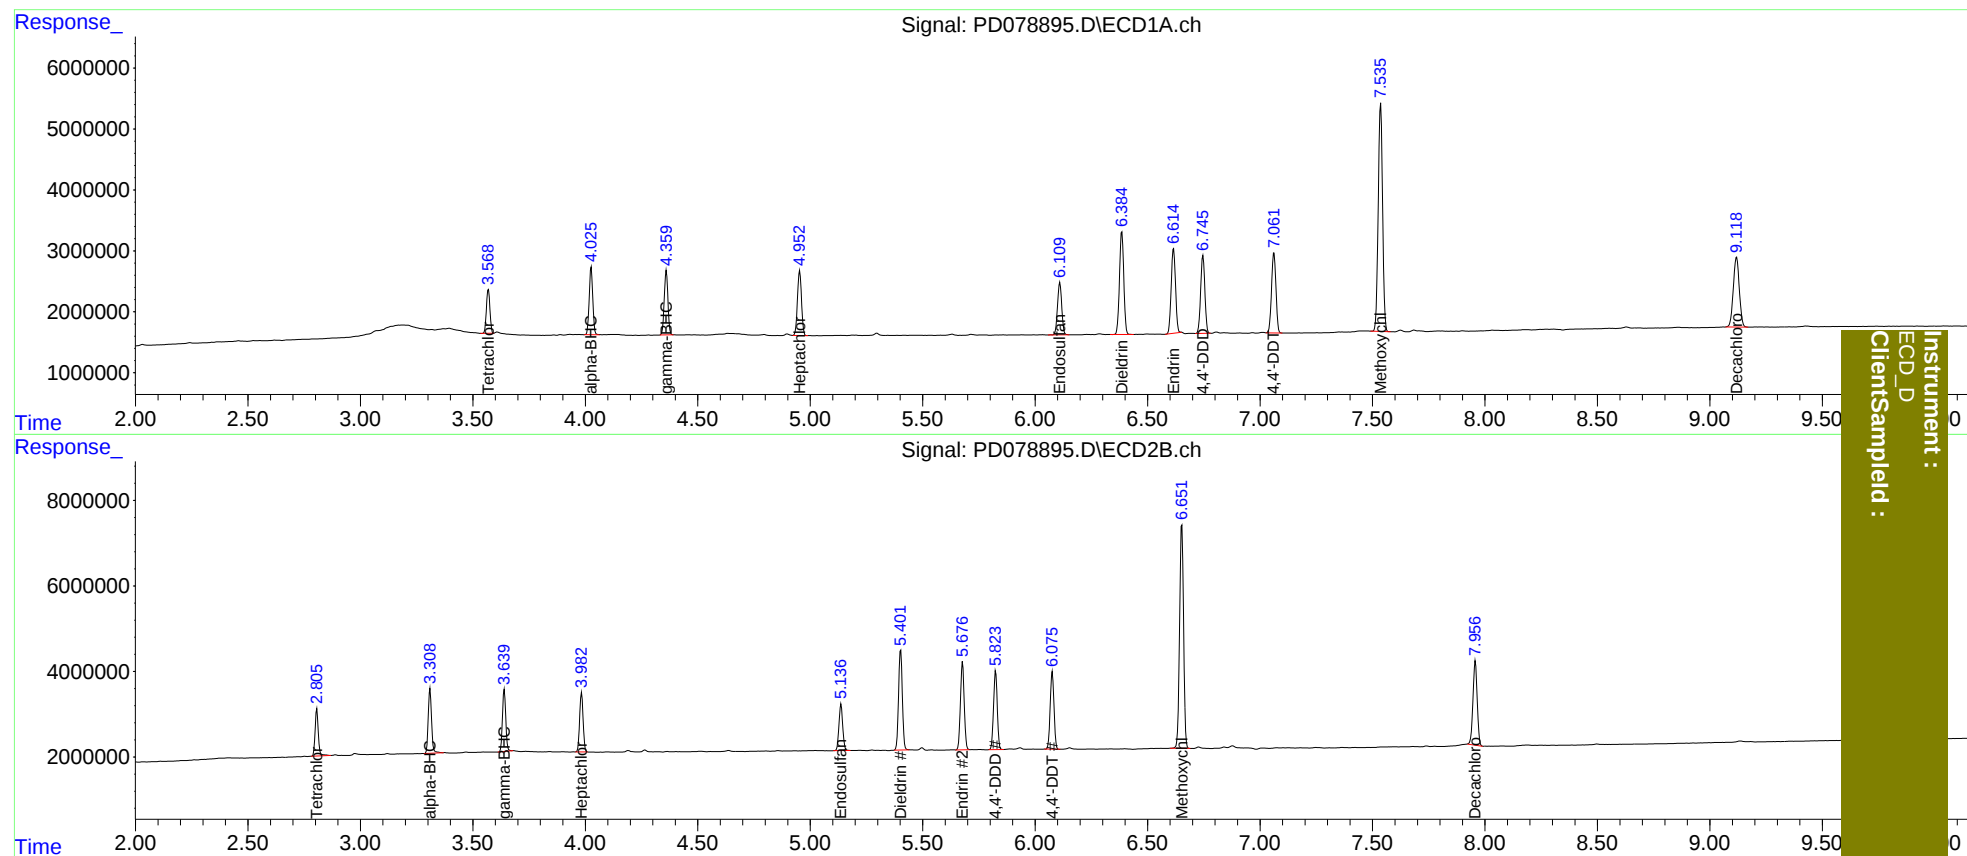


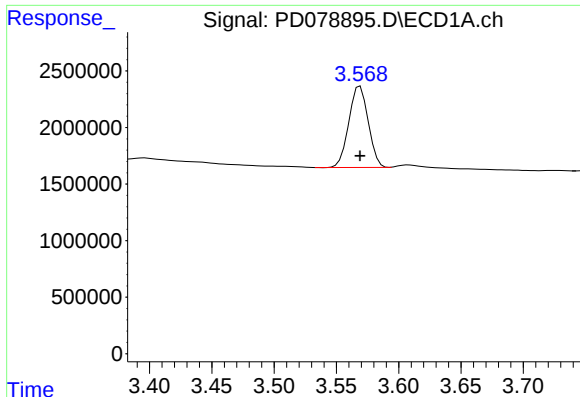

#1 Tetrachloro-m-xylene


R.T.: 3.569 min
Delta R.T.: 0.000 min
Response: 7816539
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

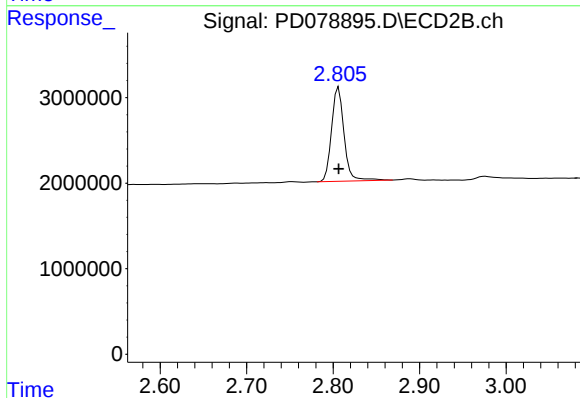


#1 Tetrachloro-m-xylene

R.T.: 2.806 min
Delta R.T.: 0.000 min
Response: 11069502
Conc: 20.00 ng/ml

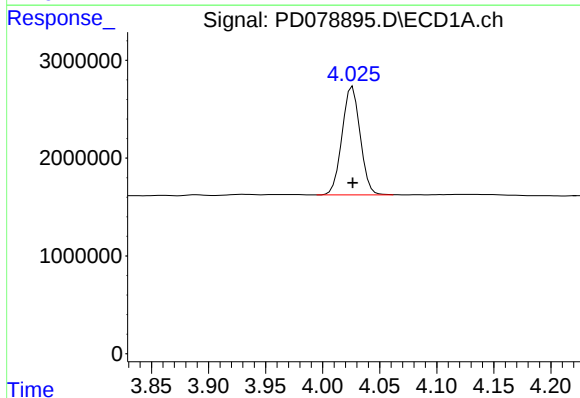


#2 alpha-BHC

R.T.: 4.026 min
Delta R.T.: 0.000 min
Response: 12272294
Conc: 20.00 ng/ml

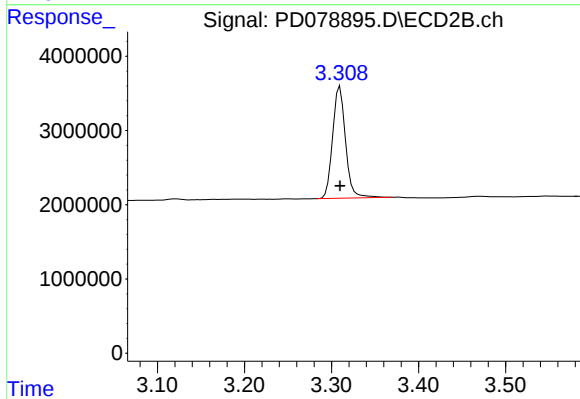

#2 alpha-BHC


R.T.: 3.310 min
Delta R.T.: 0.000 min
Response: 15548458
Conc: 20.00 ng/ml

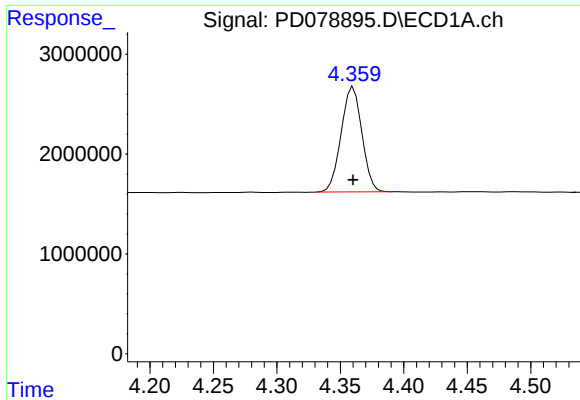

#3 gamma-BHC (Lindane)


R.T.: 4.360 min
Delta R.T.: 0.000 min
Response: 11984537
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

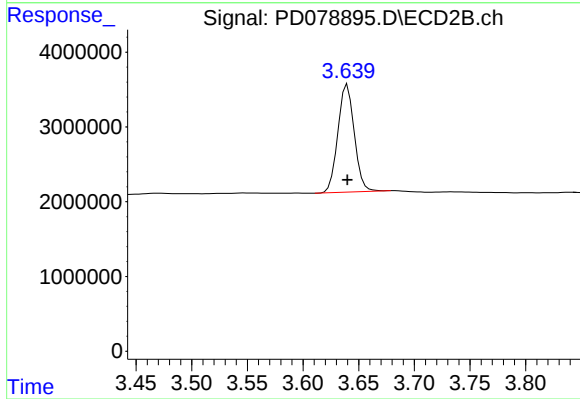


#3 gamma-BHC (Lindane)

R.T.: 3.640 min
Delta R.T.: 0.000 min
Response: 14807397
Conc: 20.00 ng/ml

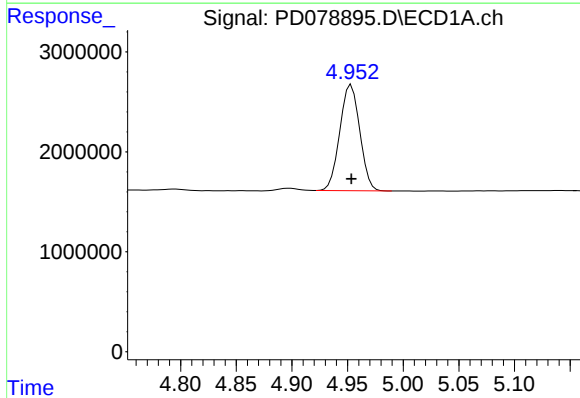


#4 Heptachlor

R.T.: 4.953 min
Delta R.T.: 0.000 min
Response: 13281205
Conc: 20.00 ng/ml

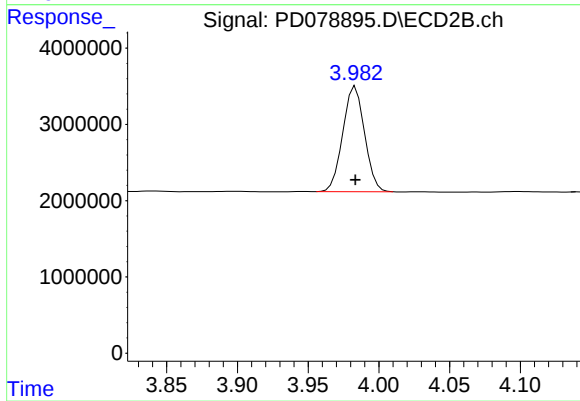

#4 Heptachlor


R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 14827690
Conc: 20.00 ng/ml

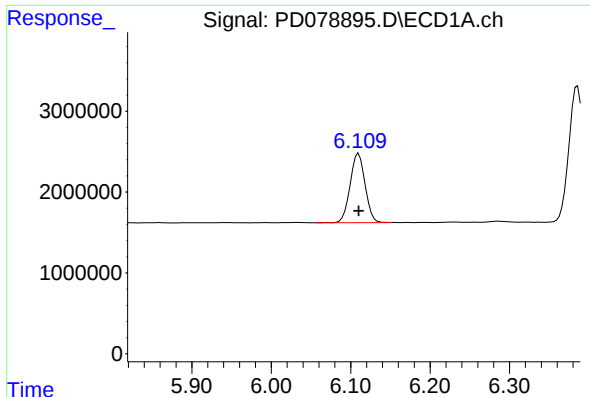

#9 Endosulfan I


R.T.: 6.110 min
Delta R.T.: 0.000 min
Response: 11221734
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

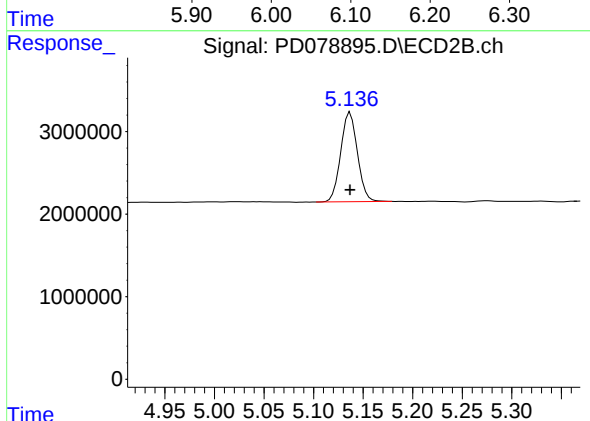


#9 Endosulfan I

R.T.: 5.137 min
Delta R.T.: 0.000 min
Response: 12724256
Conc: 20.00 ng/ml

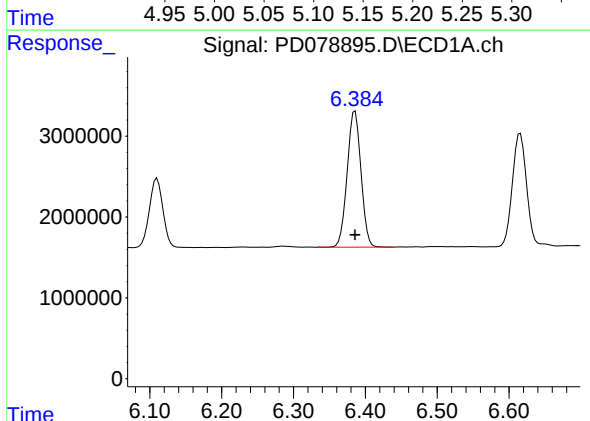


#13 Dieldrin

R.T.: 6.386 min
Delta R.T.: 0.000 min
Response: 22429486
Conc: 40.00 ng/ml

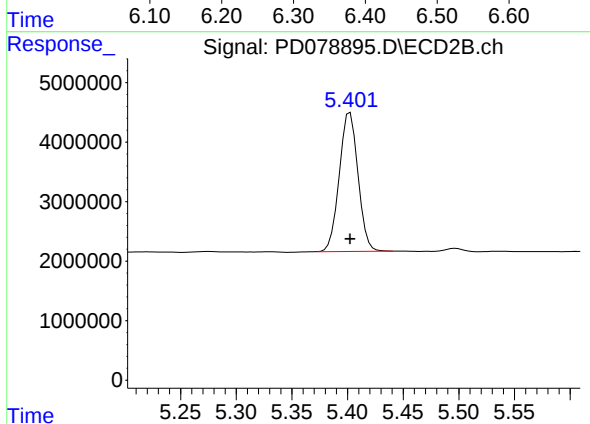

#13 Dieldrin


R.T.: 5.402 min
Delta R.T.: 0.000 min
Response: 27311433
Conc: 40.00 ng/ml

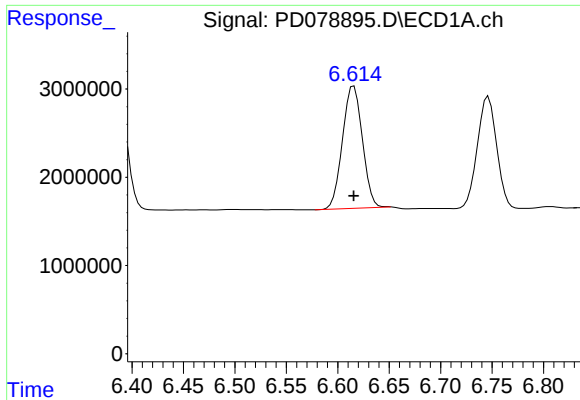

#14 Endrin


R.T.: 6.616 min
Delta R.T.: 0.000 min
Response: 18688875
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

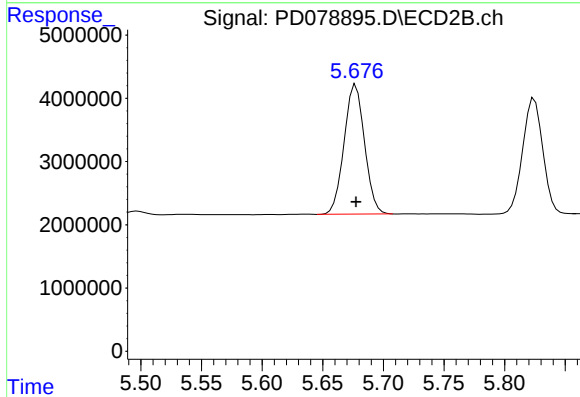


#14 Endrin

R.T.: 5.677 min
Delta R.T.: 0.000 min
Response: 24057240
Conc: 40.00 ng/ml

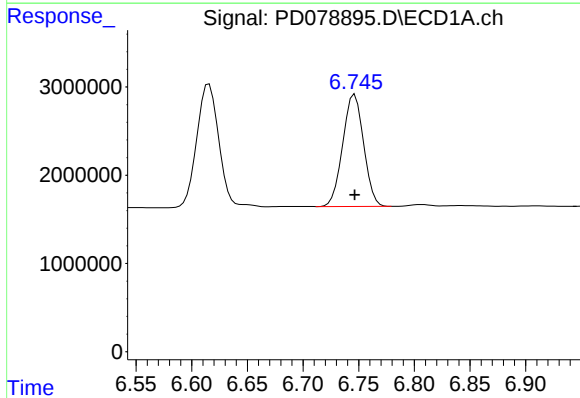


#16 4,4'-DDD

R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 16602017
Conc: 40.00 ng/ml

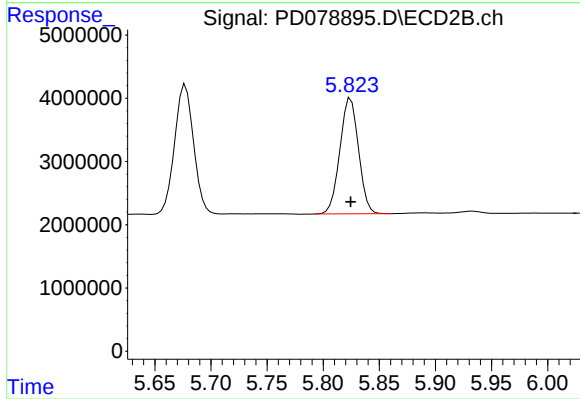

#16 4,4'-DDD


R.T.: 5.825 min
Delta R.T.: 0.000 min
Response: 21147824
Conc: 40.00 ng/ml

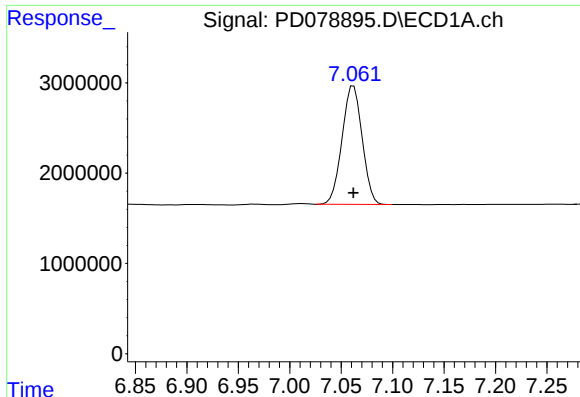

#17 4,4'-DDT


R.T.: 7.062 min
Delta R.T.: 0.000 min
Response: 17845264
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

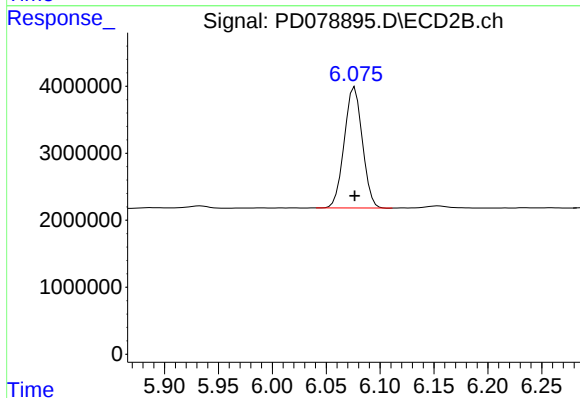


#17 4,4'-DDT

R.T.: 6.076 min
Delta R.T.: 0.000 min
Response: 21125322
Conc: 40.00 ng/ml

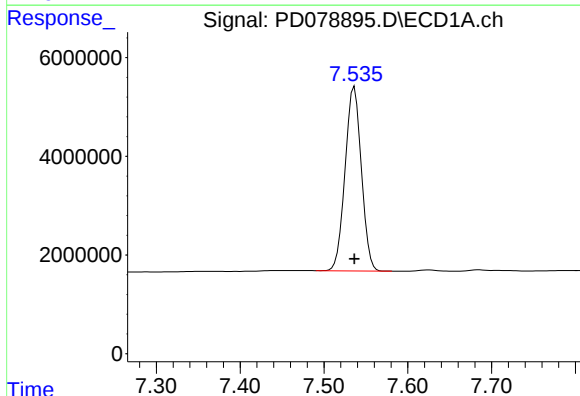


#20 Methoxychlor

R.T.: 7.536 min
Delta R.T.: 0.000 min
Response: 50445740
Conc: 200.00 ng/ml

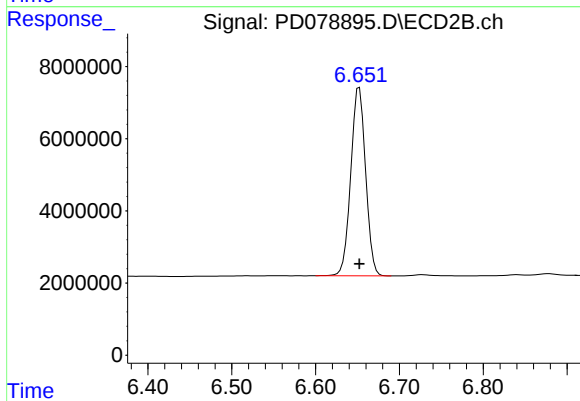

#20 Methoxychlor


R.T.: 6.652 min
Delta R.T.: 0.000 min
Response: 64329185
Conc: 200.00 ng/ml

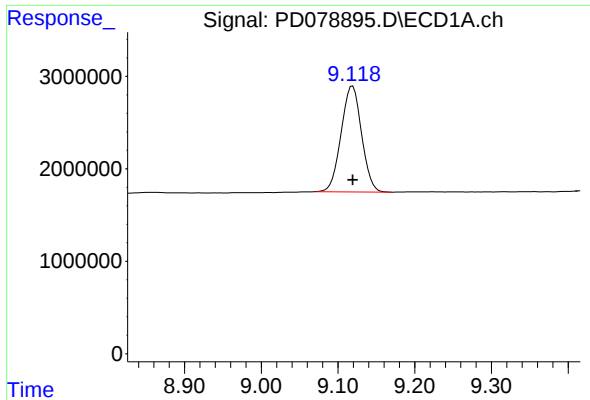

#27 Decachlorobiphenyl

R.T.: 9.119 min
Delta R.T.: 0.000 min
Response: 21287141
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

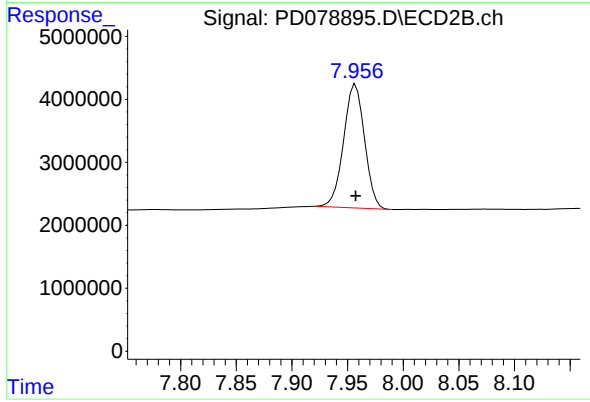

#27 Decachlorobiphenyl

R.T.: 7.957 min
Delta R.T.: 0.000 min
Response: 25684140
Conc: 40.00 ng/ml