

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101623\
 Data File : PD078897.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2023 01:44
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 05:15:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101623CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 05:13:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.806	15786688	21694623	40.393	39.197
27)	SA Decachlor...	9.118	7.958	39093010	45105508	73.458	70.246
Target Compounds							
2)	A alpha-BHC	4.026	3.310	24888516	31793908	40.560	40.897
3)	MA gamma-BHC...	4.360	3.640	24853506	30039429	41.476	40.574
4)	MA Heptachlor	4.953	3.984	27332964	29319948	41.160	39.548
9)	A Endosulfan I	6.110	5.138	21674086	25210159	38.629	39.625
13)	MA Dieldrin	6.386	5.403	44474463	55632599	79.314	81.479
14)	MA Endrin	6.616	5.678	36949876	48836936	79.084	81.201
16)	A 4,4'-DDD	6.747	5.825	33046098	42601996	79.619	80.579
17)	MA 4,4'-DDT	7.062	6.077	35499744	43336523	79.572	82.056
20)	A Methoxychlor	7.536	6.652	97656531	125.3E6	387.175	389.552


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101623\
Data File : PD078897.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2023 01:44
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 05:15:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101623CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 05:13:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

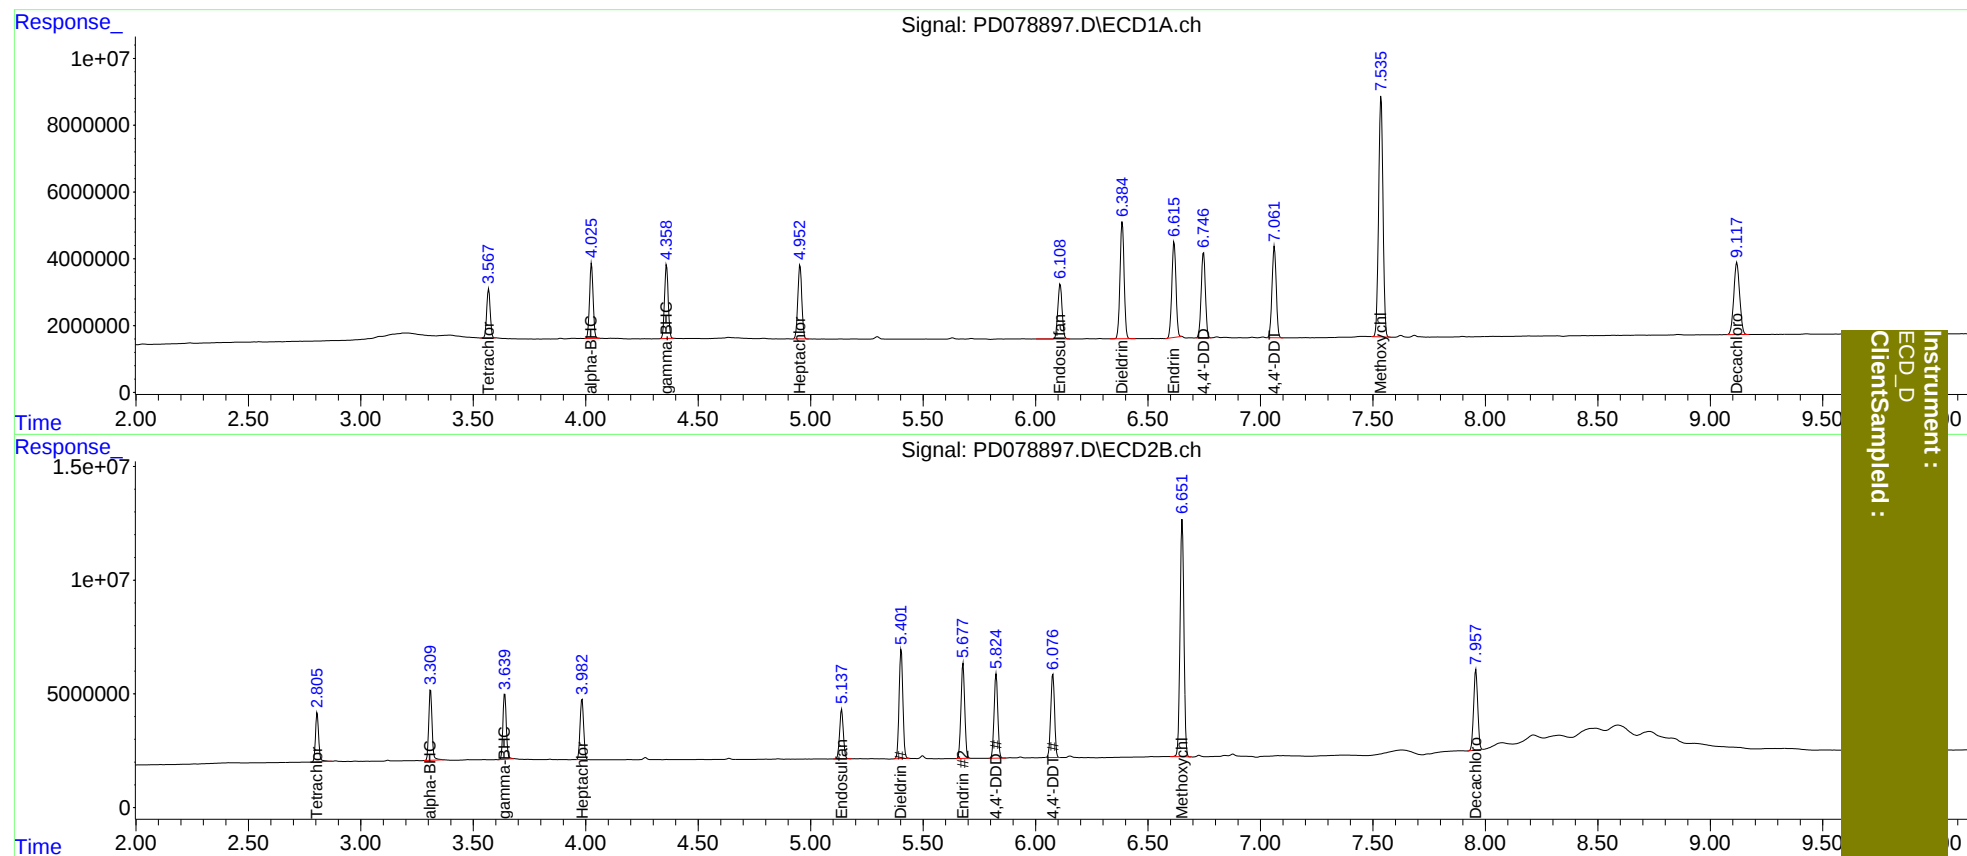


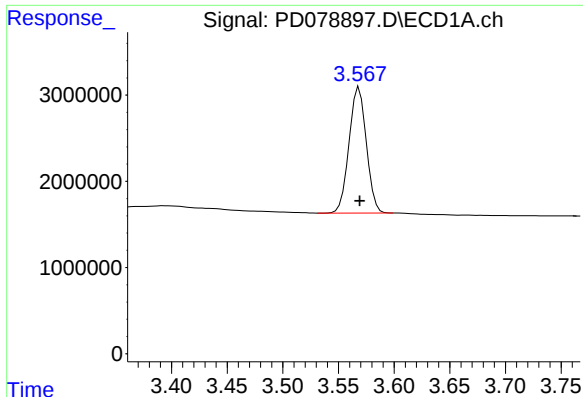

#1 Tetrachloro-m-xylene


R.T.: 3.569 min
Delta R.T.: 0.000 min
Response: 15786688
Conc: 40.39 ng/ml

Instrument :
ECD_D
ClientSampleId :

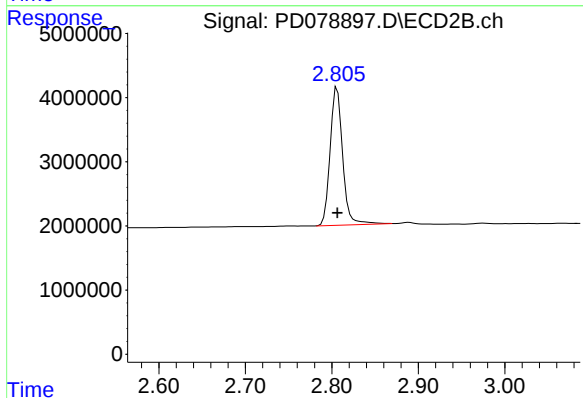


#1 Tetrachloro-m-xylene

R.T.: 2.806 min
Delta R.T.: 0.000 min
Response: 21694623
Conc: 39.20 ng/ml

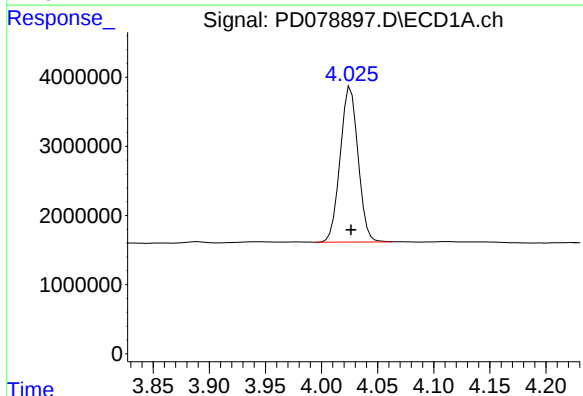


#2 alpha-BHC

R.T.: 4.026 min
Delta R.T.: 0.000 min
Response: 24888516
Conc: 40.56 ng/ml

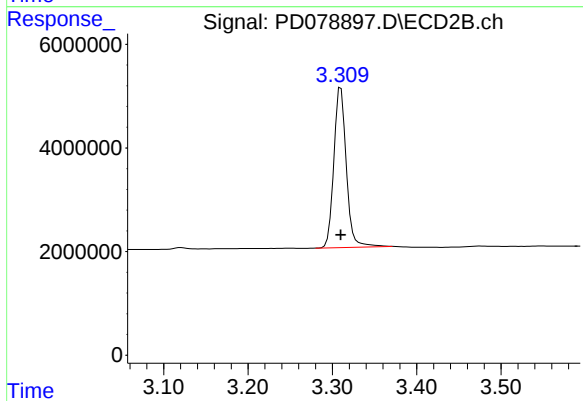

#2 alpha-BHC


R.T.: 3.310 min
Delta R.T.: 0.000 min
Response: 31793908
Conc: 40.90 ng/ml

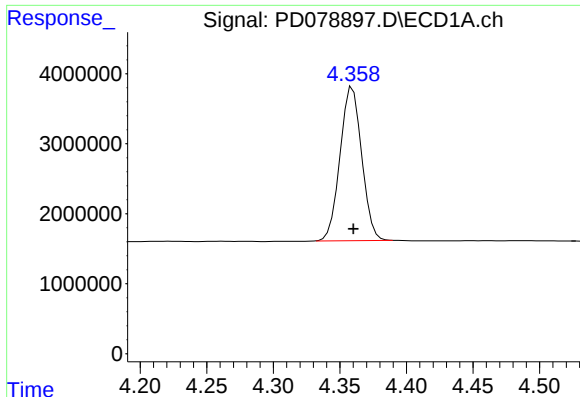

#3 gamma-BHC (Lindane)


R.T.: 4.360 min
Delta R.T.: 0.000 min
Response: 24853506
Conc: 41.48 ng/ml

Instrument :
ECD_D
ClientSampleId :

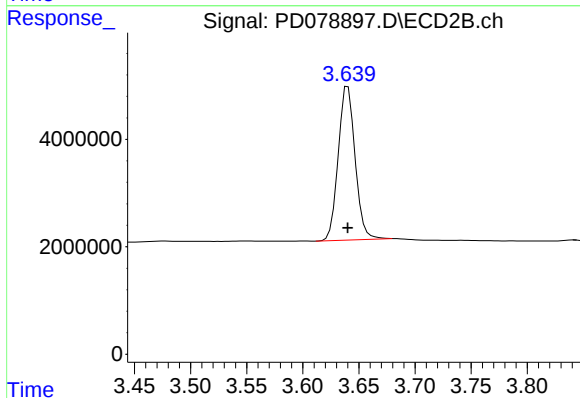


#3 gamma-BHC (Lindane)

R.T.: 3.640 min
Delta R.T.: 0.000 min
Response: 30039429
Conc: 40.57 ng/ml

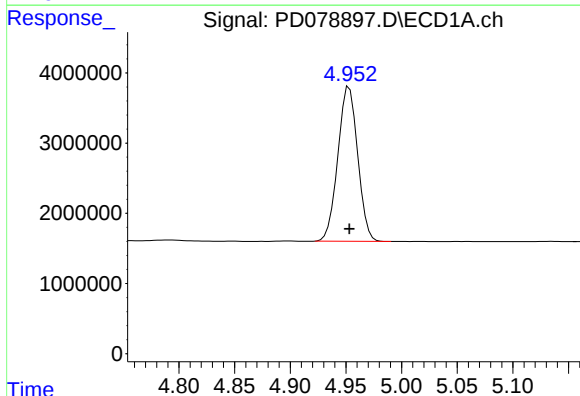


#4 Heptachlor

R.T.: 4.953 min
Delta R.T.: 0.000 min
Response: 27332964
Conc: 41.16 ng/ml

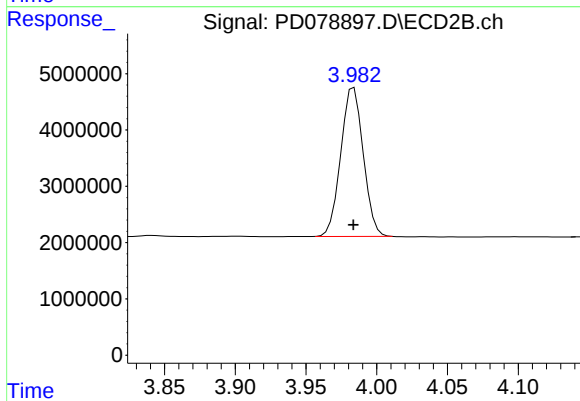

#4 Heptachlor


R.T.: 3.984 min
Delta R.T.: 0.000 min
Response: 29319948
Conc: 39.55 ng/ml

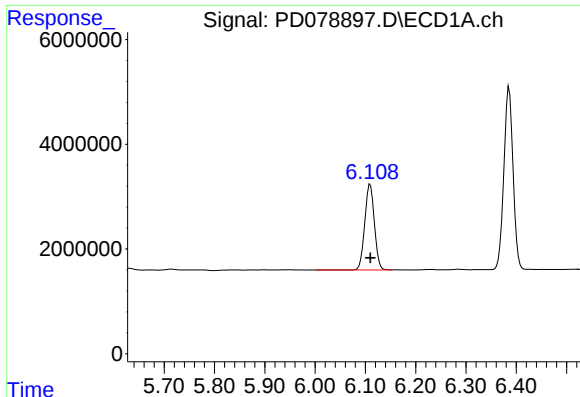

#9 Endosulfan I


R.T.: 6.110 min
Delta R.T.: 0.000 min
Response: 21674086
Conc: 38.63 ng/ml

Instrument :
ECD_D
ClientSampleId :

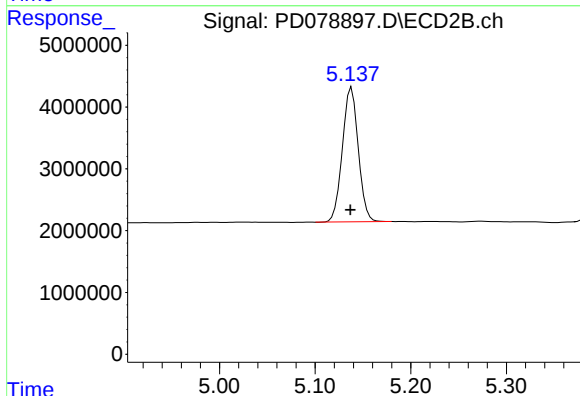


#9 Endosulfan I

R.T.: 5.138 min
Delta R.T.: 0.001 min
Response: 25210159
Conc: 39.63 ng/ml

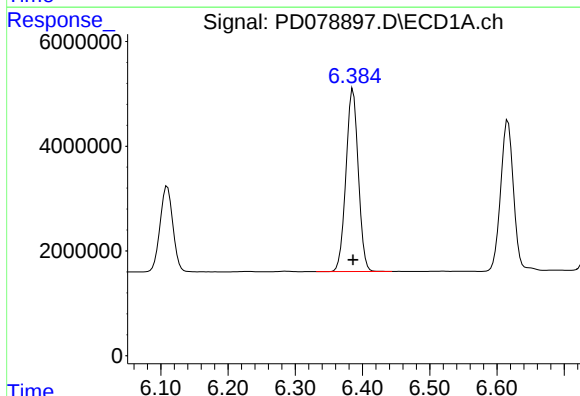


#13 Dieldrin

R.T.: 6.386 min
Delta R.T.: 0.000 min
Response: 44474463
Conc: 79.31 ng/ml

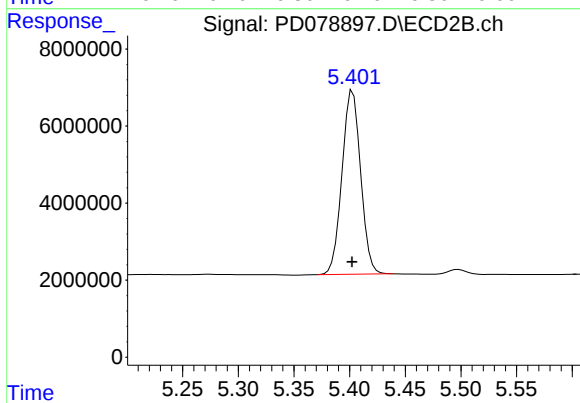

#13 Dieldrin


R.T.: 5.403 min
Delta R.T.: 0.000 min
Response: 55632599
Conc: 81.48 ng/ml

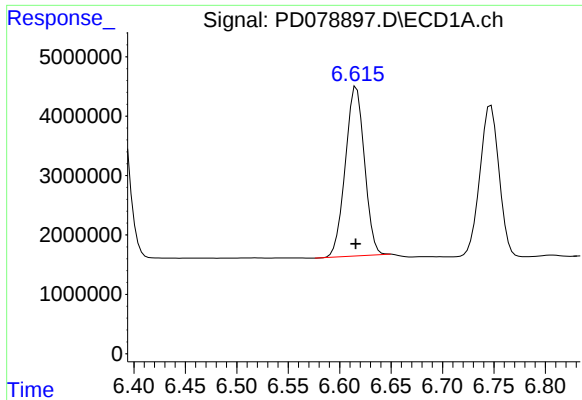

#14 Endrin


R.T.: 6.616 min
Delta R.T.: 0.000 min
Response: 36949876
Conc: 79.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

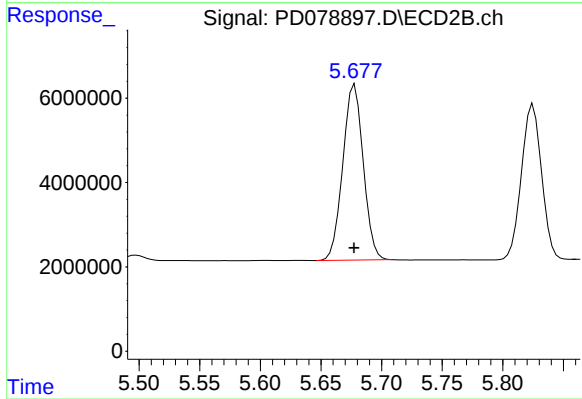


#14 Endrin

R.T.: 5.678 min
Delta R.T.: 0.000 min
Response: 48836936
Conc: 81.20 ng/ml

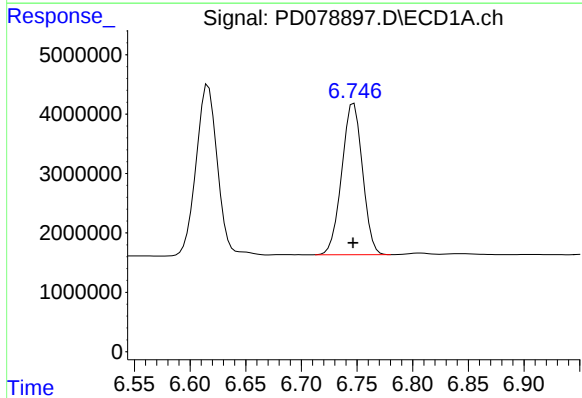


#16 4,4'-DDD

R.T.: 6.747 min
Delta R.T.: 0.000 min
Response: 33046098
Conc: 79.62 ng/ml

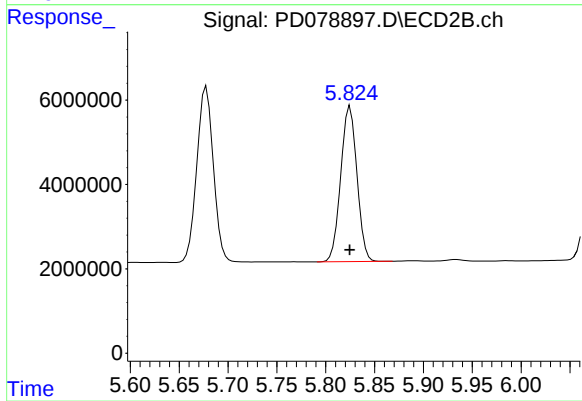

#16 4,4'-DDD


R.T.: 5.825 min
Delta R.T.: 0.000 min
Response: 42601996
Conc: 80.58 ng/ml

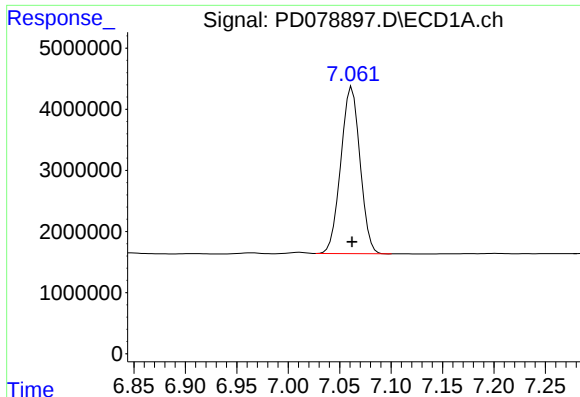

#17 4,4'-DDT


R.T.: 7.062 min
Delta R.T.: 0.000 min
Response: 35499744
Conc: 79.57 ng/ml

Instrument :
ECD_D
ClientSampleId :

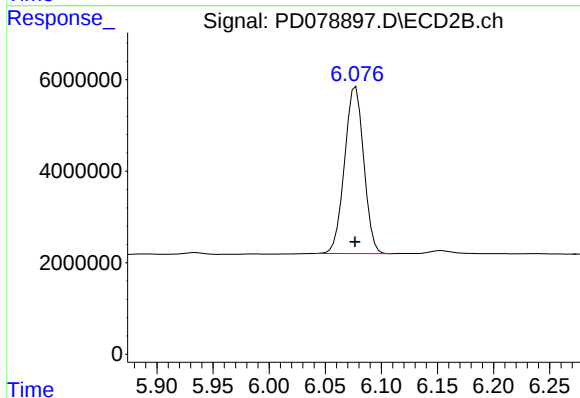


#17 4,4'-DDT

R.T.: 6.077 min
Delta R.T.: 0.000 min
Response: 43336523
Conc: 82.06 ng/ml

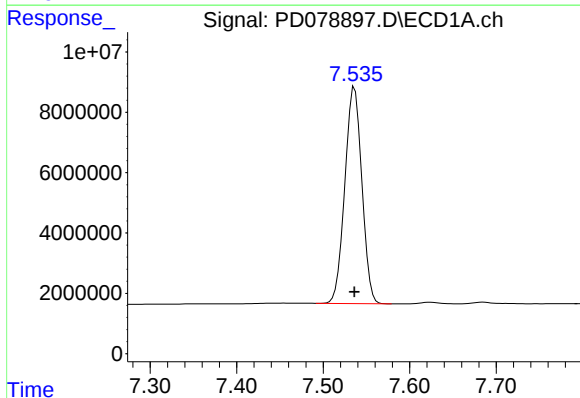


#20 Methoxychlor

R.T.: 7.536 min
Delta R.T.: 0.000 min
Response: 97656531
Conc: 387.17 ng/ml

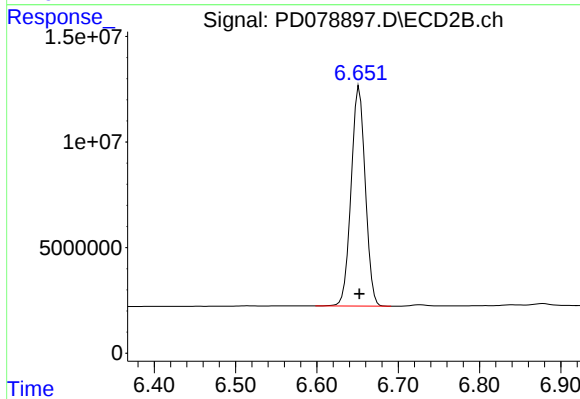

#20 Methoxychlor


R.T.: 6.652 min
Delta R.T.: 0.000 min
Response: 125297909
Conc: 389.55 ng/ml

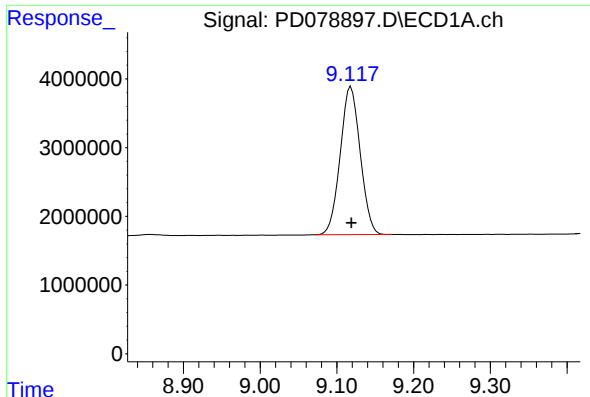

#27 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: 0.000 min
Response: 39093010
Conc: 73.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

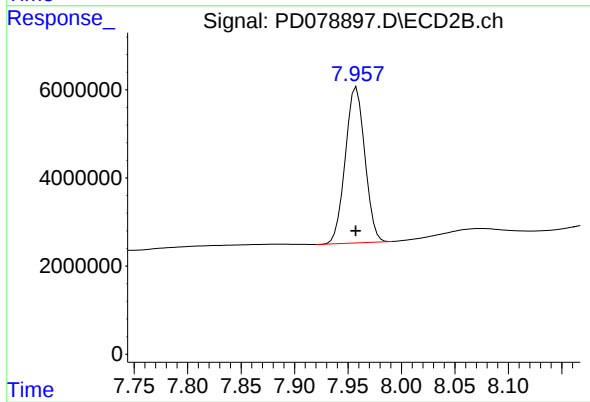

#27 Decachlorobiphenyl

R.T.: 7.958 min
Delta R.T.: 0.000 min
Response: 45105508
Conc: 70.25 ng/ml