

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101623\
 Data File : PD078901.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2023 02:37
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 05:16:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101623CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 05:13:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.806	63622557	84707443	162.790	153.047
27)	SA Decachlor...	9.118	7.957	138.5E6	176.8E6	260.163	275.280
Target Compounds							
2)	A alpha-BHC	4.026	3.309	112.1E6	135.7E6	182.713	174.535
3)	MA gamma-BHC...	4.360	3.640	105.1E6	125.8E6	175.402	169.885
4)	MA Heptachlor	4.953	3.983	109.4E6	119.7E6	164.787	161.404
9)	A Endosulfan I	6.110	5.137	82857995	101.3E6	147.674	159.153
13)	MA Dieldrin	6.385	5.402	182.1E6	233.5E6	324.697	342.030
14)	MA Endrin	6.616	5.677	150.5E6	203.1E6	322.085	337.720
16)	A 4,4'-DDD	6.746	5.824	135.1E6	177.9E6	325.438	336.527
17)	MA 4,4'-DDT	7.062	6.077	144.2E6	183.0E6	323.129	346.479
20)	A Methoxychlor	7.535	6.652	376.8E6	470.2E6	1493.865	1461.903


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101623\
Data File : PD078901.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2023 02:37
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 05:16:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101623CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 05:13:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

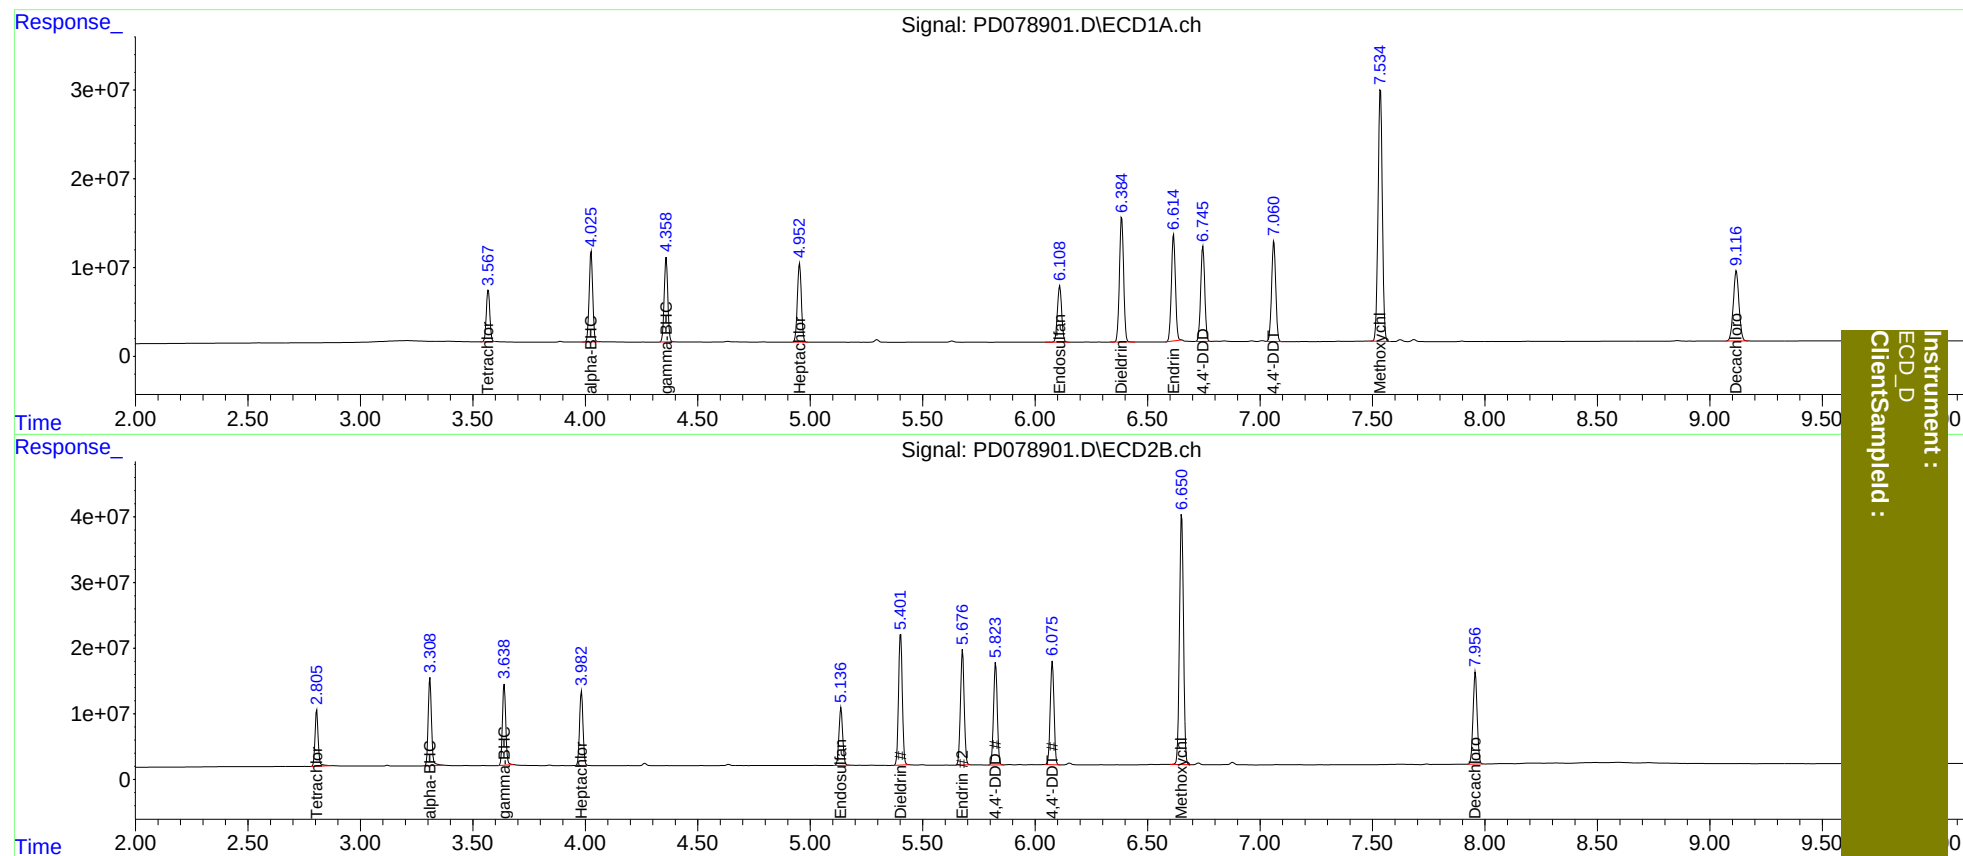


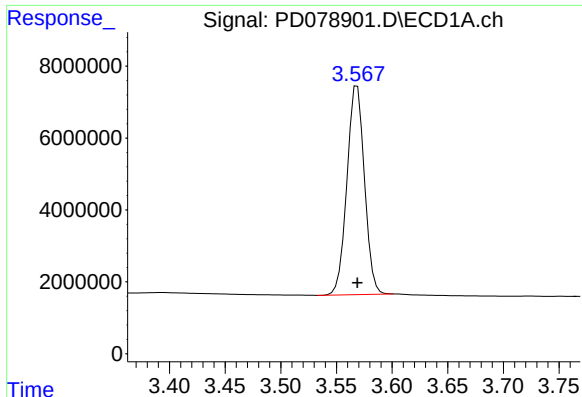

#1 Tetrachloro-m-xylene


R.T.: 3.569 min
Delta R.T.: 0.000 min
Response: 63622557
Conc: 162.79 ng/ml

Instrument :
ECD_D
ClientSampleId :

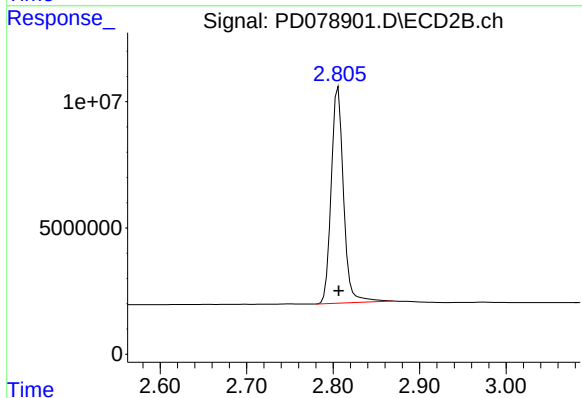


#1 Tetrachloro-m-xylene

R.T.: 2.806 min
Delta R.T.: 0.000 min
Response: 84707443
Conc: 153.05 ng/ml

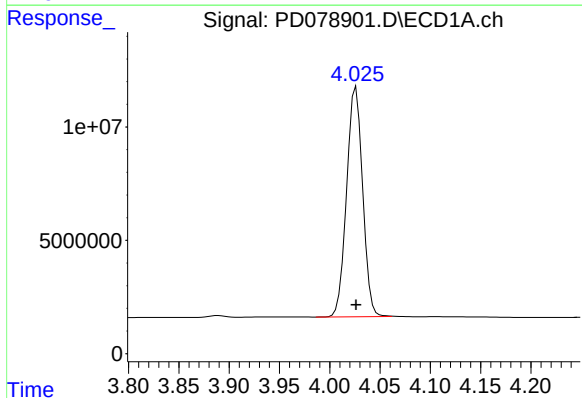


#2 alpha-BHC

R.T.: 4.026 min
Delta R.T.: 0.000 min
Response: 112115482
Conc: 182.71 ng/ml

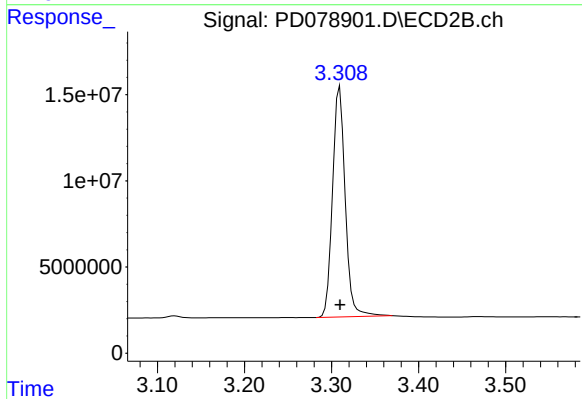

#2 alpha-BHC


R.T.: 3.309 min
Delta R.T.: 0.000 min
Response: 135687327
Conc: 174.53 ng/ml

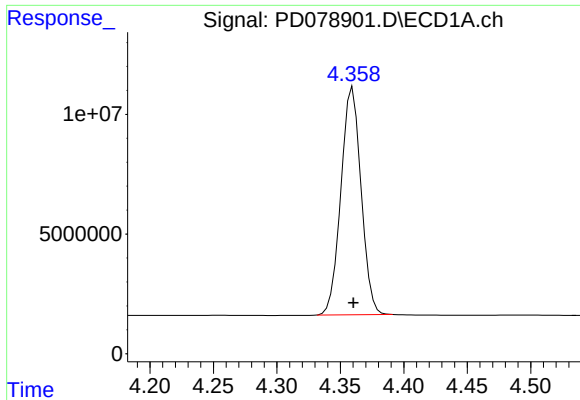

#3 gamma-BHC (Lindane)


R.T.: 4.360 min
Delta R.T.: 0.000 min
Response: 105105789
Conc: 175.40 ng/ml

Instrument :
ECD_D
ClientSampleId :

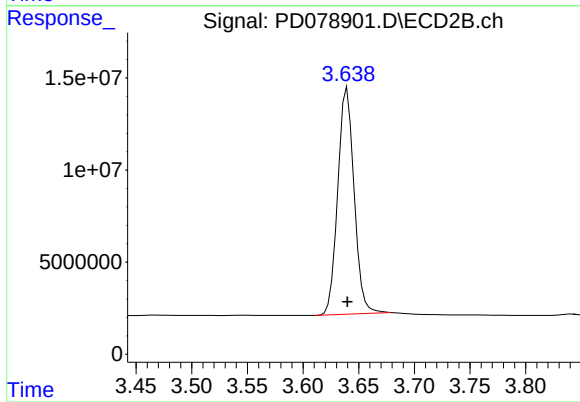


#3 gamma-BHC (Lindane)

R.T.: 3.640 min
Delta R.T.: 0.000 min
Response: 125777916
Conc: 169.89 ng/ml

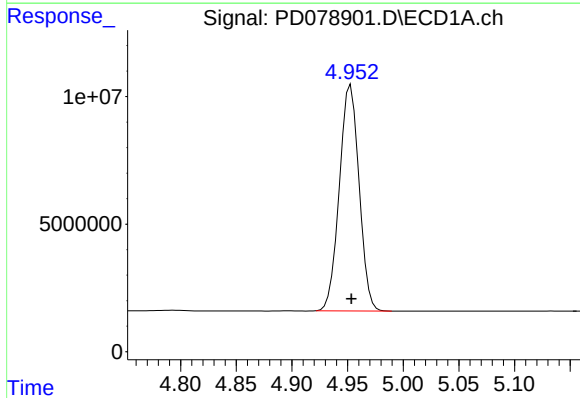


#4 Heptachlor

R.T.: 4.953 min
Delta R.T.: 0.000 min
Response: 109428317
Conc: 164.79 ng/ml

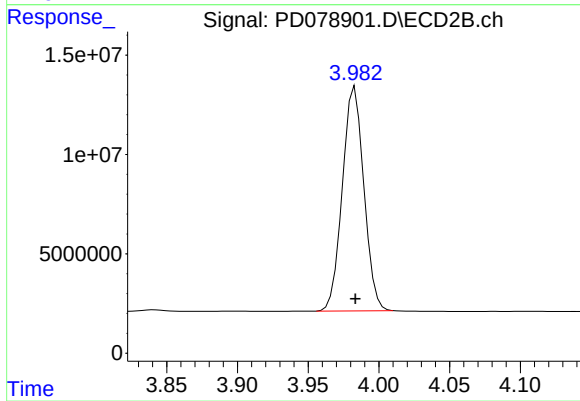

#4 Heptachlor


R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 119662143
Conc: 161.40 ng/ml

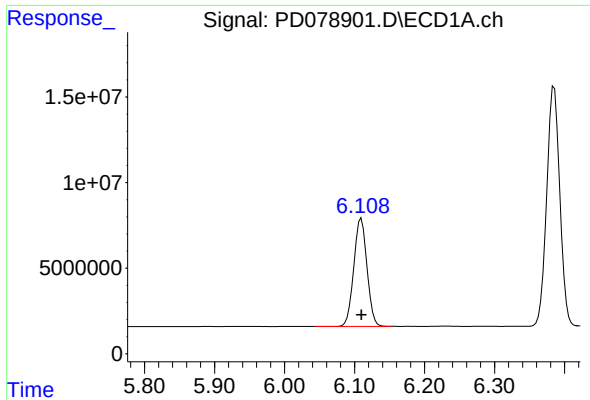

#9 Endosulfan I


R.T.: 6.110 min
Delta R.T.: 0.000 min
Response: 82857995
Conc: 147.67 ng/ml

Instrument :
ECD_D
ClientSampleId :

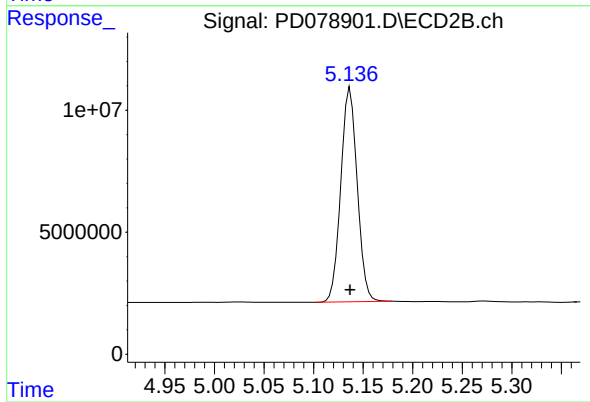


#9 Endosulfan I

R.T.: 5.137 min
Delta R.T.: 0.000 min
Response: 101254966
Conc: 159.15 ng/ml

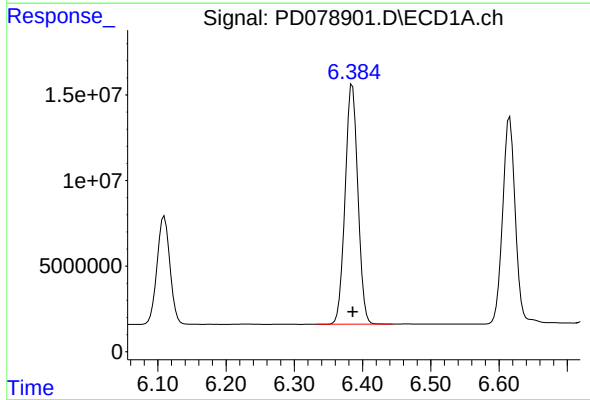


#13 Dieldrin

R.T.: 6.385 min
Delta R.T.: 0.000 min
Response: 182069582
Conc: 324.70 ng/ml

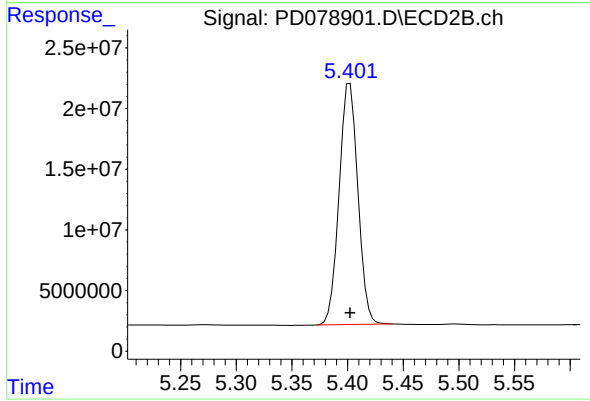

#13 Dieldrin


R.T.: 5.402 min
Delta R.T.: 0.000 min
Response: 233533511
Conc: 342.03 ng/ml

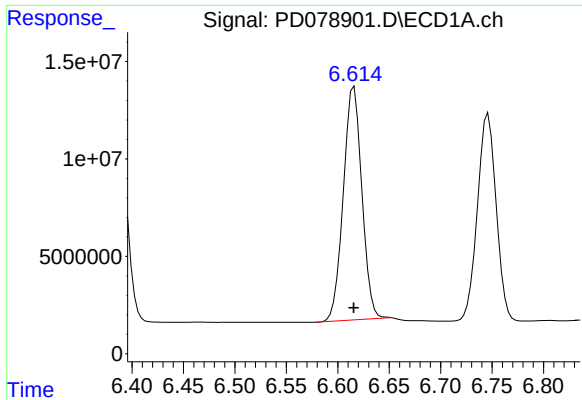

#14 Endrin


R.T.: 6.616 min
Delta R.T.: 0.000 min
Response: 150485068
Conc: 322.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

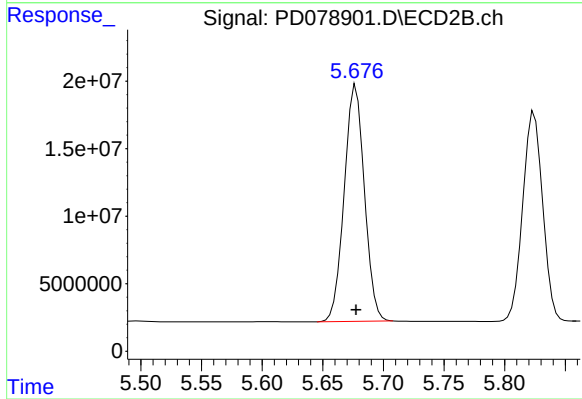


#14 Endrin

R.T.: 5.677 min
Delta R.T.: 0.000 min
Response: 203115317
Conc: 337.72 ng/ml

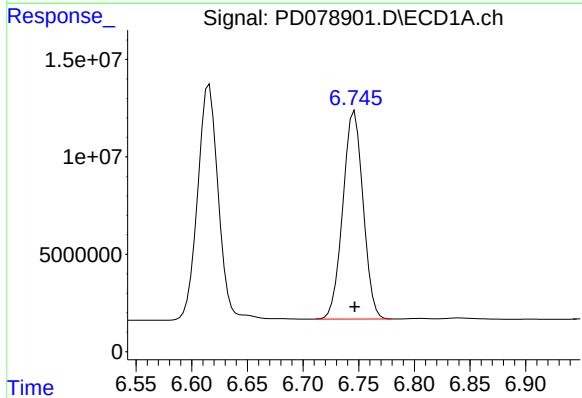


#16 4,4'-DDD

R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 135072993
Conc: 325.44 ng/ml

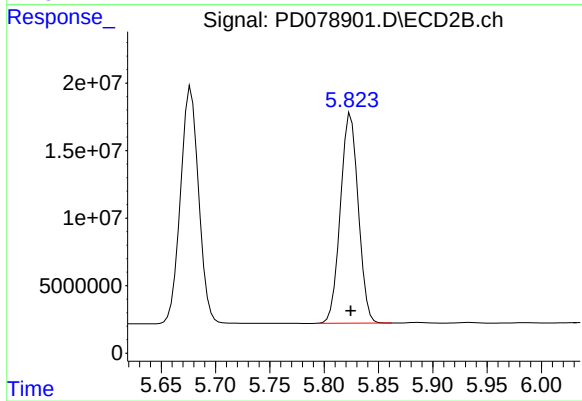

#16 4,4'-DDD


R.T.: 5.824 min
Delta R.T.: 0.000 min
Response: 177920298
Conc: 336.53 ng/ml

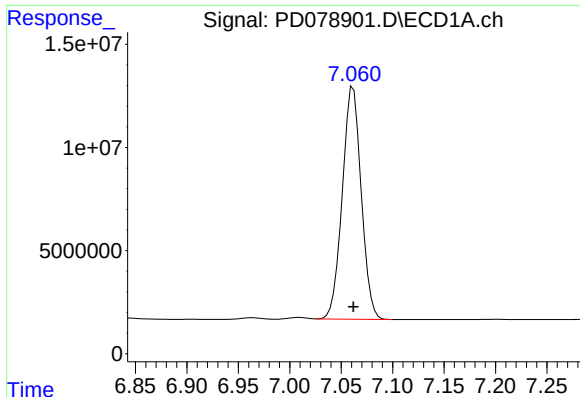

#17 4,4'-DDT


R.T.: 7.062 min
Delta R.T.: 0.000 min
Response: 144158277
Conc: 323.13 ng/ml

Instrument :
ECD_D
ClientSampleId :

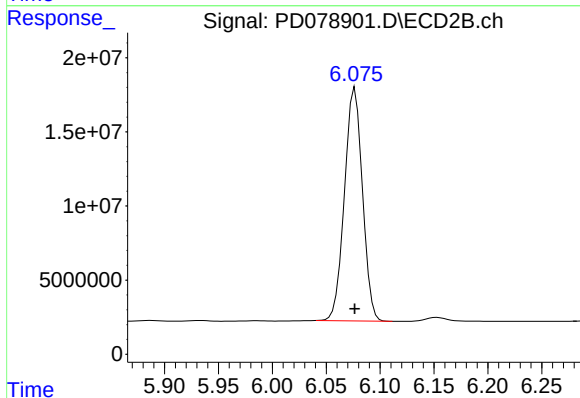


#17 4,4'-DDT

R.T.: 6.077 min
Delta R.T.: 0.000 min
Response: 182987171
Conc: 346.48 ng/ml

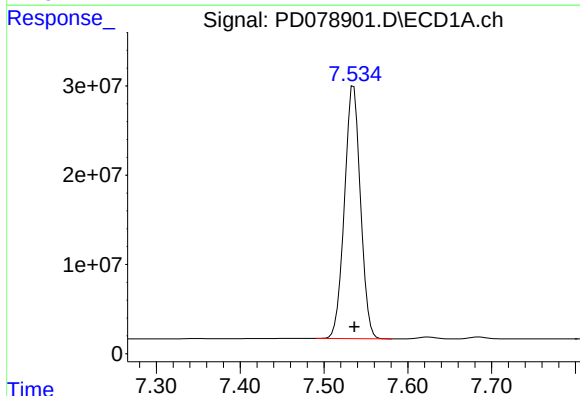


#20 Methoxychlor

R.T.: 7.535 min
Delta R.T.: 0.000 min
Response: 376795755
Conc: 1493.87 ng/ml

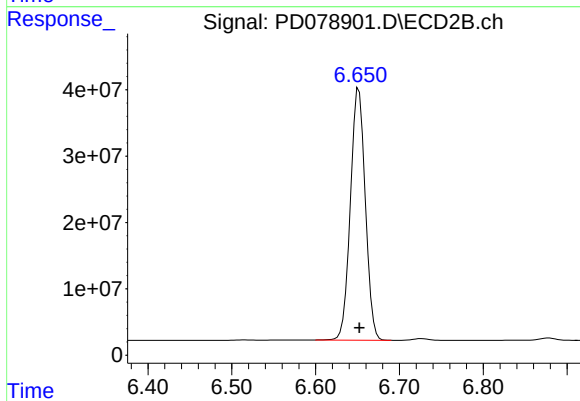

#20 Methoxychlor


R.T.: 6.652 min
Delta R.T.: 0.000 min
Response: 470215257
Conc: 1461.90 ng/ml

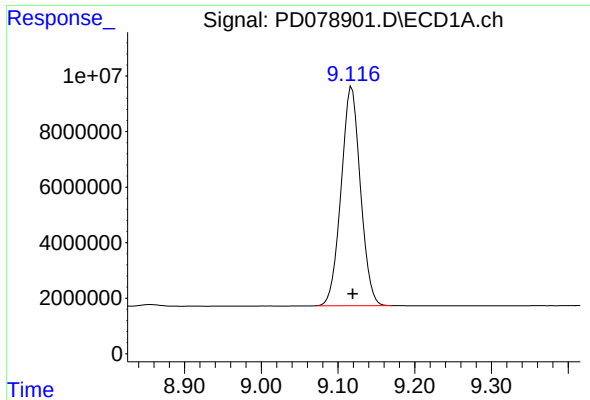

#27 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: -0.001 min
Response: 138453193
Conc: 260.16 ng/ml

Instrument :
ECD_D
ClientSampleId :

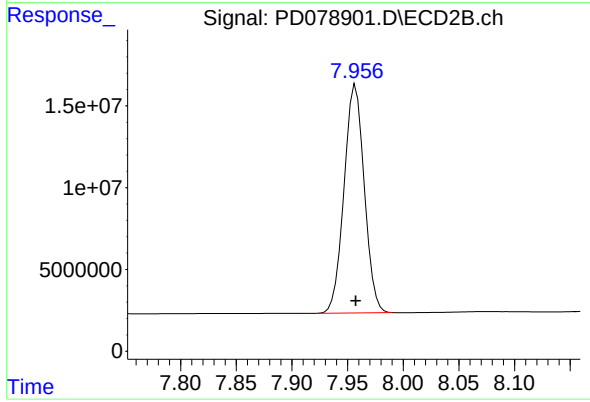

#27 Decachlorobiphenyl

R.T.: 7.957 min
Delta R.T.: 0.000 min
Response: 176758481
Conc: 275.28 ng/ml