

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101623\
 Data File : PD078903.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2023 03:03
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 05:16:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101623CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 05:13:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.568	2.806	120.7E6	168.9E6	308.740	305.103
27)	SA Decachlor...	9.119	7.957	269.9E6	350.4E6	507.236	545.760
Target Compounds							
2)	A alpha-BHC	4.026	3.310	225.2E6	281.9E6	367.046	362.573
3)	MA gamma-BHC...	4.360	3.640	212.8E6	259.4E6	355.066	350.411
4)	MA Heptachlor	4.952	3.983	223.2E6	243.6E6	336.081	328.524
9)	A Endosulfan I	6.109	5.137	165.3E6	205.1E6	294.524	322.425
13)	MA Dieldrin	6.385	5.402	376.2E6	477.8E6	670.853	699.725
14)	MA Endrin	6.616	5.677	309.5E6	412.5E6	662.453	685.910
16)	A 4,4'-DDD	6.746	5.824	278.3E6	363.5E6	670.411	687.459
17)	MA 4,4'-DDT	7.062	6.076	295.4E6	376.1E6	662.099	712.210
20)	A Methoxychlor	7.536	6.652	751.0E6	881.1E6	2977.264	2739.416


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101623\
Data File : PD078903.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2023 03:03
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 05:16:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101623CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 05:13:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

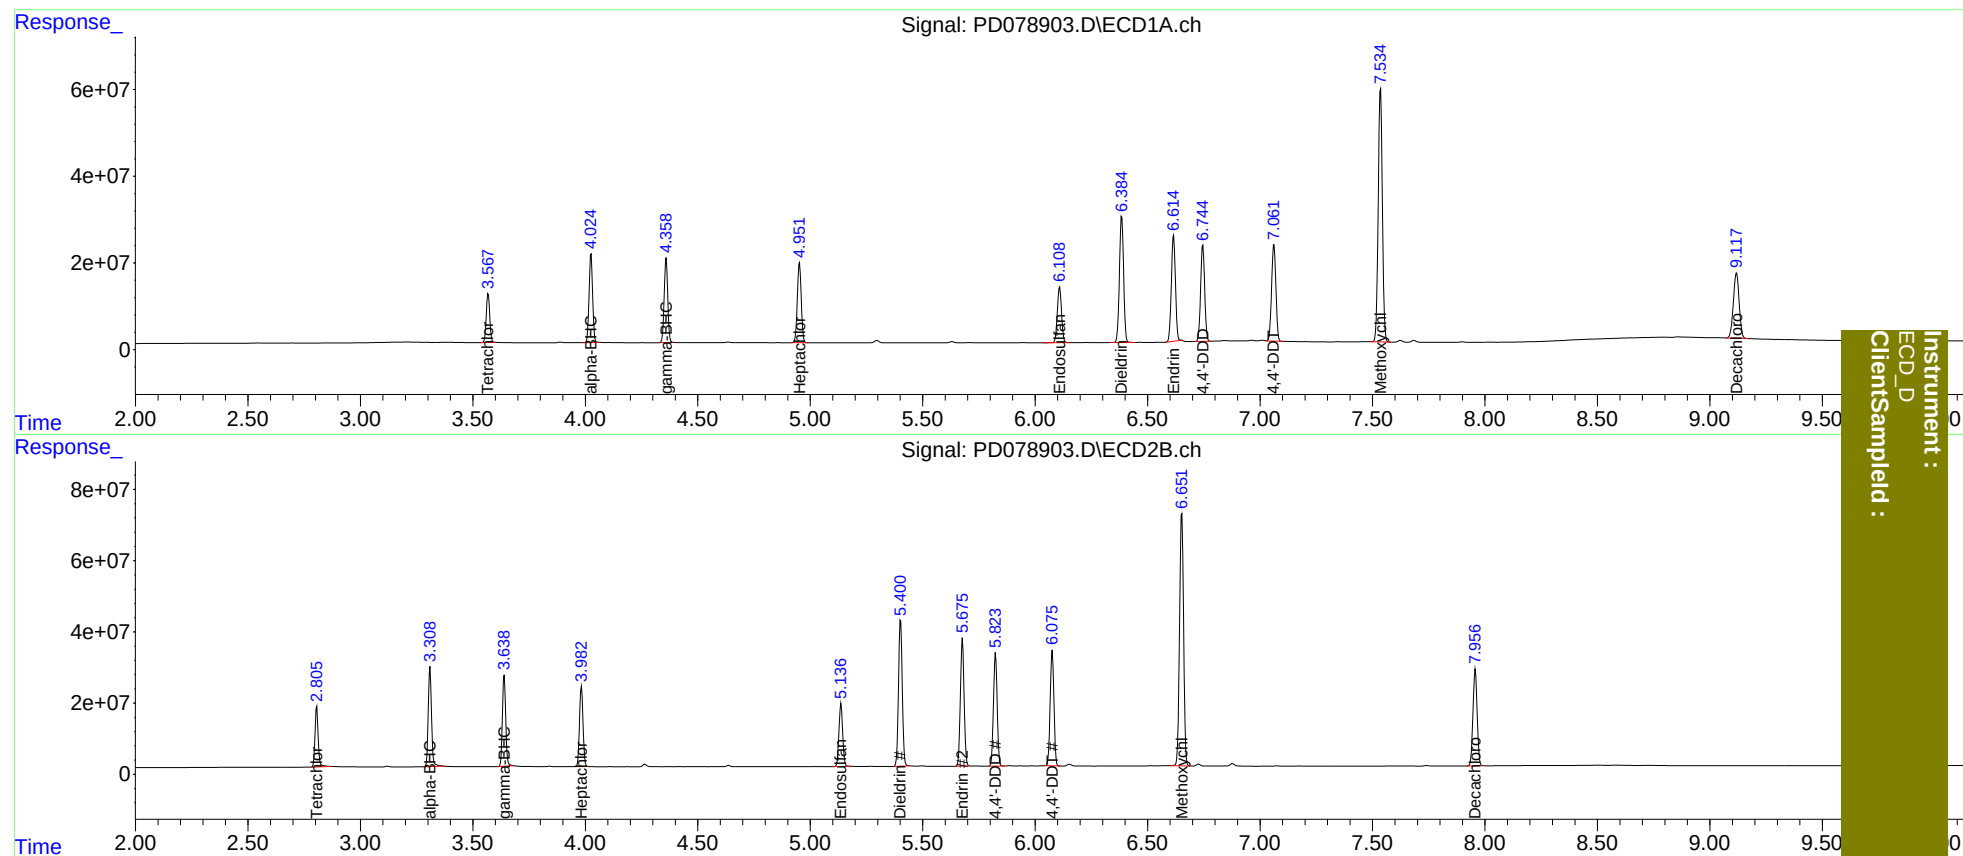


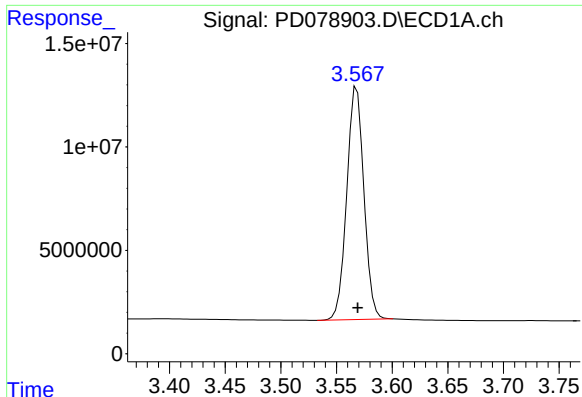

#1 Tetrachloro-m-xylene


R.T.: 3.568 min
Delta R.T.: 0.000 min
Response: 120663730
Conc: 308.74 ng/ml

Instrument :
ECD_D
ClientSampleId :

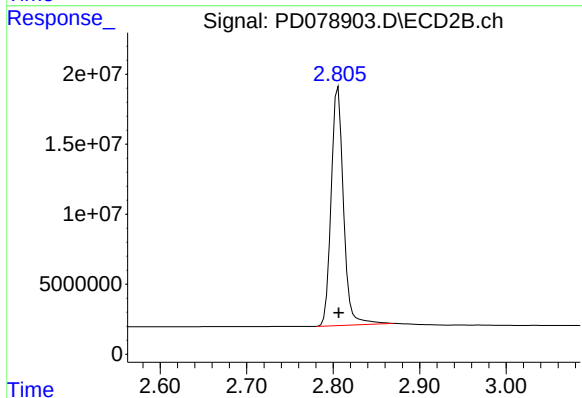


#1 Tetrachloro-m-xylene

R.T.: 2.806 min
Delta R.T.: 0.000 min
Response: 168867009
Conc: 305.10 ng/ml

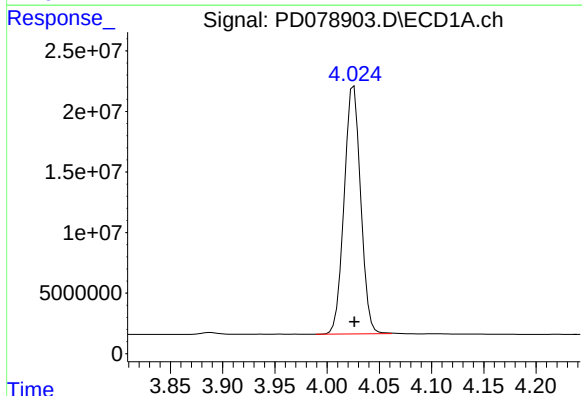


#2 alpha-BHC

R.T.: 4.026 min
Delta R.T.: 0.000 min
Response: 225225094
Conc: 367.05 ng/ml

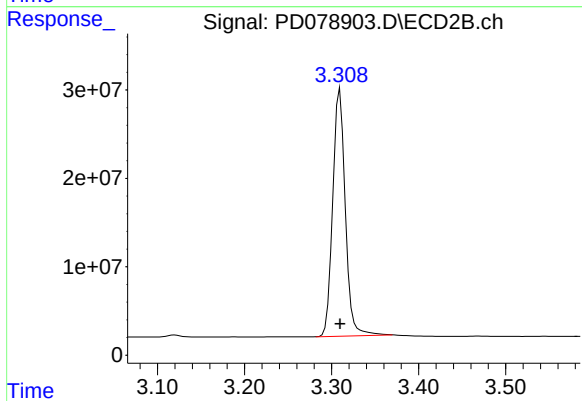

#2 alpha-BHC


R.T.: 3.310 min
Delta R.T.: 0.000 min
Response: 281872873
Conc: 362.57 ng/ml

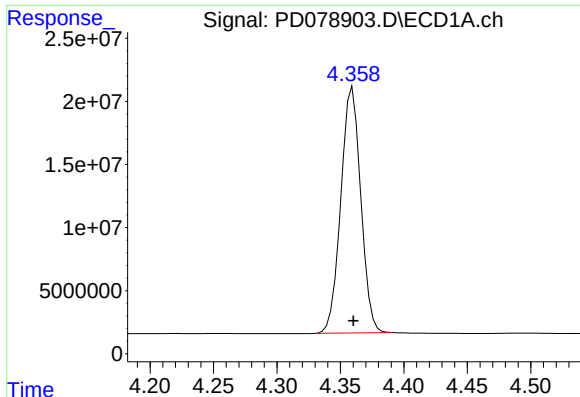

#3 gamma-BHC (Lindane)


R.T.: 4.360 min
Delta R.T.: 0.000 min
Response: 212765198
Conc: 355.07 ng/ml

Instrument :
ECD_D
ClientSampleId :

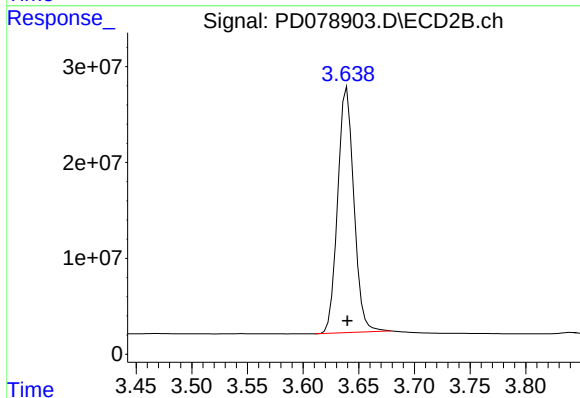


#3 gamma-BHC (Lindane)

R.T.: 3.640 min
Delta R.T.: 0.000 min
Response: 259433612
Conc: 350.41 ng/ml

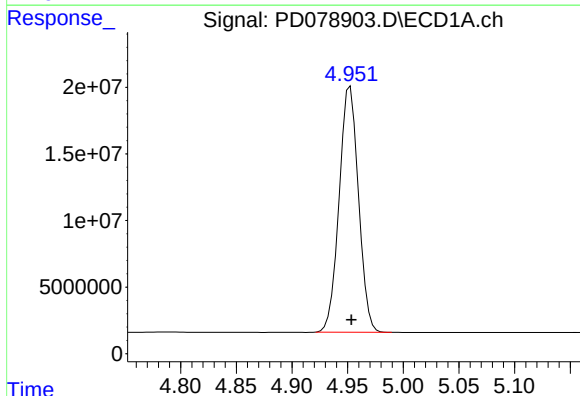


#4 Heptachlor

R.T.: 4.952 min
Delta R.T.: 0.000 min
Response: 223177835
Conc: 336.08 ng/ml

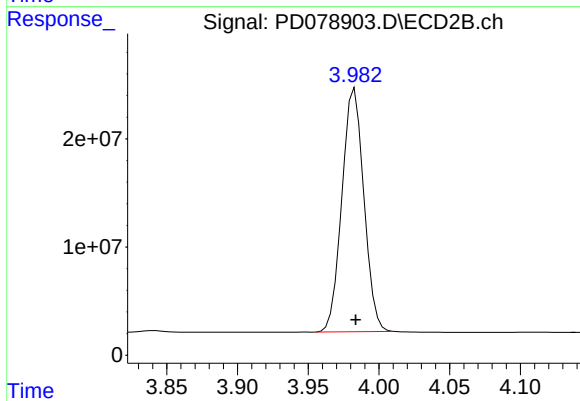

#4 Heptachlor


R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 243562264
Conc: 328.52 ng/ml

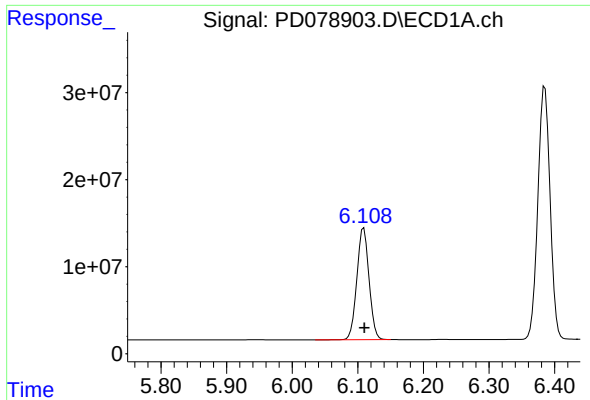

#9 Endosulfan I


R.T.: 6.109 min
Delta R.T.: 0.000 min
Response: 165253670
Conc: 294.52 ng/ml

Instrument :
ECD_D
ClientSampleId :

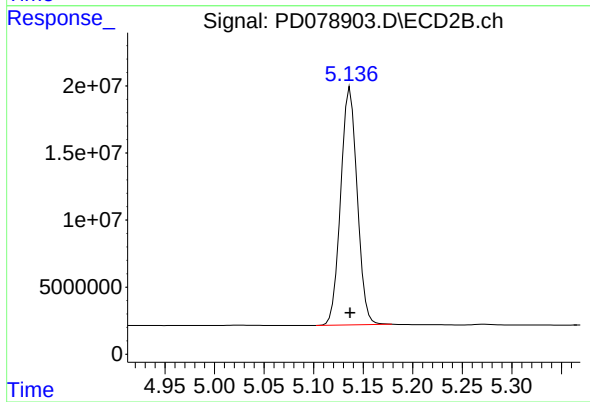


#9 Endosulfan I

R.T.: 5.137 min
Delta R.T.: 0.000 min
Response: 205130789
Conc: 322.42 ng/ml

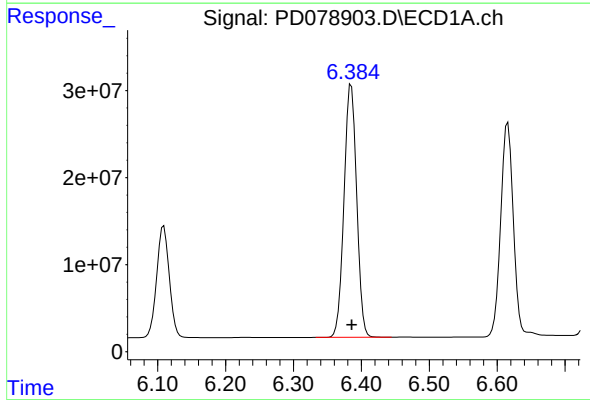


#13 Dieldrin

R.T.: 6.385 min
Delta R.T.: 0.000 min
Response: 376172370
Conc: 670.85 ng/ml

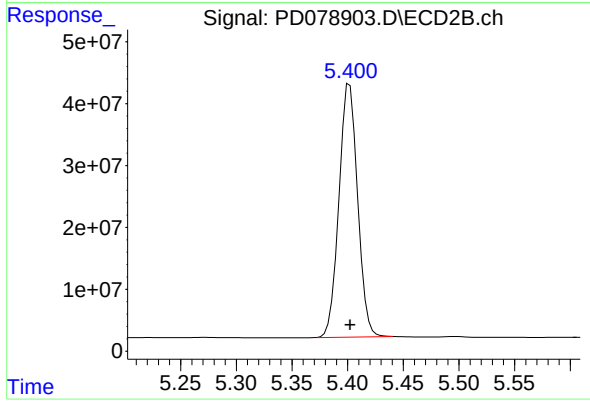

#13 Dieldrin


R.T.: 5.402 min
Delta R.T.: 0.000 min
Response: 477762067
Conc: 699.72 ng/ml

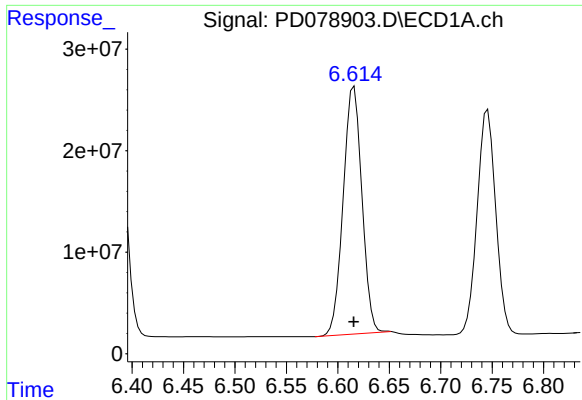

#14 Endrin


R.T.: 6.616 min
Delta R.T.: 0.000 min
Response: 309512451
Conc: 662.45 ng/ml

Instrument :
ECD_D
ClientSampleId :

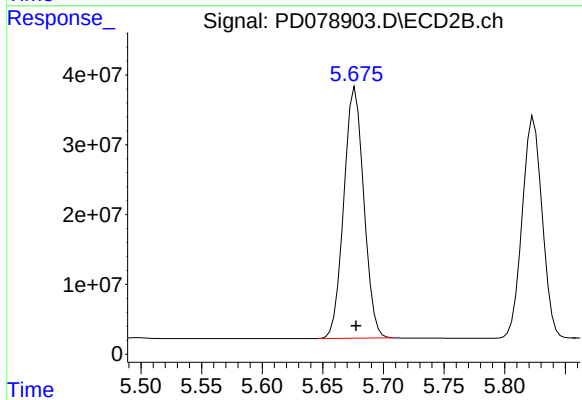


#14 Endrin

R.T.: 5.677 min
Delta R.T.: 0.000 min
Response: 412527384
Conc: 685.91 ng/ml

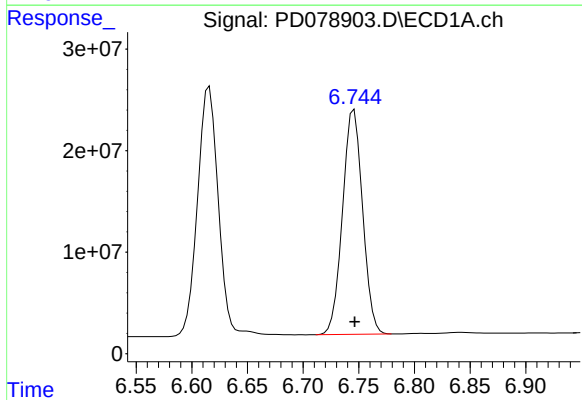


#16 4,4'-DDD

R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 278254369
Conc: 670.41 ng/ml

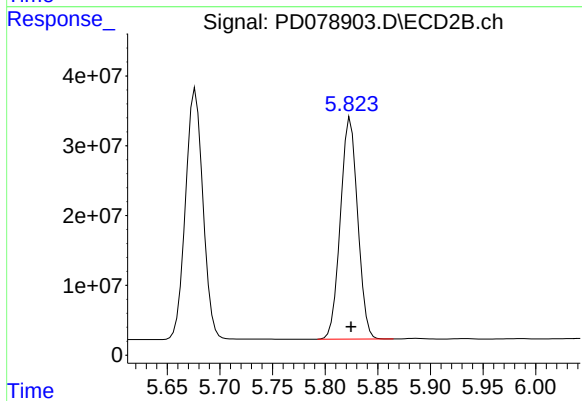

#16 4,4'-DDD


R.T.: 5.824 min
Delta R.T.: 0.000 min
Response: 363456721
Conc: 687.46 ng/ml

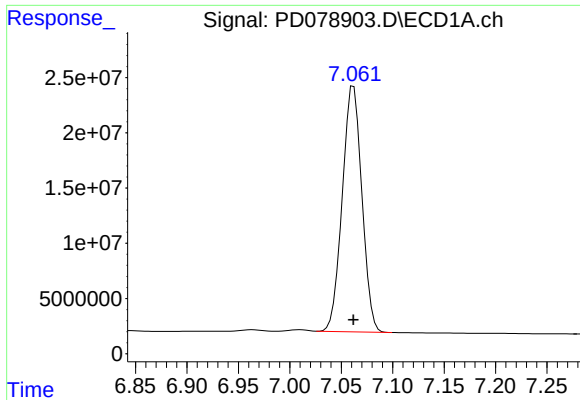

#17 4,4'-DDT


R.T.: 7.062 min
Delta R.T.: 0.000 min
Response: 295383225
Conc: 662.10 ng/ml

Instrument :
ECD_D
ClientSampleId :

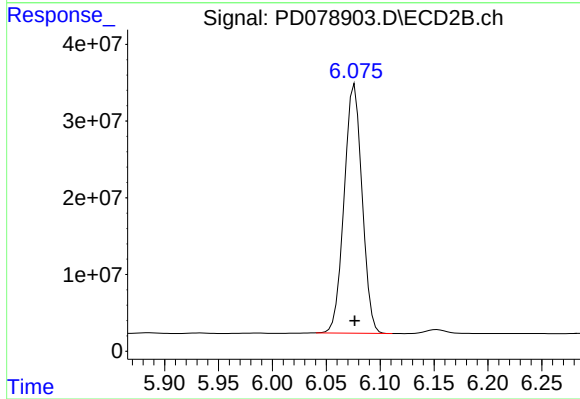


#17 4,4'-DDT

R.T.: 6.076 min
Delta R.T.: 0.000 min
Response: 376141699
Conc: 712.21 ng/ml

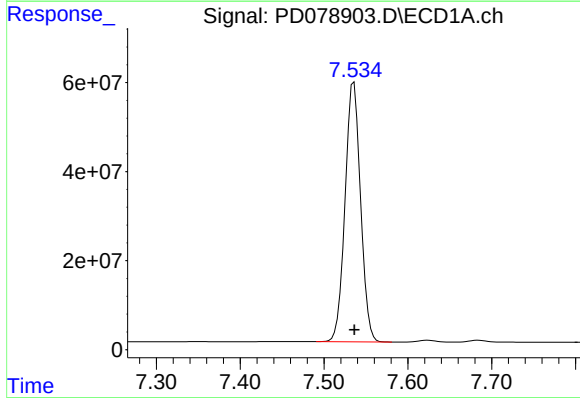


#20 Methoxychlor

R.T.: 7.536 min
Delta R.T.: 0.000 min
Response: 750951335
Conc: 2977.26 ng/ml

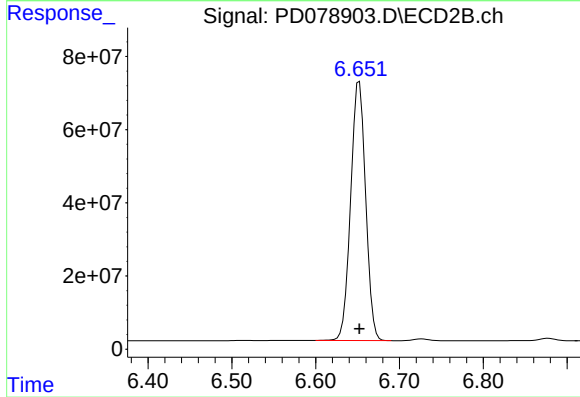

#20 Methoxychlor


R.T.: 6.652 min
Delta R.T.: 0.000 min
Response: 881122062
Conc: 2739.42 ng/ml

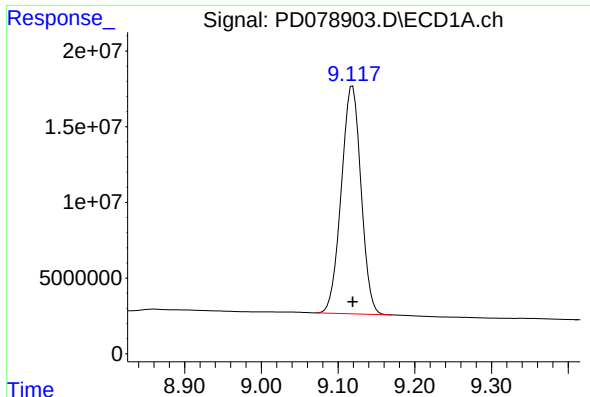

#27 Decachlorobiphenyl

R.T.: 9.119 min
Delta R.T.: 0.000 min
Response: 269940368
Conc: 507.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

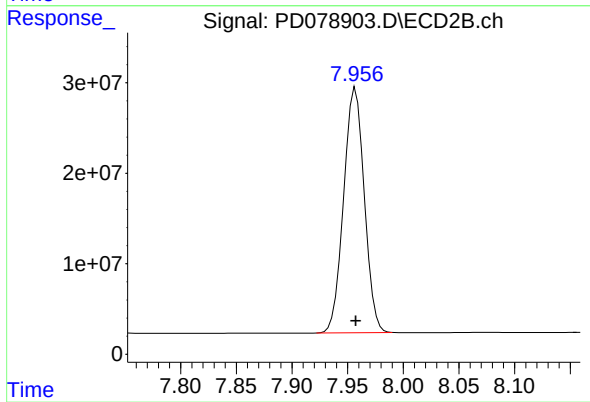

#27 Decachlorobiphenyl

R.T.: 7.957 min
Delta R.T.: 0.000 min
Response: 350434481
Conc: 545.76 ng/ml