

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101623\
 Data File : PD078905.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2023 03:30
 Operator : AR\AJ
 Sample : INDA601
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 05:16:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101623CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 05:13:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.806	236.8E6	333.3E6	605.934	602.161
27)	SA Decachlor...	9.119	7.958	506.4E6	679.1E6	951.523	1057.632
Target Compounds							
2)	A alpha-BHC	4.026	3.310	460.0E6	569.9E6	749.693	733.122
3)	MA gamma-BHC...	4.360	3.640	421.8E6	524.0E6	703.980	707.722
4)	MA Heptachlor	4.953	3.983	421.4E6	482.8E6	634.532	651.189
9)	A Endosulfan I	6.110	5.137	321.5E6	404.6E6	573.017	635.943
13)	MA Dieldrin	6.386	5.403	742.3E6	934.1E6	1323.869	1368.121
14)	MA Endrin	6.616	5.677	609.6E6	801.4E6	1304.742	1332.451
16)	A 4,4'-DDD	6.746	5.825	550.4E6	711.8E6	1326.176	1346.408
17)	MA 4,4'-DDT	7.062	6.077	586.3E6	740.7E6	1314.166	1402.560
20)	A Methoxychlor	7.537	6.652	1430.1E6	1586.1E6	5669.985	4931.169


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101623\
Data File : PD078905.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2023 03:30
Operator : AR\AJ
Sample : INDA601
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 05:16:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101623CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 05:13:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

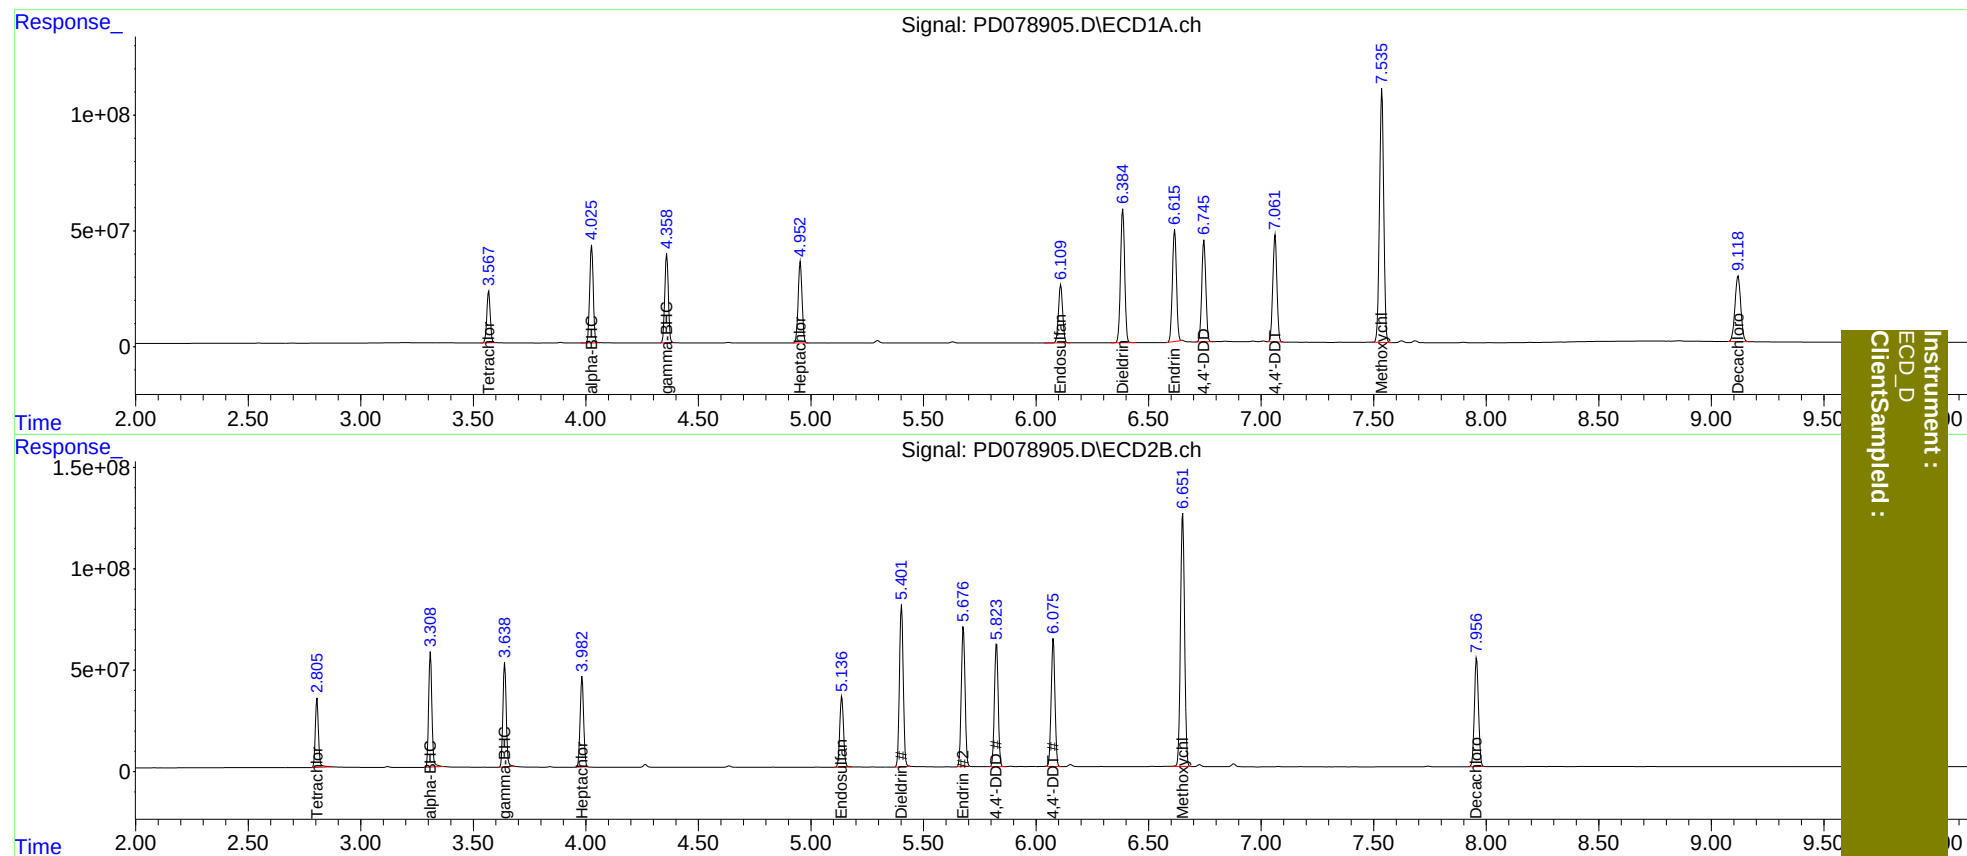


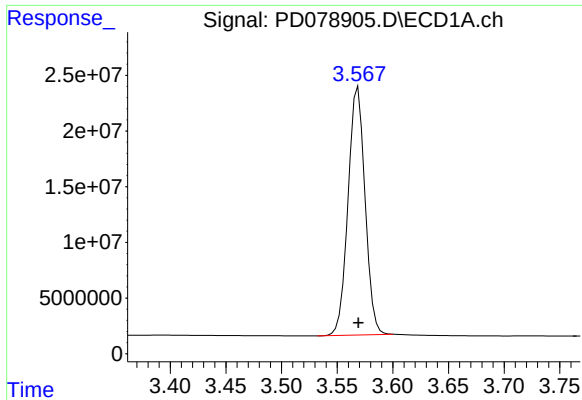

#1 Tetrachloro-m-xylene


R.T.: 3.569 min
Delta R.T.: 0.000 min
Response: 236815347
Conc: 605.93 ng/ml

Instrument :
ECD_D
ClientSampleId :

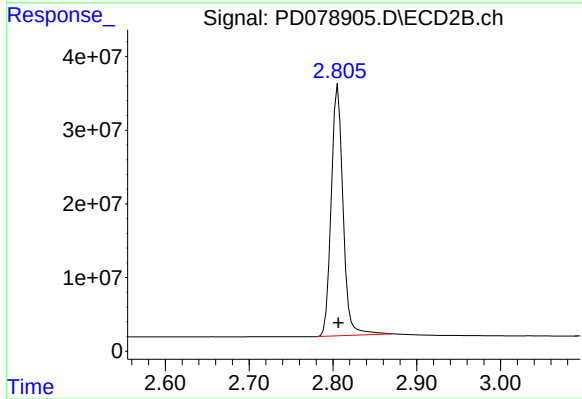


#1 Tetrachloro-m-xylene

R.T.: 2.806 min
Delta R.T.: 0.000 min
Response: 333281110
Conc: 602.16 ng/ml

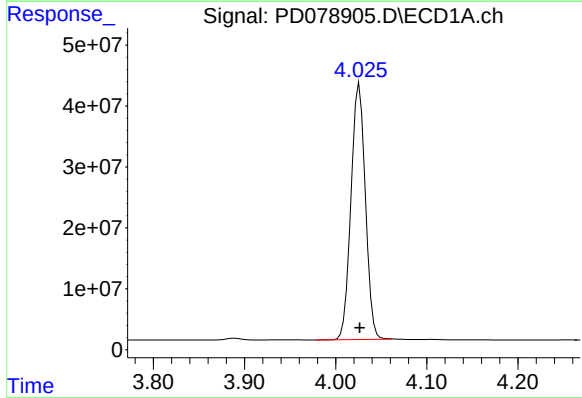


#2 alpha-BHC

R.T.: 4.026 min
Delta R.T.: 0.000 min
Response: 460022617
Conc: 749.69 ng/ml

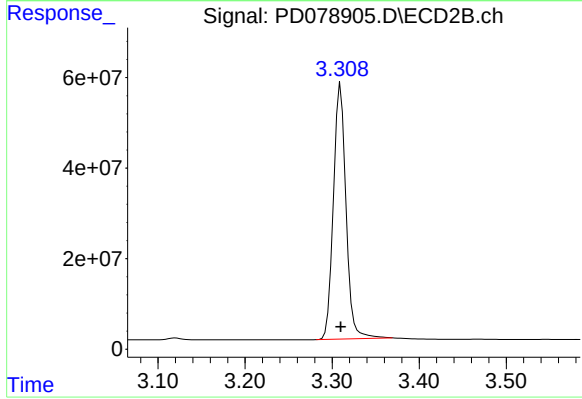

#2 alpha-BHC


R.T.: 3.310 min
Delta R.T.: 0.000 min
Response: 569946185
Conc: 733.12 ng/ml

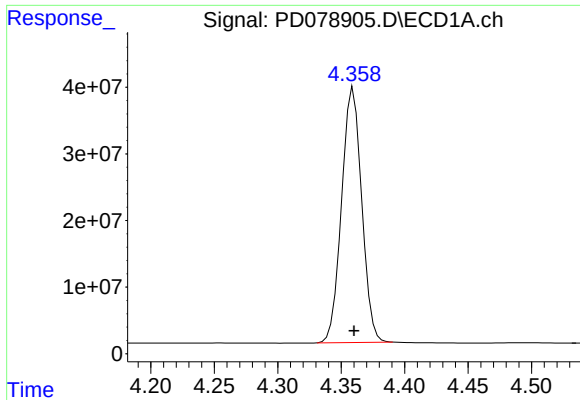

#3 gamma-BHC (Lindane)


R.T.: 4.360 min
Delta R.T.: 0.000 min
Response: 421843955
Conc: 703.98 ng/ml

Instrument :
ECD_D
ClientSampleId :

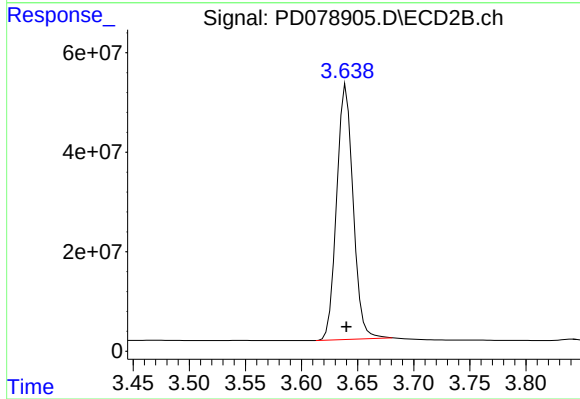


#3 gamma-BHC (Lindane)

R.T.: 3.640 min
Delta R.T.: 0.000 min
Response: 523975875
Conc: 707.72 ng/ml

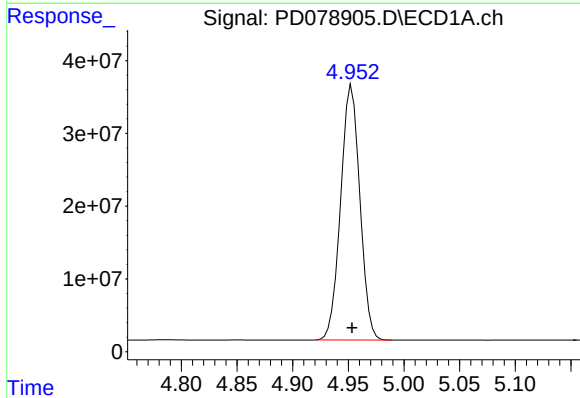


#4 Heptachlor

R.T.: 4.953 min
Delta R.T.: 0.000 min
Response: 421367655
Conc: 634.53 ng/ml

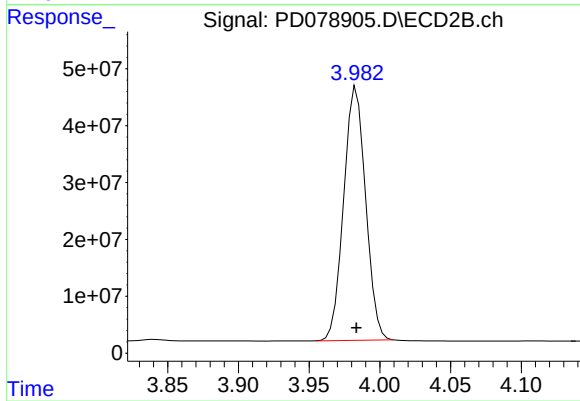

#4 Heptachlor


R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 482781522
Conc: 651.19 ng/ml

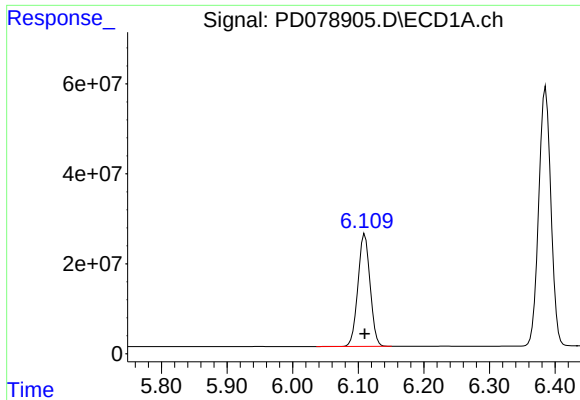

#9 Endosulfan I


R.T.: 6.110 min
Delta R.T.: 0.000 min
Response: 321512039
Conc: 573.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

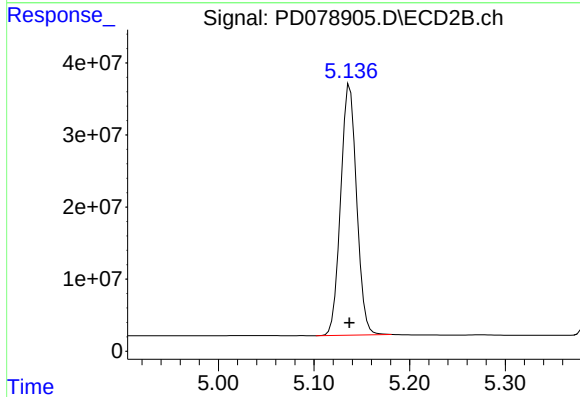


#9 Endosulfan I

R.T.: 5.137 min
Delta R.T.: 0.000 min
Response: 404595020
Conc: 635.94 ng/ml

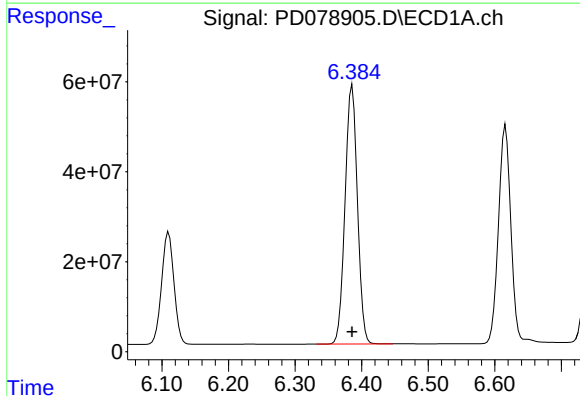


#13 Dieldrin

R.T.: 6.386 min
Delta R.T.: 0.000 min
Response: 742342640
Conc: 1323.87 ng/ml

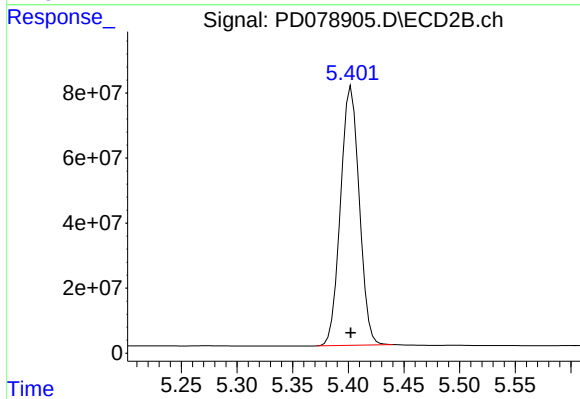

#13 Dieldrin


R.T.: 5.403 min
Delta R.T.: 0.000 min
Response: 934133737
Conc: 1368.12 ng/ml

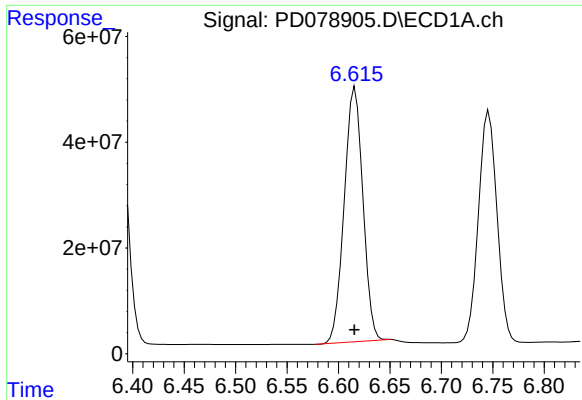

#14 Endrin


R.T.: 6.616 min
Delta R.T.: 0.000 min
Response: 609604188
Conc: 1304.74 ng/ml

Instrument :
ECD_D
ClientSampleId :

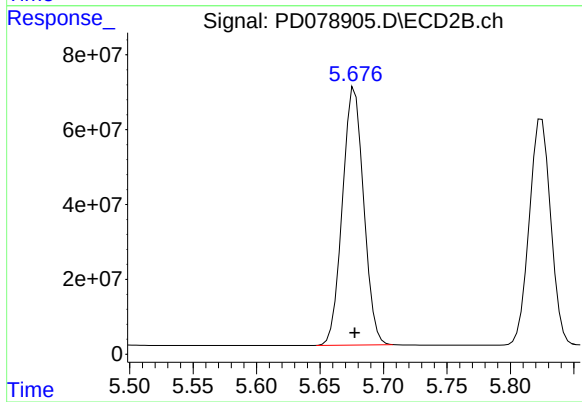


#14 Endrin

R.T.: 5.677 min
Delta R.T.: 0.000 min
Response: 801377108
Conc: 1332.45 ng/ml

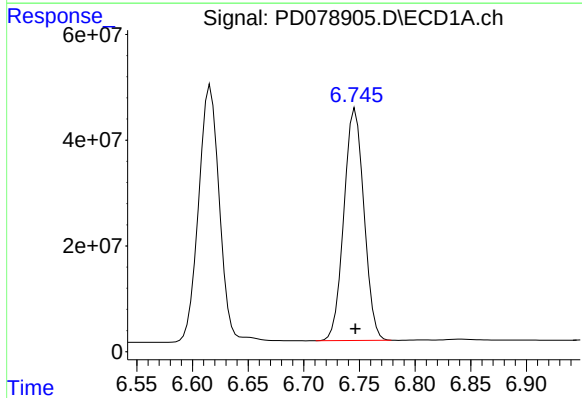


#16 4,4'-DDD

R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 550429970
Conc: 1326.18 ng/ml

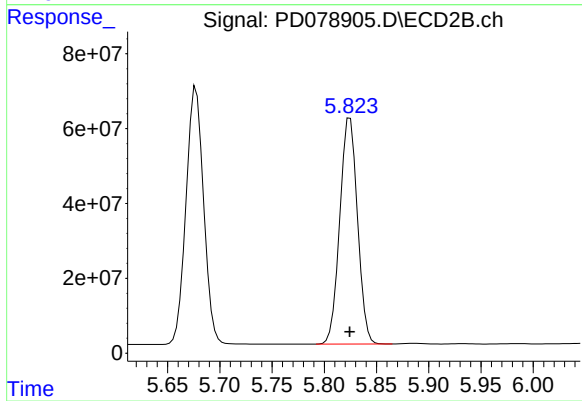

#16 4,4'-DDD


R.T.: 5.825 min
Delta R.T.: 0.000 min
Response: 711839819
Conc: 1346.41 ng/ml

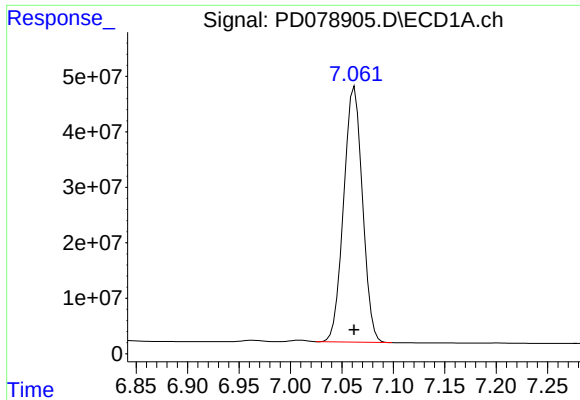

#17 4,4'-DDT


R.T.: 7.062 min
Delta R.T.: 0.000 min
Response: 586291073
Conc: 1314.17 ng/ml

Instrument :
ECD_D
ClientSampleId :

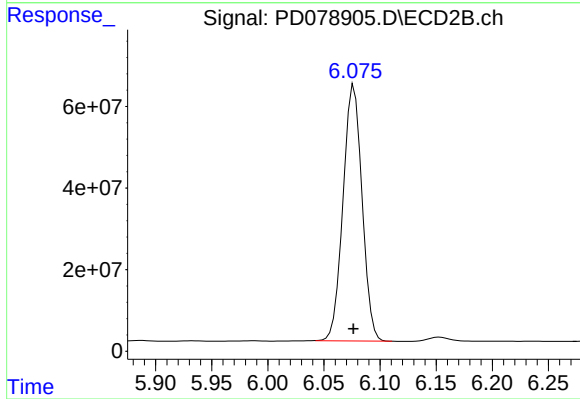


#17 4,4'-DDT

R.T.: 6.077 min
Delta R.T.: 0.000 min
Response: 740738355
Conc: 1402.56 ng/ml

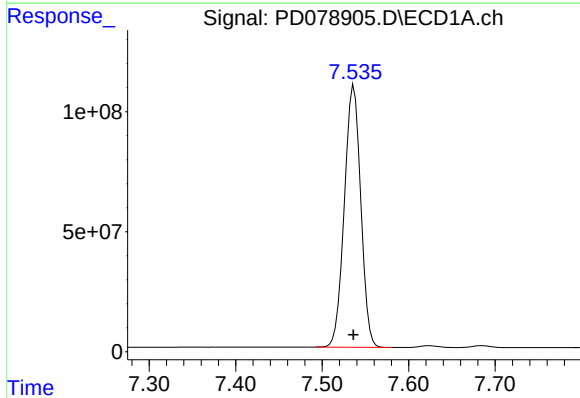


#20 Methoxychlor

R.T.: 7.537 min
Delta R.T.: 0.000 min
Response: 1430132927
Conc: 5669.98 ng/ml

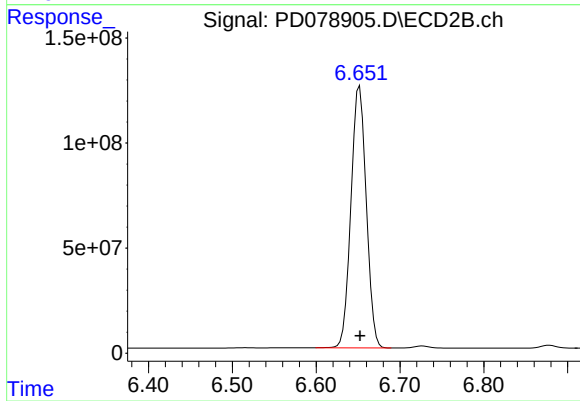

#20 Methoxychlor


R.T.: 6.652 min
Delta R.T.: 0.000 min
Response: 1586090314
Conc: 4931.17 ng/ml

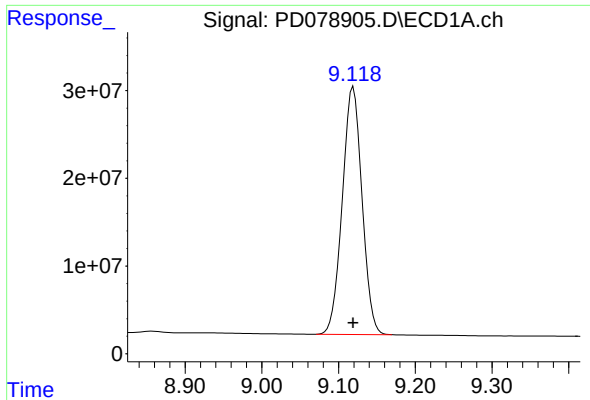

#27 Decachlorobiphenyl

R.T.: 9.119 min
Delta R.T.: 0.000 min
Response: 506380282
Conc: 951.52 ng/ml

Instrument :
ECD_D
ClientSampleId :

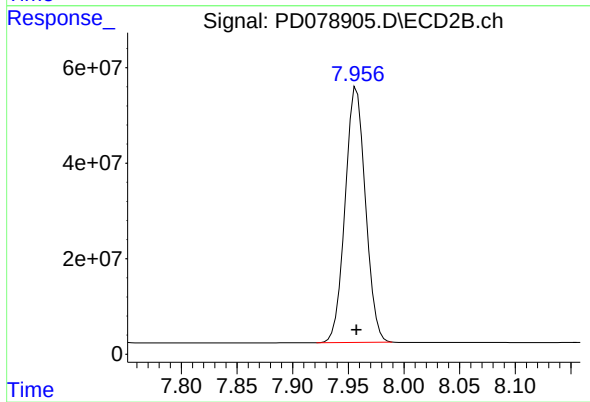

#27 Decachlorobiphenyl

R.T.: 7.958 min
Delta R.T.: 0.000 min
Response: 679109381
Conc: 1057.63 ng/ml