

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101623\
 Data File : PD078906.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2023 03:43
 Operator : AR\AJ
 Sample : INDB601
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 04:53:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101623CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 04:50:20 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.806	244.7E6	344.4E6	160.981	161.118
27)	SA Decachlor...	9.119	7.958	555.5E6	700.8E6	299.707	309.097
Target Compounds							
5)	MB Aldrin	5.296	4.265	400.9E6	506.0E6	166.662	171.063
6)	B beta-BHC	4.552	3.934	164.4E6	218.0E6	144.050	153.722
7)	B delta-BHC	4.803	4.166	456.7E6	560.6E6	172.795	178.899
8)	B Heptachlo...	5.724	4.767	358.5E6	458.2E6	159.420	164.426
10)	B trans-Chl...	5.980	5.018	355.0E6	454.9E6	164.458	170.060
11)	B cis-Chlor...	6.059	5.082	353.3E6	460.7E6	159.664	166.263
12)	B 4,4'-DDE	6.230	5.271	702.2E6	877.7E6	349.466	345.315
15)	B Endosulfa...	6.834	5.970	605.1E6	755.8E6	313.428	328.134
18)	B Endrin al...	6.964	6.149	466.6E6	574.7E6	315.357	320.048
19)	B Endosulfa...	7.199	6.372	589.1E6	707.9E6	315.479	317.412
21)	B Endrin ke...	7.685	6.879	646.0E6	810.0E6	319.455	311.825


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101623\
Data File : PD078906.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2023 03:43
Operator : AR\AJ
Sample : INDB601
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 04:53:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101623CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 04:50:20 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

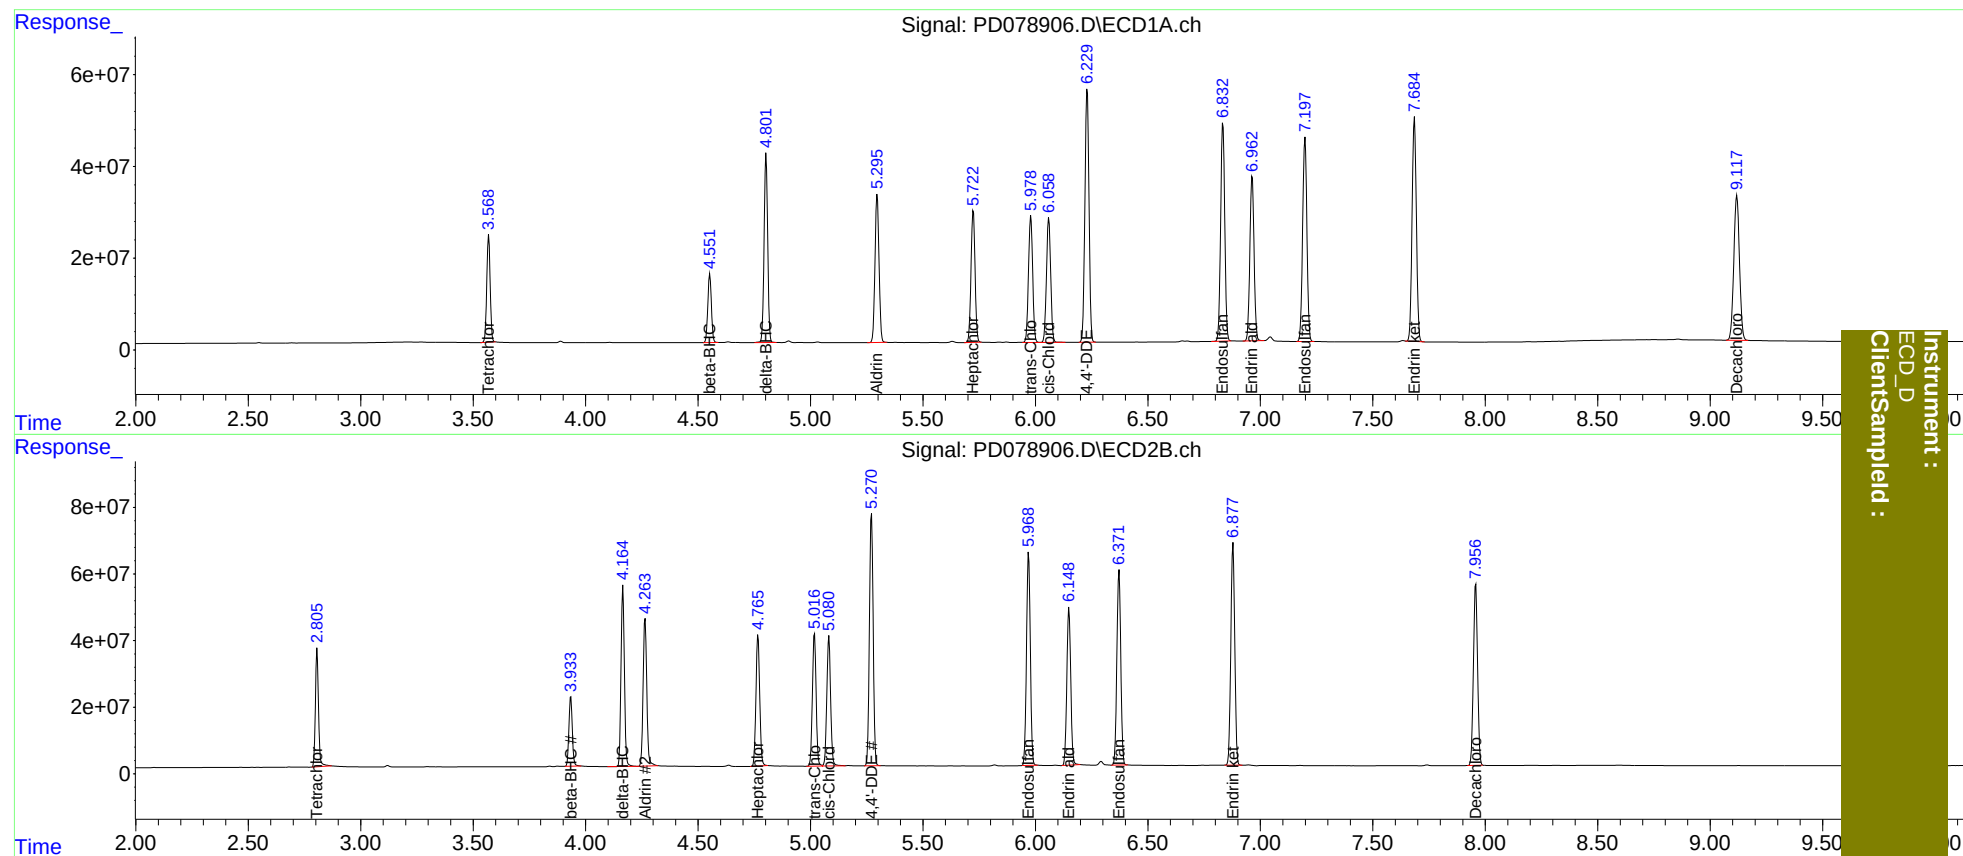


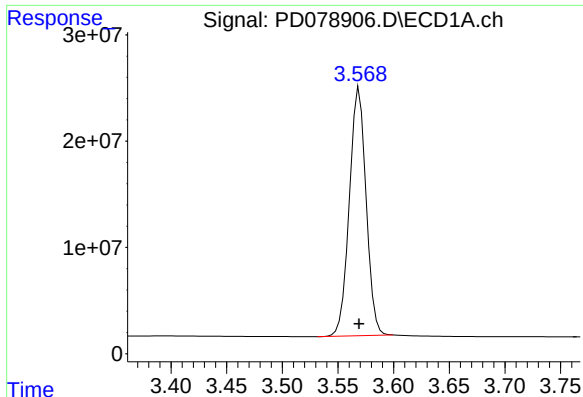

#1 Tetrachloro-m-xylene


R.T.: 3.569 min
Delta R.T.: 0.000 min
Response: 244714606
Conc: 160.98 ng/ml

Instrument :
ECD_D
ClientSampleId :

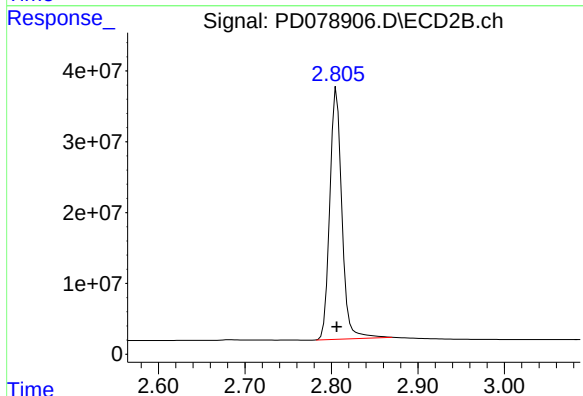


#1 Tetrachloro-m-xylene

R.T.: 2.806 min
Delta R.T.: 0.000 min
Response: 344363734
Conc: 161.12 ng/ml

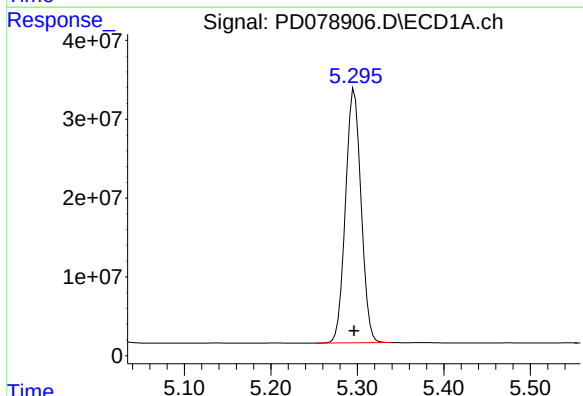


#5 Aldrin

R.T.: 5.296 min
Delta R.T.: 0.000 min
Response: 400863084
Conc: 166.66 ng/ml

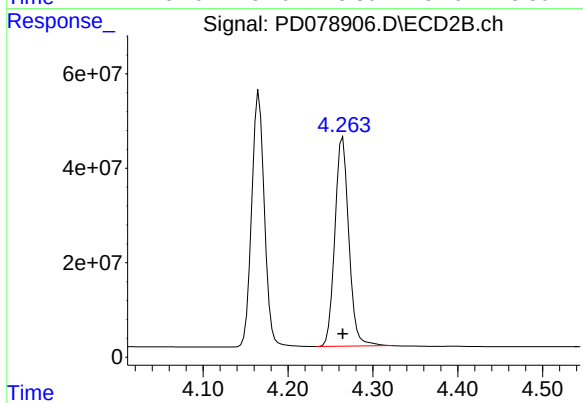

#5 Aldrin


R.T.: 4.265 min
Delta R.T.: 0.000 min
Response: 506045043
Conc: 171.06 ng/ml

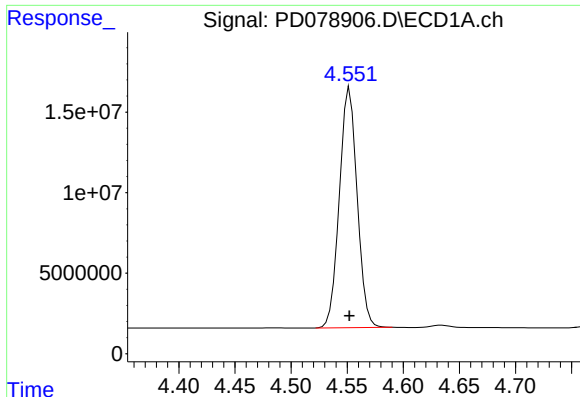

#6 beta-BHC


R.T.: 4.552 min
Delta R.T.: 0.000 min
Response: 164433891
Conc: 144.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

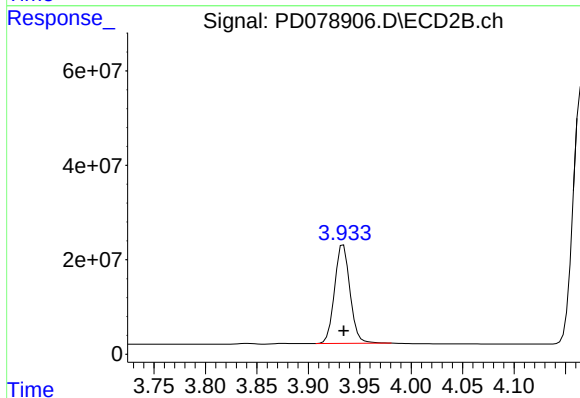


#6 beta-BHC

R.T.: 3.934 min
Delta R.T.: 0.000 min
Response: 218019067
Conc: 153.72 ng/ml

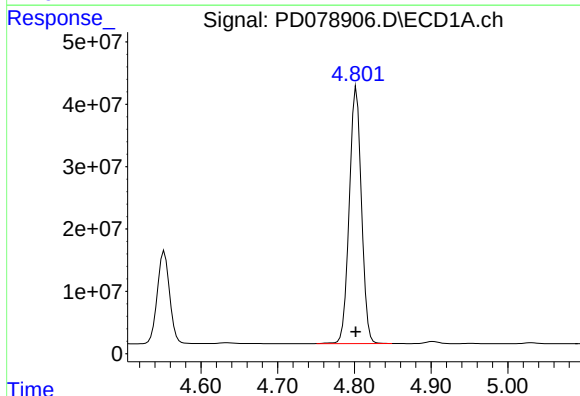


#7 delta-BHC

R.T.: 4.803 min
Delta R.T.: 0.000 min
Response: 456687581
Conc: 172.80 ng/ml

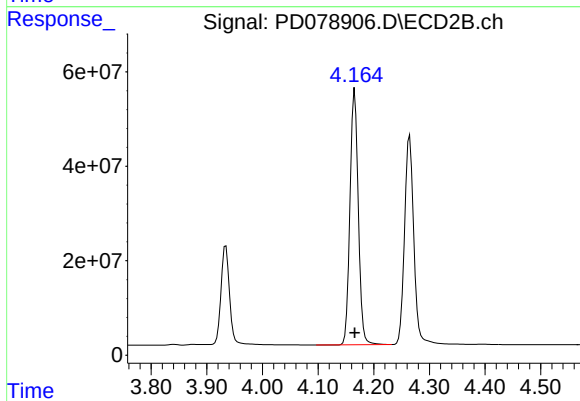

#7 delta-BHC


R.T.: 4.166 min
Delta R.T.: 0.000 min
Response: 560623370
Conc: 178.90 ng/ml

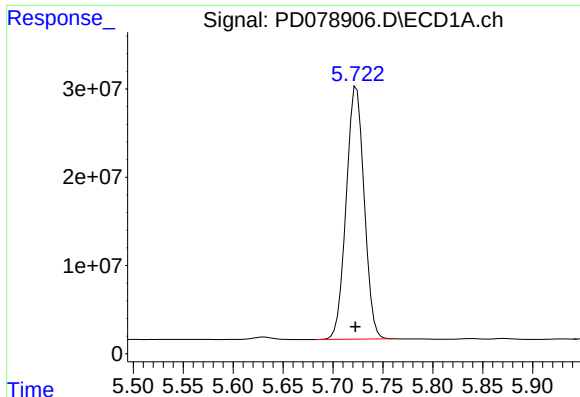

#8 Heptachlor epoxide


R.T.: 5.724 min
Delta R.T.: 0.001 min
Response: 358491447
Conc: 159.42 ng/ml

Instrument :
ECD_D
ClientSampleId :

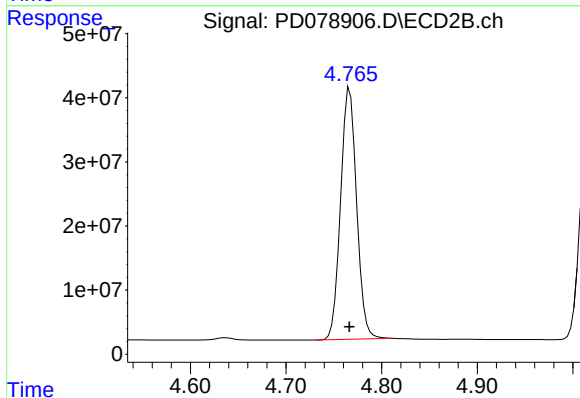


#8 Heptachlor epoxide

R.T.: 4.767 min
Delta R.T.: 0.000 min
Response: 458159327
Conc: 164.43 ng/ml

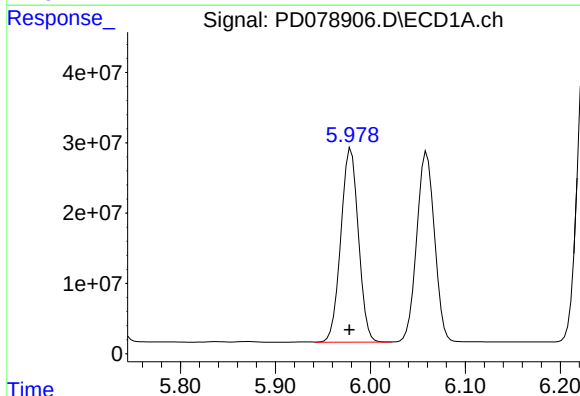


#10 trans-Chlordane

R.T.: 5.980 min
Delta R.T.: 0.001 min
Response: 354966427
Conc: 164.46 ng/ml

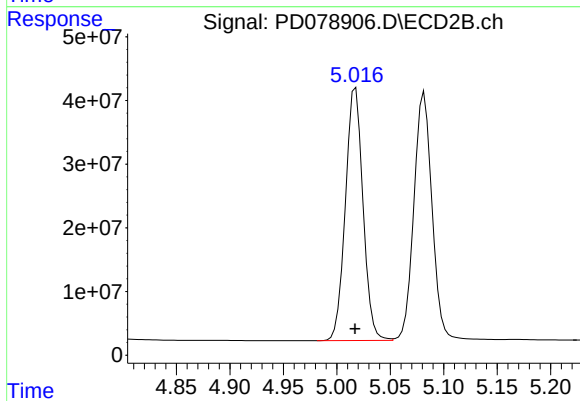

#10 trans-Chlordane


R.T.: 5.018 min
Delta R.T.: 0.000 min
Response: 454871001
Conc: 170.06 ng/ml

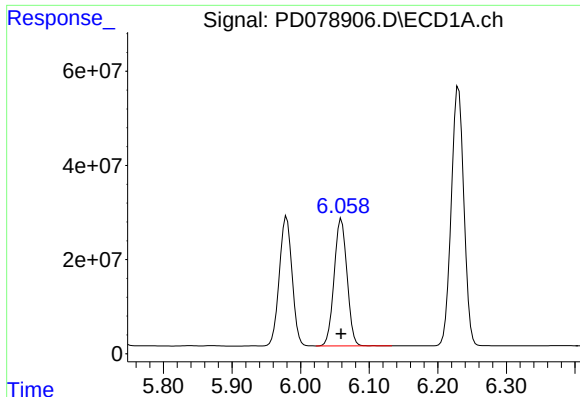

#11 cis-Chlordane


R.T.: 6.059 min
Delta R.T.: 0.000 min
Response: 353335187
Conc: 159.66 ng/ml

Instrument :
ECD_D
ClientSampleId :

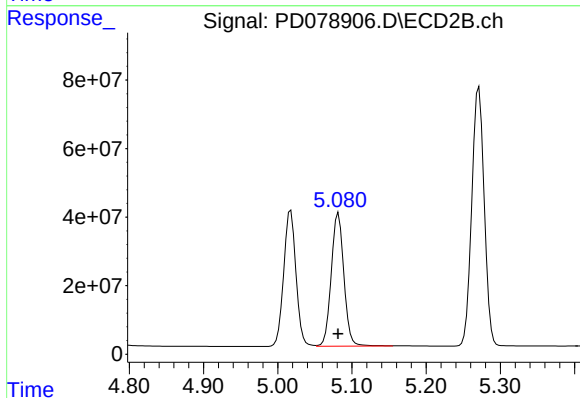


#11 cis-Chlordane

R.T.: 5.082 min
Delta R.T.: 0.000 min
Response: 460699801
Conc: 166.26 ng/ml

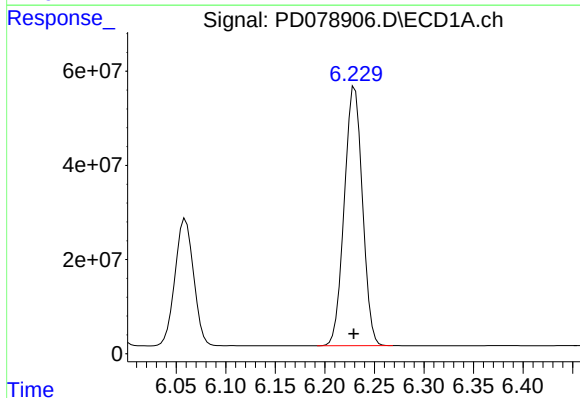


#12 4,4'-DDE

R.T.: 6.230 min
Delta R.T.: 0.001 min
Response: 702203891
Conc: 349.47 ng/ml

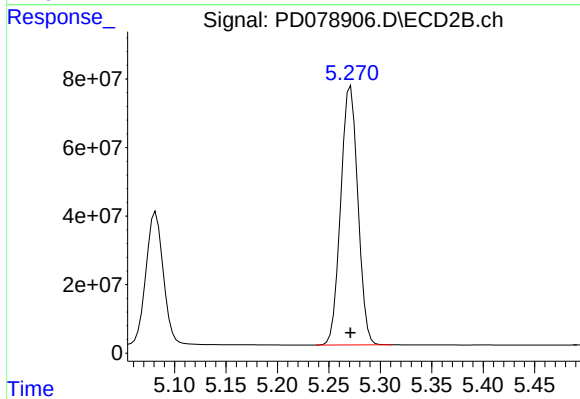

#12 4,4'-DDE


R.T.: 5.271 min
Delta R.T.: 0.000 min
Response: 877661737
Conc: 345.31 ng/ml

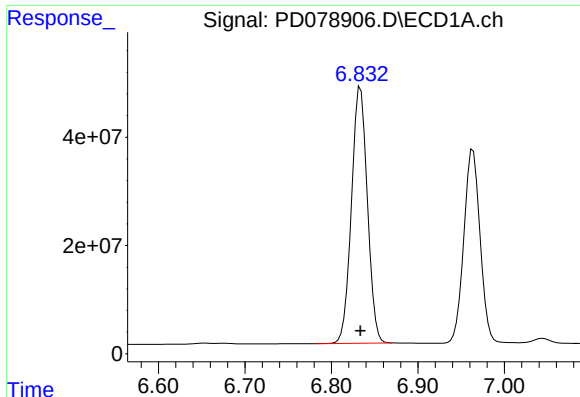

#15 Endosulfan II


R.T.: 6.834 min
Delta R.T.: 0.000 min
Response: 605054755
Conc: 313.43 ng/ml

Instrument :
ECD_D
ClientSampleId :

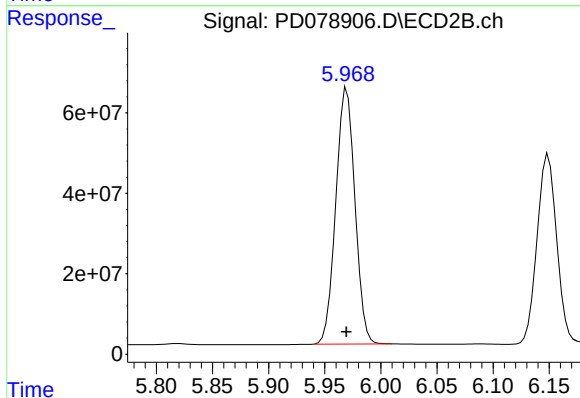


#15 Endosulfan II

R.T.: 5.970 min
Delta R.T.: 0.000 min
Response: 755799787
Conc: 328.13 ng/ml

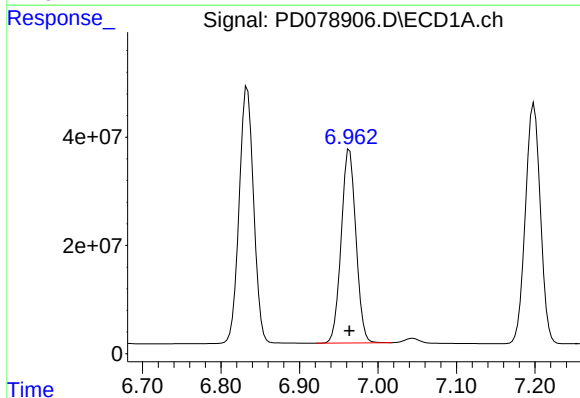


#18 Endrin aldehyde

R.T.: 6.964 min
Delta R.T.: 0.000 min
Response: 466642887
Conc: 315.36 ng/ml

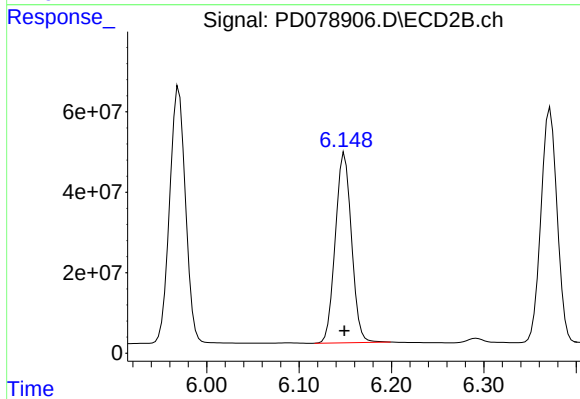

#18 Endrin aldehyde


R.T.: 6.149 min
Delta R.T.: 0.000 min
Response: 574735837
Conc: 320.05 ng/ml

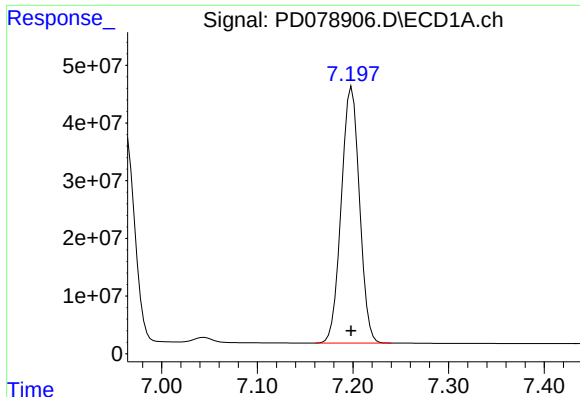

#19 Endosulfan Sulfate


R.T.: 7.199 min
Delta R.T.: 0.000 min
Response: 589103908
Conc: 315.48 ng/ml

Instrument :
ECD_D
ClientSampleId :

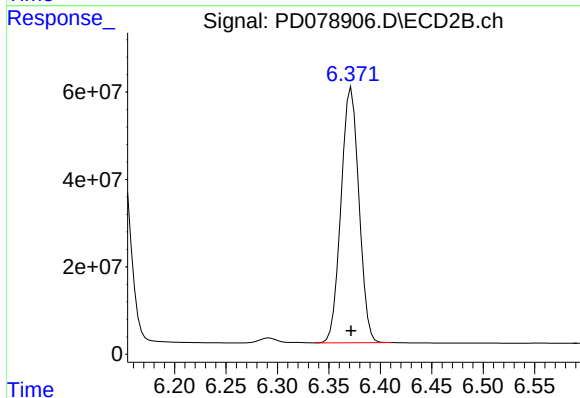


#19 Endosulfan Sulfate

R.T.: 6.372 min
Delta R.T.: 0.000 min
Response: 707876153
Conc: 317.41 ng/ml

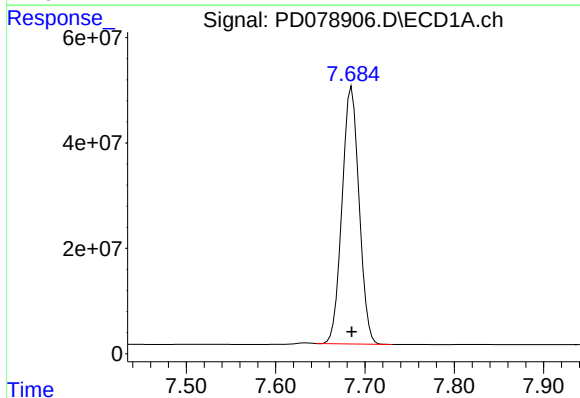


#21 Endrin ketone

R.T.: 7.685 min
Delta R.T.: 0.000 min
Response: 645994397
Conc: 319.46 ng/ml

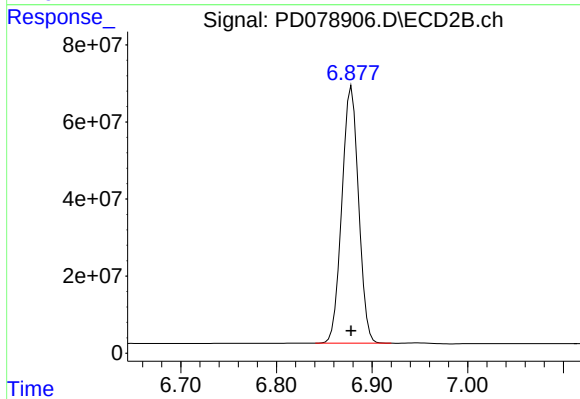

#21 Endrin ketone


R.T.: 6.879 min
Delta R.T.: 0.000 min
Response: 810013906
Conc: 311.82 ng/ml

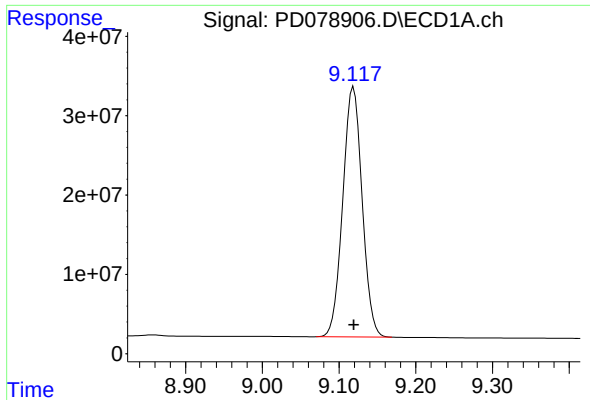

#27 Decachlorobiphenyl

R.T.: 9.119 min
Delta R.T.: 0.000 min
Response: 555472084
Conc: 299.71 ng/ml

Instrument :
ECD_D
ClientSampleId :

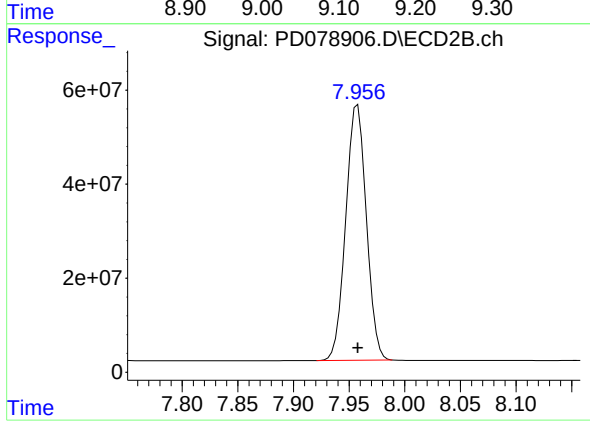

#27 Decachlorobiphenyl

R.T.: 7.958 min
Delta R.T.: 0.000 min
Response: 700752004
Conc: 309.10 ng/ml