

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101624\
 Data File : PD086074.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 10:12
 Operator : AR\AJ
 Sample : PB164033BL
 Misc : BL/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB164033BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 10:47:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101124.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 11 13:57:25 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.450	2.877	22384830	120.0E6	18.438	19.214
28) SA Decachlor...	8.908	8.061	39028965	112.1E6	18.073	21.051

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101624\
Data File : PD086074.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 10:12
Operator : AR\AJ
Sample : PB164033BL
Misc : BL/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB164033BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 10:47:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101124.M
Quant Title : GC Extractables
QLast Update : Fri Oct 11 13:57:25 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

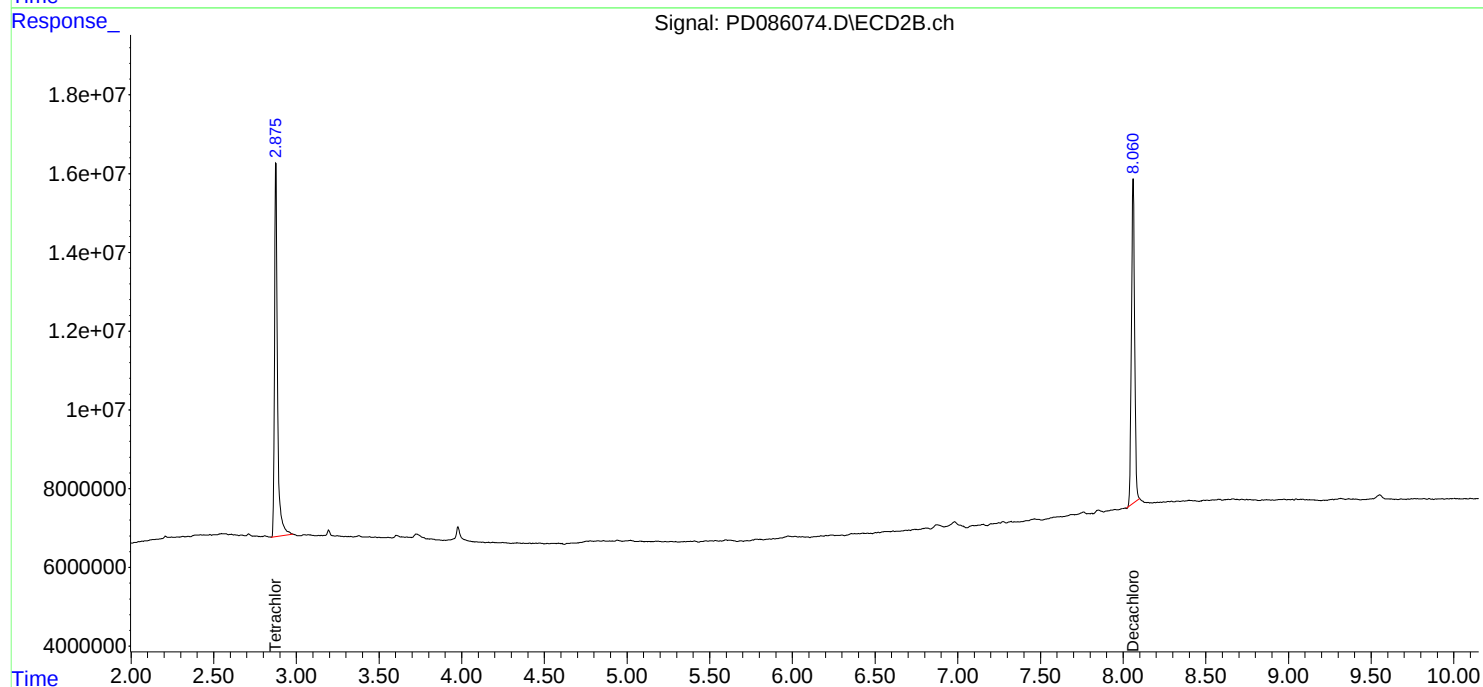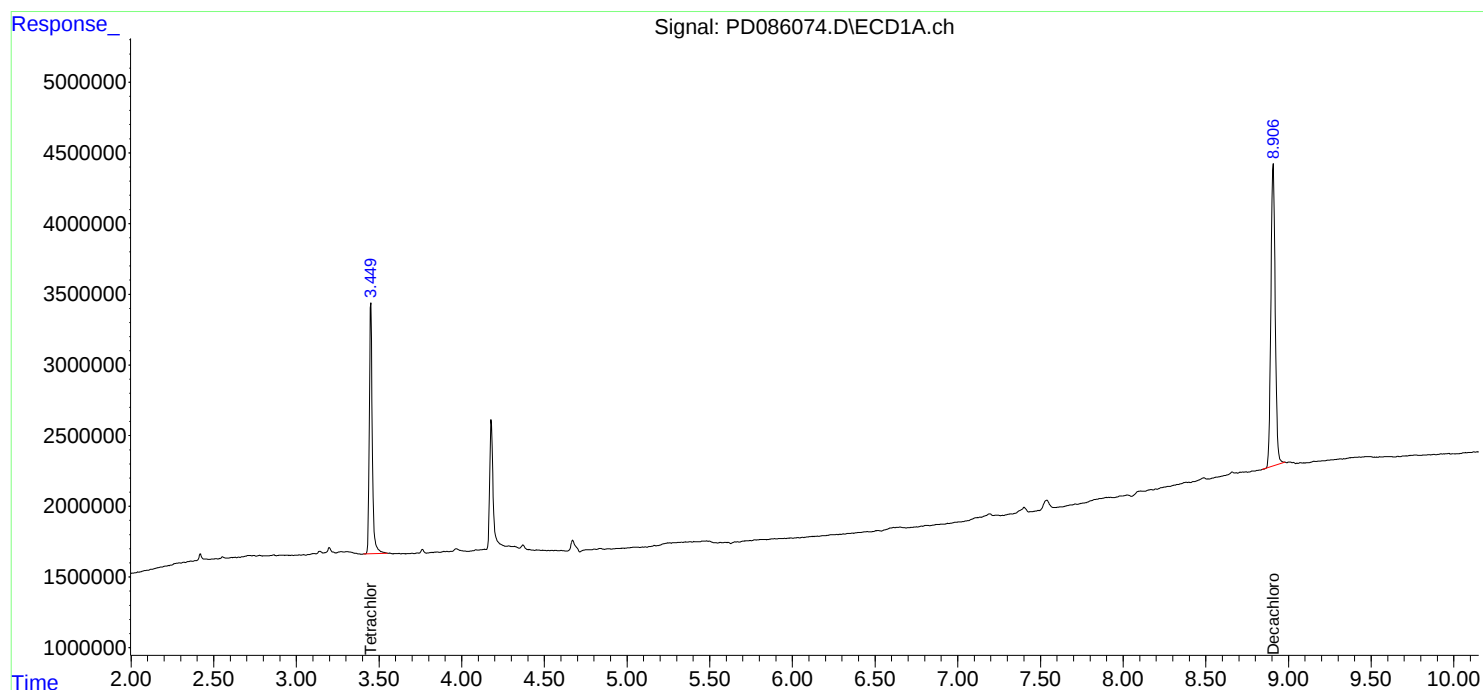


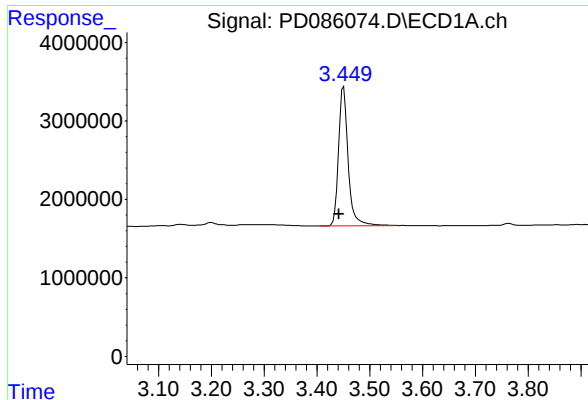

#1 Tetrachloro-m-xylene


R.T.: 3.450 min
Delta R.T.: 0.008 min
Response: 22384830
Conc: 18.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB164033BL

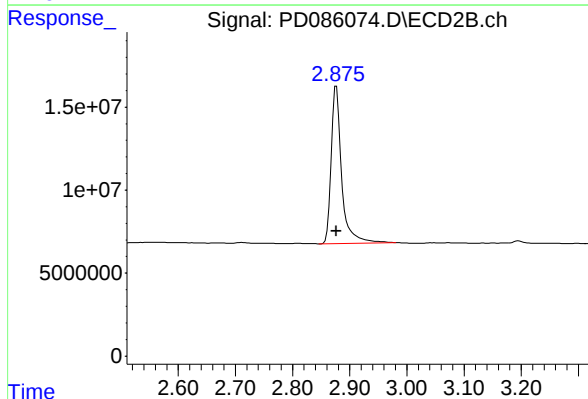


#1 Tetrachloro-m-xylene

R.T.: 2.877 min
Delta R.T.: 0.000 min
Response: 119953659
Conc: 19.21 ng/ml

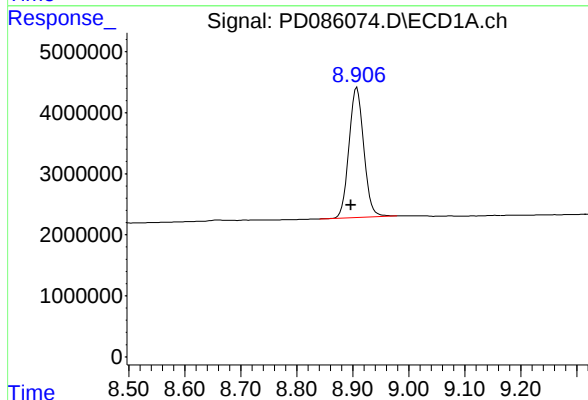

#28 Decachlorobiphenyl

R.T.: 8.908 min
Delta R.T.: 0.010 min
Response: 39028965
Conc: 18.07 ng/ml

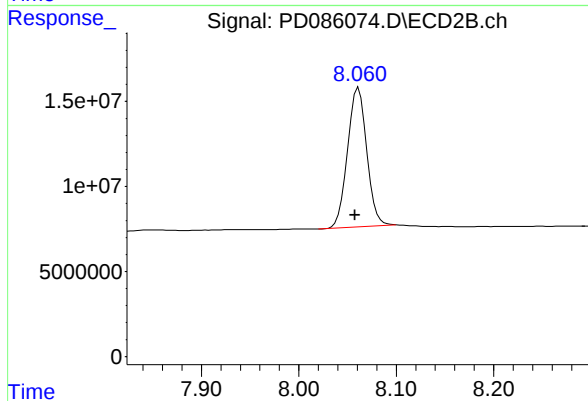

#28 Decachlorobiphenyl

R.T.: 8.061 min
Delta R.T.: 0.004 min
Response: 112132271
Conc: 21.05 ng/ml