

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101625\
 Data File : PD090631.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2025 14:38
 Operator : AR\AJ
 Sample : Q3348-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 WCS-TP1

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/17/2025
 Supervised By :Sohil Jodhani 10/17/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 04:59:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091825.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:52:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.543	2.873	59008968	567.4E6	18.154m	20.669m
28) SA Decachlor...	9.069	8.063	87880376	477.0E6	18.213	14.716

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101625\
Data File : PD090631.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2025 14:38
Operator : AR\AJ
Sample : Q3348-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
WCS-TP1


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/17/2025
Supervised By : Sohil Jodhani 10/17/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 04:59:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091825.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:52:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

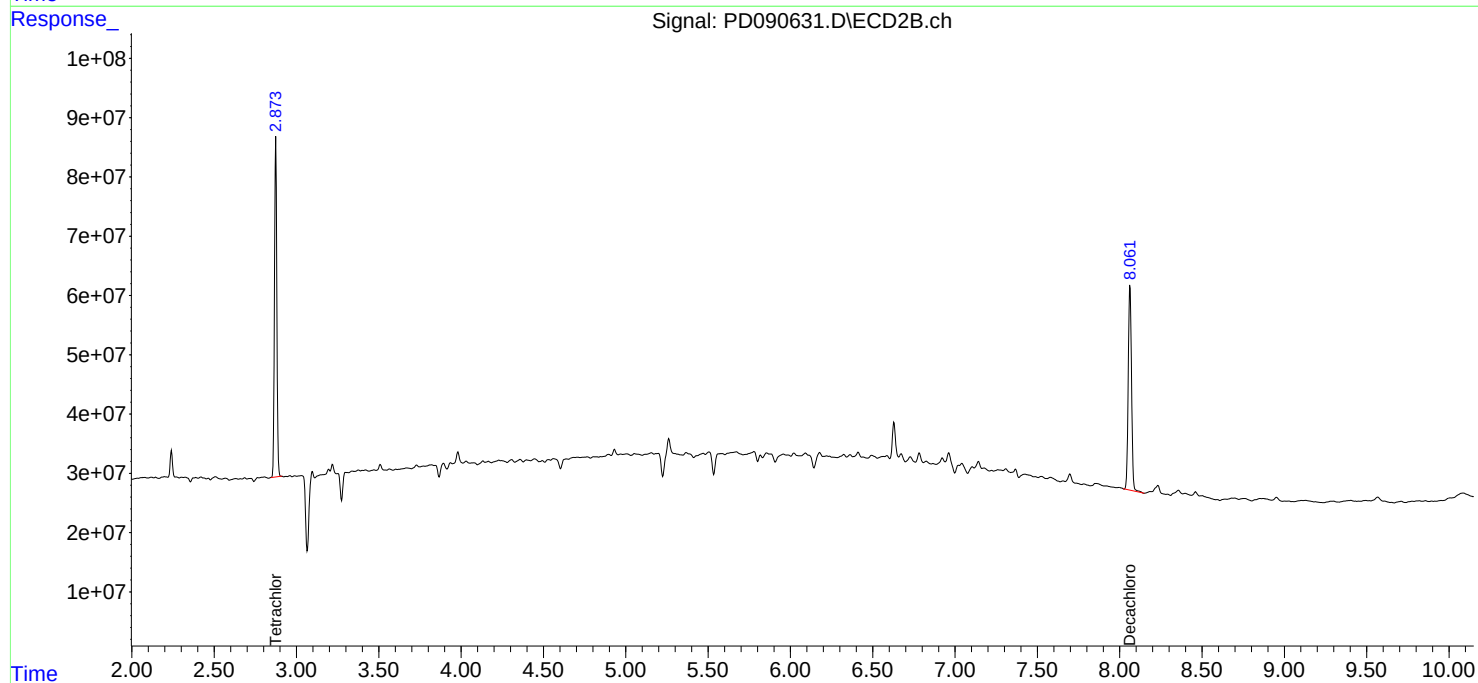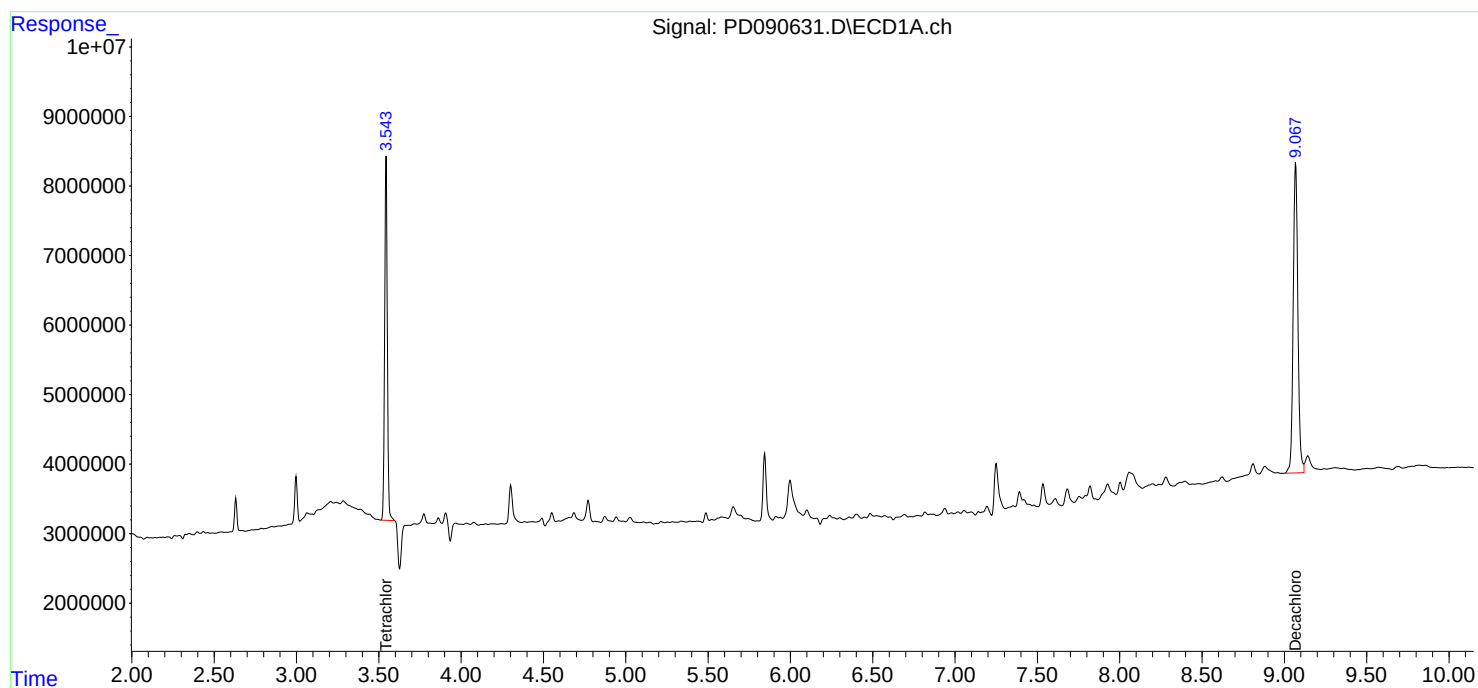

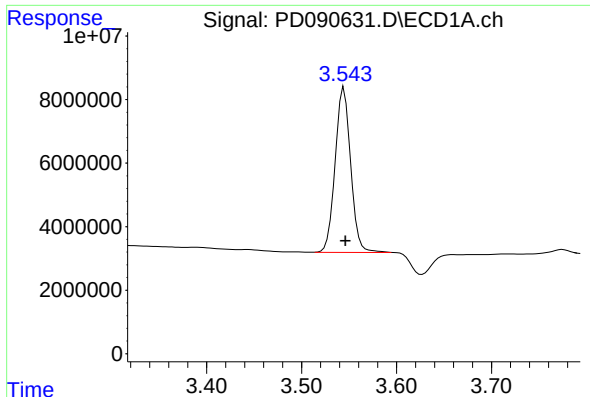


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: -0.003 min
Response: 59008968
Conc: 18.15 ng/ml

Instrument :
ECD_D
ClientSampleId :
WCS-TP1


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/17/2025
Supervised By :Sohil Jodhani 10/17/2025

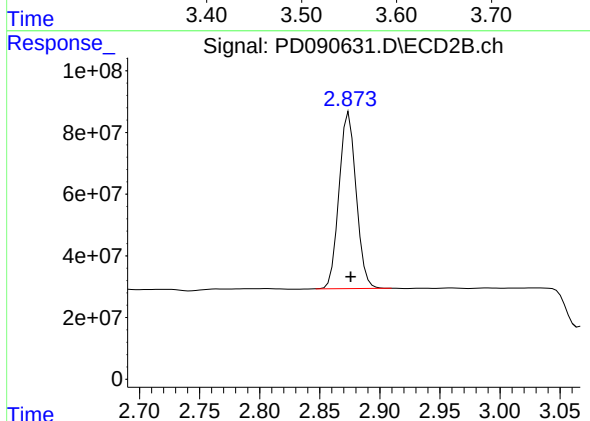


#1 Tetrachloro-m-xylene

R.T.: 2.873 min
Delta R.T.: -0.003 min
Response: 567354095
Conc: 20.67 ng/ml m

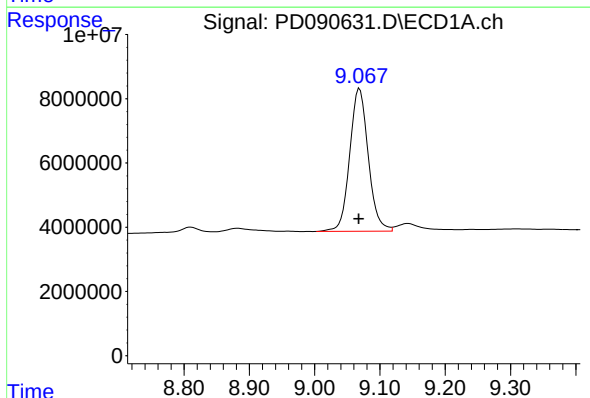

#28 Decachlorobiphenyl

R.T.: 9.069 min
Delta R.T.: 0.001 min
Response: 87880376
Conc: 18.21 ng/ml

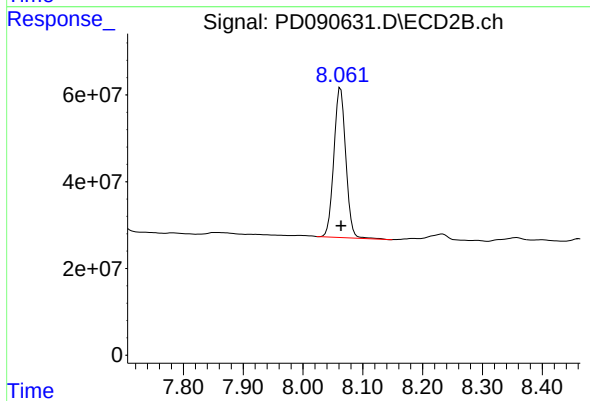

#28 Decachlorobiphenyl

R.T.: 8.063 min
Delta R.T.: -0.001 min
Response: 477014367
Conc: 14.72 ng/ml