

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101625\
 Data File : PD090635.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2025 15:34
 Operator : AR\AJ
 Sample : Q3352-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-3

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/17/2025
 Supervised By : Sohil Jodhani 10/17/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 05:00:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091825.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:52:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.543	2.873	58195543	559.9E6	17.904m	20.395m
28) SA Decachlor...	9.068	8.063	77647687	456.0E6	16.093	14.067

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101625\
Data File : PD090635.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2025 15:34
Operator : AR\AJ
Sample : Q3352-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/17/2025
Supervised By : Sohil Jodhani 10/17/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 05:00:13 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091825.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:52:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

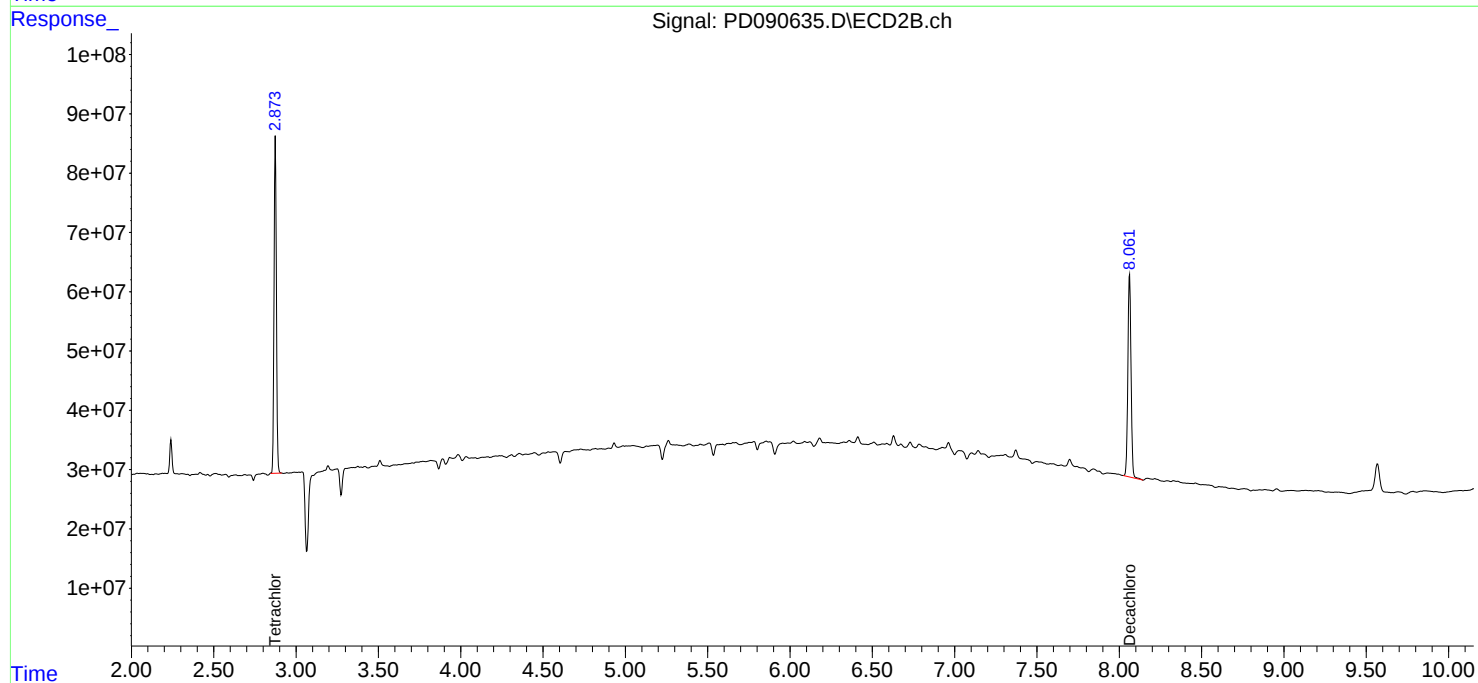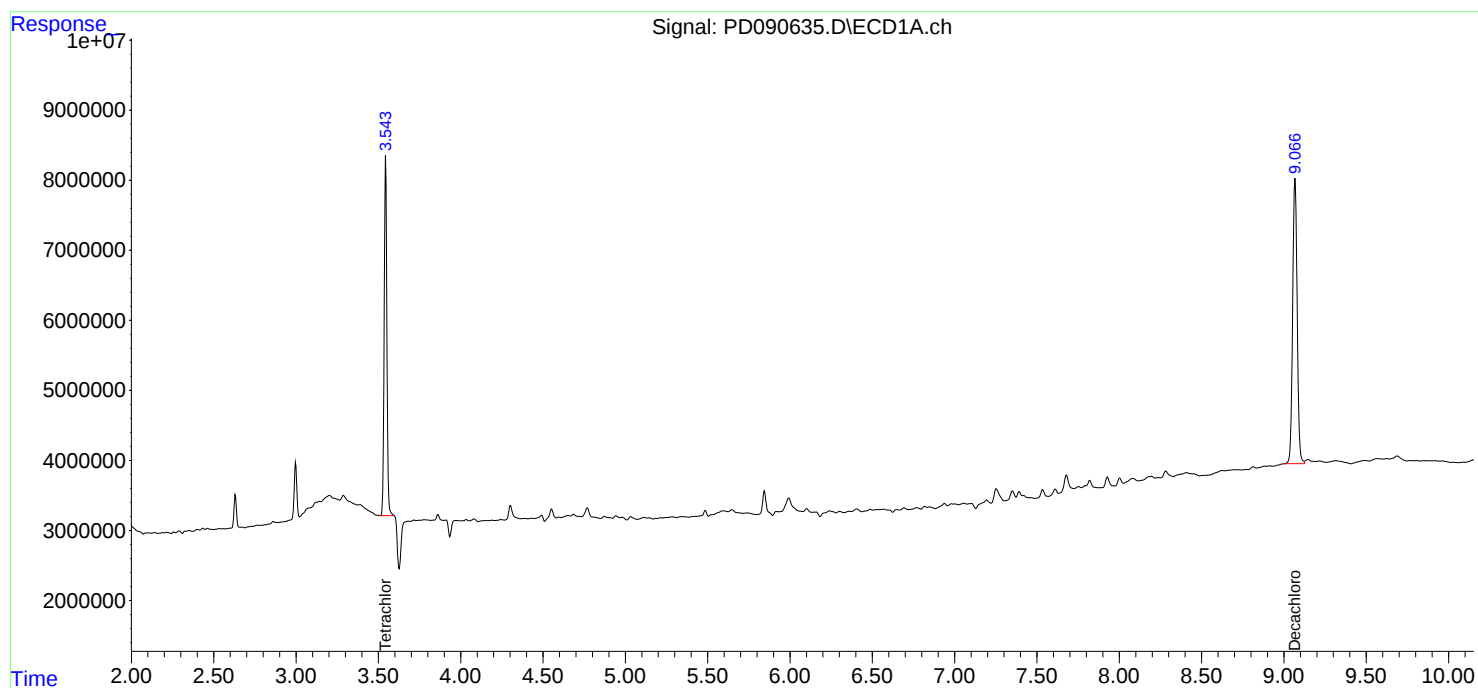

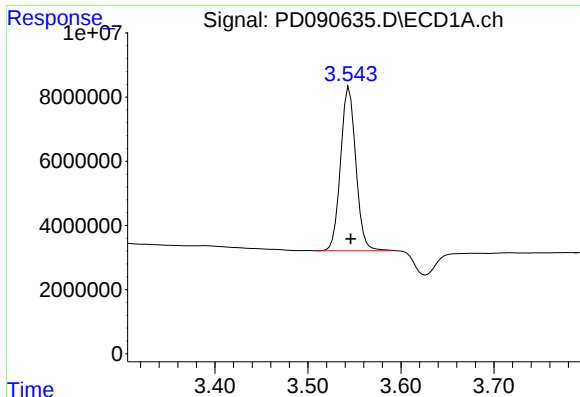


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: -0.003 min
Response: 58195543
Conc: 17.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/17/2025
Supervised By :Sohil Jodhani 10/17/2025

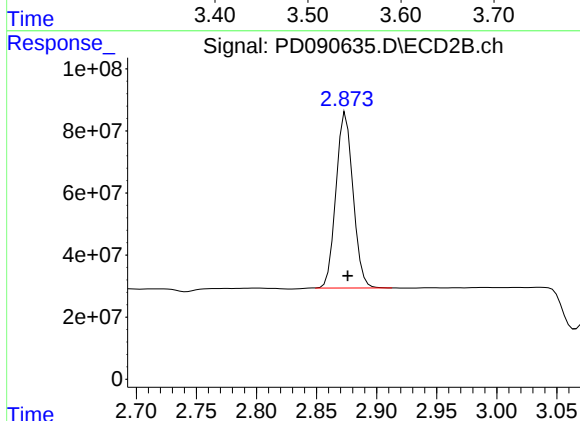


#1 Tetrachloro-m-xylene

R.T.: 2.873 min
Delta R.T.: -0.003 min
Response: 559851798
Conc: 20.40 ng/ml m

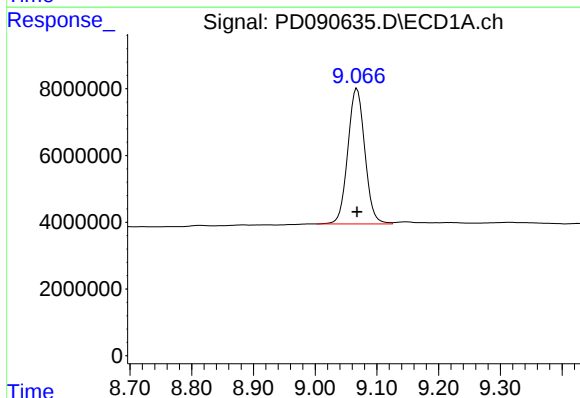

#28 Decachlorobiphenyl

R.T.: 9.068 min
Delta R.T.: 0.000 min
Response: 77647687
Conc: 16.09 ng/ml

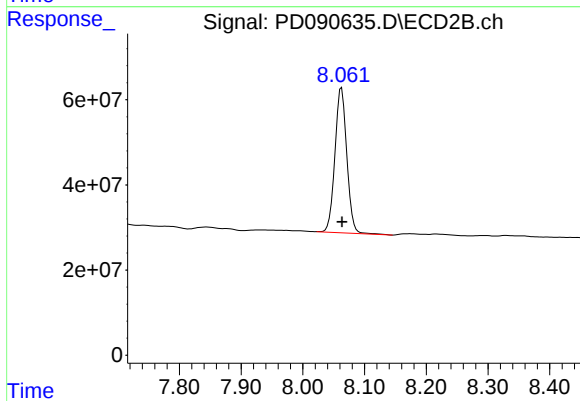

#28 Decachlorobiphenyl

R.T.: 8.063 min
Delta R.T.: 0.000 min
Response: 455972177
Conc: 14.07 ng/ml