

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101722\
 Data File : PD072449.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2022 16:12
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 17:37:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 17 17:34:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.707	3.468	13616321	211.7E6	5.467	5.697
27)	SA Decachlor...	7.845	8.928	22138948	100.2E6	11.327	11.208
Target Compounds							
2)	A alpha-BHC	3.212	3.933	18430419	280.6E6	5.044	5.824
3)	MA gamma-BHC...	3.543	4.267	16265412	249.8E6	5.066	6.184
4)	MA Heptachlor	3.875	4.834	17756824	171.8E6	5.256	6.069
9)	A Endosulfan I	5.030	5.991	14152602	92939607	5.360	5.846
13)	MA Dieldrin	5.297	6.268	29487523	185.2E6	10.241	11.545
14)	MA Endrin	5.573	6.500	25708813	161.2E6	10.215	12.055
16)	A 4,4'-DDD	5.721	6.634	23003632	141.5E6	10.258	11.598
17)	MA 4,4'-DDT	5.970	6.942	21753187	131.7E6	9.998	11.089
20)	A Methoxychlor	6.554	7.421	63464472	310.9E6	53.719	57.279


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101722\
Data File : PD072449.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2022 16:12
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 17:37:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
Quant Title : GC Extractables
QLast Update : Mon Oct 17 17:34:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

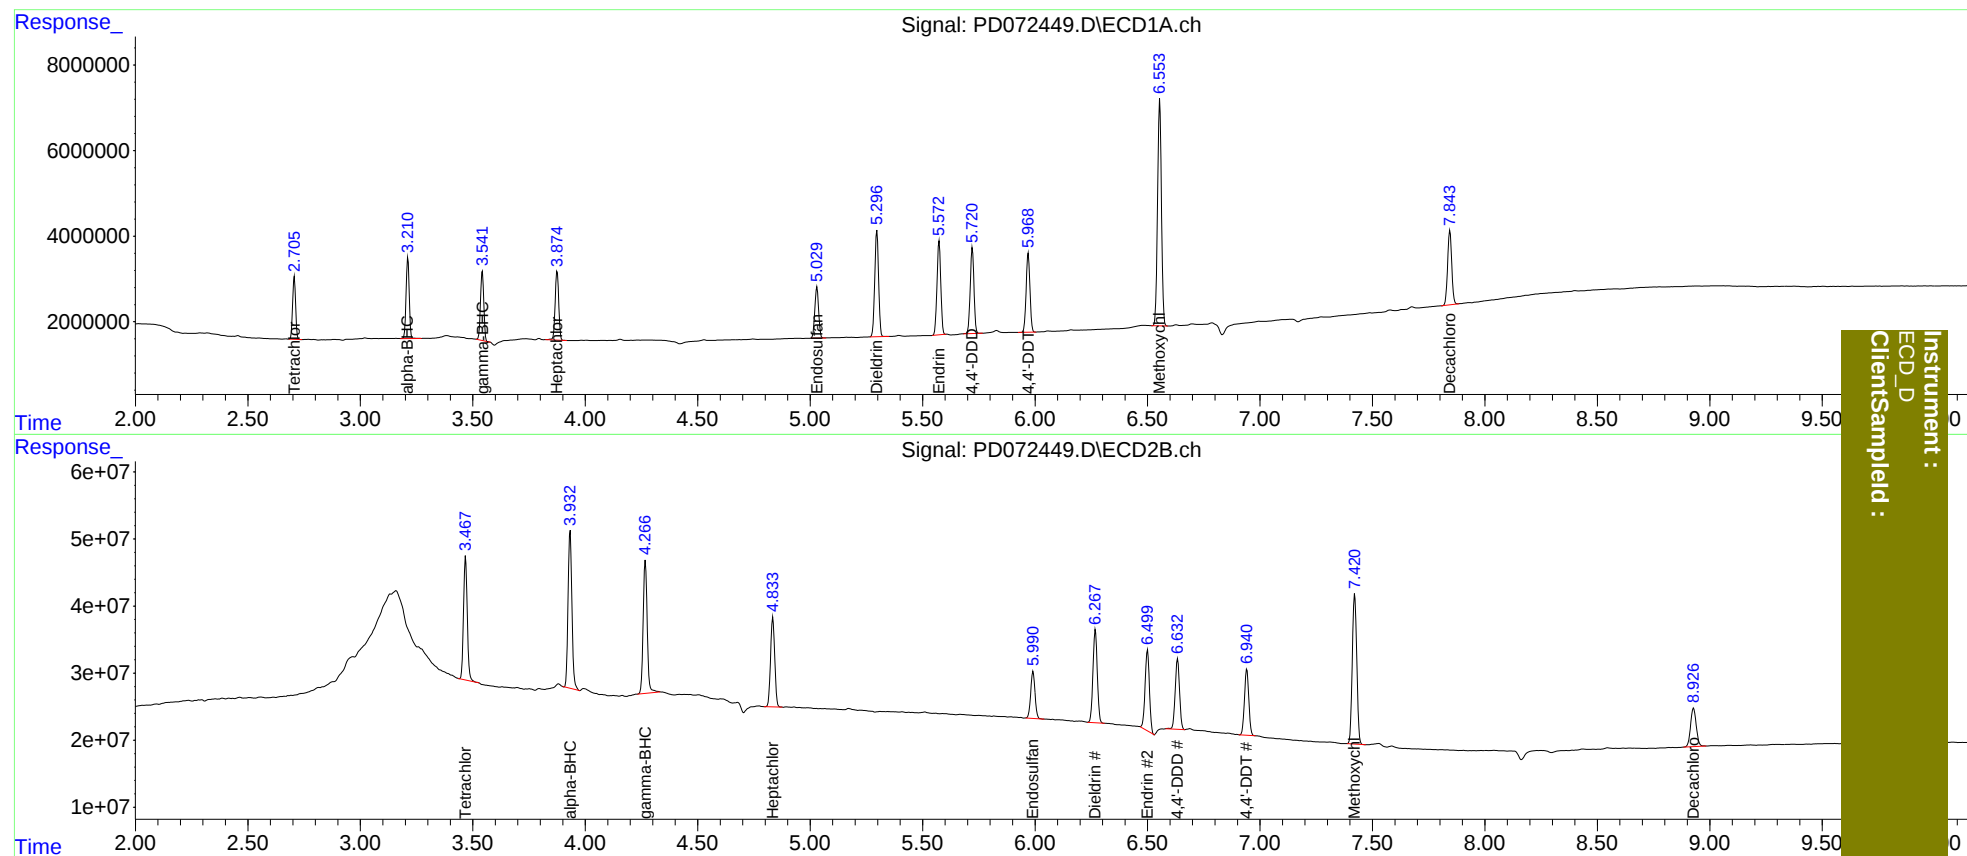


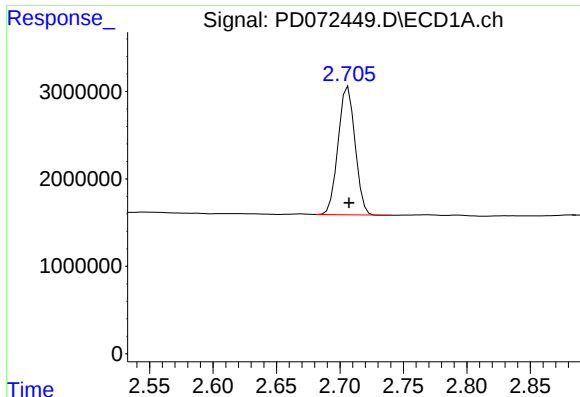

#1 Tetrachloro-m-xylene


R.T.: 2.707 min
Delta R.T.: 0.000 min
Response: 13616321
Conc: 5.47 ng/ml

Instrument :
ECD_D
ClientSampleId :

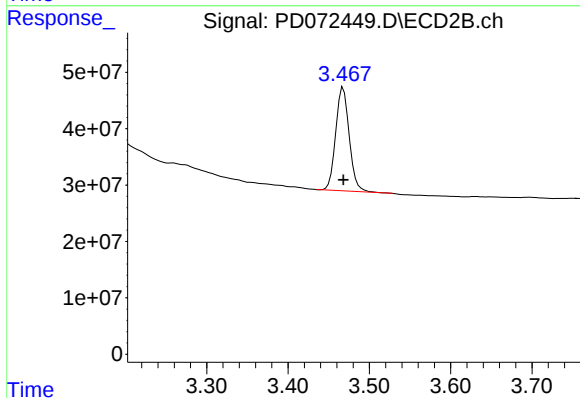


#1 Tetrachloro-m-xylene

R.T.: 3.468 min
Delta R.T.: 0.000 min
Response: 211686247
Conc: 5.70 ng/ml

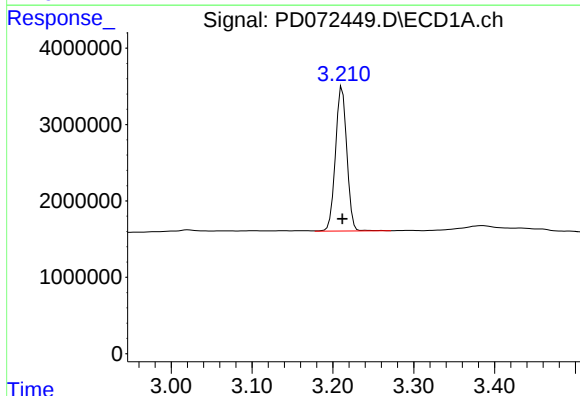


#2 alpha-BHC

R.T.: 3.212 min
Delta R.T.: 0.000 min
Response: 18430419
Conc: 5.04 ng/ml

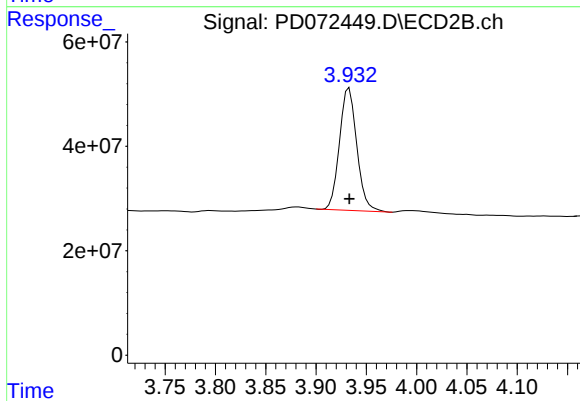

#2 alpha-BHC


R.T.: 3.933 min
Delta R.T.: 0.000 min
Response: 280618252
Conc: 5.82 ng/ml

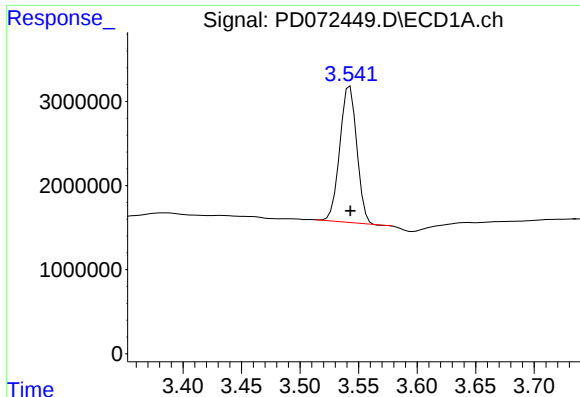

#3 gamma-BHC (Lindane)


R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 16265412
Conc: 5.07 ng/ml

Instrument :
ECD_D
ClientSampleId :

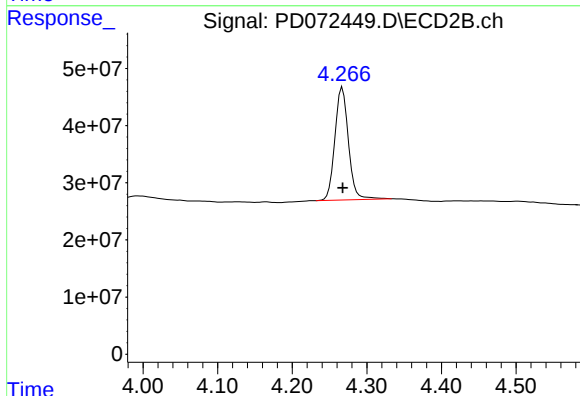


#3 gamma-BHC (Lindane)

R.T.: 4.267 min
Delta R.T.: 0.000 min
Response: 249838028
Conc: 6.18 ng/ml

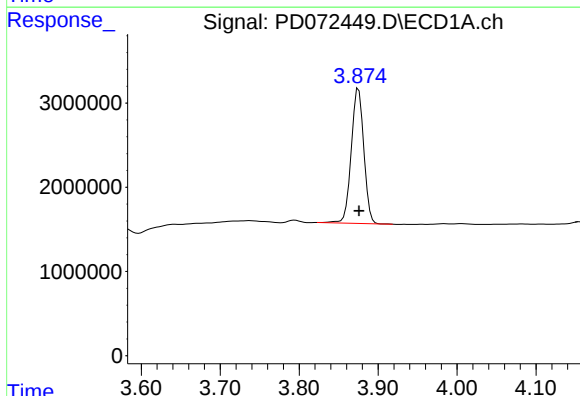


#4 Heptachlor

R.T.: 3.875 min
Delta R.T.: 0.000 min
Response: 17756824
Conc: 5.26 ng/ml

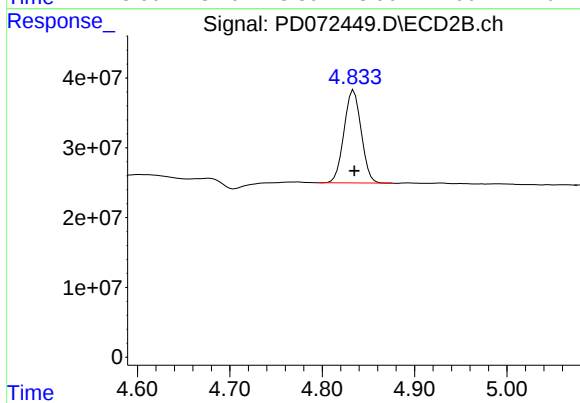

#4 Heptachlor


R.T.: 4.834 min
Delta R.T.: 0.000 min
Response: 171777487
Conc: 6.07 ng/ml

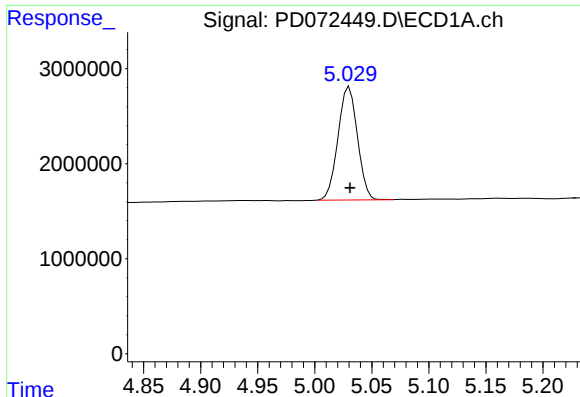

#9 Endosulfan I


R.T.: 5.030 min
Delta R.T.: 0.000 min
Response: 14152602
Conc: 5.36 ng/ml

Instrument :
ECD_D
ClientSampleId :

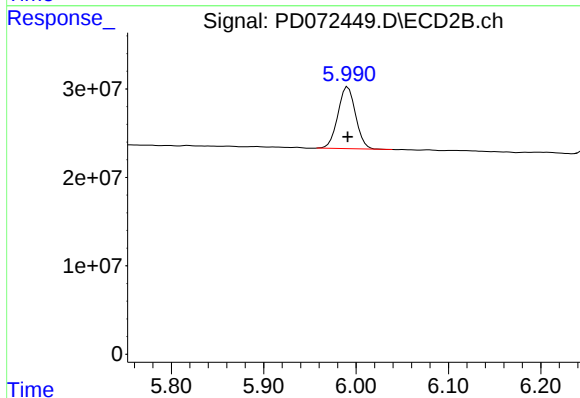


#9 Endosulfan I

R.T.: 5.991 min
Delta R.T.: 0.000 min
Response: 92939607
Conc: 5.85 ng/ml

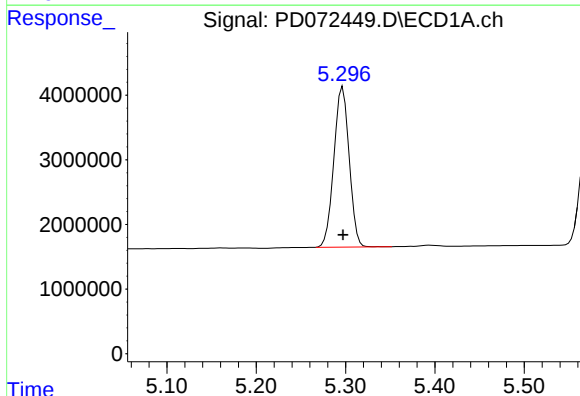


#13 Dieldrin

R.T.: 5.297 min
Delta R.T.: 0.000 min
Response: 29487523
Conc: 10.24 ng/ml

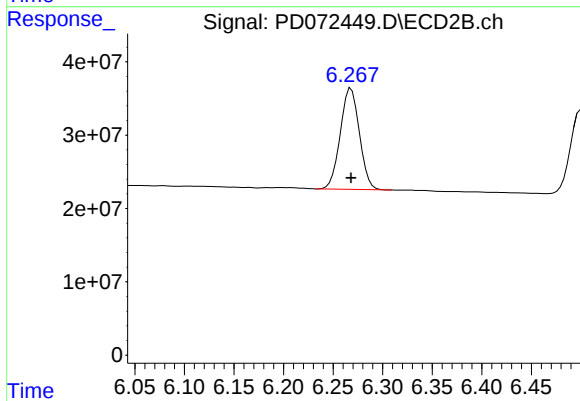

#13 Dieldrin


R.T.: 6.268 min
Delta R.T.: 0.000 min
Response: 185183212
Conc: 11.55 ng/ml

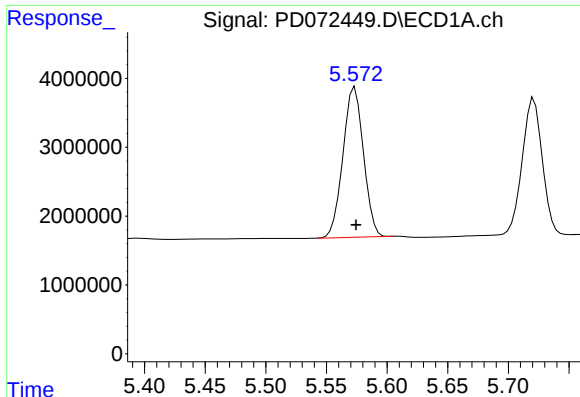

#14 Endrin


R.T.: 5.573 min
Delta R.T.: -0.001 min
Response: 25708813
Conc: 10.22 ng/ml

Instrument :
ECD_D
ClientSampleId :

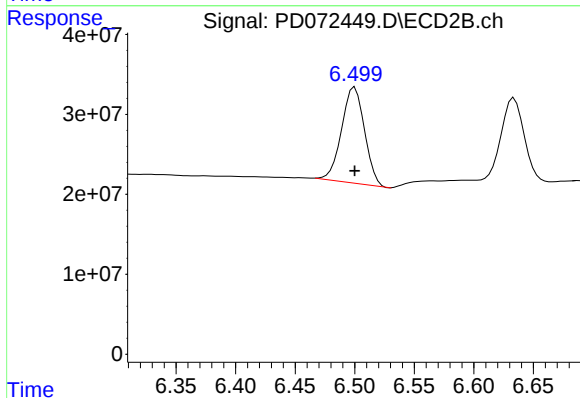


#14 Endrin

R.T.: 6.500 min
Delta R.T.: 0.000 min
Response: 161232164
Conc: 12.06 ng/ml

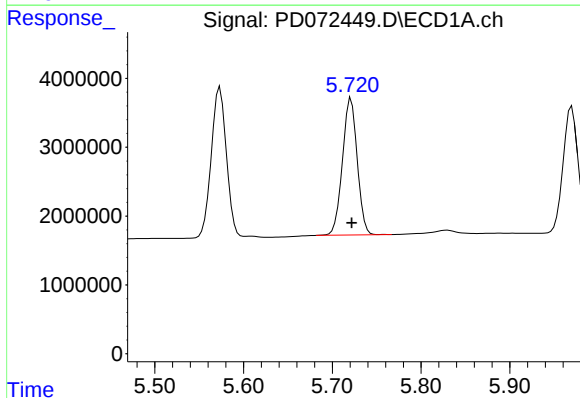


#16 4,4'-DDD

R.T.: 5.721 min
Delta R.T.: 0.000 min
Response: 23003632
Conc: 10.26 ng/ml

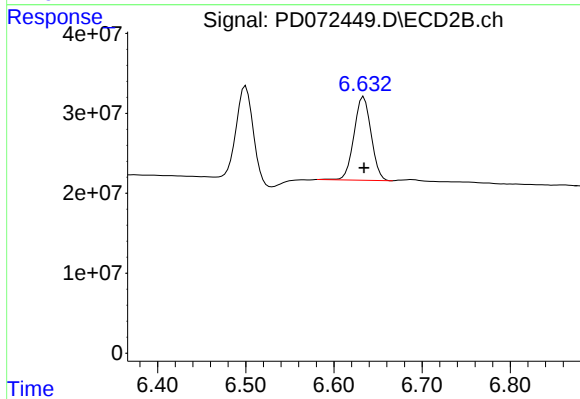

#16 4,4'-DDD


R.T.: 6.634 min
Delta R.T.: 0.000 min
Response: 141453101
Conc: 11.60 ng/ml

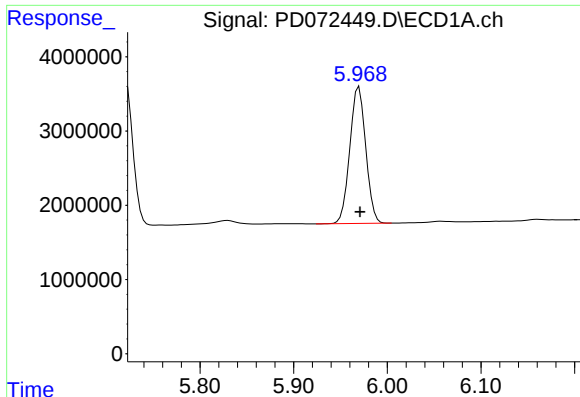

#17 4,4'-DDT


R.T.: 5.970 min
Delta R.T.: -0.001 min
Response: 21753187
Conc: 10.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

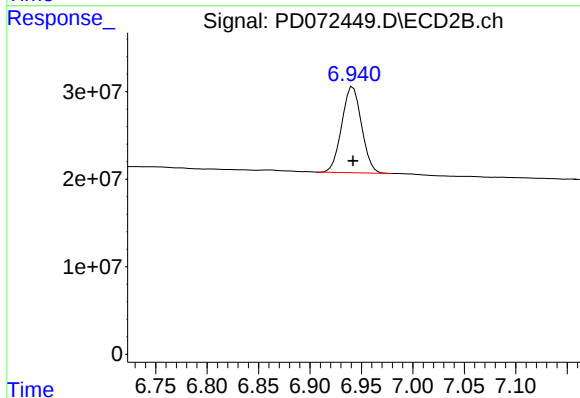


#17 4,4'-DDT

R.T.: 6.942 min
Delta R.T.: 0.000 min
Response: 131659090
Conc: 11.09 ng/ml

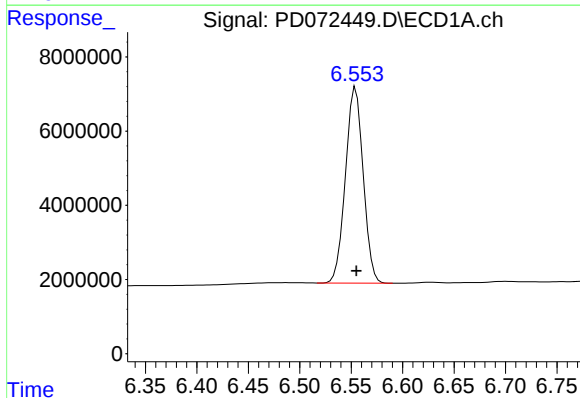


#20 Methoxychlor

R.T.: 6.554 min
Delta R.T.: 0.000 min
Response: 63464472
Conc: 53.72 ng/ml

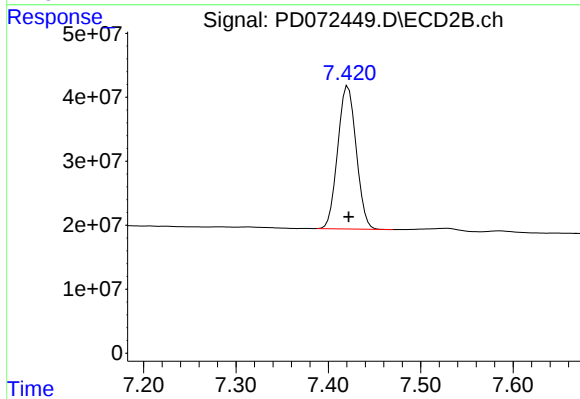

#20 Methoxychlor


R.T.: 7.421 min
Delta R.T.: 0.000 min
Response: 310892782
Conc: 57.28 ng/ml

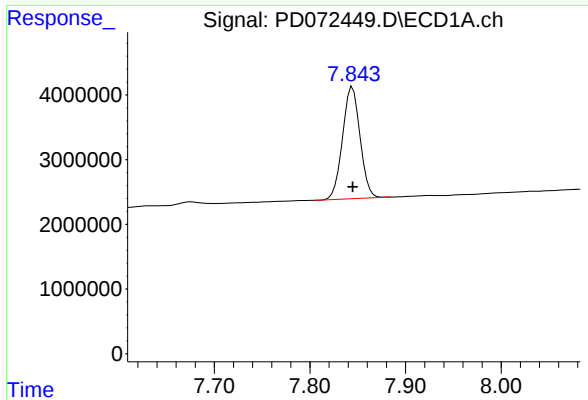

#27 Decachlorobiphenyl

R.T.: 7.845 min
Delta R.T.: 0.000 min
Response: 22138948
Conc: 11.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

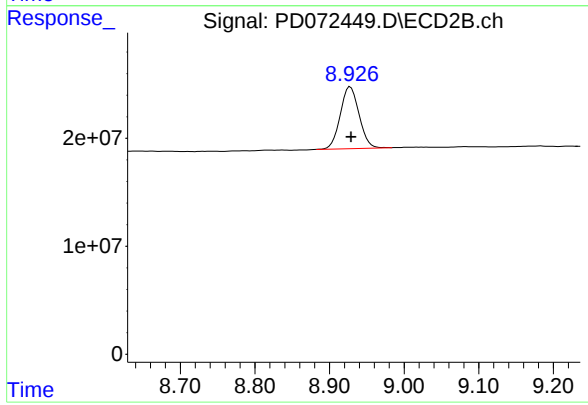

#27 Decachlorobiphenyl

R.T.: 8.928 min
Delta R.T.: -0.001 min
Response: 100192169
Conc: 11.21 ng/ml