

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101722\
 Data File : PD072451.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2022 16:39
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 17:37:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 17 17:34:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.706	3.468	26060640	398.5E6	10.463	10.725
27)	SA Decachlor...	7.845	8.929	41803442	188.6E6	21.387	21.103
Target Compounds							
2)	A alpha-BHC	3.212	3.933	36356399	517.5E6	9.950	10.741
3)	MA gamma-BHC...	3.543	4.267	32368889	445.7E6	10.082	11.031
4)	MA Heptachlor	3.875	4.834	34420549	310.3E6	10.189	10.964
9)	A Endosulfan I	5.030	5.991	27335581	170.3E6	10.352	10.711
13)	MA Dieldrin	5.297	6.268	57626459	342.1E6	20.013	21.330
14)	MA Endrin	5.574	6.500	50549554	288.2E6	20.085	21.552
16)	A 4,4'-DDD	5.721	6.634	44084957	259.2E6	19.658	21.251
17)	MA 4,4'-DDT	5.970	6.941	42984726	248.8E6	19.756	20.955
20)	A Methoxychlor	6.554	7.422	121.7E6	576.4E6	103.009	106.200


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101722\
Data File : PD072451.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2022 16:39
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 17:37:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
Quant Title : GC Extractables
QLast Update : Mon Oct 17 17:34:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

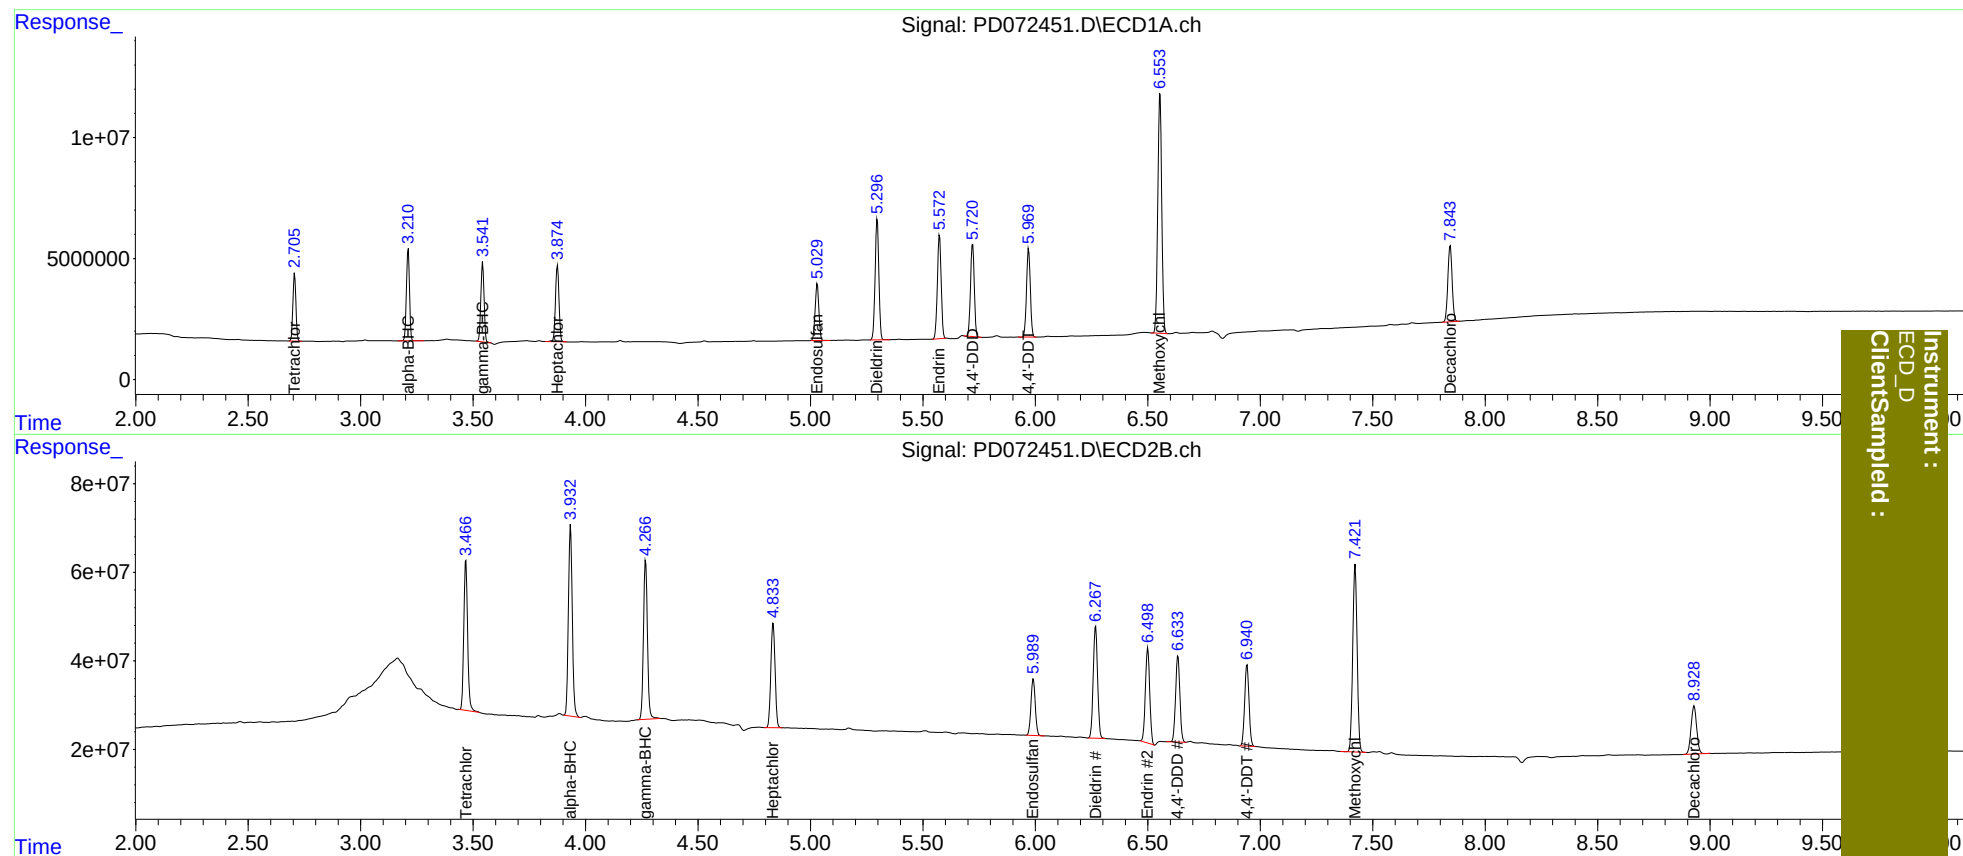


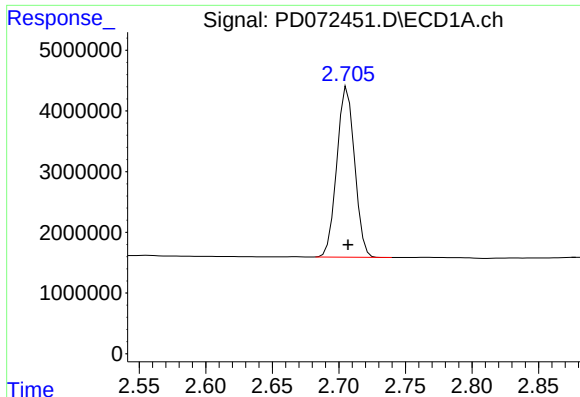

#1 Tetrachloro-m-xylene


R.T.: 2.706 min
Delta R.T.: 0.000 min
Response: 26060640
Conc: 10.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

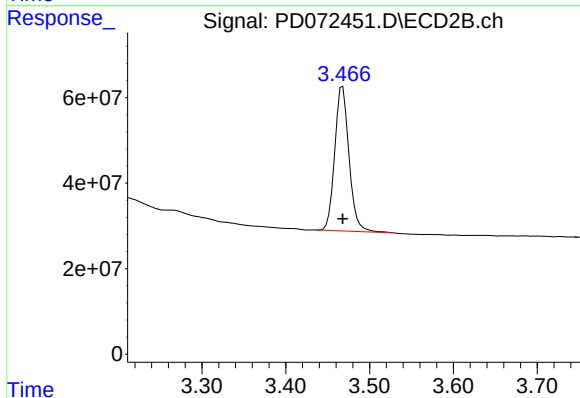


#1 Tetrachloro-m-xylene

R.T.: 3.468 min
Delta R.T.: 0.000 min
Response: 398495806
Conc: 10.73 ng/ml

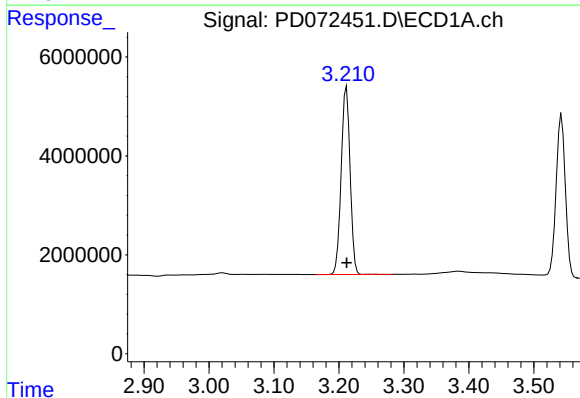


#2 alpha-BHC

R.T.: 3.212 min
Delta R.T.: 0.000 min
Response: 36356399
Conc: 9.95 ng/ml

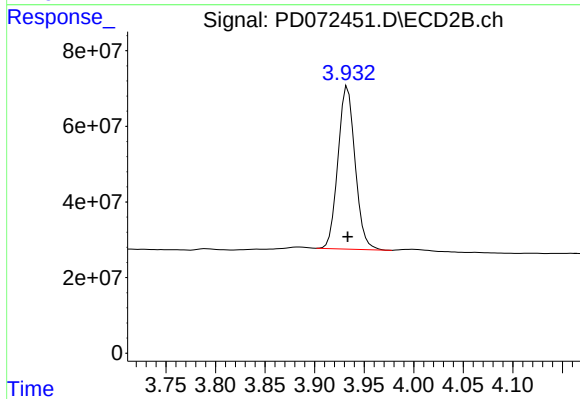

#2 alpha-BHC


R.T.: 3.933 min
Delta R.T.: 0.000 min
Response: 517549727
Conc: 10.74 ng/ml

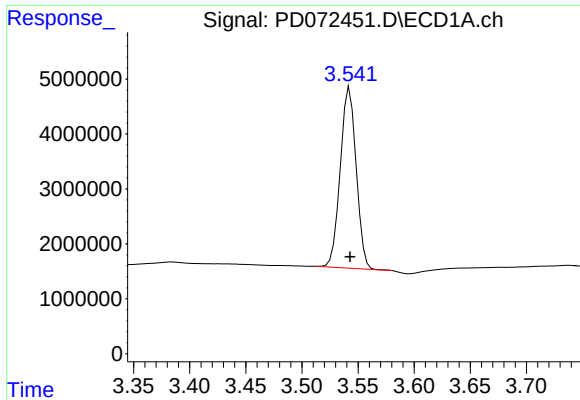

#3 gamma-BHC (Lindane)


R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 32368889
Conc: 10.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

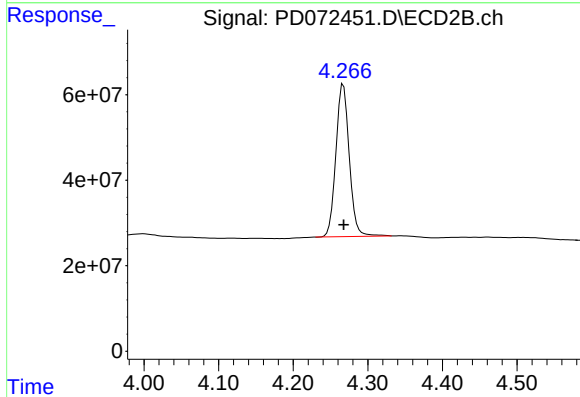


#3 gamma-BHC (Lindane)

R.T.: 4.267 min
Delta R.T.: 0.000 min
Response: 445667850
Conc: 11.03 ng/ml

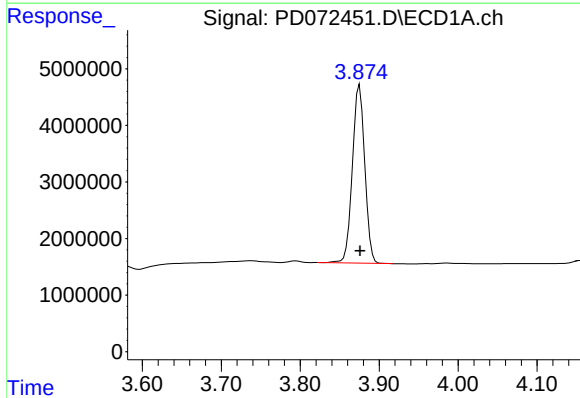


#4 Heptachlor

R.T.: 3.875 min
Delta R.T.: 0.000 min
Response: 34420549
Conc: 10.19 ng/ml

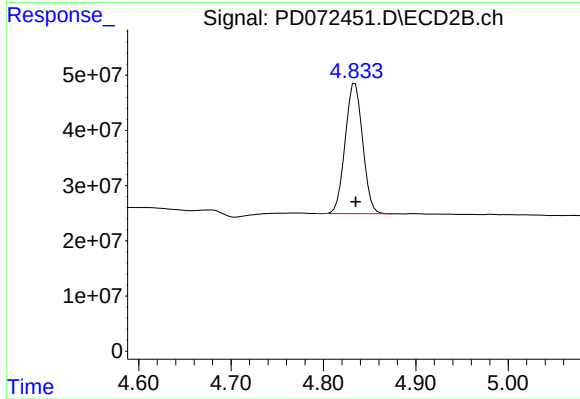

#4 Heptachlor


R.T.: 4.834 min
Delta R.T.: 0.000 min
Response: 310347141
Conc: 10.96 ng/ml

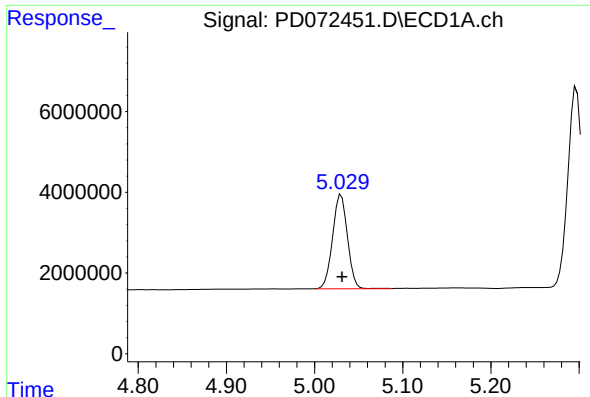

#9 Endosulfan I


R.T.: 5.030 min
Delta R.T.: 0.000 min
Response: 27335581
Conc: 10.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

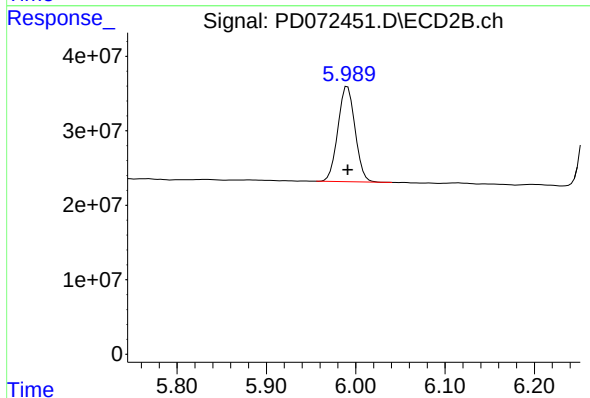


#9 Endosulfan I

R.T.: 5.991 min
Delta R.T.: 0.000 min
Response: 170268090
Conc: 10.71 ng/ml

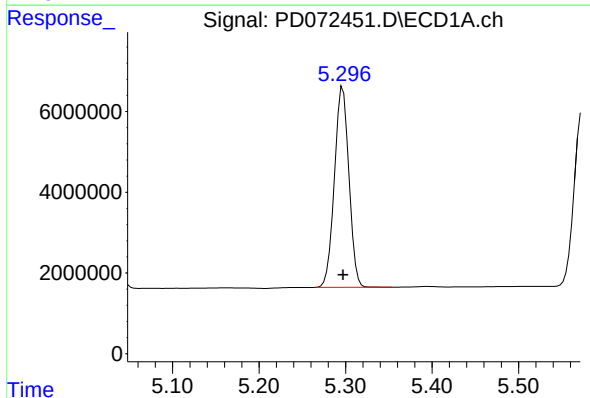


#13 Dieldrin

R.T.: 5.297 min
Delta R.T.: 0.000 min
Response: 57626459
Conc: 20.01 ng/ml

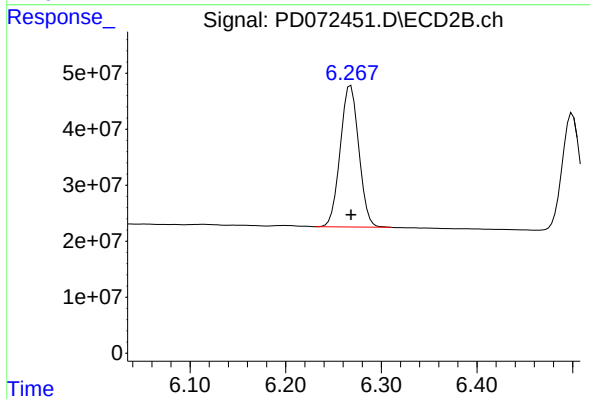

#13 Dieldrin


R.T.: 6.268 min
Delta R.T.: 0.000 min
Response: 342118830
Conc: 21.33 ng/ml

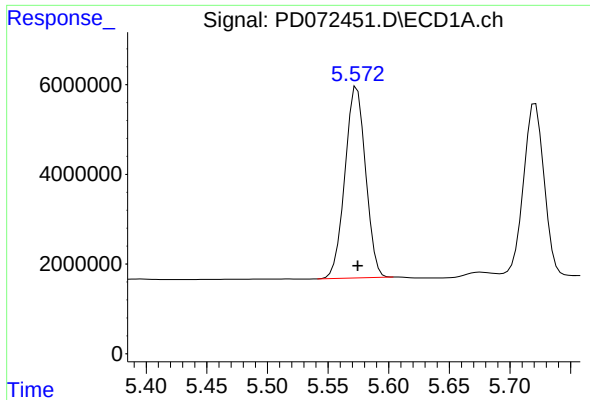

#14 Endrin


R.T.: 5.574 min
Delta R.T.: 0.000 min
Response: 50549554
Conc: 20.09 ng/ml

Instrument :
ECD_D
ClientSampleId :

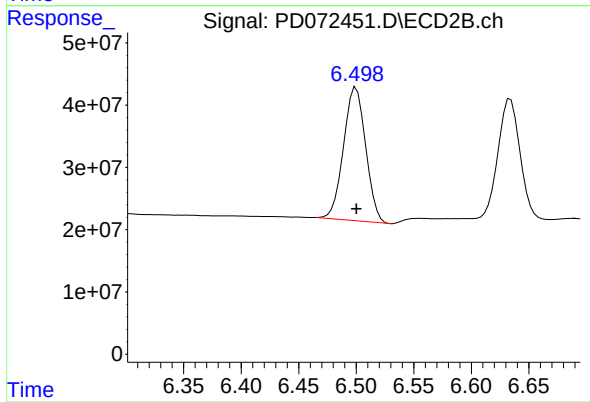


#14 Endrin

R.T.: 6.500 min
Delta R.T.: 0.000 min
Response: 288244260
Conc: 21.55 ng/ml

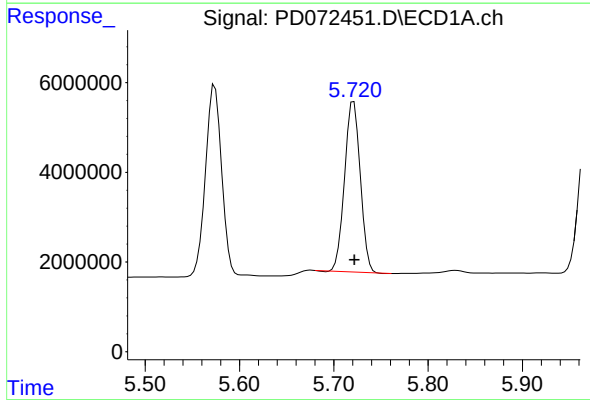


#16 4,4'-DDD

R.T.: 5.721 min
Delta R.T.: 0.000 min
Response: 44084957
Conc: 19.66 ng/ml

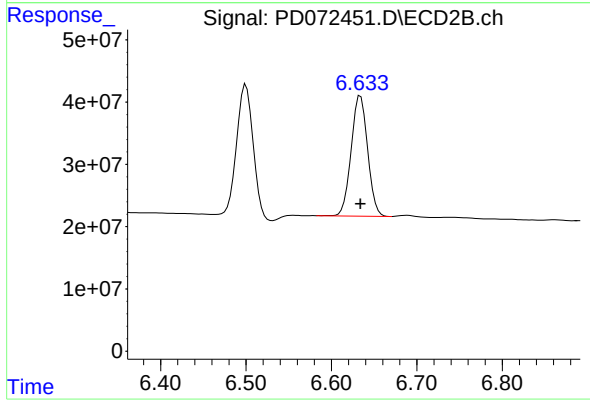

#16 4,4'-DDD


R.T.: 6.634 min
Delta R.T.: 0.000 min
Response: 259172213
Conc: 21.25 ng/ml

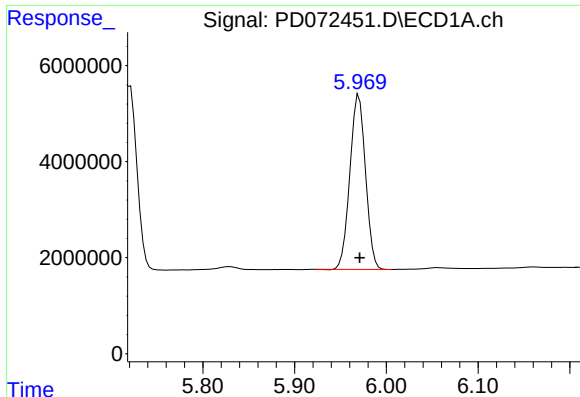

#17 4,4'-DDT


R.T.: 5.970 min
Delta R.T.: 0.000 min
Response: 42984726
Conc: 19.76 ng/ml

Instrument :
ECD_D
ClientSampleId :

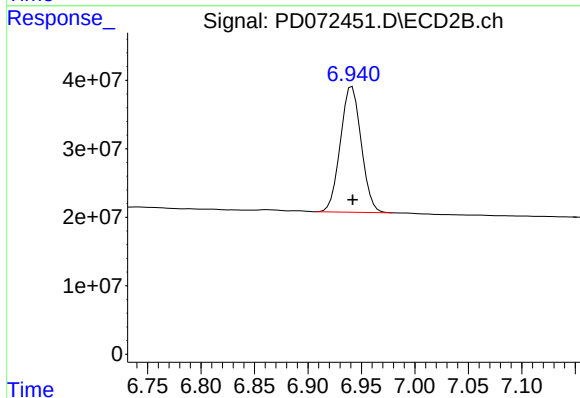


#17 4,4'-DDT

R.T.: 6.941 min
Delta R.T.: 0.000 min
Response: 248807930
Conc: 20.96 ng/ml

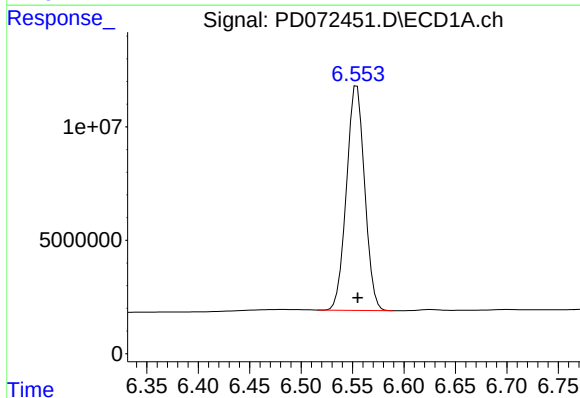


#20 Methoxychlor

R.T.: 6.554 min
Delta R.T.: 0.000 min
Response: 121696190
Conc: 103.01 ng/ml

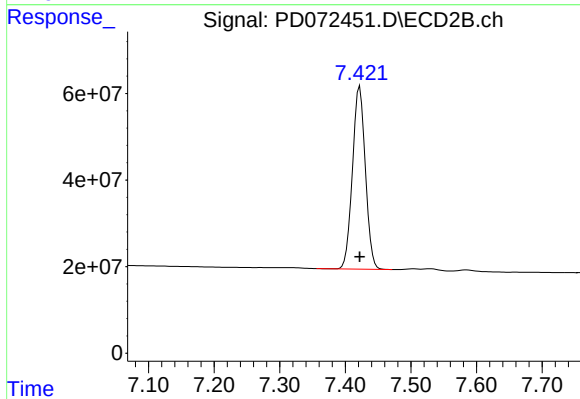

#20 Methoxychlor


R.T.: 7.422 min
Delta R.T.: 0.000 min
Response: 576422397
Conc: 106.20 ng/ml

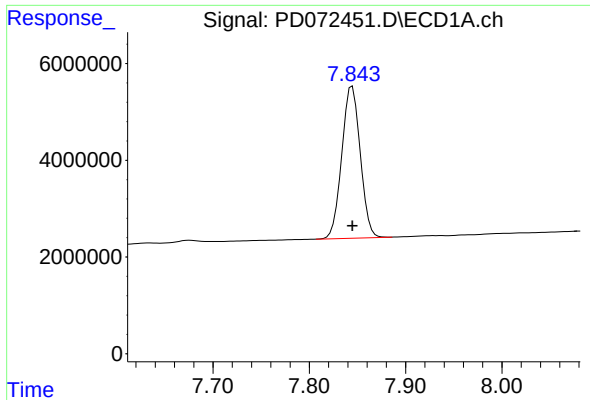

#27 Decachlorobiphenyl

R.T.: 7.845 min
Delta R.T.: 0.000 min
Response: 41803442
Conc: 21.39 ng/ml

Instrument :
ECD_D
ClientSampleId :

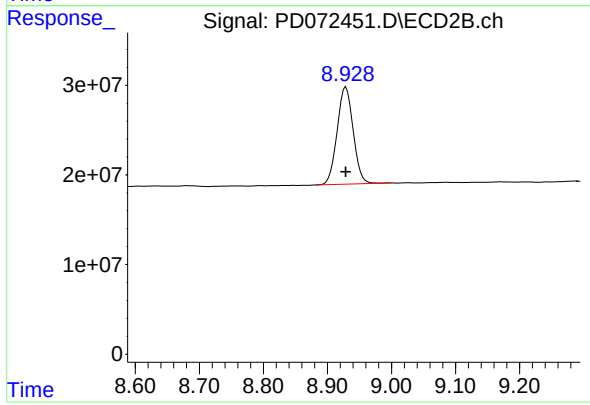

#27 Decachlorobiphenyl

R.T.: 8.929 min
Delta R.T.: 0.000 min
Response: 188641228
Conc: 21.10 ng/ml