

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101722\
 Data File : PD072455.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2022 17:32
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 17:58:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 17 17:34:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.706	3.468	99578472	1418.8E6	39.979	38.185
27)	SA Decachlor...	7.845	8.928	152.6E6	685.8E6	78.049	76.715
Target Compounds							
2)	A alpha-BHC	3.212	3.933	153.2E6	1850.7E6	41.931	38.410
3)	MA gamma-BHC...	3.543	4.267	134.2E6	1519.5E6	41.809	37.610
4)	MA Heptachlor	3.876	4.835	138.1E6	1049.2E6	40.885	37.065
9)	A Endosulfan I	5.030	5.991	105.2E6	597.6E6	39.845	37.593
13)	MA Dieldrin	5.297	6.268	236.9E6	1229.4E6	82.287	76.648
14)	MA Endrin	5.574	6.500	207.4E6	1023.3E6	82.389	76.508
16)	A 4,4'-DDD	5.721	6.634	183.9E6	935.3E6	82.011	76.687
17)	MA 4,4'-DDT	5.970	6.942	180.6E6	926.1E6	82.985	77.995
20)	A Methoxychlor	6.555	7.422	467.1E6	2077.9E6	395.397	382.833


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101722\
Data File : PD072455.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2022 17:32
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 17:58:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
Quant Title : GC Extractables
QLast Update : Mon Oct 17 17:34:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

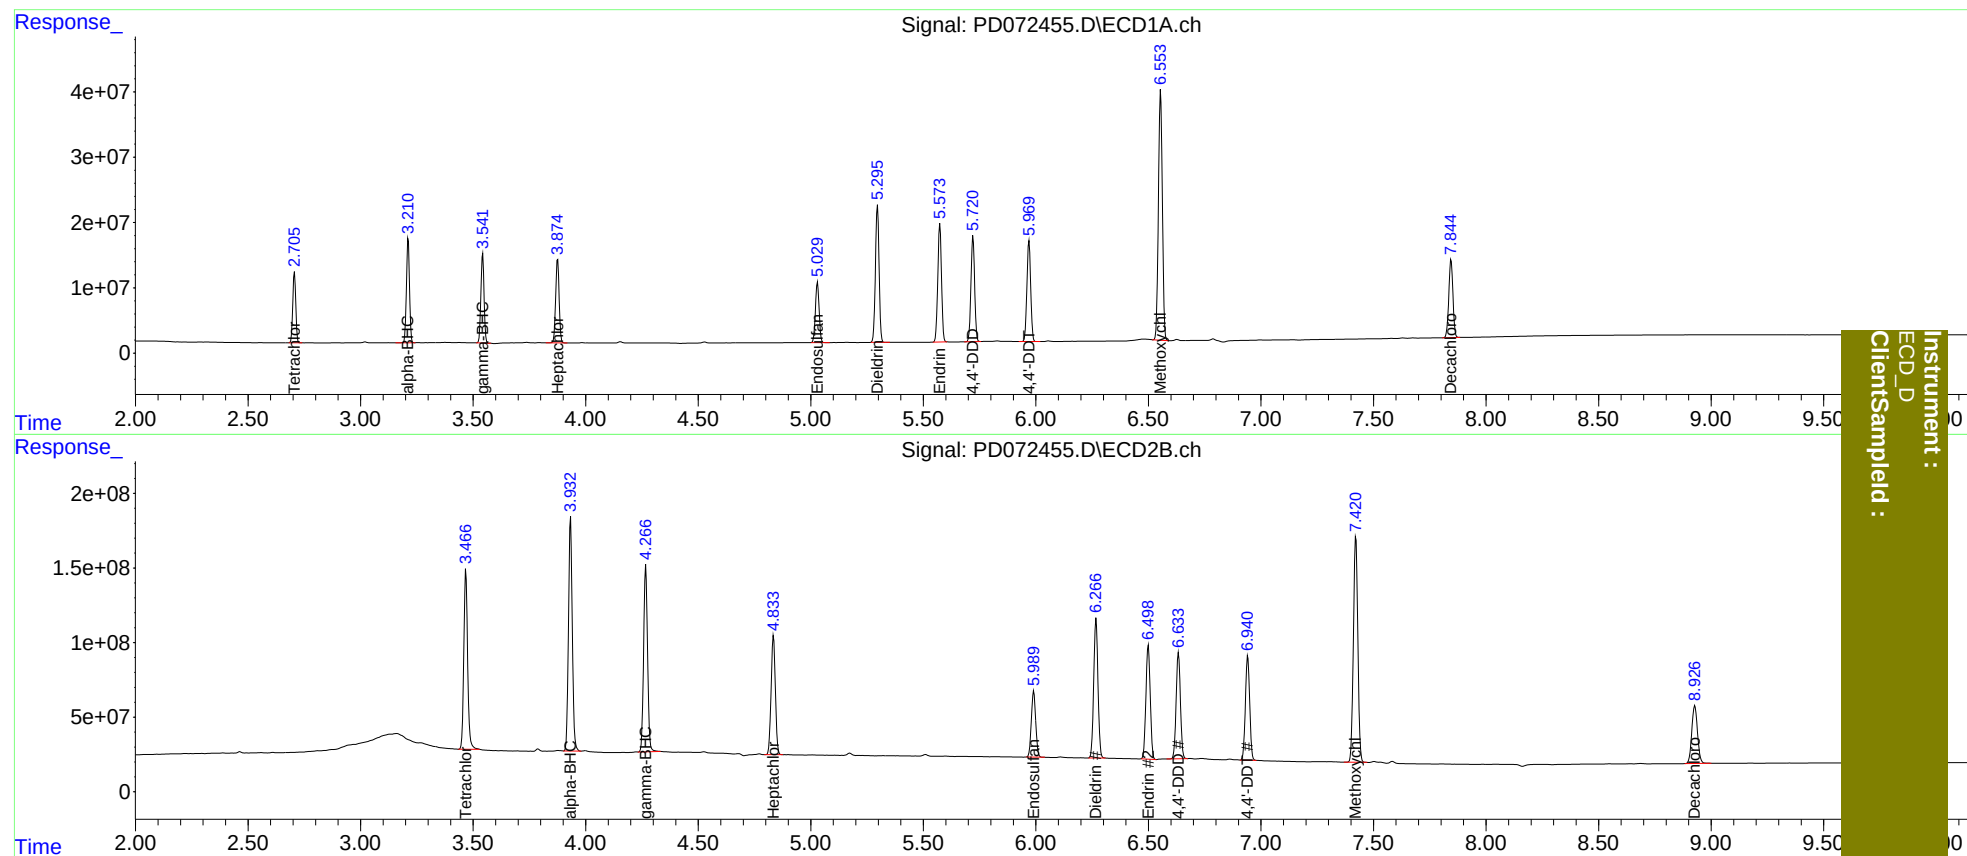


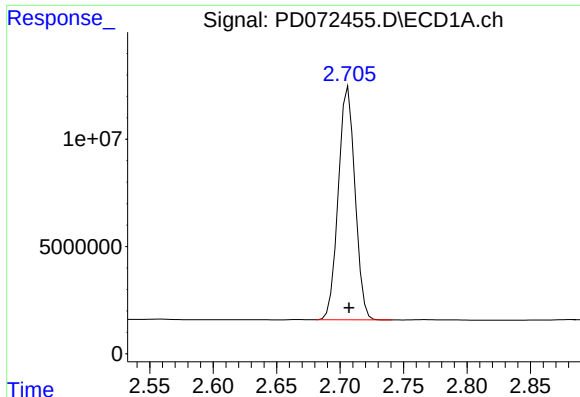

#1 Tetrachloro-m-xylene


R.T.: 2.706 min
Delta R.T.: 0.000 min
Response: 99578472
Conc: 39.98 ng/ml

Instrument :
ECD_D
ClientSampleId :

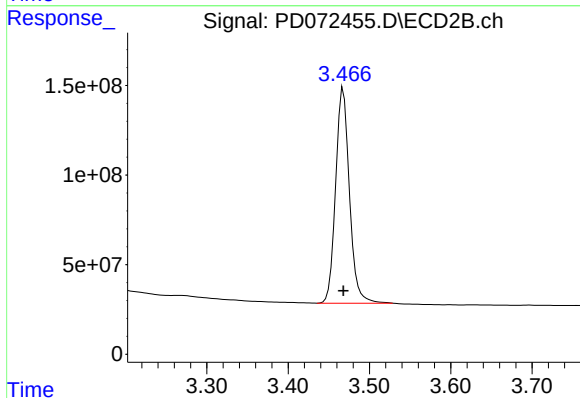


#1 Tetrachloro-m-xylene

R.T.: 3.468 min
Delta R.T.: 0.000 min
Response: 1418770551
Conc: 38.18 ng/ml

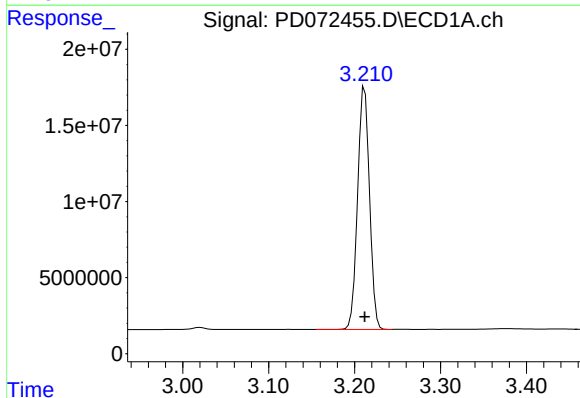


#2 alpha-BHC

R.T.: 3.212 min
Delta R.T.: 0.000 min
Response: 153208552
Conc: 41.93 ng/ml

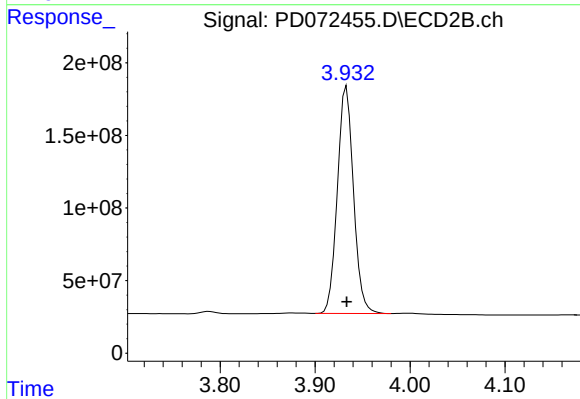

#2 alpha-BHC


R.T.: 3.933 min
Delta R.T.: 0.000 min
Response: 1850728322
Conc: 38.41 ng/ml

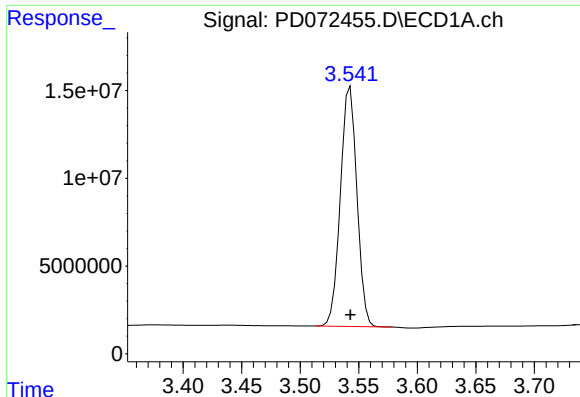

#3 gamma-BHC (Lindane)


R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 134228097
Conc: 41.81 ng/ml

Instrument :
ECD_D
ClientSampleId :

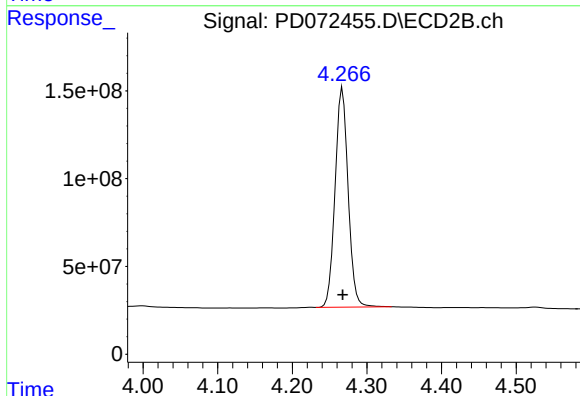


#3 gamma-BHC (Lindane)

R.T.: 4.267 min
Delta R.T.: 0.000 min
Response: 1519524607
Conc: 37.61 ng/ml

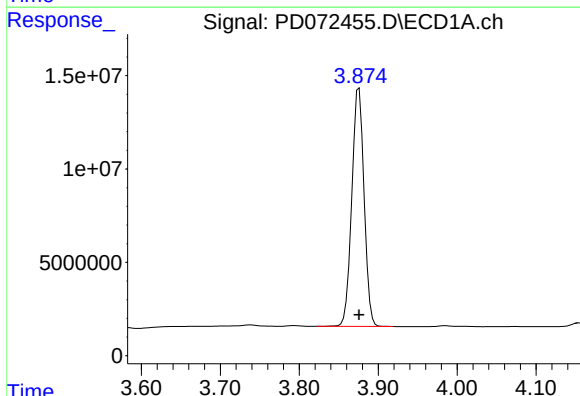


#4 Heptachlor

R.T.: 3.876 min
Delta R.T.: 0.000 min
Response: 138116169
Conc: 40.89 ng/ml

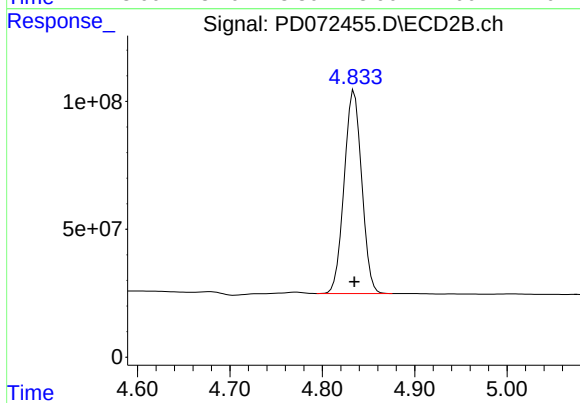

#4 Heptachlor


R.T.: 4.835 min
Delta R.T.: 0.000 min
Response: 1049155403
Conc: 37.07 ng/ml

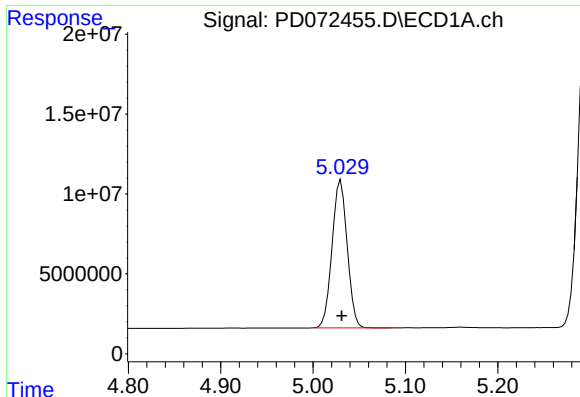

#9 Endosulfan I


R.T.: 5.030 min
Delta R.T.: -0.001 min
Response: 105212431
Conc: 39.85 ng/ml

Instrument :
ECD_D
ClientSampleId :

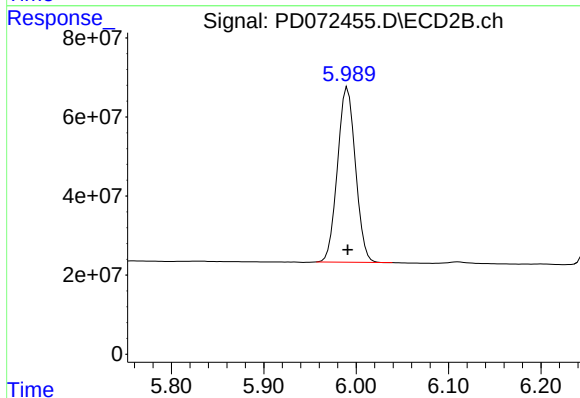


#9 Endosulfan I

R.T.: 5.991 min
Delta R.T.: 0.000 min
Response: 597612564
Conc: 37.59 ng/ml

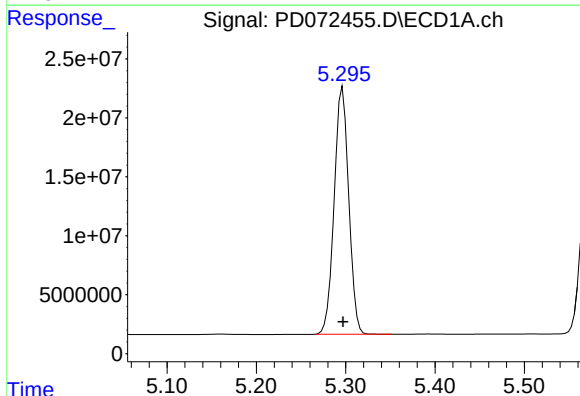


#13 Dieldrin

R.T.: 5.297 min
Delta R.T.: 0.000 min
Response: 236942500
Conc: 82.29 ng/ml

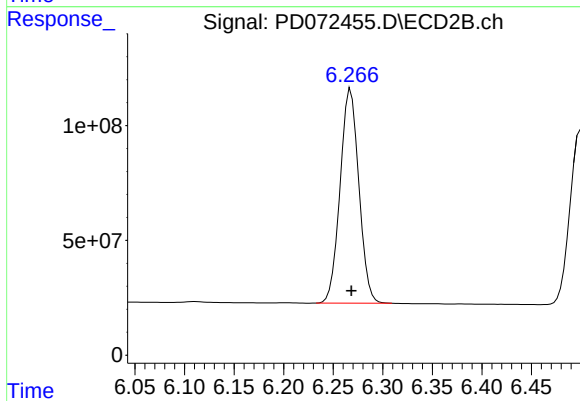

#13 Dieldrin


R.T.: 6.268 min
Delta R.T.: 0.000 min
Response: 1229387682
Conc: 76.65 ng/ml

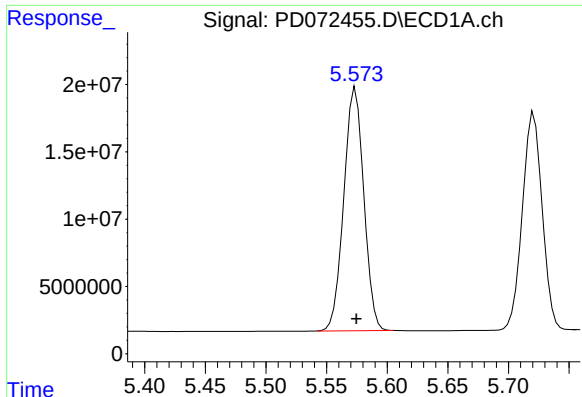

#14 Endrin


R.T.: 5.574 min
Delta R.T.: 0.000 min
Response: 207350385
Conc: 82.39 ng/ml

Instrument :
ECD_D
ClientSampleId :

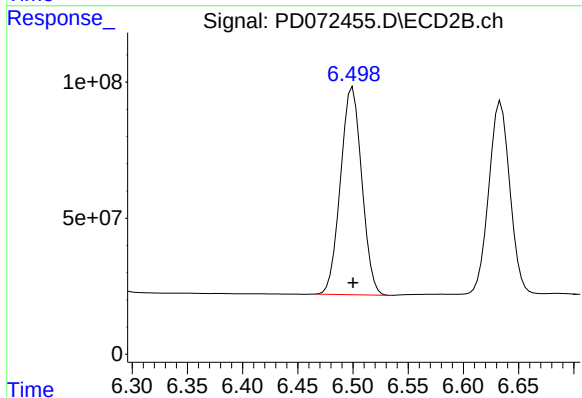


#14 Endrin

R.T.: 6.500 min
Delta R.T.: 0.000 min
Response: 1023257309
Conc: 76.51 ng/ml

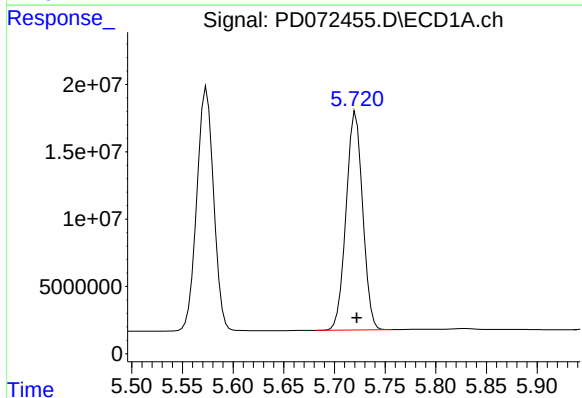


#16 4,4'-DDD

R.T.: 5.721 min
Delta R.T.: 0.000 min
Response: 183916806
Conc: 82.01 ng/ml

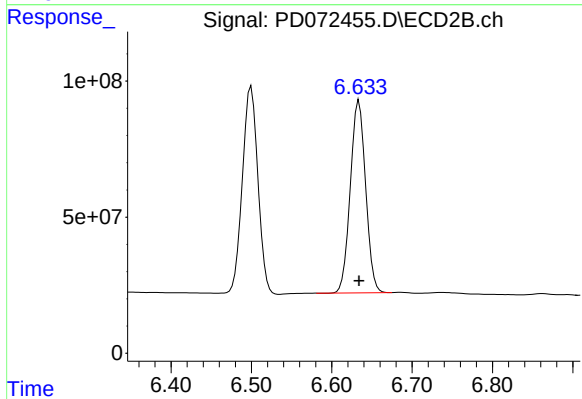

#16 4,4'-DDD


R.T.: 6.634 min
Delta R.T.: 0.000 min
Response: 935272609
Conc: 76.69 ng/ml

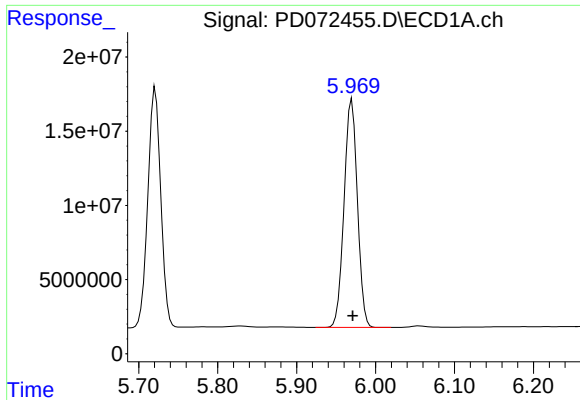

#17 4,4'-DDT


R.T.: 5.970 min
Delta R.T.: 0.000 min
Response: 180554208
Conc: 82.99 ng/ml

Instrument :
ECD_D
ClientSampleId :

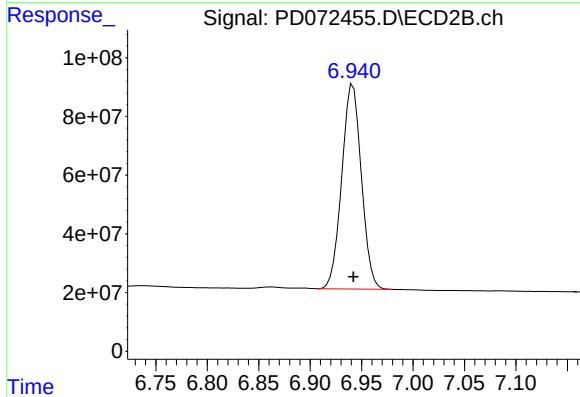


#17 4,4'-DDT

R.T.: 6.942 min
Delta R.T.: 0.000 min
Response: 926061330
Conc: 78.00 ng/ml

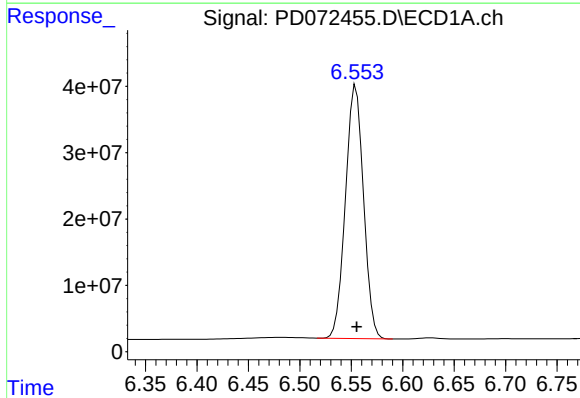


#20 Methoxychlor

R.T.: 6.555 min
Delta R.T.: 0.000 min
Response: 467125308
Conc: 395.40 ng/ml

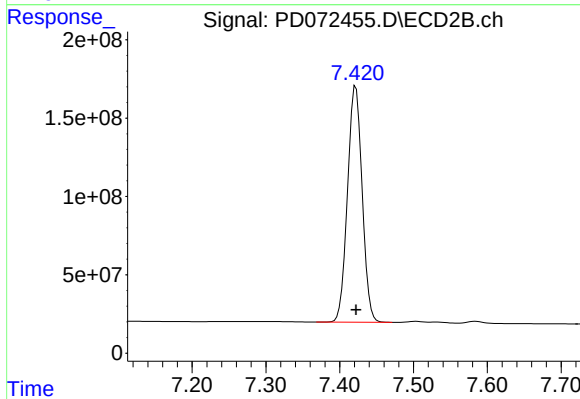

#20 Methoxychlor


R.T.: 7.422 min
Delta R.T.: 0.000 min
Response: 2077902678
Conc: 382.83 ng/ml

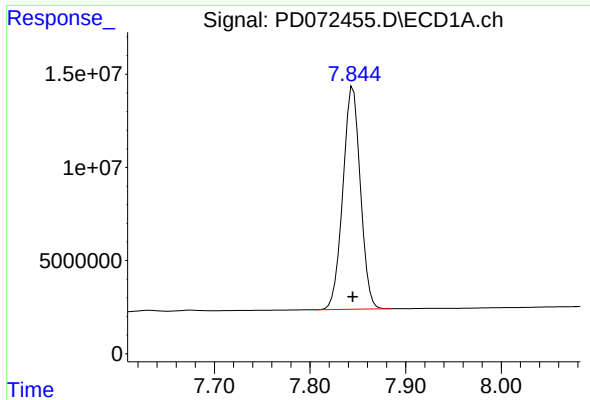

#27 Decachlorobiphenyl

R.T.: 7.845 min
Delta R.T.: 0.000 min
Response: 152554050
Conc: 78.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

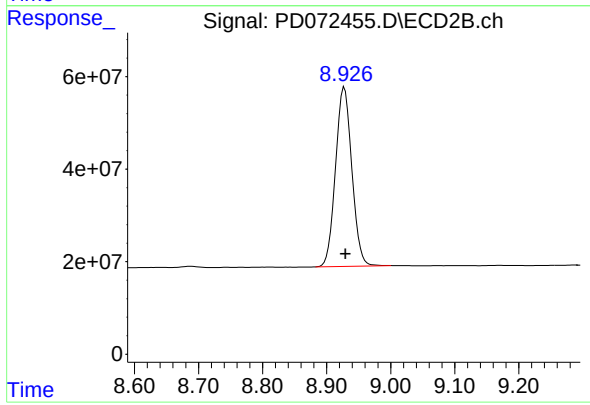

#27 Decachlorobiphenyl

R.T.: 8.928 min
Delta R.T.: -0.001 min
Response: 685757844
Conc: 76.71 ng/ml