

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101722\
 Data File : PD072457.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2022 17:59
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 18:11:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 17 17:34:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.706	3.468	195.2E6	2638.8E6	78.353	71.021
27)	SA Decachlor...	7.844	8.928	294.8E6	1287.8E6	150.832	144.060
Target Compounds							
2)	A alpha-BHC	3.211	3.933	312.7E6	3500.5E6	85.579	72.649
3)	MA gamma-BHC...	3.542	4.267	272.4E6	2837.3E6	84.834	70.227
4)	MA Heptachlor	3.875	4.835	276.6E6	1922.3E6	81.880	67.913
9)	A Endosulfan I	5.030	5.990	208.6E6	1109.7E6	78.998	69.805
13)	MA Dieldrin	5.297	6.268	475.6E6	2332.4E6	165.157	145.419
14)	MA Endrin	5.574	6.500	415.0E6	1928.7E6	164.908	144.207
16)	A 4,4'-DDD	5.721	6.634	370.0E6	1763.0E6	164.990	144.557
17)	MA 4,4'-DDT	5.970	6.942	367.1E6	1774.2E6	168.735	149.428
20)	A Methoxychlor	6.554	7.422	905.6E6	3873.7E6	766.577	713.693

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101722\
Data File : PD072457.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2022 17:59
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 18:11:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
Quant Title : GC Extractables
QLast Update : Mon Oct 17 17:34:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

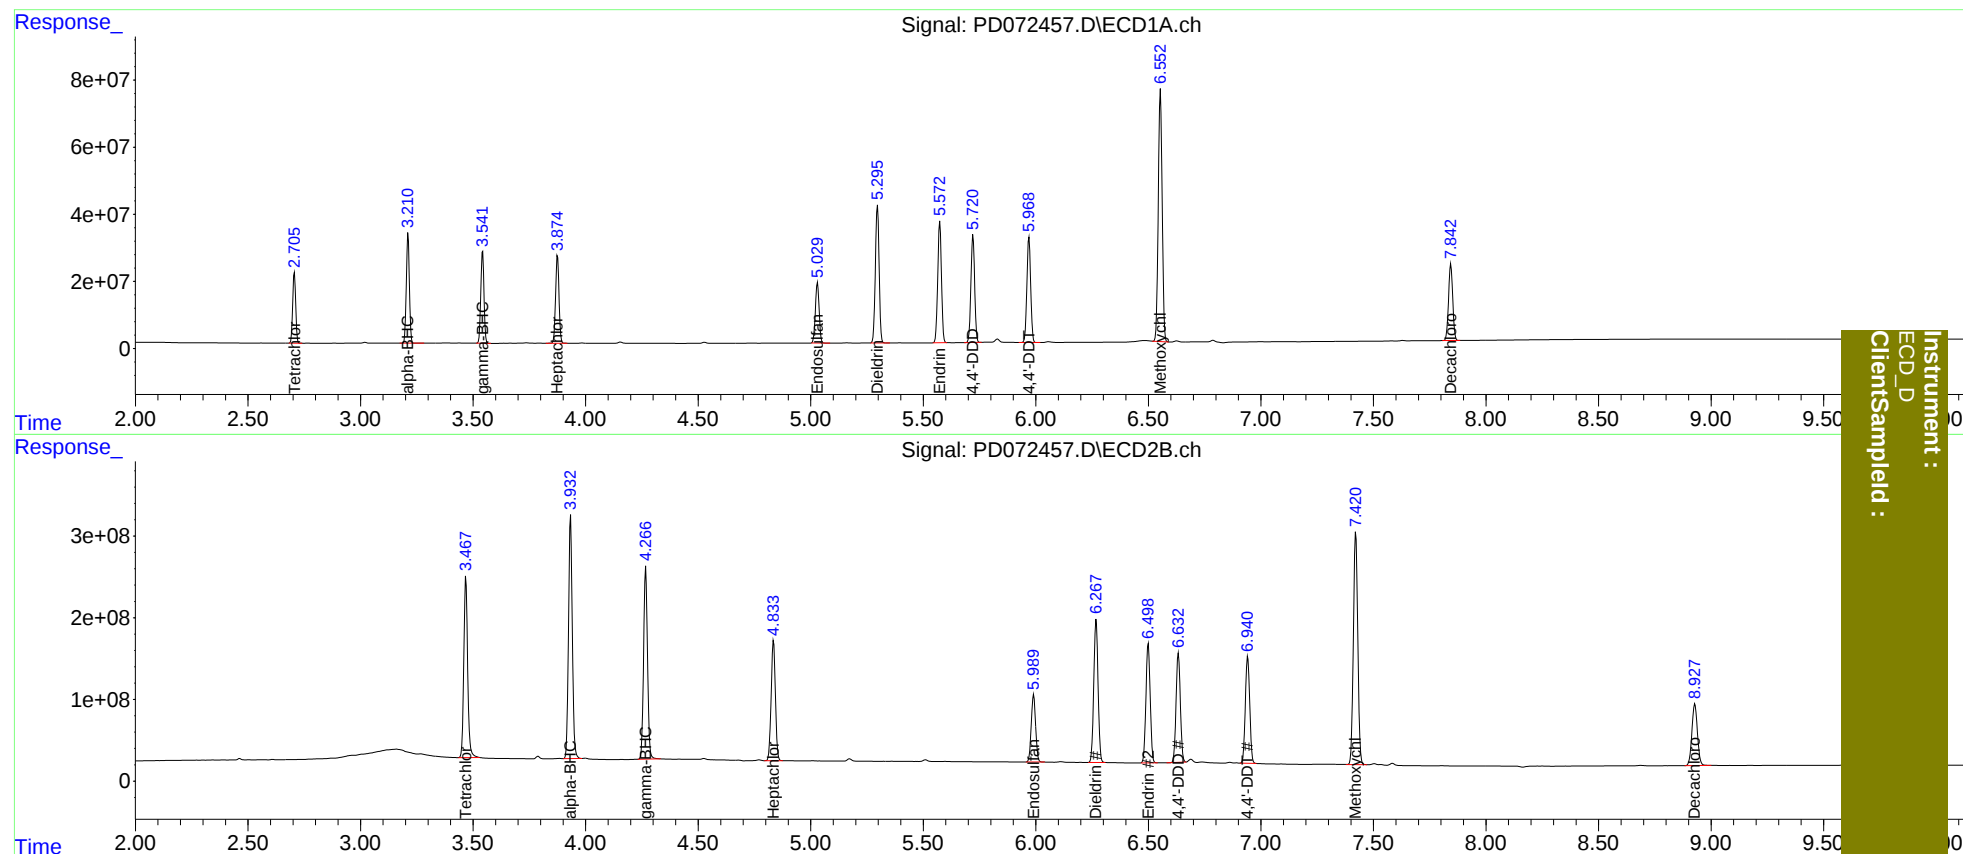


Instrument :
ECD_D
ClientSampled :
10

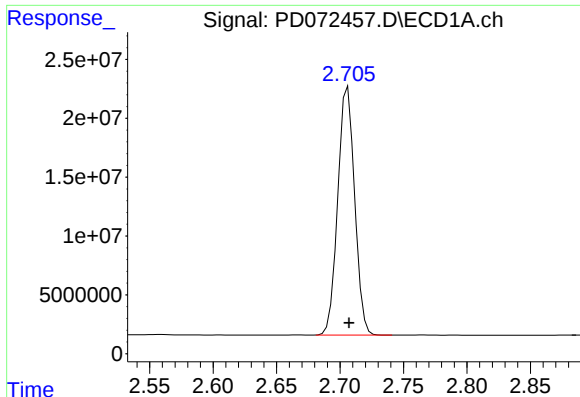

#1 Tetrachloro-m-xylene


R.T.: 2.706 min
Delta R.T.: 0.000 min
Response: 195156788
Conc: 78.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

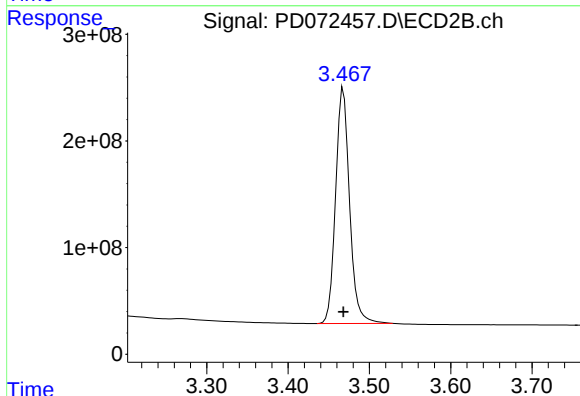


#1 Tetrachloro-m-xylene

R.T.: 3.468 min
Delta R.T.: 0.000 min
Response: 2638833387
Conc: 71.02 ng/ml

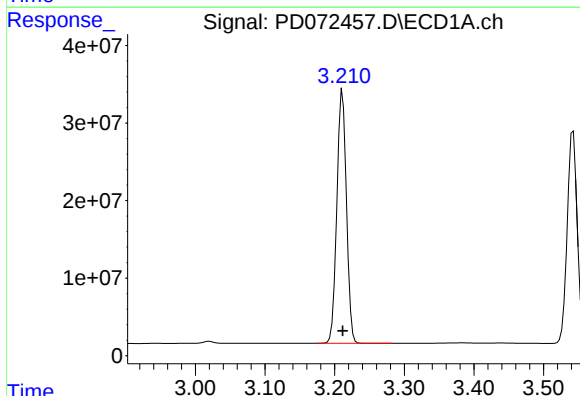


#2 alpha-BHC

R.T.: 3.211 min
Delta R.T.: 0.000 min
Response: 312688824
Conc: 85.58 ng/ml

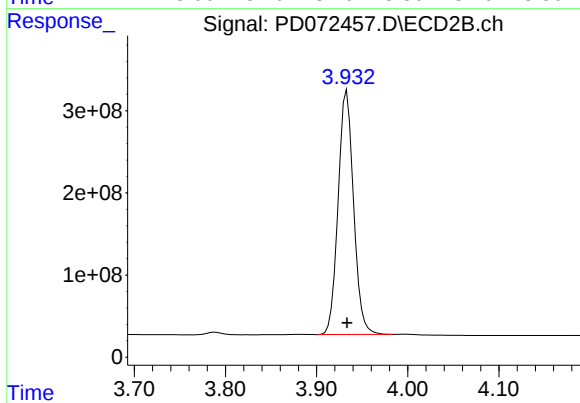

#2 alpha-BHC


R.T.: 3.933 min
Delta R.T.: 0.000 min
Response: 3500459160
Conc: 72.65 ng/ml

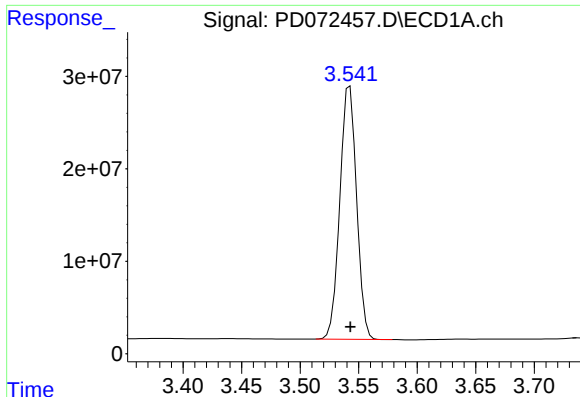

#3 gamma-BHC (Lindane)


R.T.: 3.542 min
Delta R.T.: 0.000 min
Response: 272364339
Conc: 84.83 ng/ml

Instrument :
ECD_D
ClientSampleId :

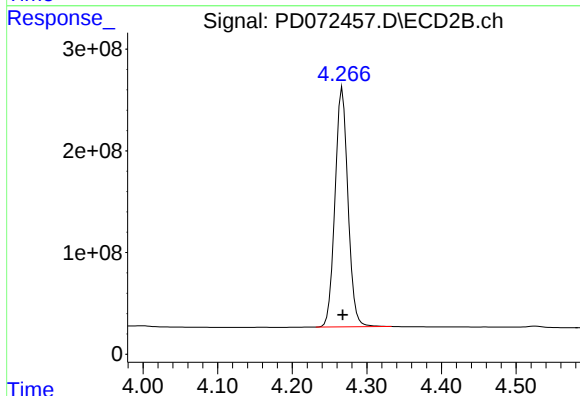


#3 gamma-BHC (Lindane)

R.T.: 4.267 min
Delta R.T.: 0.000 min
Response: 2837300006
Conc: 70.23 ng/ml

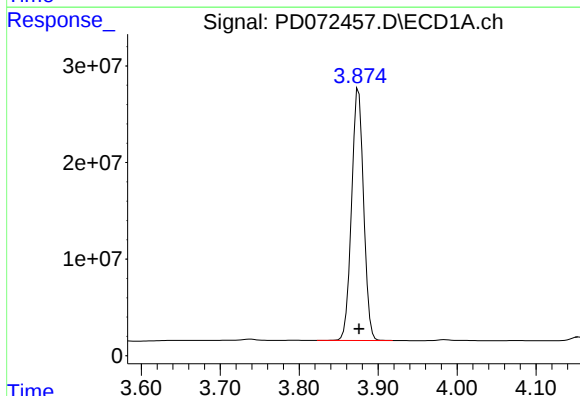


#4 Heptachlor

R.T.: 3.875 min
Delta R.T.: 0.000 min
Response: 276603505
Conc: 81.88 ng/ml

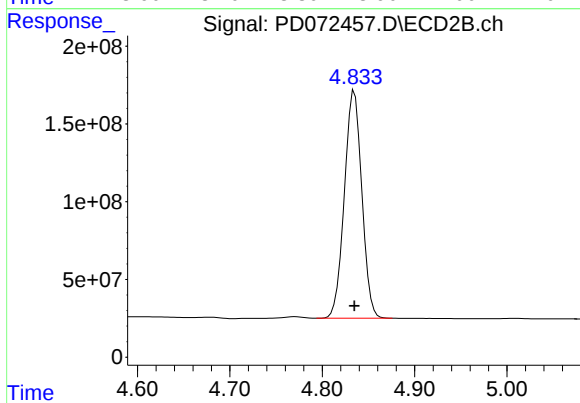

#4 Heptachlor


R.T.: 4.835 min
Delta R.T.: 0.000 min
Response: 1922330679
Conc: 67.91 ng/ml

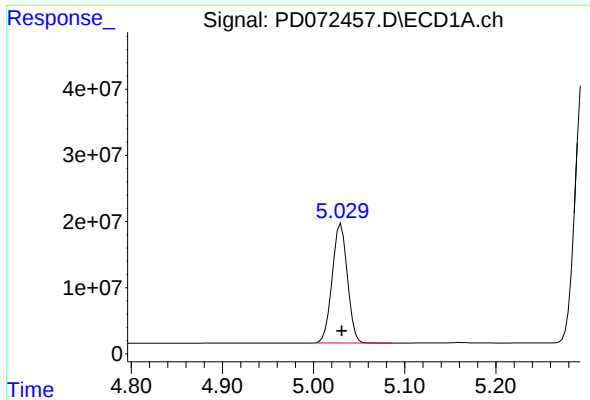

#9 Endosulfan I


R.T.: 5.030 min
Delta R.T.: 0.000 min
Response: 208596768
Conc: 79.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

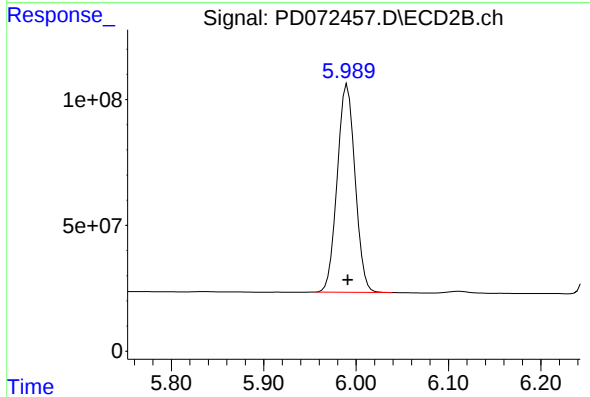


#9 Endosulfan I

R.T.: 5.990 min
Delta R.T.: 0.000 min
Response: 1109693092
Conc: 69.80 ng/ml

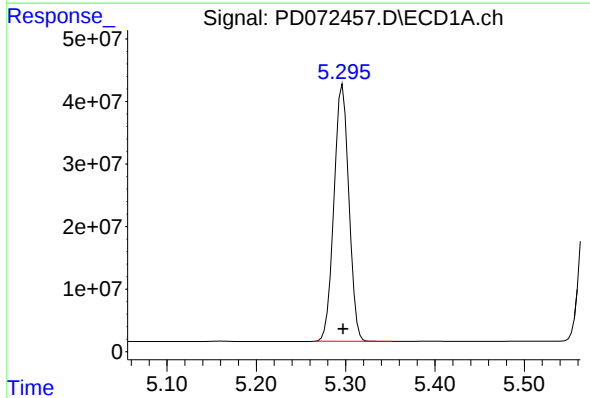


#13 Dieldrin

R.T.: 5.297 min
Delta R.T.: 0.000 min
Response: 475563051
Conc: 165.16 ng/ml

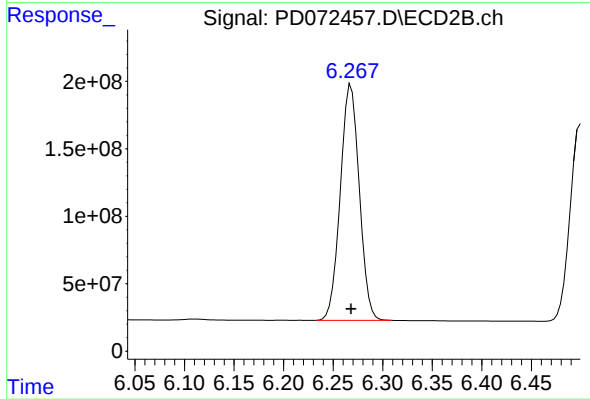

#13 Dieldrin


R.T.: 6.268 min
Delta R.T.: 0.000 min
Response: 2332442044
Conc: 145.42 ng/ml

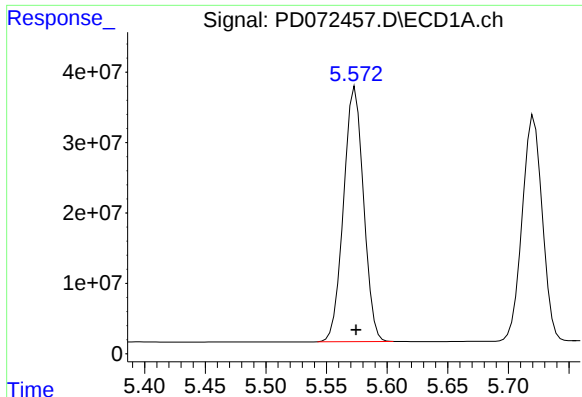

#14 Endrin


R.T.: 5.574 min
Delta R.T.: 0.000 min
Response: 415029578
Conc: 164.91 ng/ml

Instrument :
ECD_D
ClientSampleId :

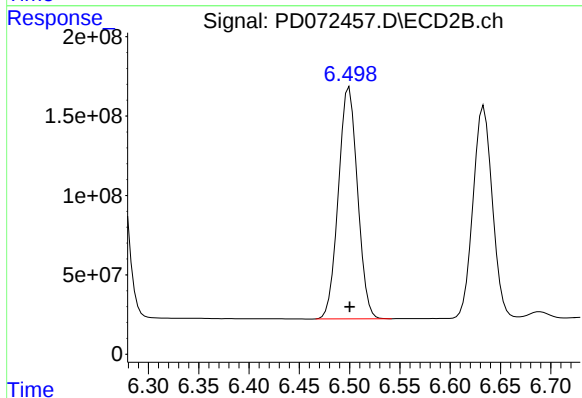


#14 Endrin

R.T.: 6.500 min
Delta R.T.: 0.000 min
Response: 1928693338
Conc: 144.21 ng/ml

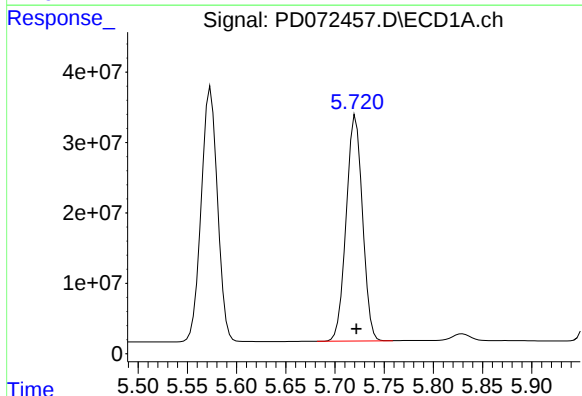


#16 4,4'-DDD

R.T.: 5.721 min
Delta R.T.: 0.000 min
Response: 370005931
Conc: 164.99 ng/ml

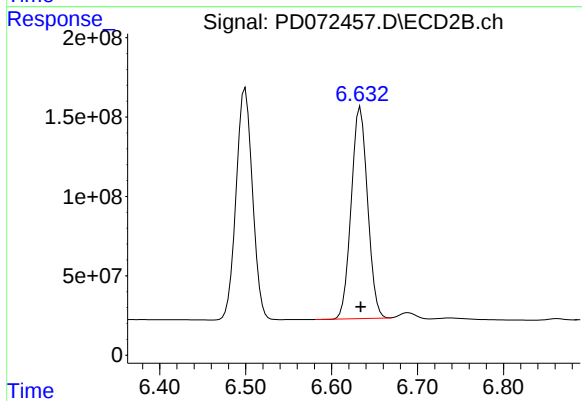

#16 4,4'-DDD


R.T.: 6.634 min
Delta R.T.: 0.000 min
Response: 1763003413
Conc: 144.56 ng/ml

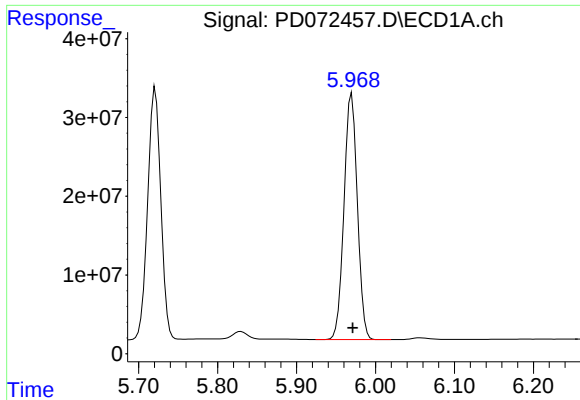

#17 4,4'-DDT


R.T.: 5.970 min
Delta R.T.: -0.001 min
Response: 367123198
Conc: 168.74 ng/ml

Instrument :
ECD_D
ClientSampleId :

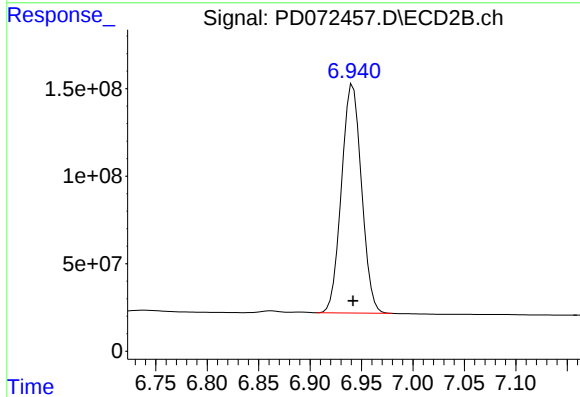


#17 4,4'-DDT

R.T.: 6.942 min
Delta R.T.: 0.000 min
Response: 1774203225
Conc: 149.43 ng/ml

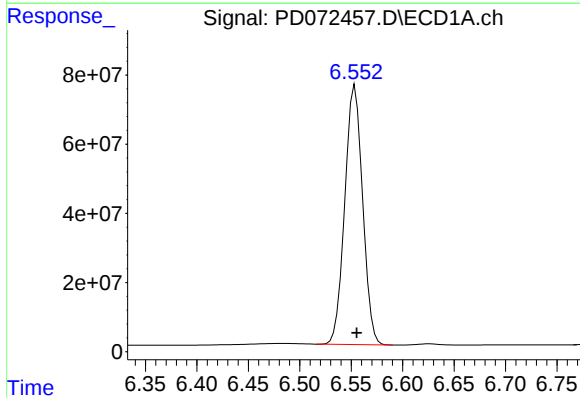


#20 Methoxychlor

R.T.: 6.554 min
Delta R.T.: -0.001 min
Response: 905639560
Conc: 766.58 ng/ml

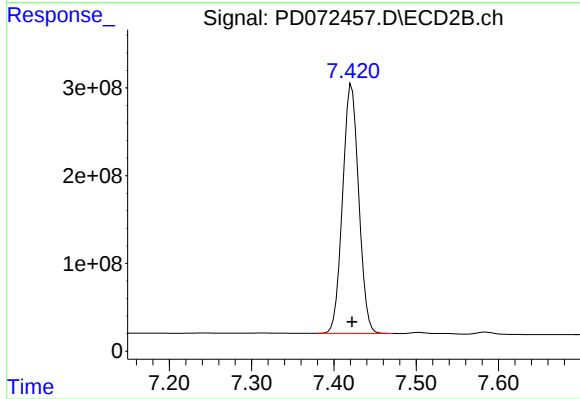

#20 Methoxychlor


R.T.: 7.422 min
Delta R.T.: 0.000 min
Response: 3873716824
Conc: 713.69 ng/ml

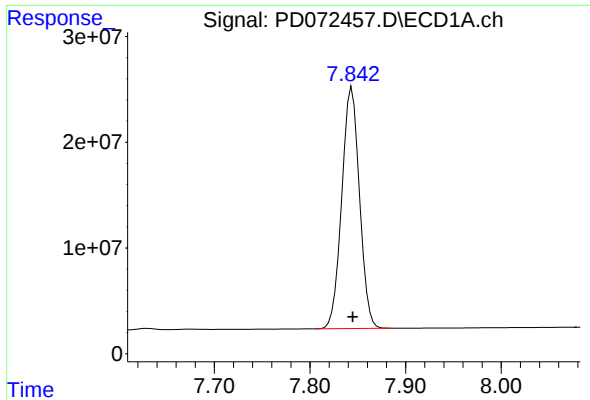

#27 Decachlorobiphenyl

R.T.: 7.844 min
Delta R.T.: 0.000 min
Response: 294814567
Conc: 150.83 ng/ml

Instrument :
ECD_D
ClientSampleId :

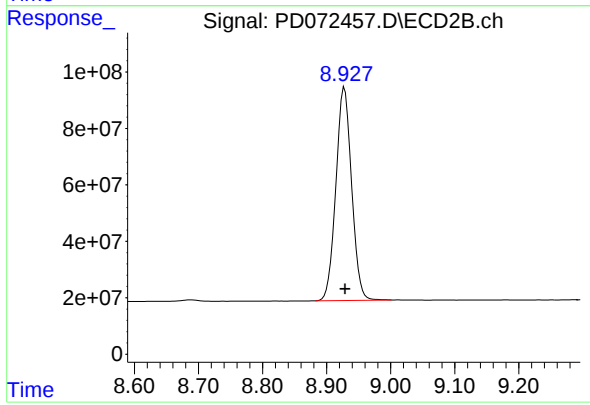

#27 Decachlorobiphenyl

R.T.: 8.928 min
Delta R.T.: -0.001 min
Response: 1287758249
Conc: 144.06 ng/ml