

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101722\
 Data File : PD072442.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2022 14:39
 Operator : AR\AJ
 Sample : RESC039
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC041

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/18/2022
 Supervised By :Ankita Jodhani 10/19/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 06:23:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 18 06:21:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.706	3.468	49045209	726.3E6	19.235	19.339
27)	SA Decachlor...	7.844	8.928	78574841	357.9E6	39.255	39.762
Target Compounds							
2)	A alpha-BHC	3.211	3.933	35100833	501.3E6	9.378	10.186
3)	MA gamma-BHC...	3.542	4.267	29971148	427.5E6	9.104	10.258
4)	MA Heptachlor	3.873	4.834	31889548	303.0E6	9.226m	10.526
5)	MB Aldrin	4.154	5.173	32271789	255.9E6	9.526	10.634
6)	B beta-BHC	3.843	4.483	15941186	172.7E6	9.972m	10.374
7)	B delta-BHC	4.075	4.727	32584831	322.3E6	9.188	10.115
8)	B Heptachlo...	4.660	5.606	28798692	201.1E6	9.494	10.334
9)	A Endosulfan I	5.030	5.990	25751690	167.9E6	9.579	10.453m
10)	B trans-Chl...	4.909	5.860	29533087	188.7E6	9.500	10.084
11)	B cis-Chlor...	4.973	5.936	28703884	177.3E6	9.504	9.912
12)	B 4,4'-DDE	5.161	6.109	53968760	330.7E6	18.526	20.217
13)	MA Dieldrin	5.296	6.268	54975133	331.2E6	18.771	20.291
14)	MA Endrin	5.573	6.500	48053229	282.1E6	18.769	20.514
15)	B Endosulfa...	5.872	6.730	45591717	257.2E6	18.927	20.158
16)	A 4,4'-DDD	5.721	6.634	43271769	253.7E6	19.048	20.456
17)	MA 4,4'-DDT	5.970	6.942	41345969	242.7E6	18.706	20.178
18)	B Endrin al...	6.054	6.862	40160284	219.1E6	19.652	20.366
19)	B Endosulfa...	6.278	7.094	46675719	238.8E6	19.338	20.001
20)	A Methoxychlor	6.554	7.422	117.5E6	561.9E6	98.408	102.356
21)	B Endrin ke...	6.789	7.584	56082874	261.6E6	19.679	20.402

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101722\
Data File : PD072442.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2022 14:39
Operator : AR\AJ
Sample : RESC039
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 06:23:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 18 06:21:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

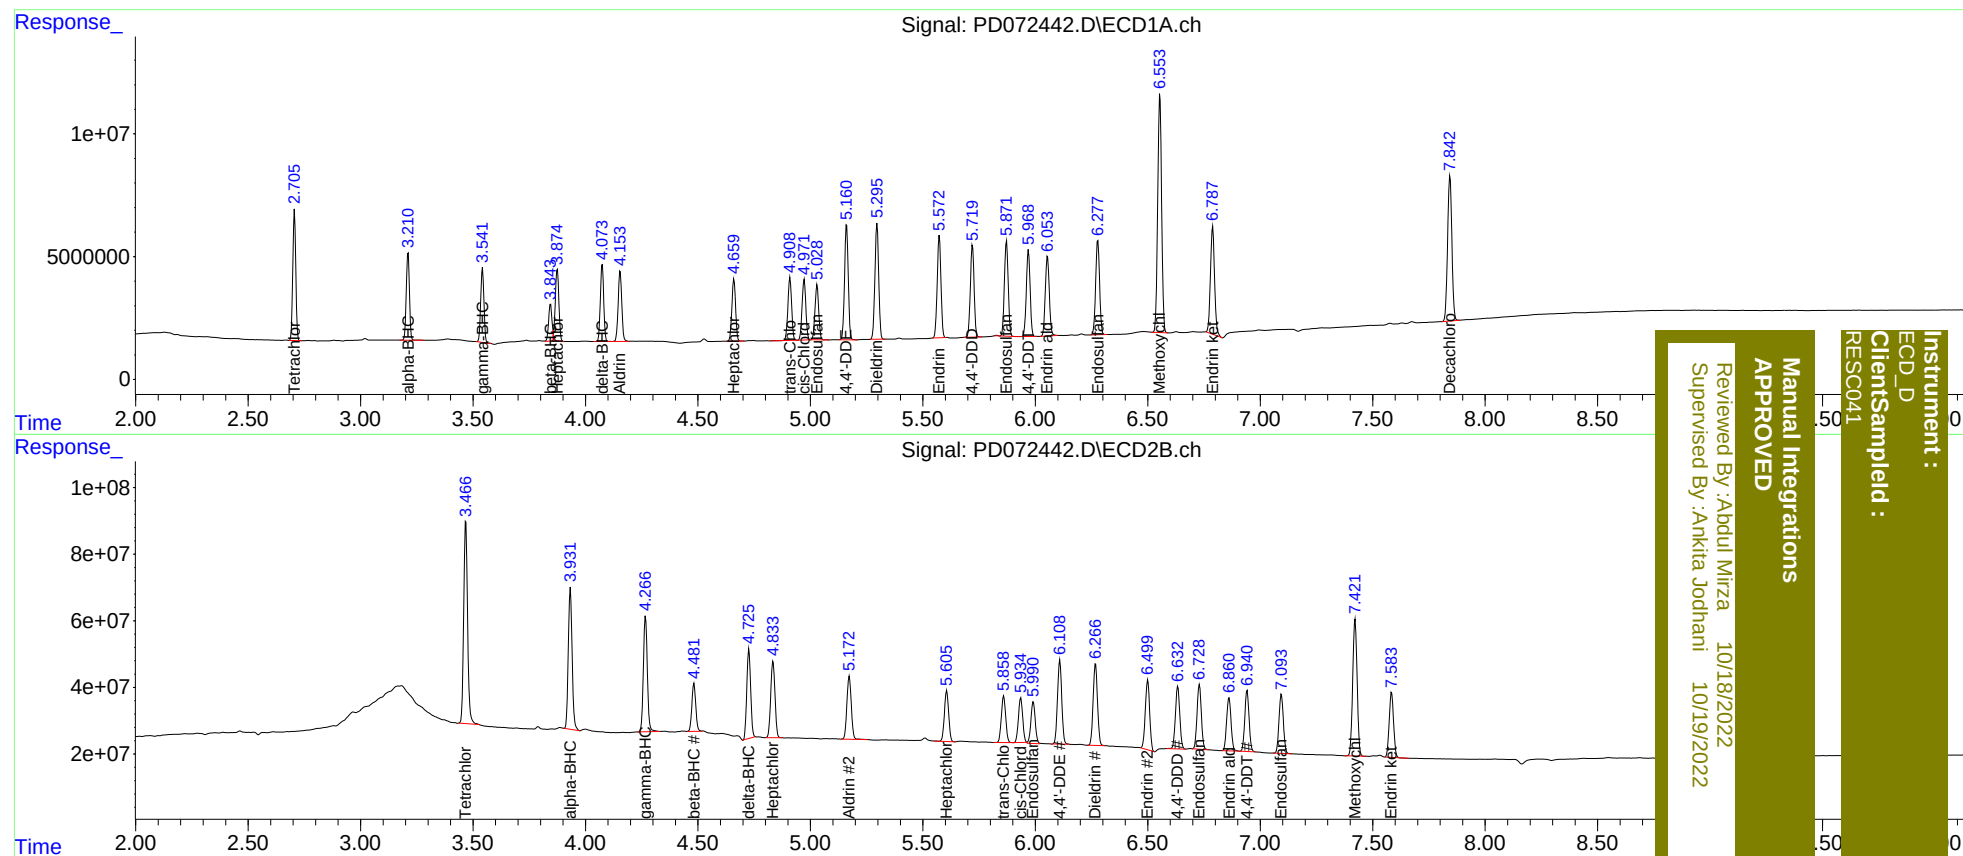

Instrument :
ECD_D
ClientSampled :
RESC041

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/18/2022
Supervised By :Ankita Jodhani 10/19/2022