

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101722\
 Data File : PD072465.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2022 19:45
 Operator : AR\AJ
 Sample : N4950-05MSD
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB8T0MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/20/2022
 Supervised By : Ankita Jodhani 10/20/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 06:25:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 18 06:21:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.707	3.469	30266481	516.2E6	11.870	13.742
27)	SA Decachlor...	7.845	8.927	30988285	751.5E6	15.481m	83.477 #
Target Compounds							
2)	A alpha-BHC	3.212	3.933	170.4E6	1847.9E6	45.523	37.546
3)	MA gamma-BHC...	3.546	4.266	270.4E6	1779.3E6	82.133	42.691m#
4)	MA Heptachlor	3.874	4.833	164.7E6	1089.5E6	47.652m	37.842m
5)	MB Aldrin	4.155	5.173	168.3E6	1136.8E6	49.686	47.250
6)	B beta-BHC	3.844	4.481	58005396	707.9E6	36.285m	42.523m
7)	B delta-BHC	4.075	4.727	61469112	467.4E6	17.332	14.671
8)	B Heptachlo...	4.661	5.606	139.9E6	699.3E6	46.107	35.940
9)	A Endosulfan I	5.030	5.989	93647985	665.7E6	34.833	41.436m
10)	B trans-Chl...	4.910	5.871	157.2E6	2855.8E6	50.585	152.624 #
11)	B cis-Chlor...	4.973	5.933	149.3E6	782.9E6	49.447	43.761m
12)	B 4,4'-DDE	5.162	6.108	287.9E6	1134.8E6	98.822	69.370 #
13)	MA Dieldrin	5.298	6.268	789.4E6	1224.6E6	269.552	75.031 #
14)	MA Endrin	5.574	6.500	267.9E6	1047.8E6	104.641	76.197 #
15)	B Endosulfa...	5.872	6.729	269.5E6	1187.2E6	111.866	93.058
16)	A 4,4'-DDD	5.720	6.632	230.9E6	1213.3E6	101.659m	97.832m
17)	MA 4,4'-DDT	5.970	6.941	208.9E6	1081.2E6	94.502	89.887
18)	B Endrin al...	6.055	6.860	209.6E6	842.1E6	102.549	78.280
19)	B Endosulfa...	6.278	7.093	180.3E6	844.5E6	74.707	70.731
20)	A Methoxychlor	6.553	7.421	511.4E6	2554.8E6	428.507m	465.406
21)	B Endrin ke...	6.789	7.582	228.1E6	1094.8E6	80.044	85.384m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101722\
Data File : PD072465.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2022 19:45
Operator : AR\AJ
Sample : N4950-05MSD
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 06:25:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 18 06:21:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

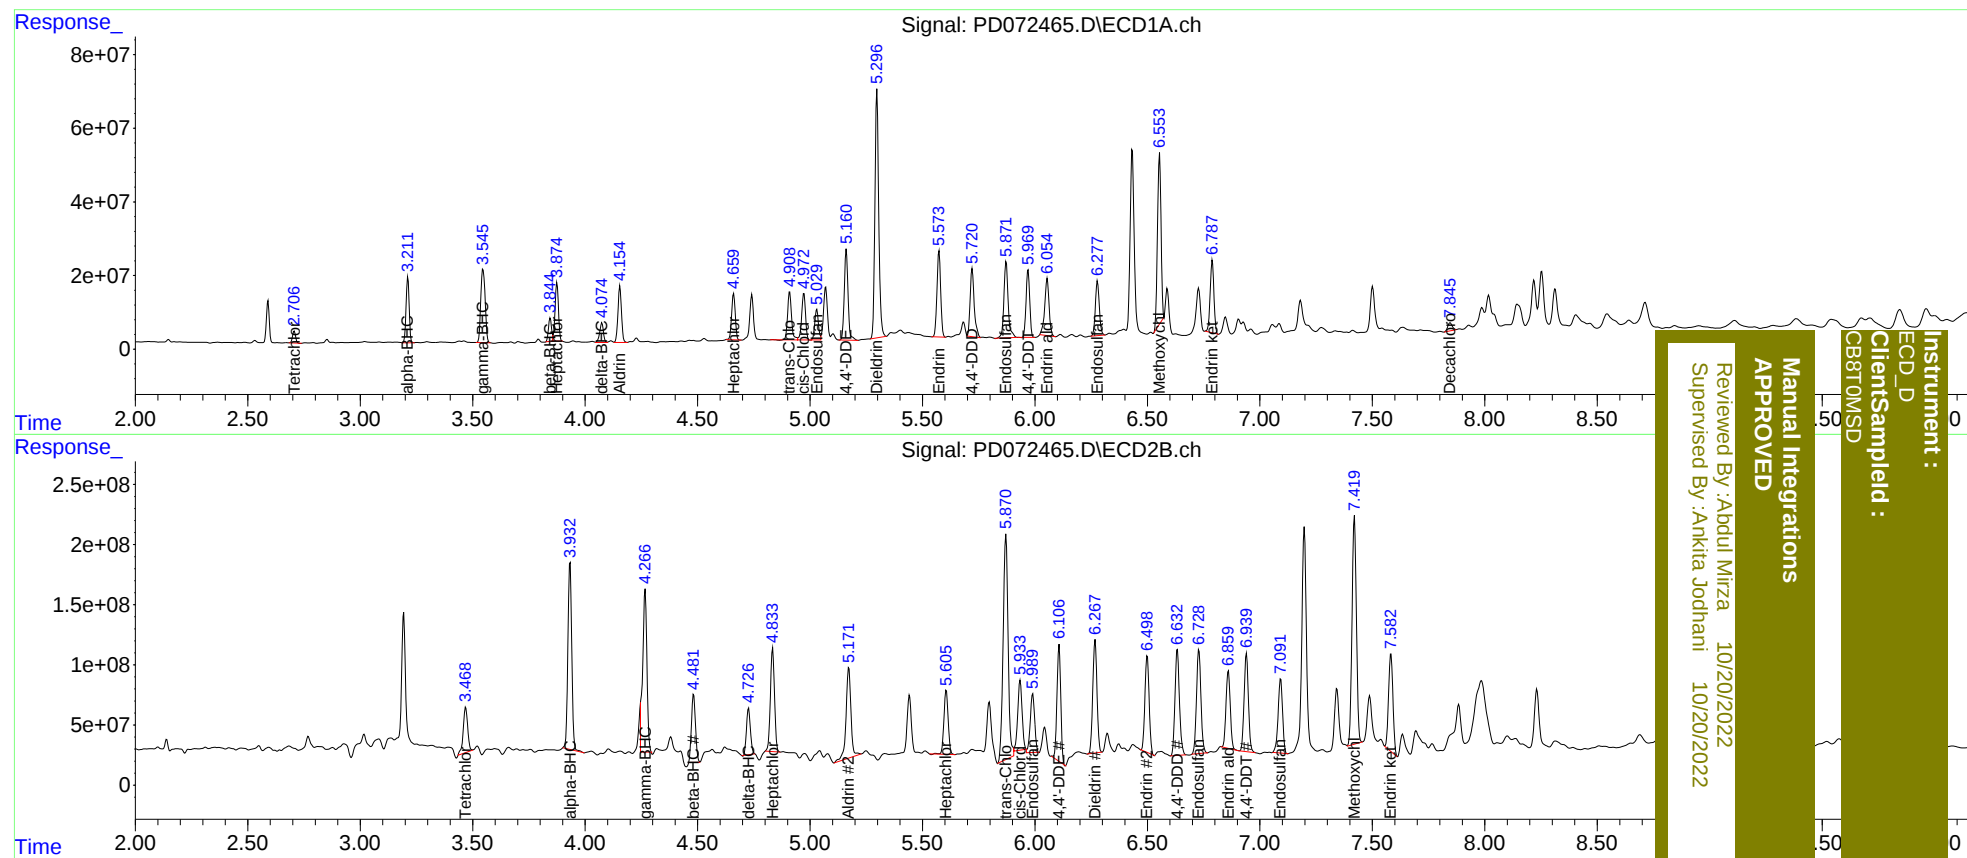

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 10/20/2022
Supervised By: Ankita Jodhani 10/20/2022

Instrument :
ECD_D
Client Sampled :
CB8TOMSD