

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101722\
 Data File : PD072470.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2022 20:52
 Operator : AR\AJ
 Sample : N4984-04MSD
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGNC4MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/20/2022
 Supervised By : Ankita Jodhani 10/20/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 06:27:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 18 06:21:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.707	3.469	39400957	717.1E6	15.453	19.091
27)	SA Decachlor...	7.844	8.927	61127109	282.0E6	30.539	31.330
Target Compounds							
2)	A alpha-BHC	3.212	3.932	174.8E6	1988.1E6	46.703	40.395
3)	MA gamma-BHC...	3.543	4.267	161.3E6	1716.3E6	48.981	41.179
4)	MA Heptachlor	3.875	4.834	167.0E6	1237.8E6	48.322m	42.991
5)	MB Aldrin	4.155	5.173	182.7E6	1029.6E6	53.940	42.794
6)	B beta-BHC	3.844	4.482	68989326	624.9E6	43.156m	37.541
7)	B delta-BHC	4.075	4.726	55765839	515.0E6	15.724	16.166
8)	B Heptachlo...	4.661	5.605	143.6E6	851.7E6	47.345	43.772
9)	A Endosulfan I	5.031	5.989	130.6E6	720.0E6	48.561	44.819m
10)	B trans-Chl...	4.908	5.858	149.0E6	791.7E6	47.926m	42.309
11)	B cis-Chlor...	4.973	5.935	143.8E6	743.6E6	47.623	41.561
12)	B 4,4'-DDE	5.162	6.108	296.8E6	1480.4E6	101.899	90.502
13)	MA Dieldrin	5.297	6.267	306.5E6	1516.3E6	104.650	92.901
14)	MA Endrin	5.573	6.499	265.4E6	1203.1E6	103.653	87.492
15)	B Endosulfa...	5.872	6.729	245.3E6	1195.5E6	101.815	93.711
16)	A 4,4'-DDD	5.721	6.633	232.6E6	1157.5E6	102.368	93.333
17)	MA 4,4'-DDT	5.970	6.940	233.4E6	1209.7E6	105.604	100.566
18)	B Endrin al...	6.055	6.860	178.3E6	884.8E6	87.239	82.252
19)	B Endosulfa...	6.278	7.093	189.0E6	900.8E6	78.299	75.451
20)	A Methoxychlor	6.554	7.421	606.8E6	2726.7E6	508.434	496.725
21)	B Endrin ke...	6.789	7.583	276.2E6	1197.7E6	96.919	93.412

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101722\
Data File : PD072470.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2022 20:52
Operator : AR\AJ
Sample : N4984-04MSD
Misc :
ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 06:27:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 18 06:21:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

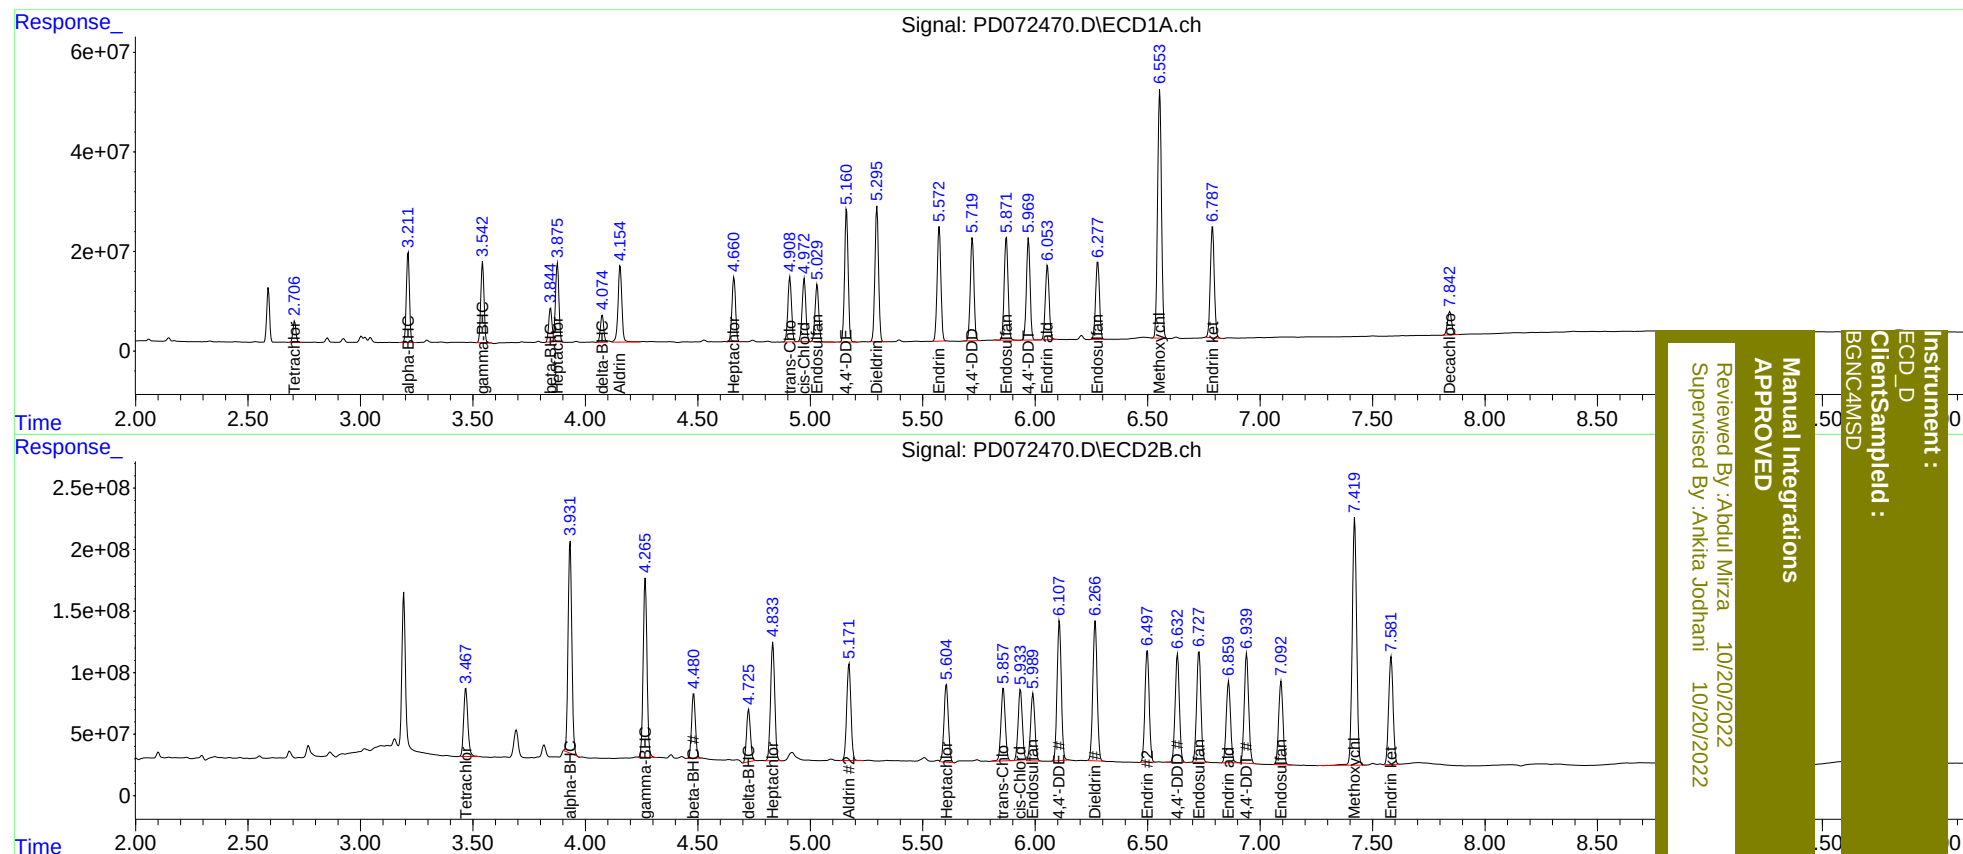

Reviewed By: Abdul Mirza 10/20/2022
Supervised By: Ankita Jodhani 10/20/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
BGCAMSD