

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101722\
 Data File : PD072475.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2022 21:59
 Operator : AR\AJ
 Sample : N4984-10
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGNM2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/20/2022
 Supervised By : Ankita Jodhani 10/20/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 08:30:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 18 06:21:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.707	3.468	29488436	430.1E6	11.565	11.450
2)	SA Decachlor...	7.844	8.926	32753727	231.0E6	16.363	25.658 #
Target Compounds							
3)	MA gamma-BHC...	3.553	4.247	13597559	70090533	4.130	1.682m#
16)	A 4,4'-DDD	5.738	6.630	5532477	30328258	2.435m	2.445m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101722\
Data File : PD072475.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2022 21:59
Operator : AR\AJ
Sample : N4984-10
Misc :
ALS Vial : 35 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 08:30:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 18 06:21:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

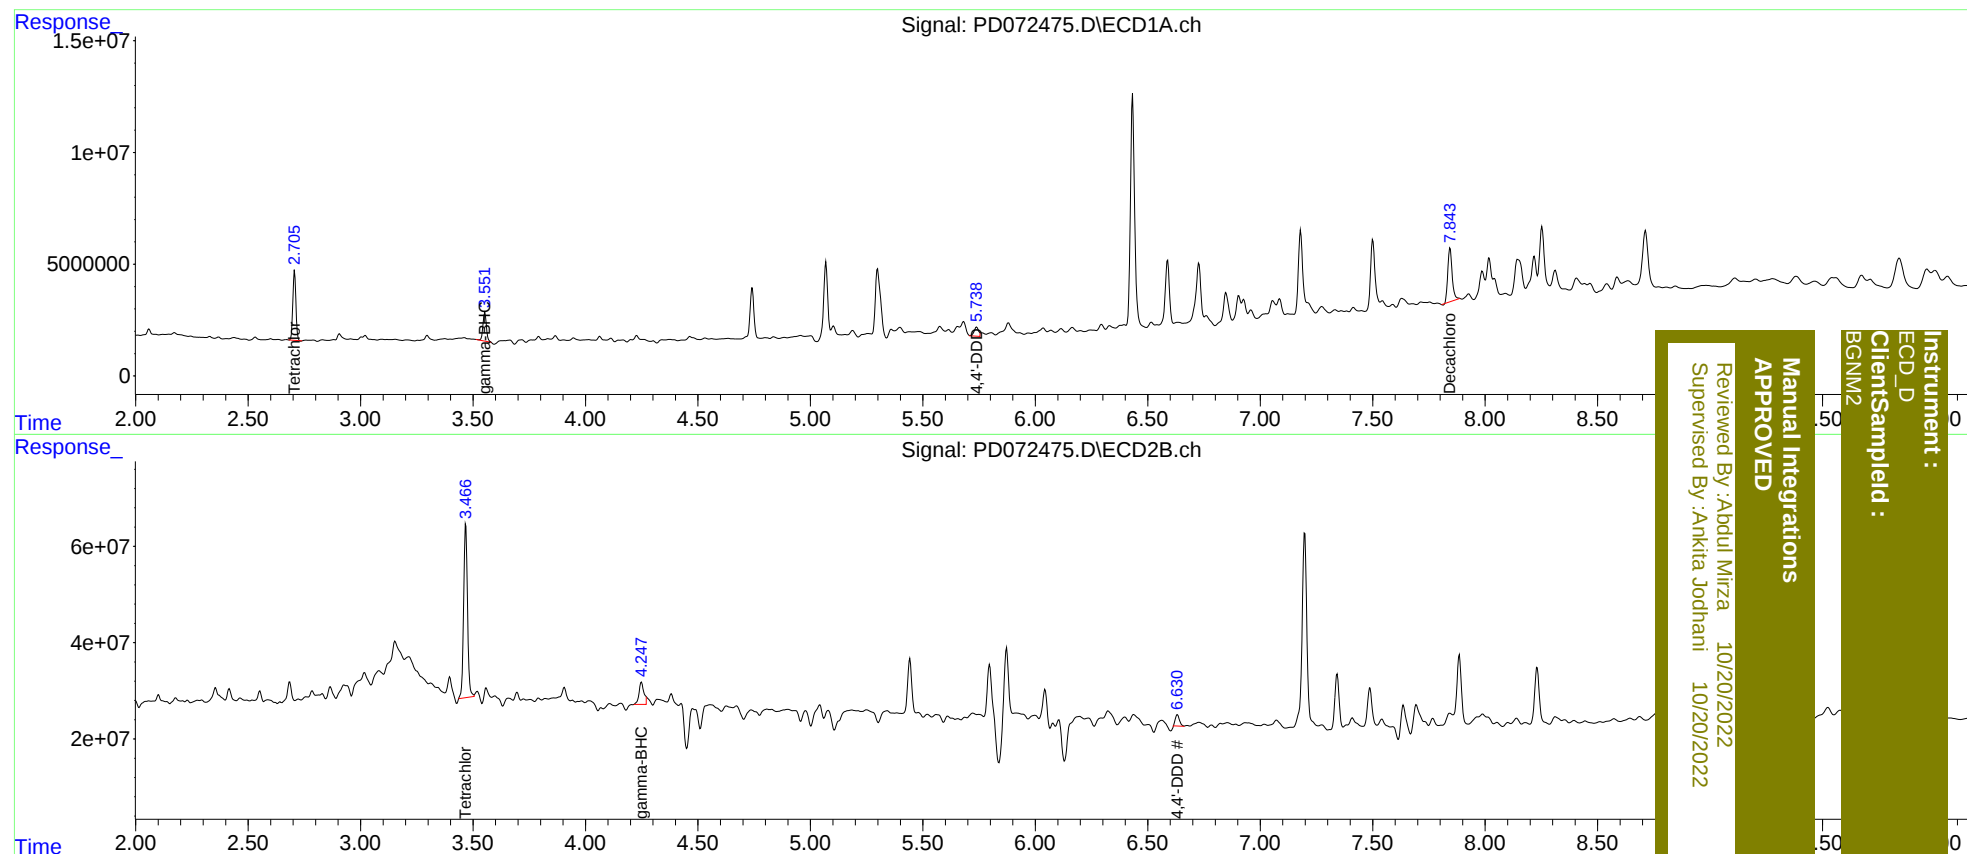

Reviewed By: Abdul Mirza 10/20/2022
Supervised By: Ankita Jodhani 10/20/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
BGM2