

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101722\
 Data File : PD072464.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2022 19:32
 Operator : AR\AJ
 Sample : N4950-04MS
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB8TOMS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/20/2022
 Supervised By : Ankita Jodhani 10/20/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 06:25:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 18 06:21:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.707	3.469	31198840	514.9E6	12.236	13.709
27)	SA Decachlor...	7.844	8.927	32863814	755.8E6	16.418m	83.952 #
Target Compounds							
2)	A alpha-BHC	3.212	3.933	171.1E6	1857.5E6	45.715	37.741
3)	MA gamma-BHC...	3.546	4.266	271.3E6	1770.9E6	82.413	42.491m#
4)	MA Heptachlor	3.874	4.832	170.0E6	1096.2E6	49.172m	38.074m
5)	MB Aldrin	4.155	5.173	169.5E6	1130.0E6	50.038	46.967
6)	B beta-BHC	3.844	4.482	61296458	733.6E6	38.344m	44.066
7)	B delta-BHC	4.074	4.727	61463049	472.5E6	17.330	14.830
8)	B Heptachlo...	4.660	5.606	139.5E6	708.5E6	45.989	36.414
9)	A Endosulfan I	5.030	5.989	94644471	709.2E6	35.204	44.149m#
10)	B trans-Chl...	4.909	5.871	158.3E6	2848.2E6	50.916	152.221 #
11)	B cis-Chlor...	4.973	5.934	151.5E6	827.6E6	50.153	46.258m
12)	B 4,4'-DDE	5.161	6.108	290.9E6	1149.5E6	99.859	70.272 #
13)	MA Dieldrin	5.297	6.268	788.6E6	1254.1E6	269.266	76.833 #
14)	MA Endrin	5.573	6.499	271.3E6	1064.7E6	105.988	77.425 #
15)	B Endosulfa...	5.872	6.729	272.4E6	1214.0E6	113.101	95.157
16)	A 4,4'-DDD	5.719	6.632	231.5E6	1223.6E6	101.901m	98.663m
17)	MA 4,4'-DDT	5.968	6.941	212.7E6	1107.5E6	96.219	92.071
18)	B Endrin al...	6.054	6.860	209.2E6	838.7E6	102.360	77.959
19)	B Endosulfa...	6.278	7.093	182.5E6	864.7E6	75.629	72.425
20)	A Methoxychlor	6.553	7.421	495.6E6	2592.9E6	415.228	472.356
21)	B Endrin ke...	6.788	7.583	230.6E6	1105.3E6	80.907	86.207

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101722\
Data File : PD072464.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2022 19:32
Operator : AR\AJ
Sample : N4950-04MS
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 06:25:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 18 06:21:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

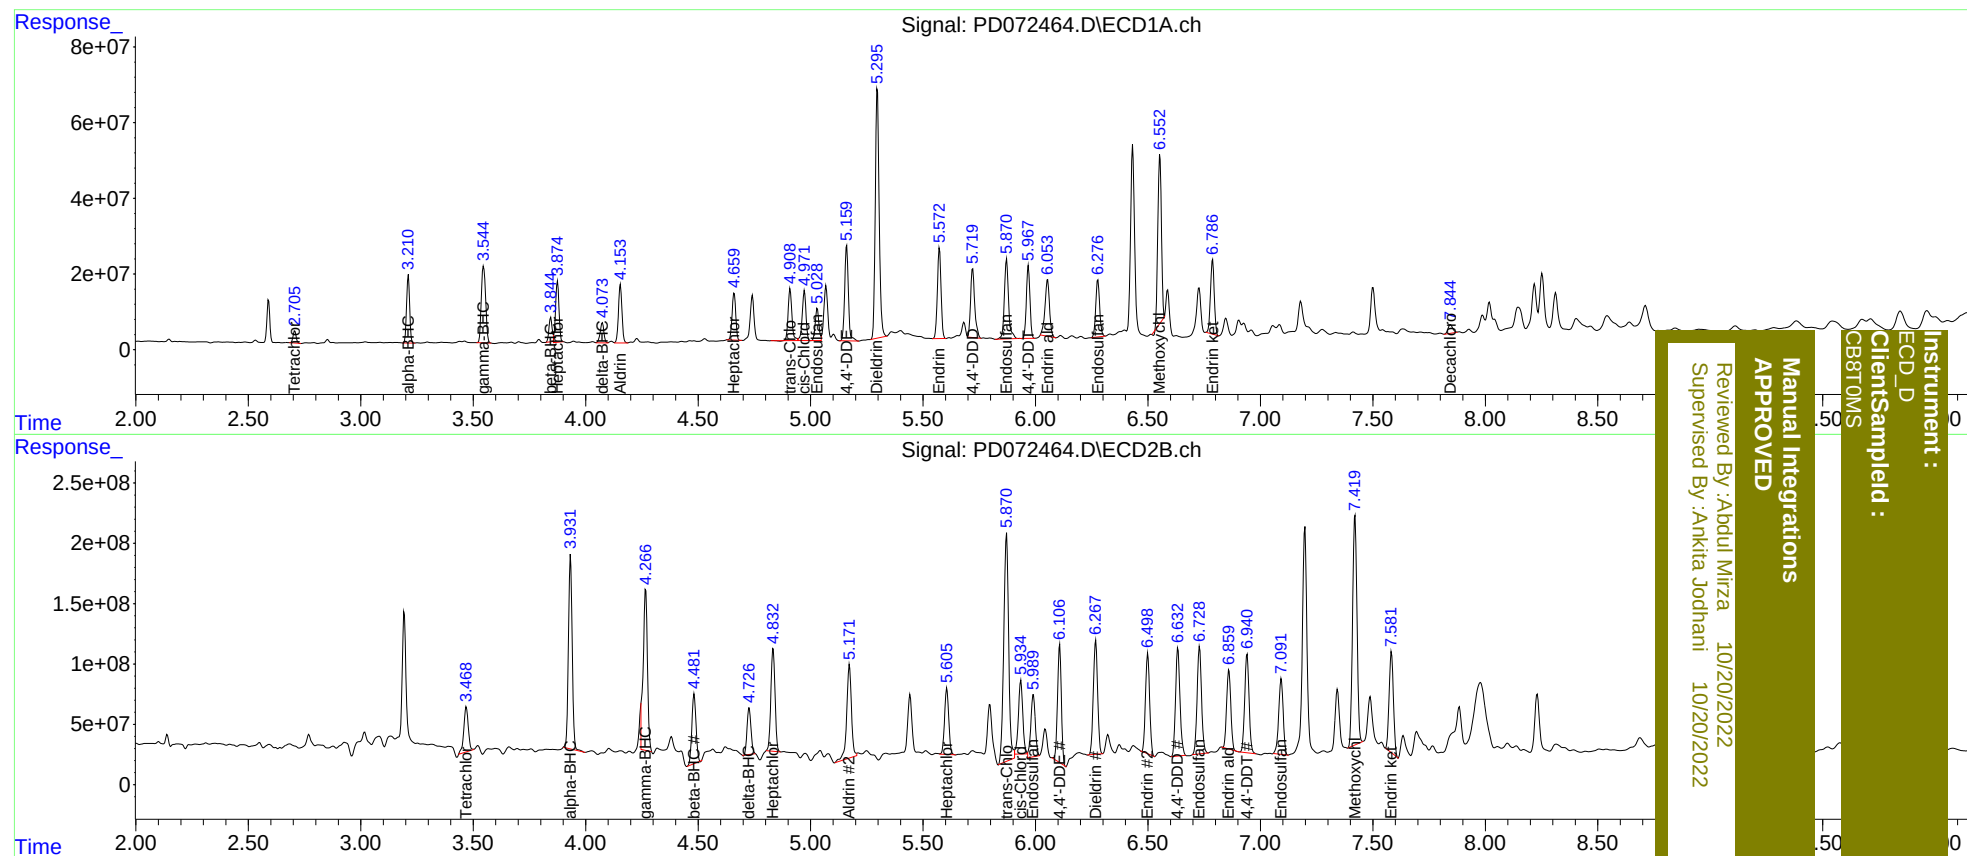

Instrument :
ECD_D
ClientSampled :
CB8TOMS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 10/20/2022
Supervised By: Ankita Jodhani 10/20/2022