

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101722\
 Data File : PD072469.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2022 20:39
 Operator : AR\AJ
 Sample : N4984-03MS
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGNC4MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/20/2022
 Supervised By : Ankita Jodhani 10/20/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 06:27:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 18 06:21:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.706	3.469	40636565	725.2E6	15.937	19.307
27)	SA Decachlor...	7.843	8.926	58431031	288.5E6	29.192	32.049
Target Compounds							
2)	A alpha-BHC	3.212	3.933	179.2E6	2010.4E6	47.864	40.848
3)	MA gamma-BHC...	3.543	4.267	165.4E6	1745.3E6	50.248	41.876
4)	MA Heptachlor	3.874	4.834	172.3E6	1248.7E6	49.836m	43.371
5)	MB Aldrin	4.154	5.173	183.4E6	1045.8E6	54.143	43.466
6)	B beta-BHC	3.843	4.482	65232845	638.9E6	40.806m	38.377
7)	B delta-BHC	4.075	4.726	56646391	520.3E6	15.972	16.331
8)	B Heptachlo...	4.660	5.605	146.5E6	830.9E6	48.291	42.703
9)	A Endosulfan I	5.030	5.988	133.6E6	737.3E6	49.696	45.898m
10)	B trans-Chl...	4.909	5.859	146.8E6	804.0E6	47.228	42.967
11)	B cis-Chlor...	4.973	5.935	146.5E6	753.4E6	48.497	42.112
12)	B 4,4'-DDE	5.161	6.108	301.6E6	1503.4E6	103.543	91.905
13)	MA Dieldrin	5.296	6.267	311.6E6	1534.1E6	106.401	93.990
14)	MA Endrin	5.573	6.498	270.0E6	1266.2E6	105.470	92.082
15)	B Endosulfa...	5.871	6.729	250.0E6	1210.2E6	103.802	94.856
16)	A 4,4'-DDD	5.720	6.633	236.0E6	1175.7E6	103.872	94.800
17)	MA 4,4'-DDT	5.969	6.941	237.2E6	1224.2E6	107.299	101.775
18)	B Endrin al...	6.054	6.860	180.8E6	894.6E6	88.493	83.161
19)	B Endosulfa...	6.278	7.093	190.5E6	909.4E6	78.921	76.173
20)	A Methoxychlor	6.553	7.421	611.2E6	2721.6E6	512.067	495.806
21)	B Endrin ke...	6.788	7.583	276.6E6	1208.2E6	97.049	94.231

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101722\
Data File : PD072469.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2022 20:39
Operator : AR\AJ
Sample : N4984-03MS
Misc :
ALS Vial : 29 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 06:27:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 18 06:21:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

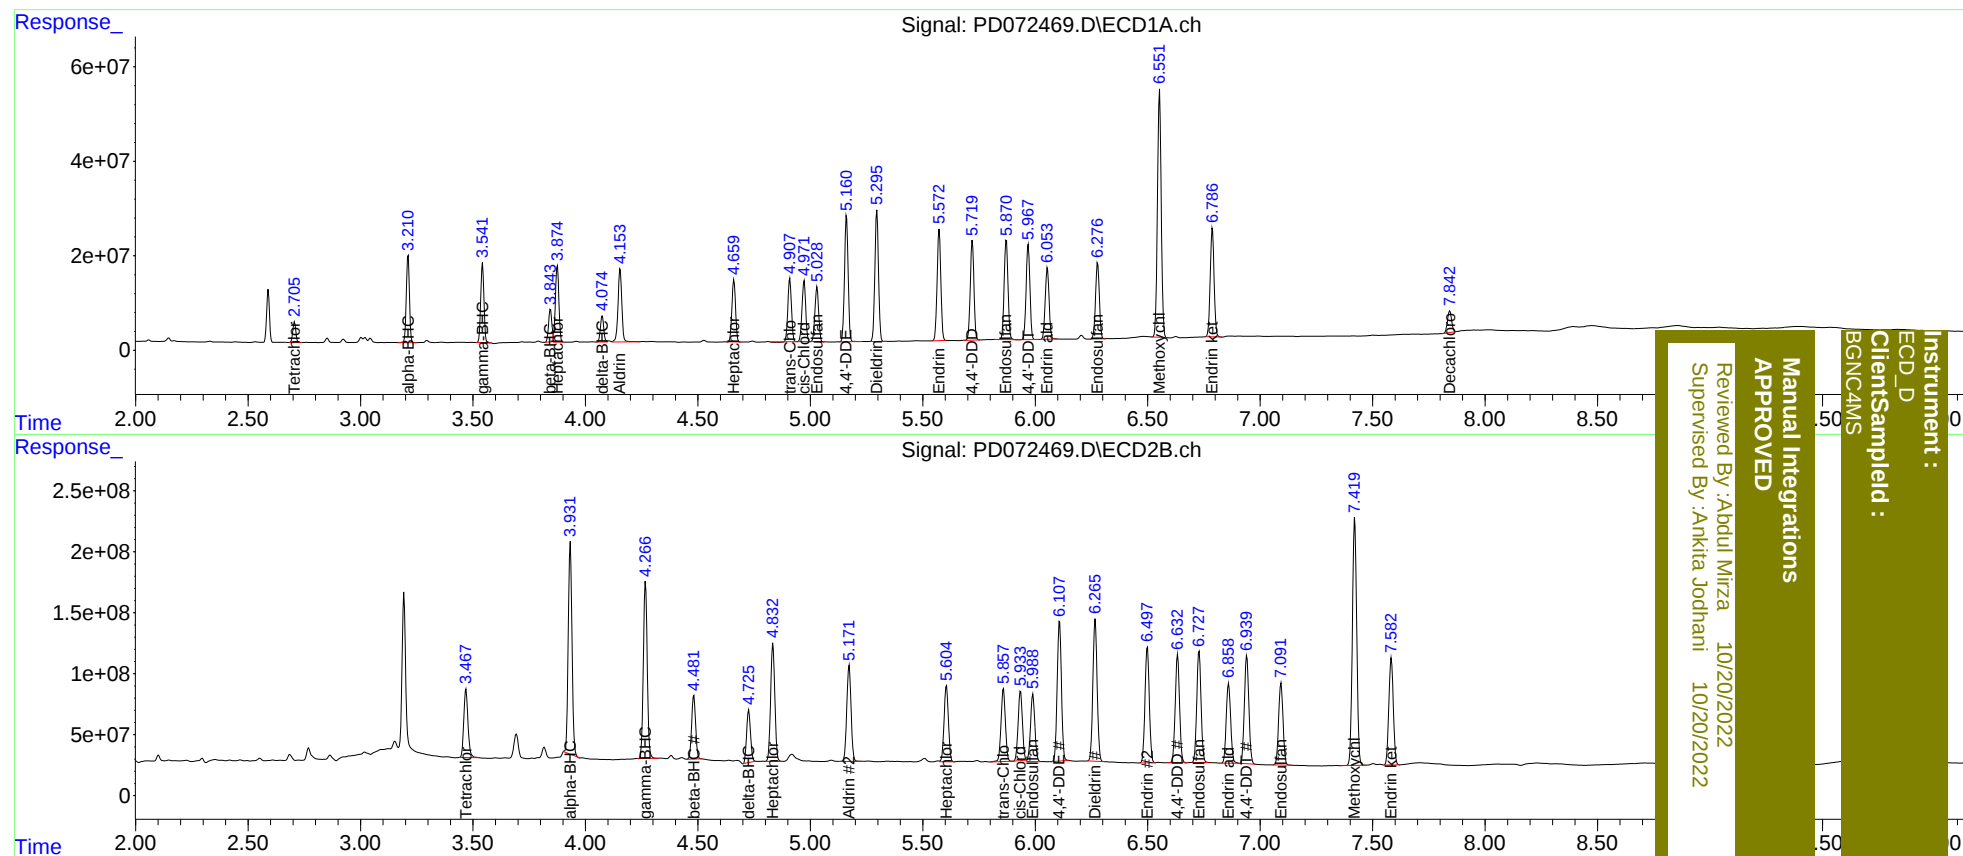

Instrument :
ECD_D
ClientSampled :
BGC/CAMS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 10/20/2022
Supervised By: Ankita Jodhani 10/20/2022