

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101723\
 Data File : PD078917.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2023 06:23
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 08:27:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 07:37:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.806	8075785	11282583	5.388	5.302
27)	SA Decachlor...	9.119	7.957	21201084	25656002	11.395	11.365
Target Compounds							
2)	A alpha-BHC	4.026	3.309	12420288	16395701	4.919	4.915
3)	MA gamma-BHC...	4.360	3.639	12312025	16001304	5.114	5.066
4)	MA Heptachlor	4.953	3.983	13564427	15339290	5.351	5.150
9)	A Endosulfan I	6.110	5.137	11438411	13186503	5.478	5.318
13)	MA Dieldrin	6.385	5.401	22861633	28497727	10.391	9.836
14)	MA Endrin	6.616	5.677	18992236	24816719	10.317	9.963
16)	A 4,4'-DDD	6.746	5.824	16834911	21738937	10.343	10.003
17)	MA 4,4'-DDT	7.062	6.076	18052287	21914464	10.413	9.899
20)	A Methoxychlor	7.536	6.652	51071457	65867659	55.088	54.049


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101723\
Data File : PD078917.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2023 06:23
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 08:27:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 07:37:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

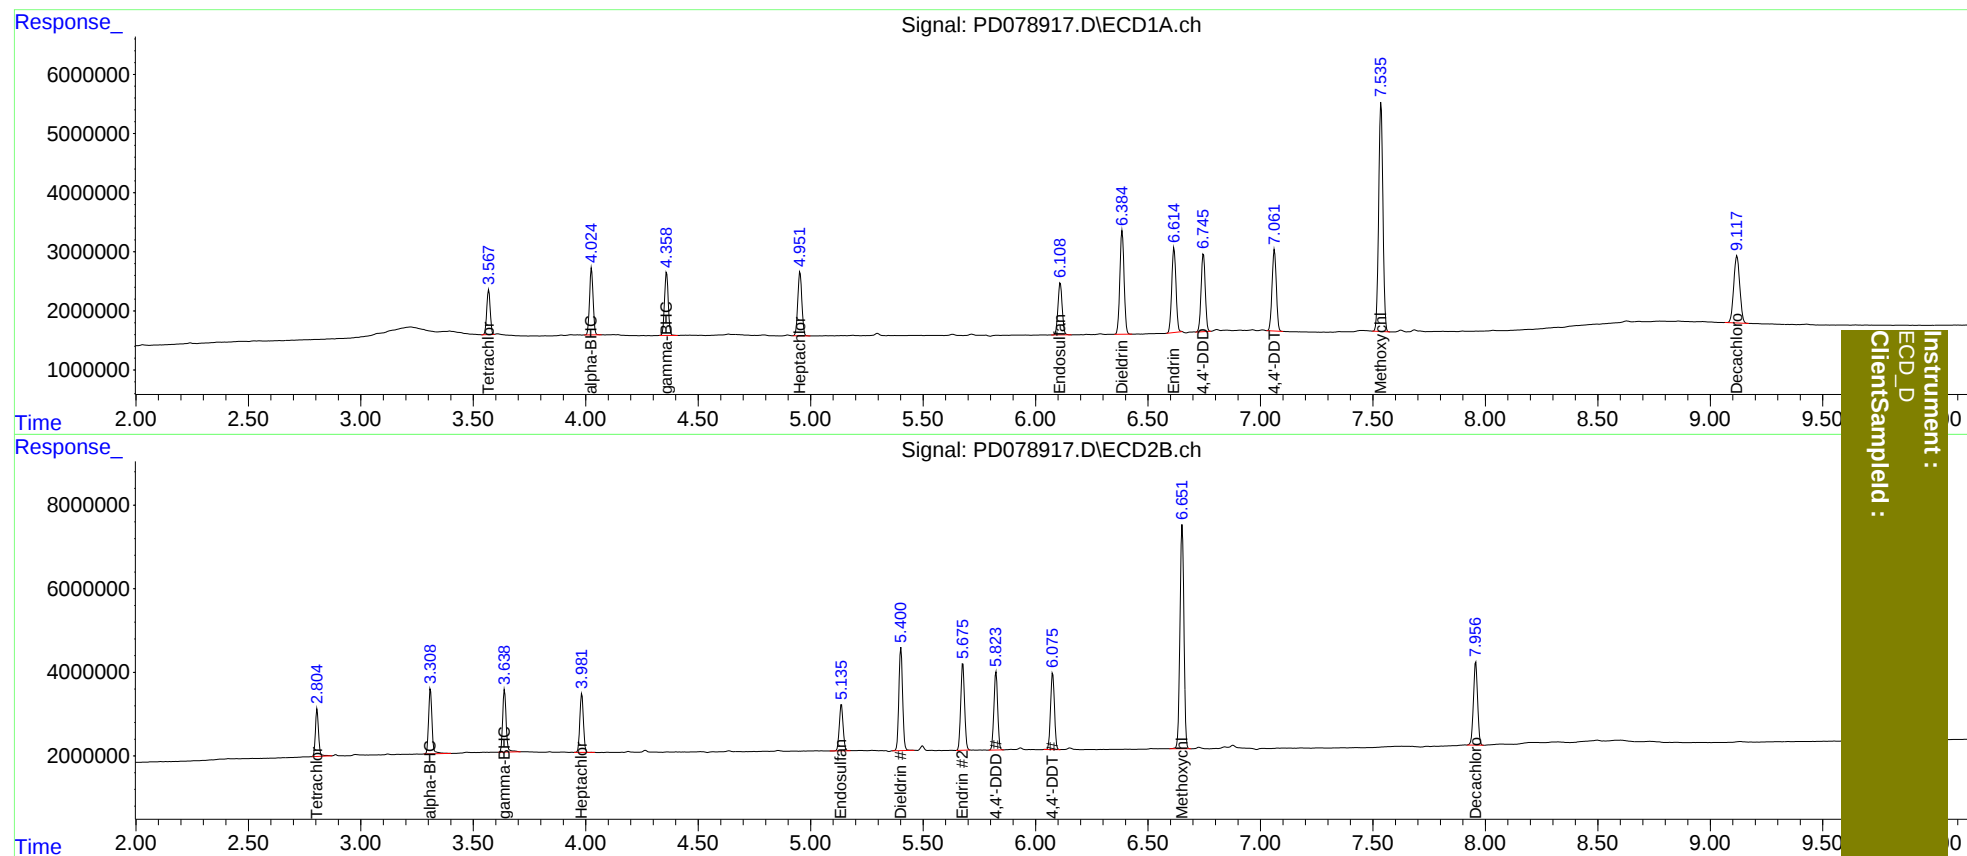


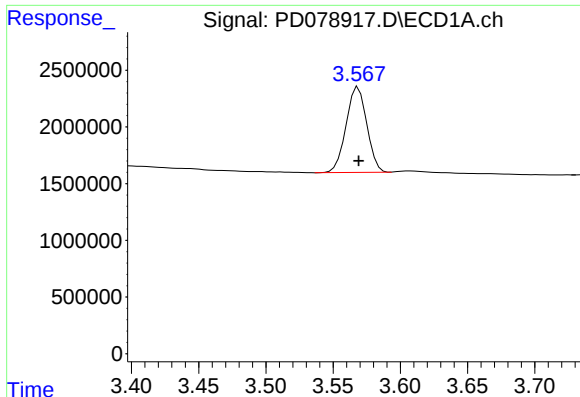

#1 Tetrachloro-m-xylene


R.T.: 3.569 min
Delta R.T.: 0.000 min
Response: 8075785
Conc: 5.39 ng/ml

Instrument :
ECD_D
ClientSampleId :

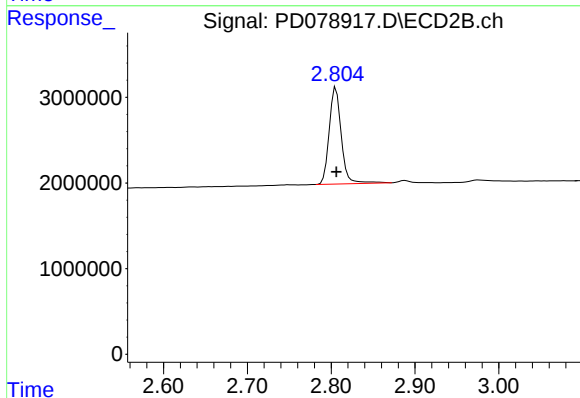


#1 Tetrachloro-m-xylene

R.T.: 2.806 min
Delta R.T.: 0.000 min
Response: 11282583
Conc: 5.30 ng/ml

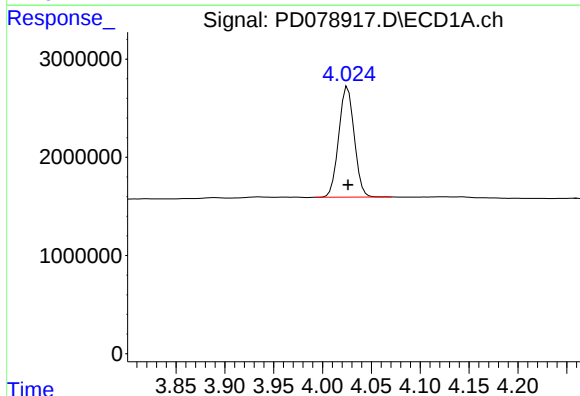


#2 alpha-BHC

R.T.: 4.026 min
Delta R.T.: 0.000 min
Response: 12420288
Conc: 4.92 ng/ml

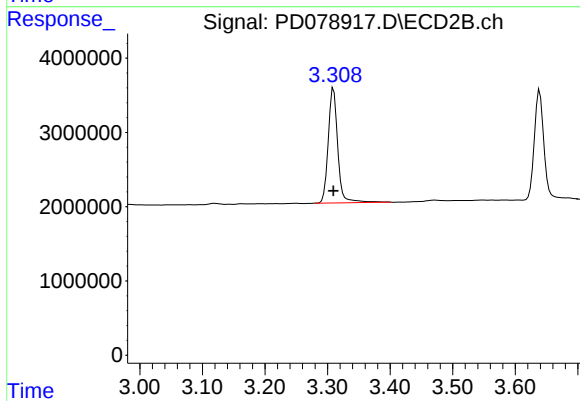

#2 alpha-BHC


R.T.: 3.309 min
Delta R.T.: 0.000 min
Response: 16395701
Conc: 4.92 ng/ml

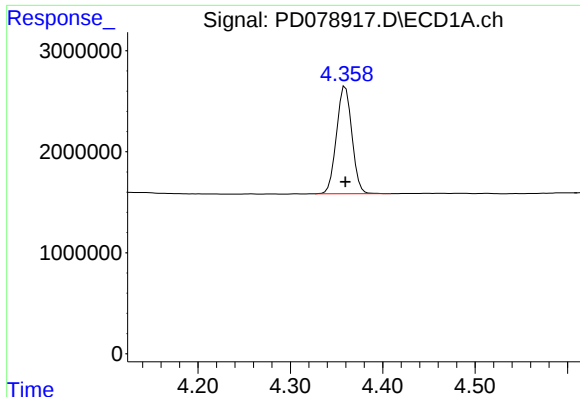

#3 gamma-BHC (Lindane)


R.T.: 4.360 min
Delta R.T.: 0.000 min
Response: 12312025
Conc: 5.11 ng/ml

Instrument :
ECD_D
ClientSampleId :

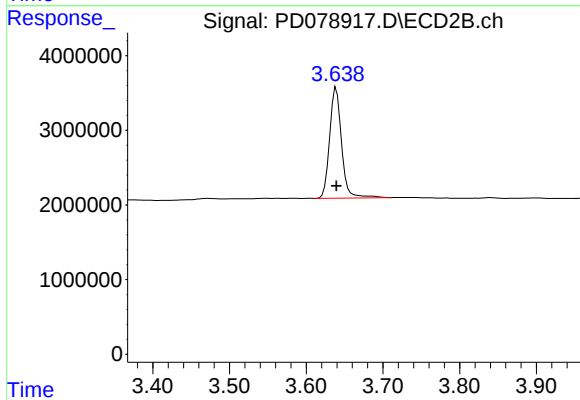


#3 gamma-BHC (Lindane)

R.T.: 3.639 min
Delta R.T.: 0.000 min
Response: 16001304
Conc: 5.07 ng/ml

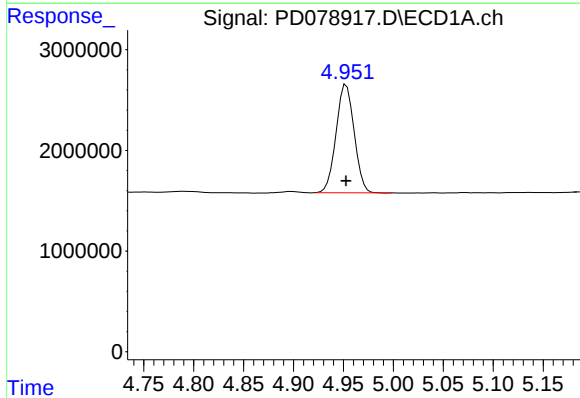


#4 Heptachlor

R.T.: 4.953 min
Delta R.T.: 0.000 min
Response: 13564427
Conc: 5.35 ng/ml

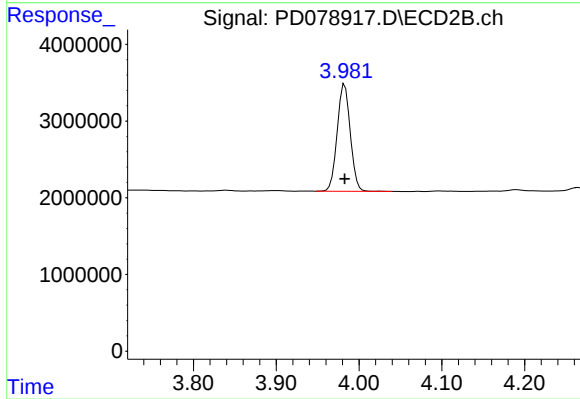

#4 Heptachlor


R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 15339290
Conc: 5.15 ng/ml

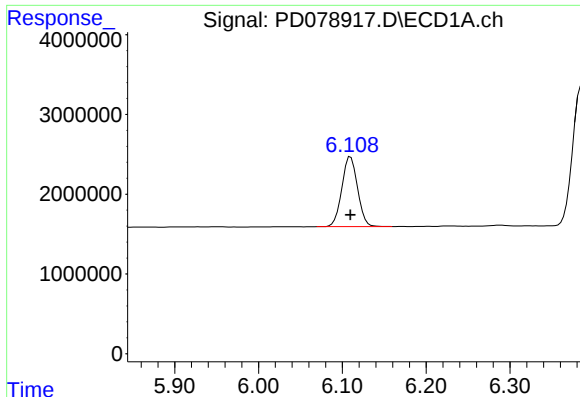

#9 Endosulfan I


R.T.: 6.110 min
Delta R.T.: 0.000 min
Response: 11438411
Conc: 5.48 ng/ml

Instrument :
ECD_D
ClientSampleId :

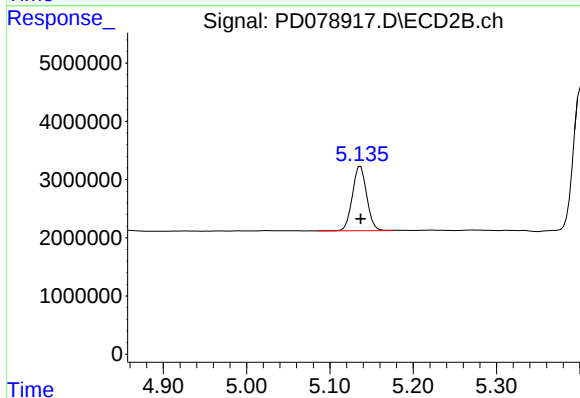


#9 Endosulfan I

R.T.: 5.137 min
Delta R.T.: 0.000 min
Response: 13186503
Conc: 5.32 ng/ml

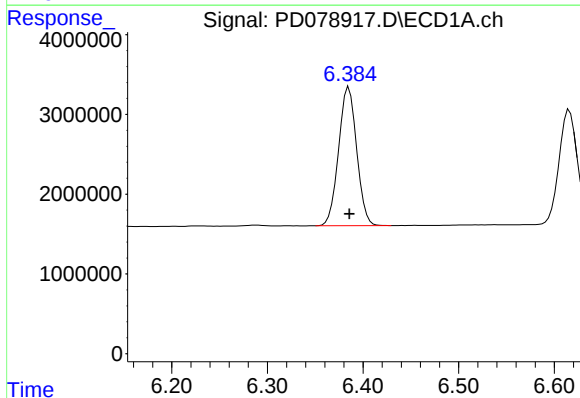


#13 Dieldrin

R.T.: 6.385 min
Delta R.T.: 0.000 min
Response: 22861633
Conc: 10.39 ng/ml

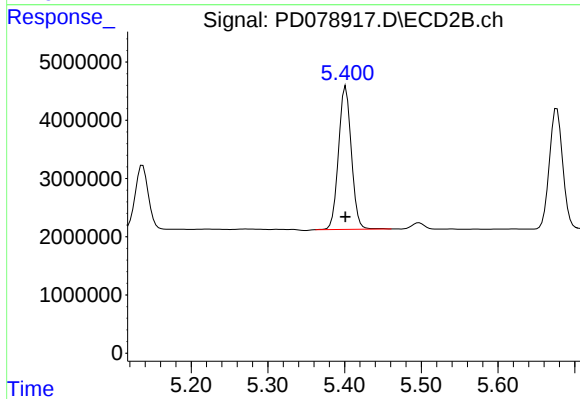

#13 Dieldrin


R.T.: 5.401 min
Delta R.T.: 0.000 min
Response: 28497727
Conc: 9.84 ng/ml

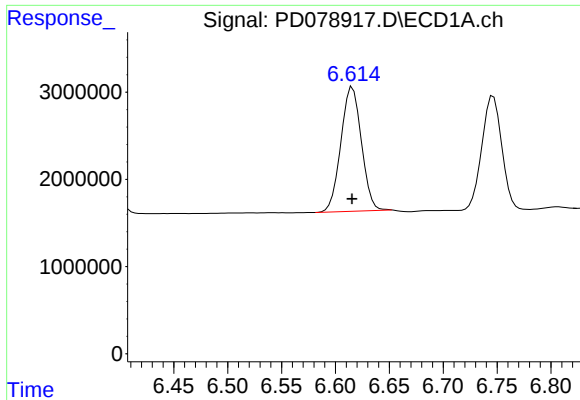

#14 Endrin


R.T.: 6.616 min
Delta R.T.: 0.000 min
Response: 18992236
Conc: 10.32 ng/ml

Instrument :
ECD_D
ClientSampleId :

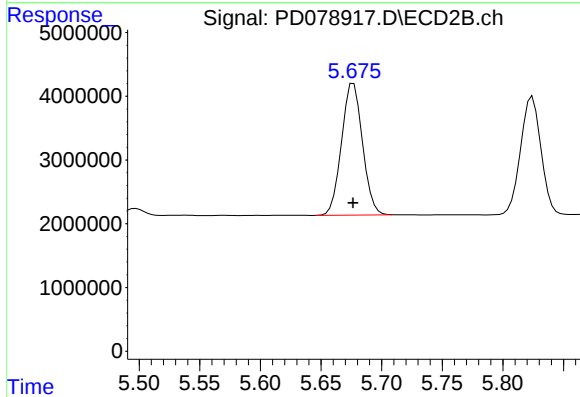


#14 Endrin

R.T.: 5.677 min
Delta R.T.: 0.000 min
Response: 24816719
Conc: 9.96 ng/ml

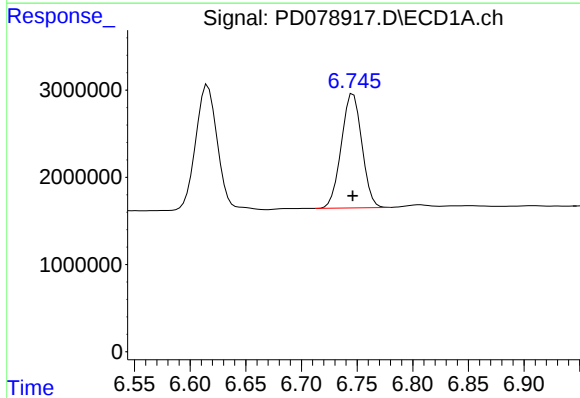


#16 4,4'-DDD

R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 16834911
Conc: 10.34 ng/ml

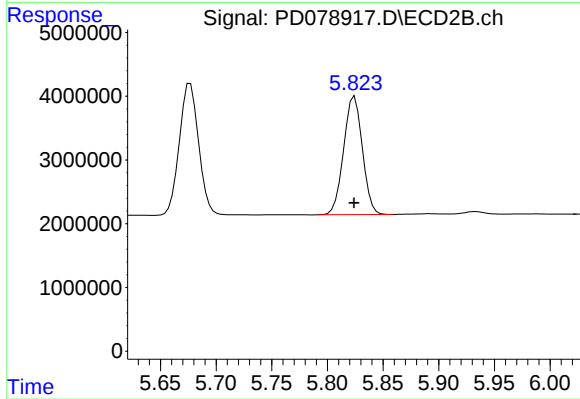

#16 4,4'-DDD


R.T.: 5.824 min
Delta R.T.: 0.000 min
Response: 21738937
Conc: 10.00 ng/ml

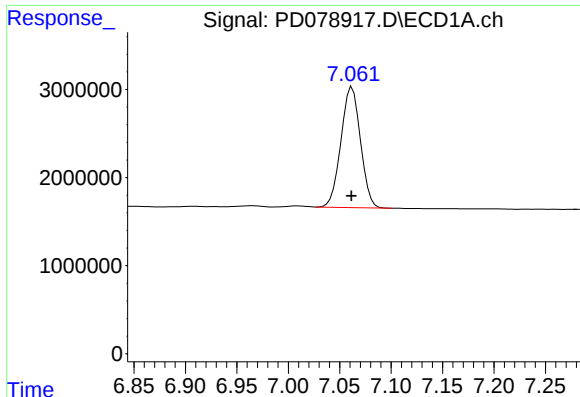

#17 4,4'-DDT


R.T.: 7.062 min
Delta R.T.: 0.000 min
Response: 18052287
Conc: 10.41 ng/ml

Instrument :
ECD_D
ClientSampleId :

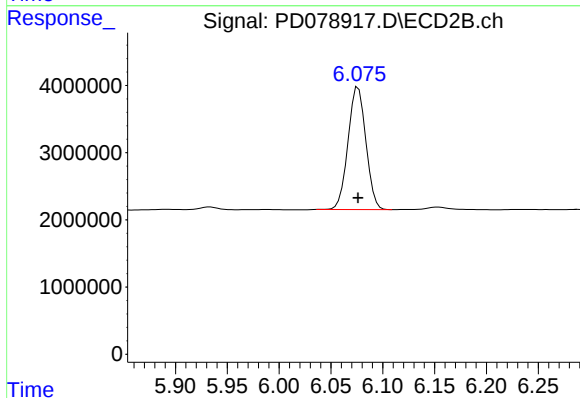


#17 4,4'-DDT

R.T.: 6.076 min
Delta R.T.: 0.000 min
Response: 21914464
Conc: 9.90 ng/ml

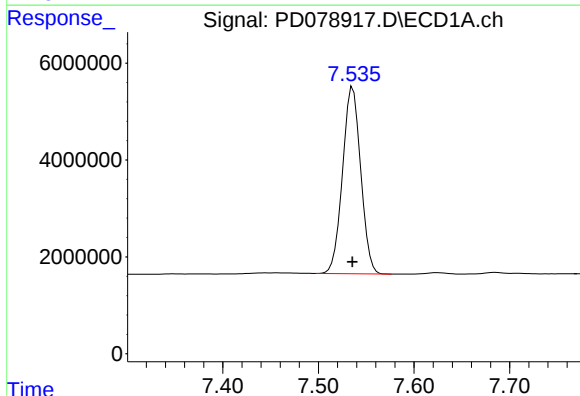


#20 Methoxychlor

R.T.: 7.536 min
Delta R.T.: 0.000 min
Response: 51071457
Conc: 55.09 ng/ml

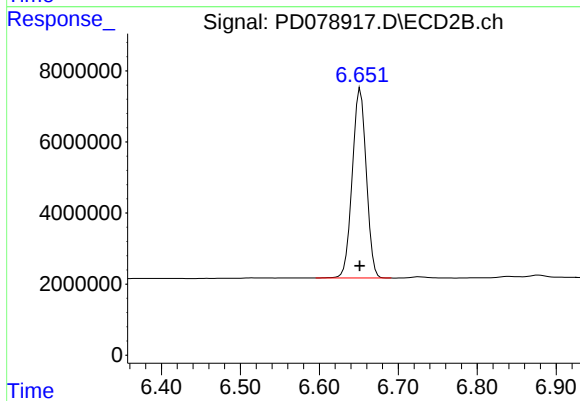

#20 Methoxychlor


R.T.: 6.652 min
Delta R.T.: 0.000 min
Response: 65867659
Conc: 54.05 ng/ml

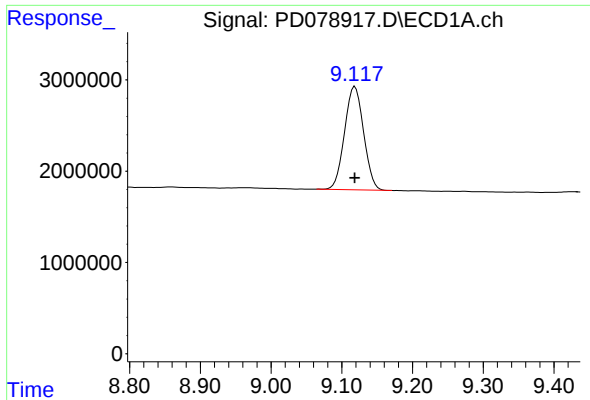

#27 Decachlorobiphenyl

R.T.: 9.119 min
Delta R.T.: 0.000 min
Response: 21201084
Conc: 11.40 ng/ml

Instrument :
ECD_D
ClientSampleId :

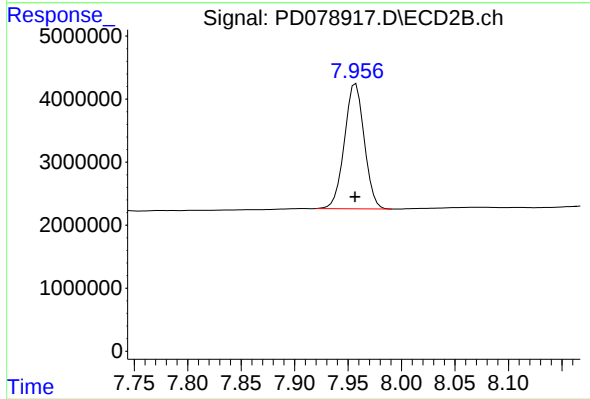

#27 Decachlorobiphenyl

R.T.: 7.957 min
Delta R.T.: 0.000 min
Response: 25656002
Conc: 11.37 ng/ml