

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101723\
 Data File : PD078921.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2023 07:16
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 08:27:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 07:37:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.806	29979432	42561628	20.000	20.000
27)	SA Decachlor...	9.118	7.957	74421308	90298280	40.000	40.000
Target Compounds							
2)	A alpha-BHC	4.026	3.309	50495503	66712623	20.000	20.000
3)	MA gamma-BHC...	4.360	3.639	48146609	63174384	20.000	20.000
4)	MA Heptachlor	4.953	3.983	50697495	59572981	20.000	20.000
9)	A Endosulfan I	6.110	5.137	41761328	49589976	20.000	20.000
13)	MA Dieldrin	6.386	5.401	88001972	115.9E6	40.000	40.000
14)	MA Endrin	6.615	5.676	73637765	99637927	40.000	40.000
16)	A 4,4'-DDD	6.746	5.824	65106249	86933600	40.000	40.000
17)	MA 4,4'-DDT	7.061	6.076	69343504	88548674	40.000	40.000
20)	A Methoxychlor	7.535	6.651	185.4E6	243.7E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101723\
Data File : PD078921.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2023 07:16
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 08:27:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 07:37:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

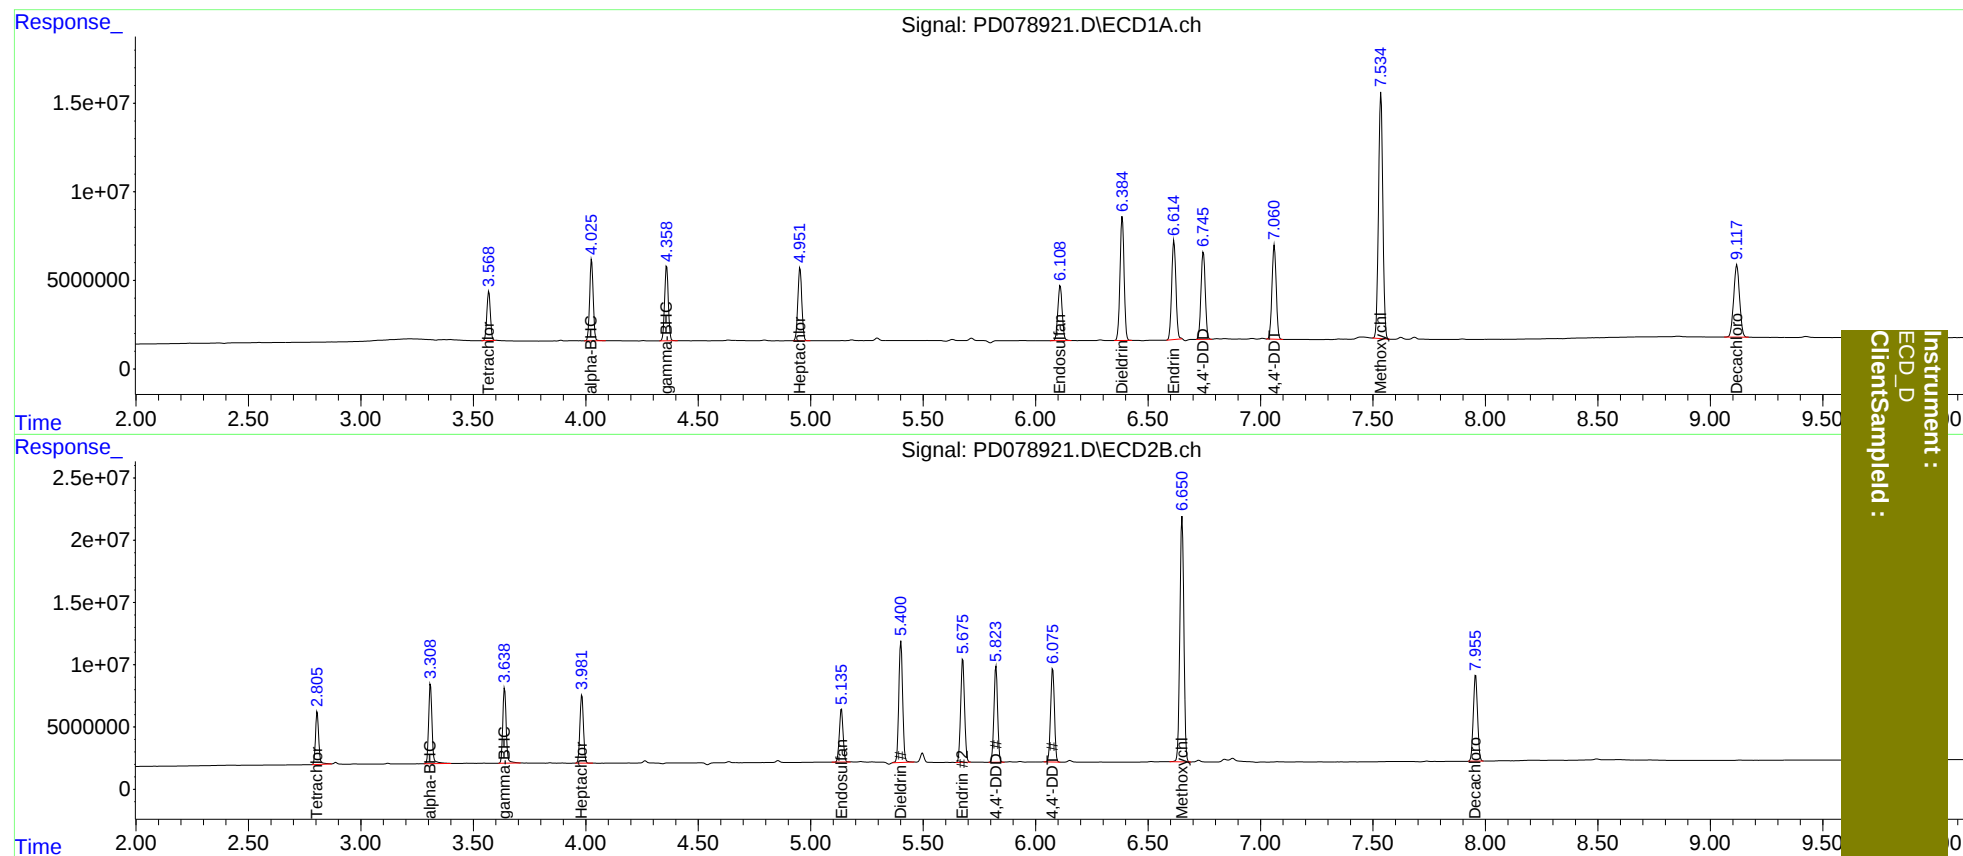


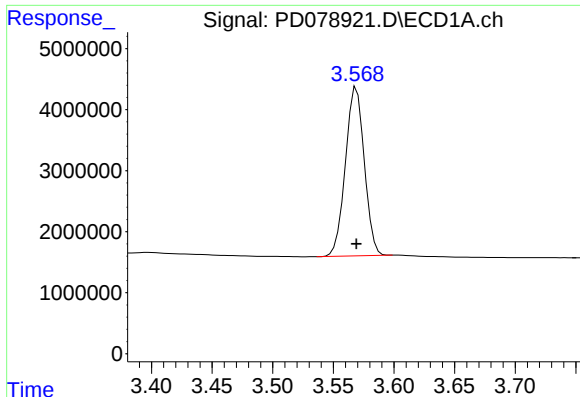

#1 Tetrachloro-m-xylene


R.T.: 3.569 min
Delta R.T.: 0.000 min
Response: 29979432
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

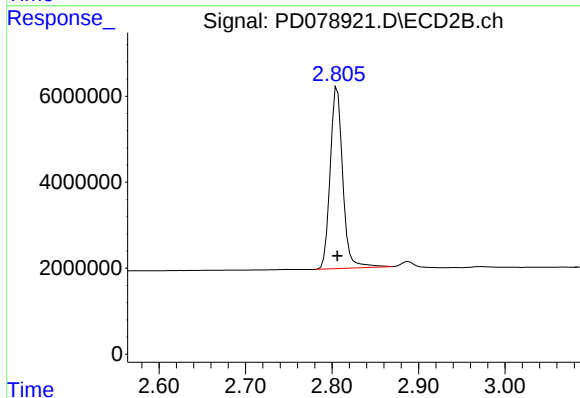


#1 Tetrachloro-m-xylene

R.T.: 2.806 min
Delta R.T.: 0.000 min
Response: 42561628
Conc: 20.00 ng/ml

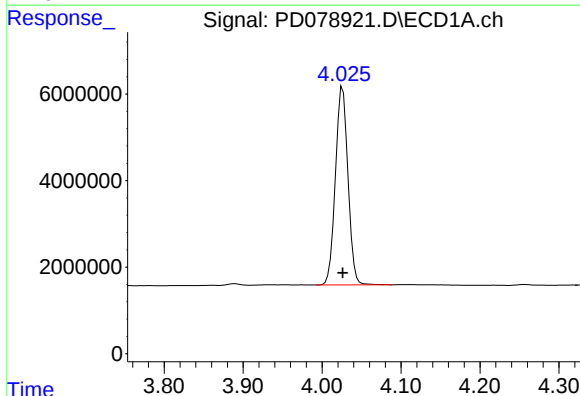


#2 alpha-BHC

R.T.: 4.026 min
Delta R.T.: 0.000 min
Response: 50495503
Conc: 20.00 ng/ml

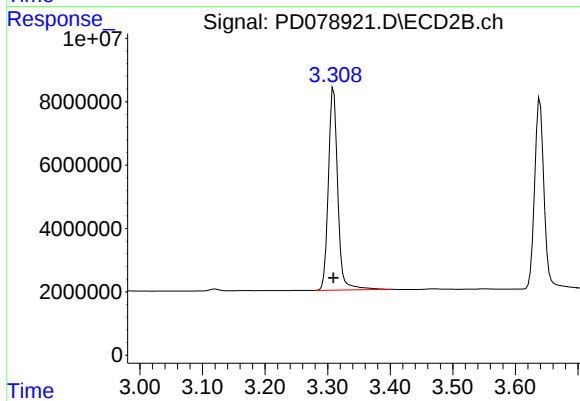

#2 alpha-BHC


R.T.: 3.309 min
Delta R.T.: 0.000 min
Response: 66712623
Conc: 20.00 ng/ml

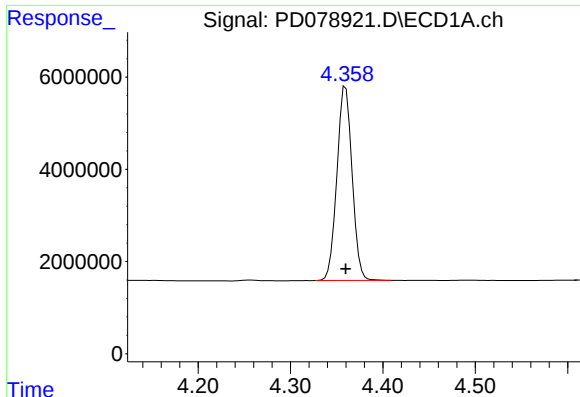

#3 gamma-BHC (Lindane)


R.T.: 4.360 min
Delta R.T.: 0.000 min
Response: 48146609
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

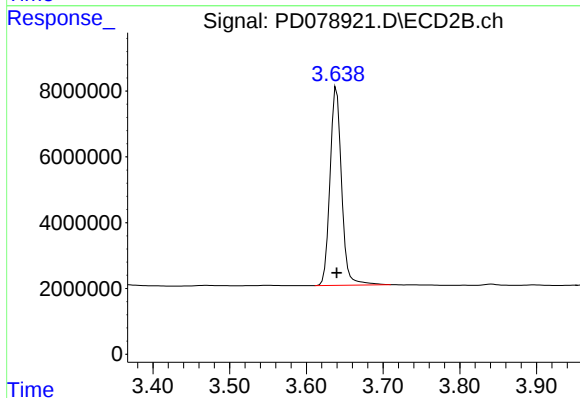


#3 gamma-BHC (Lindane)

R.T.: 3.639 min
Delta R.T.: 0.000 min
Response: 63174384
Conc: 20.00 ng/ml

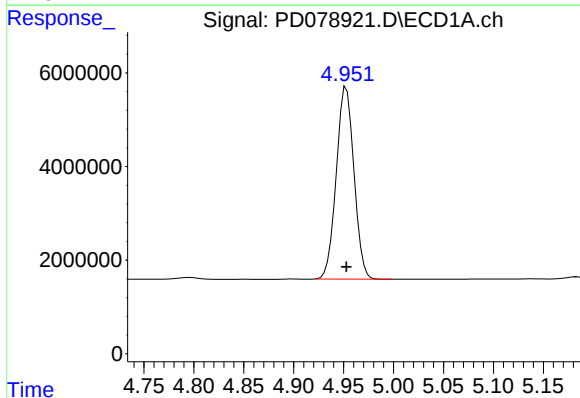


#4 Heptachlor

R.T.: 4.953 min
Delta R.T.: 0.000 min
Response: 50697495
Conc: 20.00 ng/ml

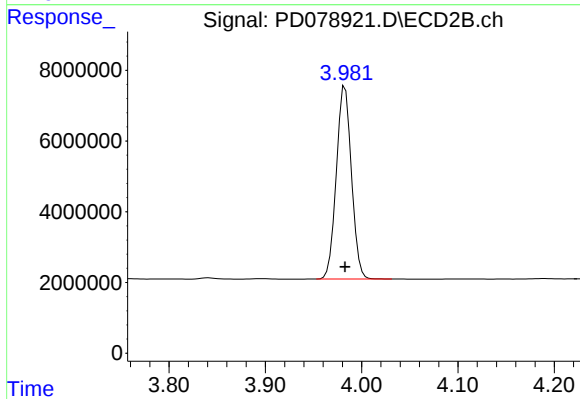

#4 Heptachlor


R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 59572981
Conc: 20.00 ng/ml

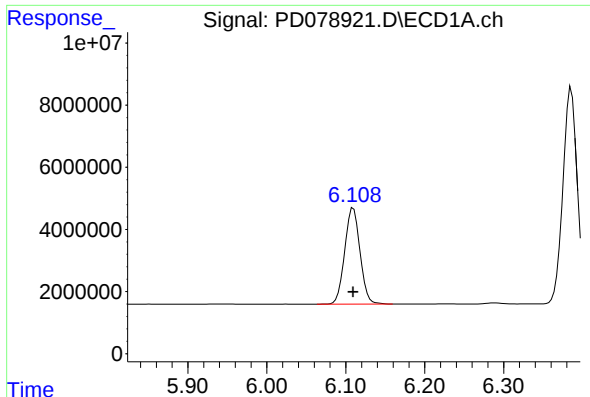

#9 Endosulfan I


R.T.: 6.110 min
Delta R.T.: 0.000 min
Response: 41761328
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

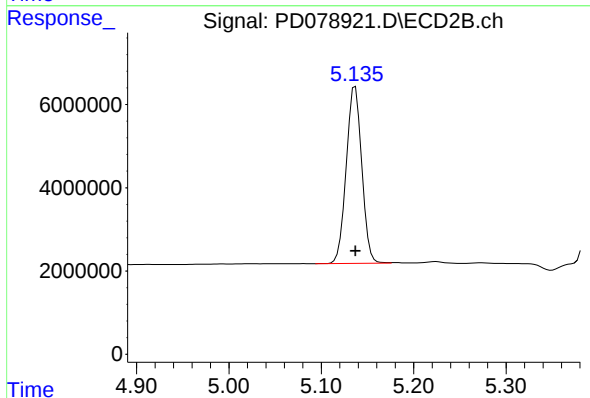


#9 Endosulfan I

R.T.: 5.137 min
Delta R.T.: 0.000 min
Response: 49589976
Conc: 20.00 ng/ml

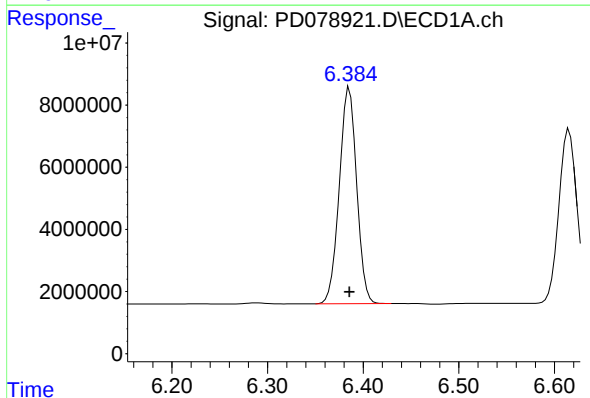


#13 Dieldrin

R.T.: 6.386 min
Delta R.T.: 0.000 min
Response: 88001972
Conc: 40.00 ng/ml

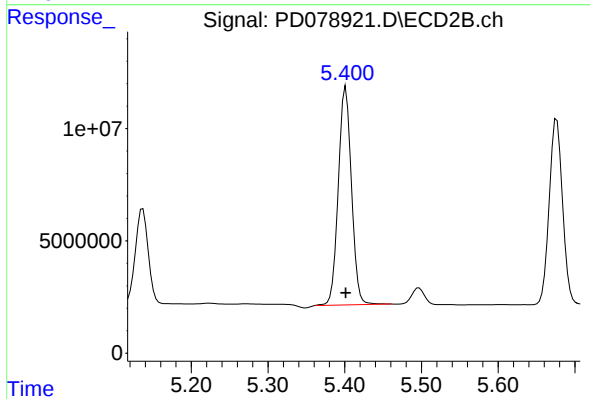

#13 Dieldrin


R.T.: 5.401 min
Delta R.T.: 0.000 min
Response: 115889677
Conc: 40.00 ng/ml

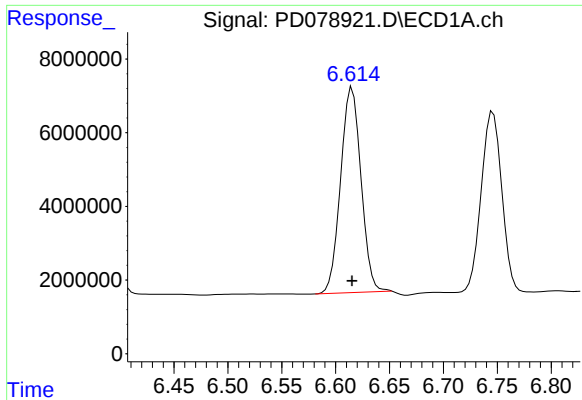

#14 Endrin


R.T.: 6.615 min
Delta R.T.: 0.000 min
Response: 73637765
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

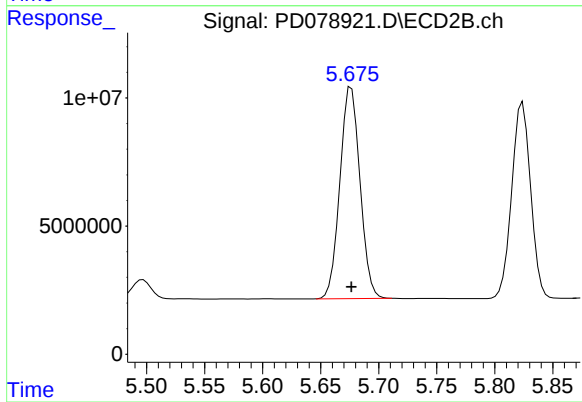


#14 Endrin

R.T.: 5.676 min
Delta R.T.: 0.000 min
Response: 99637927
Conc: 40.00 ng/ml

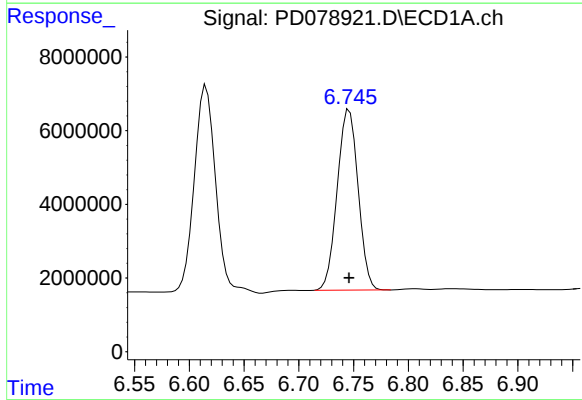


#16 4,4'-DDD

R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 65106249
Conc: 40.00 ng/ml

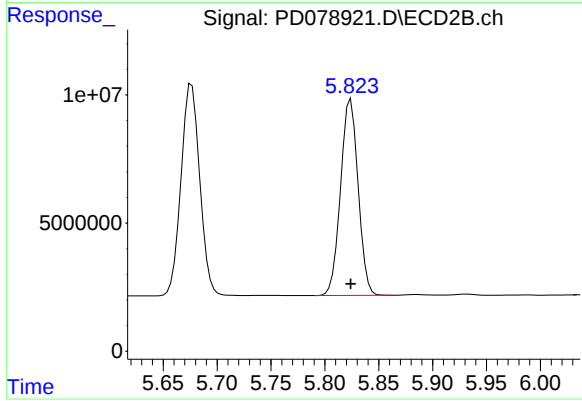

#16 4,4'-DDD


R.T.: 5.824 min
Delta R.T.: 0.000 min
Response: 86933600
Conc: 40.00 ng/ml

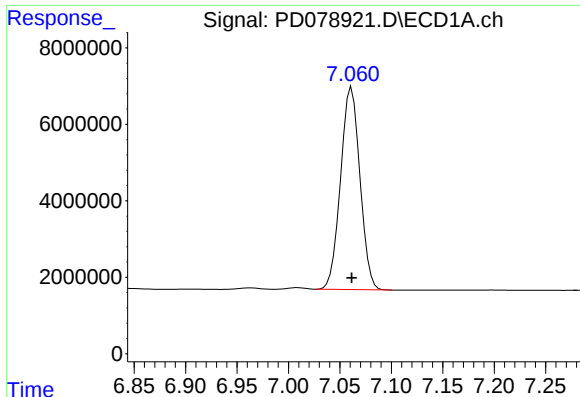

#17 4,4'-DDT


R.T.: 7.061 min
Delta R.T.: 0.000 min
Response: 69343504
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

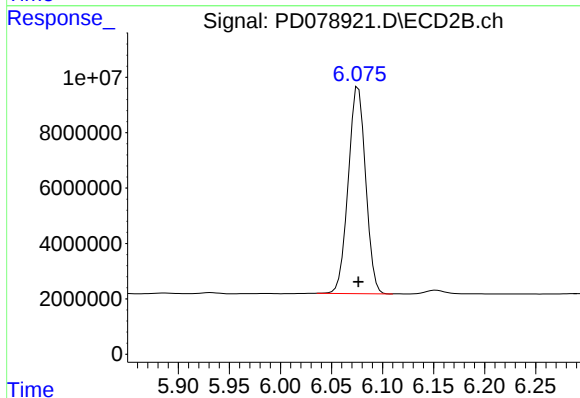


#17 4,4'-DDT

R.T.: 6.076 min
Delta R.T.: 0.000 min
Response: 88548674
Conc: 40.00 ng/ml

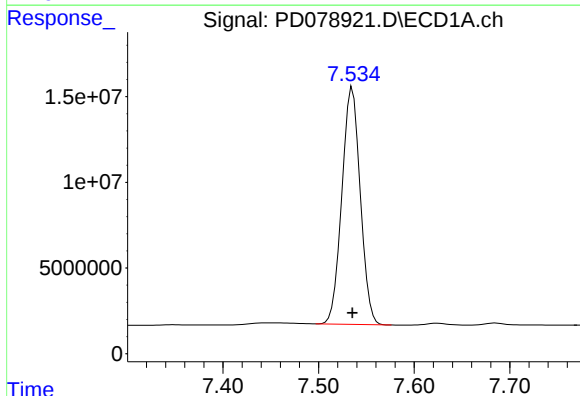


#20 Methoxychlor

R.T.: 7.535 min
Delta R.T.: 0.000 min
Response: 185417228
Conc: 200.00 ng/ml

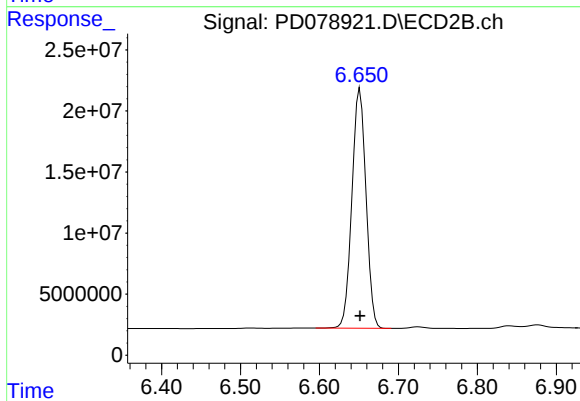

#20 Methoxychlor


R.T.: 6.651 min
Delta R.T.: 0.000 min
Response: 243732360
Conc: 200.00 ng/ml

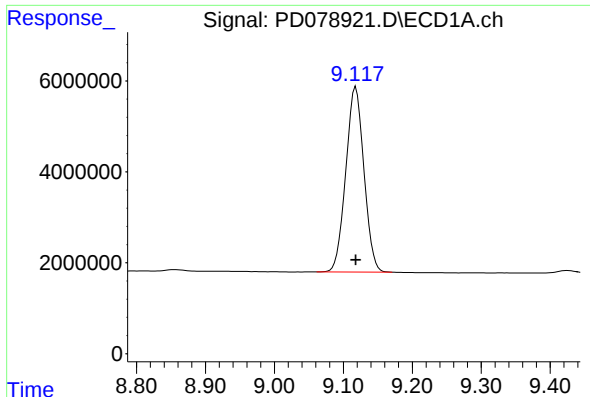

#27 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: 0.000 min
Response: 74421308
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

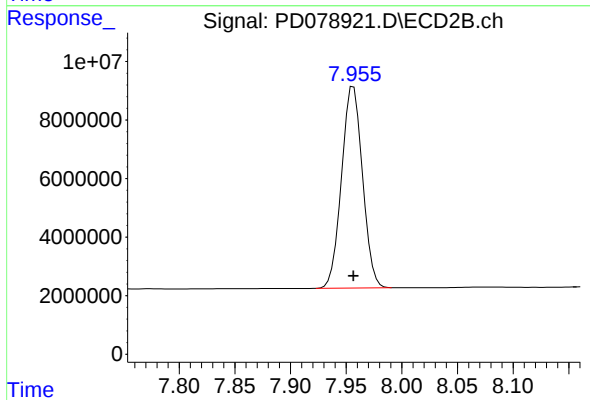

#27 Decachlorobiphenyl

R.T.: 7.957 min
Delta R.T.: 0.000 min
Response: 90298280
Conc: 40.00 ng/ml