

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101723\
 Data File : PD078923.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2023 07:43
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 08:28:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 07:37:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.806	60386077	85969684	40.285	40.398
27)	SA Decachlor...	9.119	7.957	144.1E6	180.3E6	77.469	79.880
Target Compounds							
2)	A alpha-BHC	4.026	3.309	107.9E6	141.3E6	42.720	42.347
3)	MA gamma-BHC...	4.360	3.639	101.1E6	131.9E6	41.998	41.755
4)	MA Heptachlor	4.953	3.983	104.0E6	123.0E6	41.043	41.285
9)	A Endosulfan I	6.109	5.137	82975604	102.3E6	39.738	41.245
13)	MA Dieldrin	6.386	5.401	182.5E6	241.1E6	82.947	83.214
14)	MA Endrin	6.616	5.677	151.4E6	206.4E6	82.230	82.880
16)	A 4,4'-DDD	6.746	5.824	135.5E6	180.9E6	83.277	83.229
17)	MA 4,4'-DDT	7.062	6.076	143.6E6	185.5E6	82.824	83.805
20)	A Methoxychlor	7.535	6.651	374.2E6	475.3E6	403.673	390.020


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101723\
Data File : PD078923.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2023 07:43
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 08:28:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 07:37:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

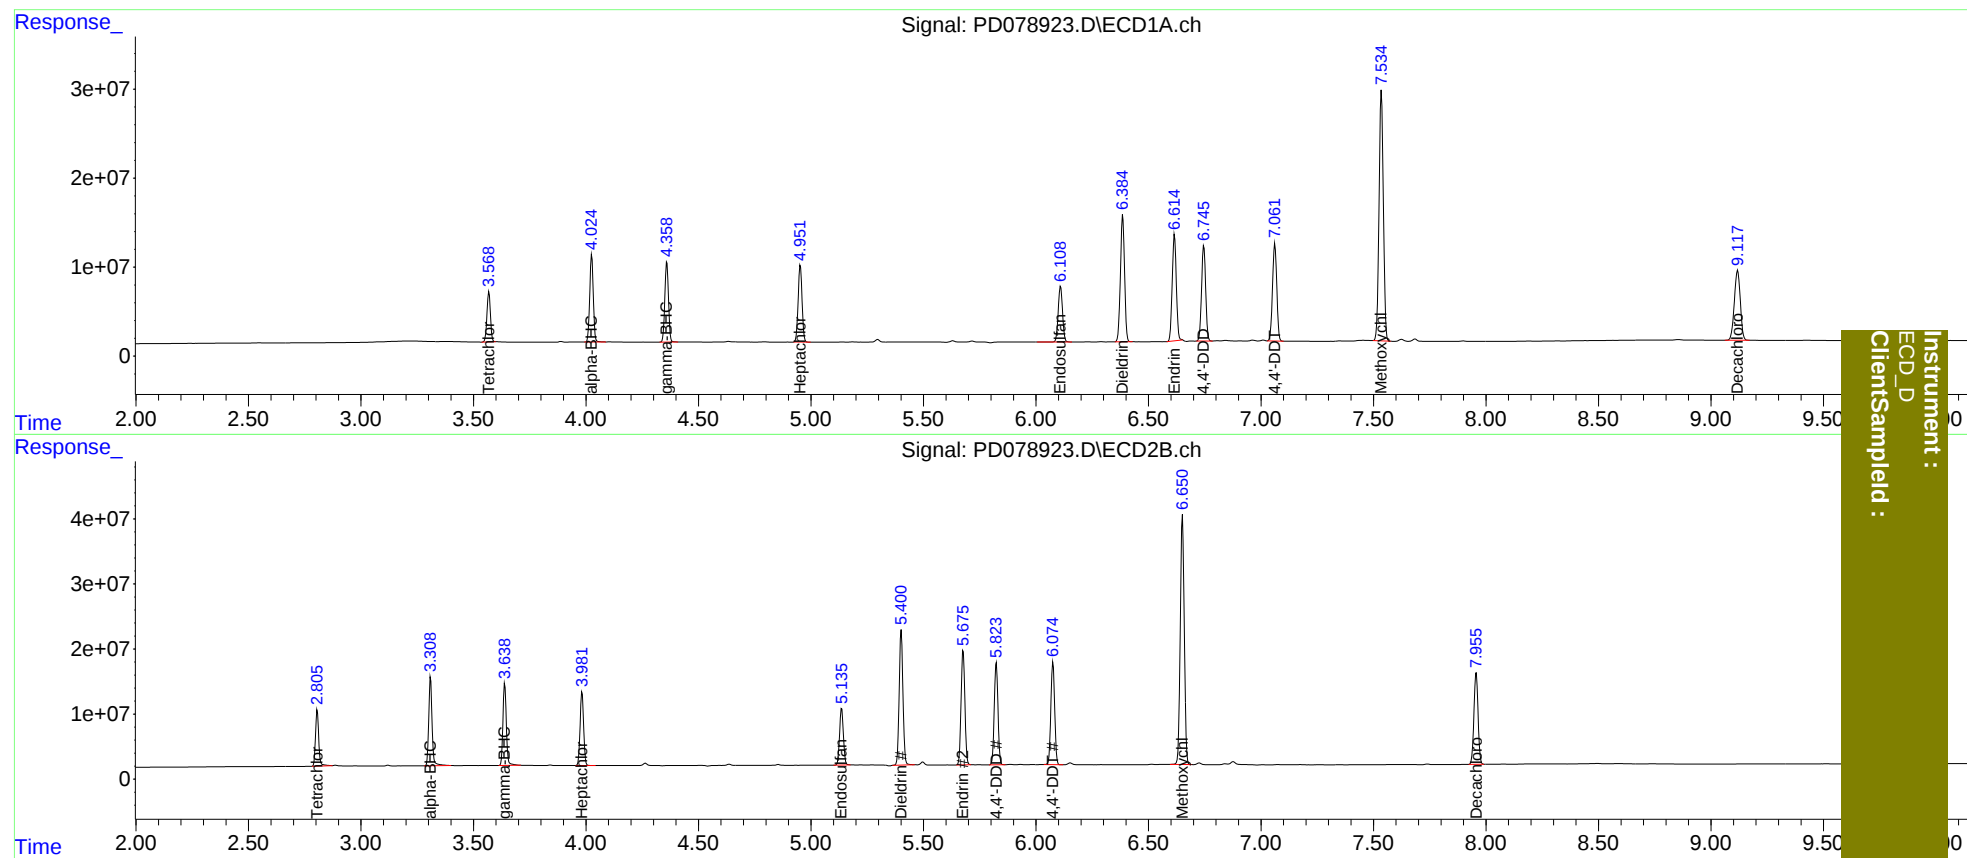


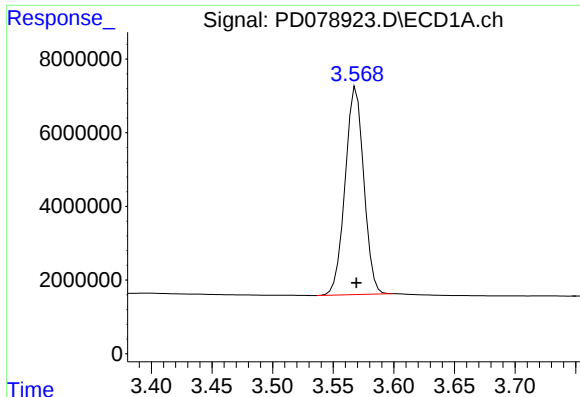

#1 Tetrachloro-m-xylene


R.T.: 3.569 min
Delta R.T.: 0.000 min
Response: 60386077
Conc: 40.29 ng/ml

Instrument :
ECD_D
ClientSampleId :

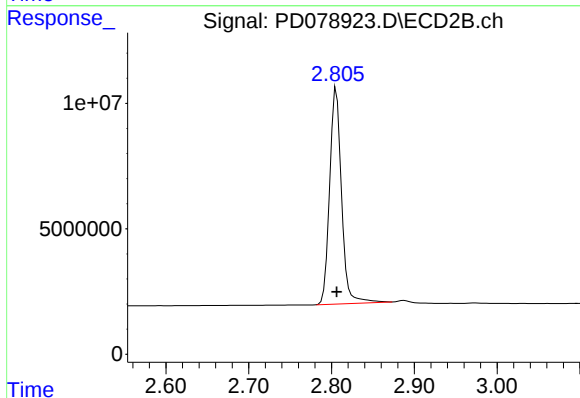


#1 Tetrachloro-m-xylene

R.T.: 2.806 min
Delta R.T.: 0.000 min
Response: 85969684
Conc: 40.40 ng/ml

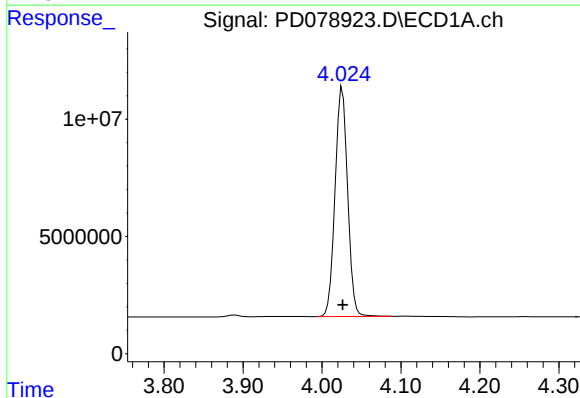


#2 alpha-BHC

R.T.: 4.026 min
Delta R.T.: 0.000 min
Response: 107858522
Conc: 42.72 ng/ml

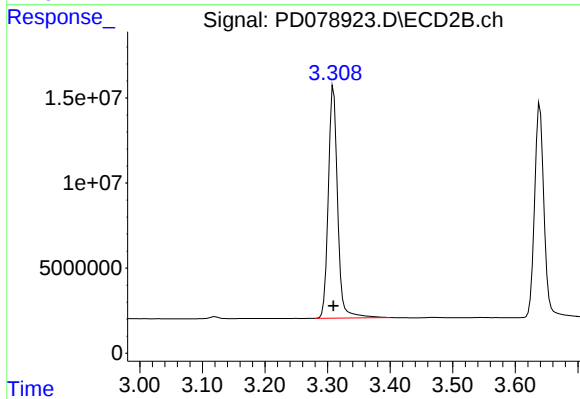

#2 alpha-BHC


R.T.: 3.309 min
Delta R.T.: 0.000 min
Response: 141253264
Conc: 42.35 ng/ml

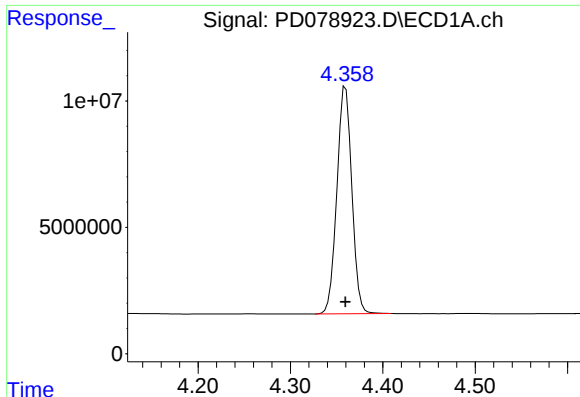

#3 gamma-BHC (Lindane)


R.T.: 4.360 min
Delta R.T.: 0.000 min
Response: 101103665
Conc: 42.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

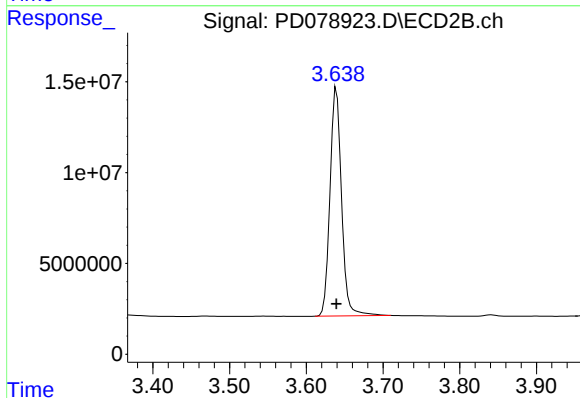


#3 gamma-BHC (Lindane)

R.T.: 3.639 min
Delta R.T.: 0.000 min
Response: 131892179
Conc: 41.75 ng/ml

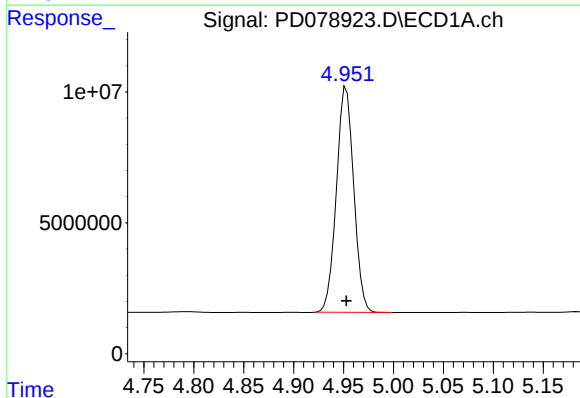


#4 Heptachlor

R.T.: 4.953 min
Delta R.T.: 0.000 min
Response: 104038472
Conc: 41.04 ng/ml

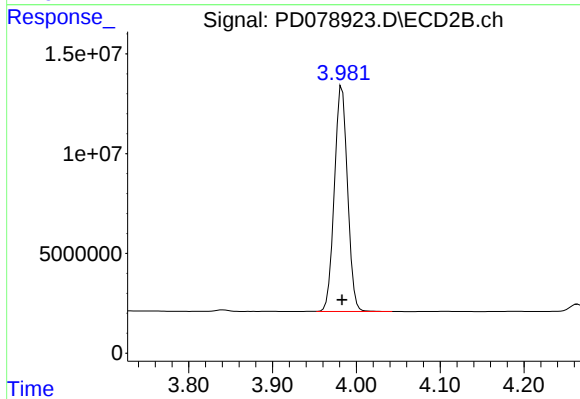

#4 Heptachlor


R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 122973371
Conc: 41.28 ng/ml

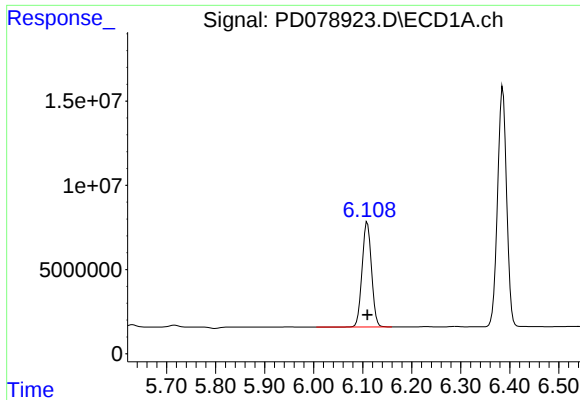

#9 Endosulfan I


R.T.: 6.109 min
Delta R.T.: 0.000 min
Response: 82975604
Conc: 39.74 ng/ml

Instrument :
ECD_D
ClientSampleId :

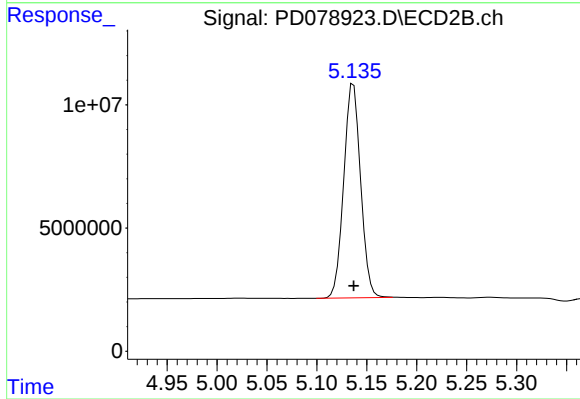


#9 Endosulfan I

R.T.: 5.137 min
Delta R.T.: 0.000 min
Response: 102267789
Conc: 41.25 ng/ml

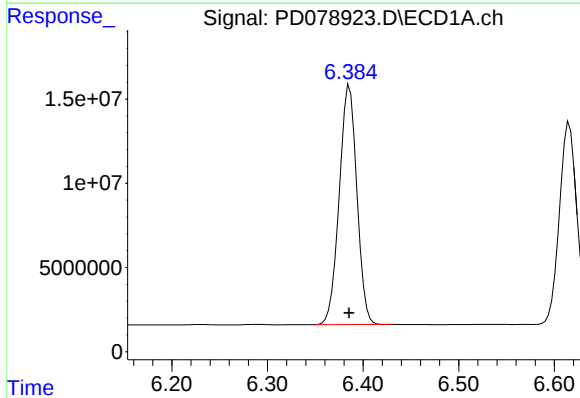


#13 Dieldrin

R.T.: 6.386 min
Delta R.T.: 0.000 min
Response: 182487725
Conc: 82.95 ng/ml

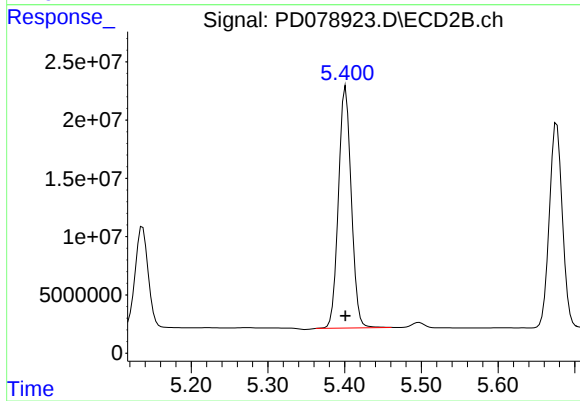

#13 Dieldrin


R.T.: 5.401 min
Delta R.T.: 0.000 min
Response: 241091277
Conc: 83.21 ng/ml

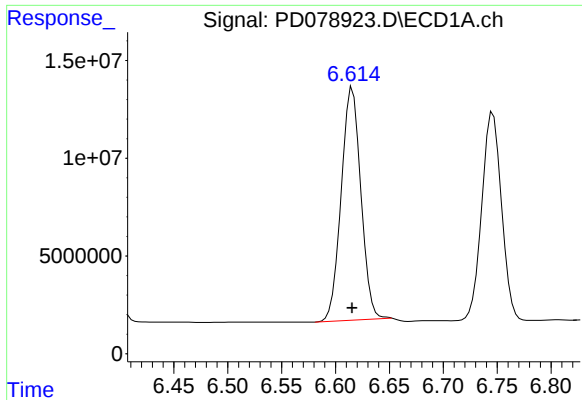

#14 Endrin


R.T.: 6.616 min
Delta R.T.: 0.000 min
Response: 151381237
Conc: 82.23 ng/ml

Instrument :
ECD_D
ClientSampleId :

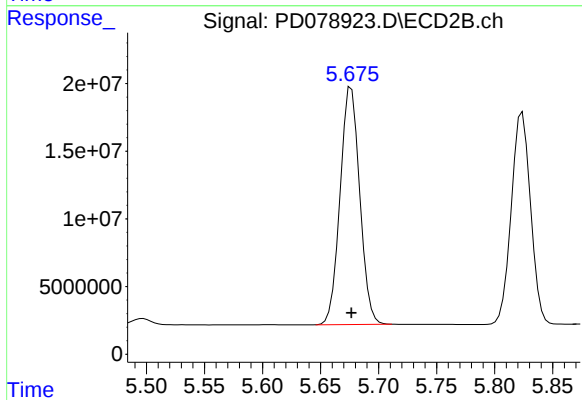


#14 Endrin

R.T.: 5.677 min
Delta R.T.: 0.000 min
Response: 206449676
Conc: 82.88 ng/ml

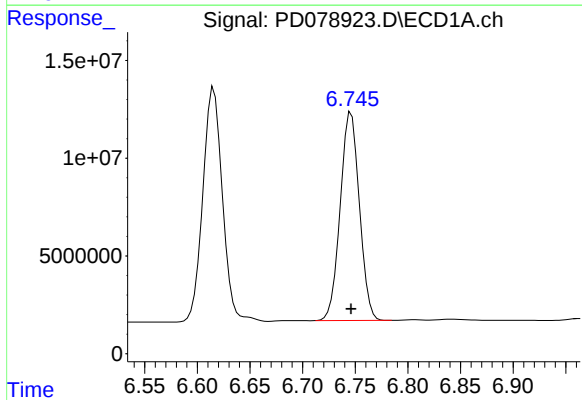


#16 4,4'-DDD

R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 135546719
Conc: 83.28 ng/ml

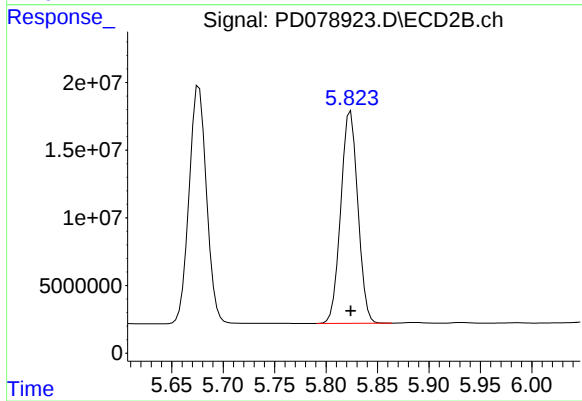

#16 4,4'-DDD


R.T.: 5.824 min
Delta R.T.: 0.000 min
Response: 180883927
Conc: 83.23 ng/ml

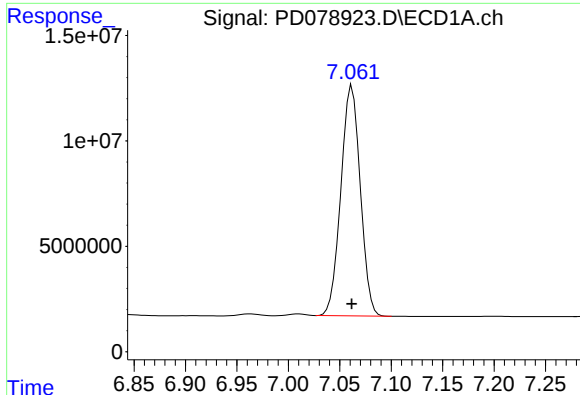

#17 4,4'-DDT


R.T.: 7.062 min
Delta R.T.: 0.000 min
Response: 143582377
Conc: 82.82 ng/ml

Instrument :
ECD_D
ClientSampleId :

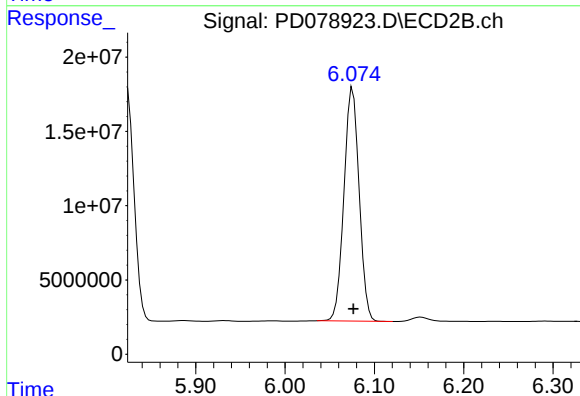


#17 4,4'-DDT

R.T.: 6.076 min
Delta R.T.: 0.000 min
Response: 185519538
Conc: 83.80 ng/ml

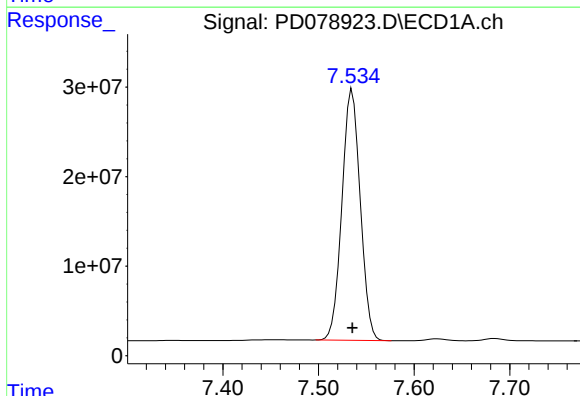


#20 Methoxychlor

R.T.: 7.535 min
Delta R.T.: 0.000 min
Response: 374239670
Conc: 403.67 ng/ml

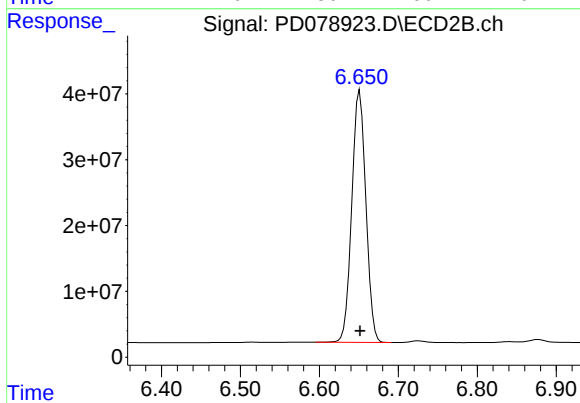

#20 Methoxychlor


R.T.: 6.651 min
Delta R.T.: 0.000 min
Response: 475302926
Conc: 390.02 ng/ml

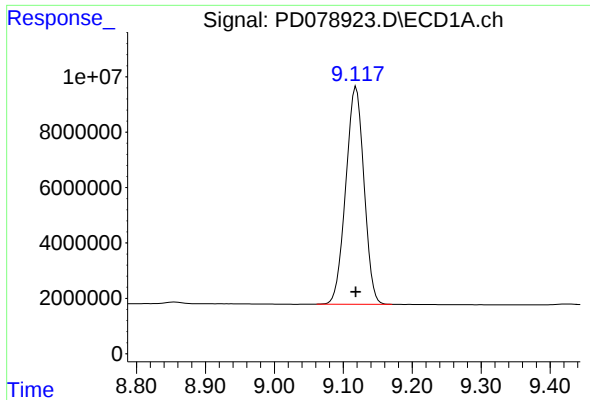

#27 Decachlorobiphenyl

R.T.: 9.119 min
Delta R.T.: 0.000 min
Response: 144133388
Conc: 77.47 ng/ml

Instrument :
ECD_D
ClientSampleId :

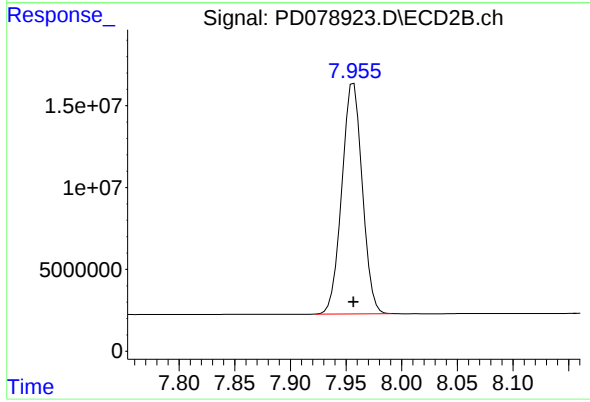

#27 Decachlorobiphenyl

R.T.: 7.957 min
Delta R.T.: 0.000 min
Response: 180325340
Conc: 79.88 ng/ml