

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101725\
 Data File : PD090656.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2025 12:56
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 13:55:00 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 17 13:48:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.875	158.9E6	1788.1E6	74.500	74.676
28)	SA Decachlor...	9.066	8.062	243.4E6	1612.3E6	74.640	74.503
Target Compounds							
23)	Chlordane-1	4.709	3.897	138.2E6	879.2E6	747.855	745.314
24)	Chlordane-2	5.236	4.479	134.2E6	909.2E6	743.636	745.838
25)	Chlordane-3	5.941	5.117	574.9E6	2751.6E6	749.591	747.247
26)	Chlordane-4	6.026	5.181	680.9E6	2339.6E6	743.974	741.430
27)	Chlordane-5	6.865	6.081	111.1E6	1068.4E6	746.235	747.201



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101725\
Data File : PD090656.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2025 12:56
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 13:55:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
Quant Title : GC Extractables
QLast Update : Fri Oct 17 13:48:57 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

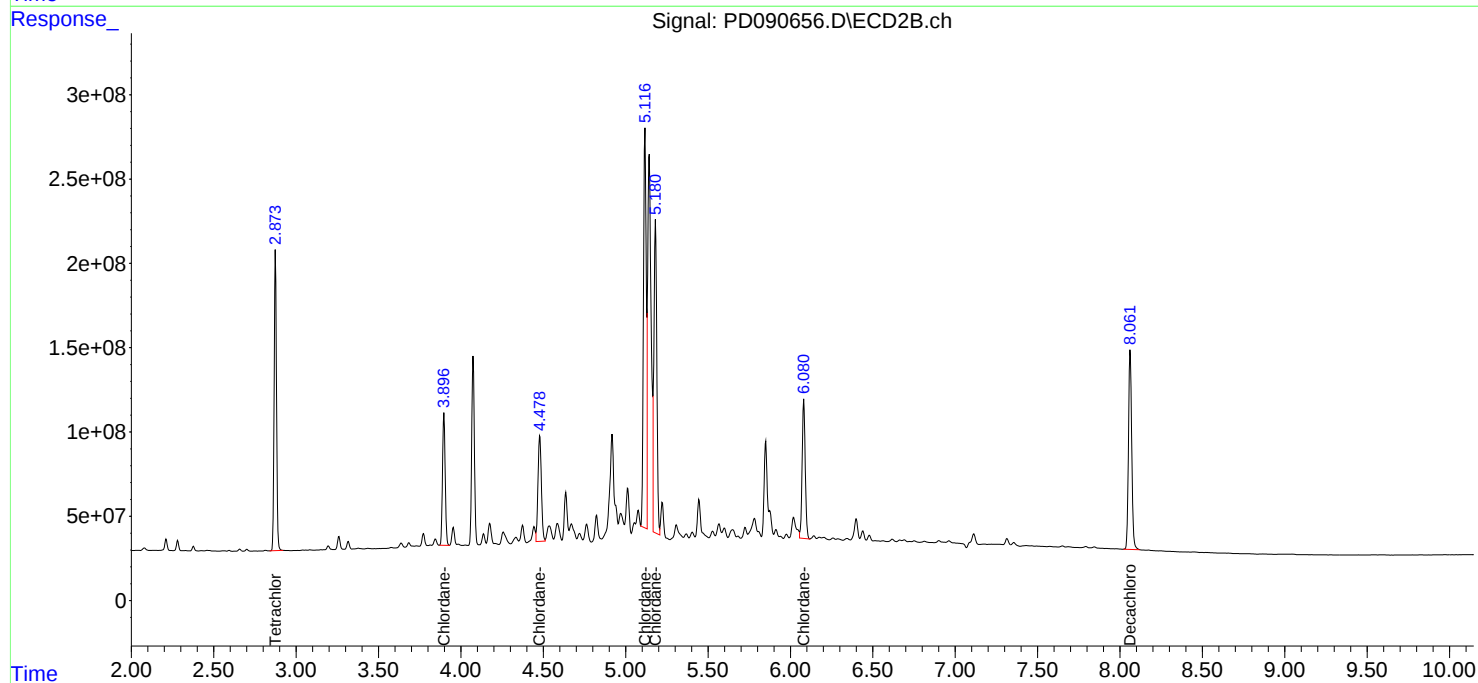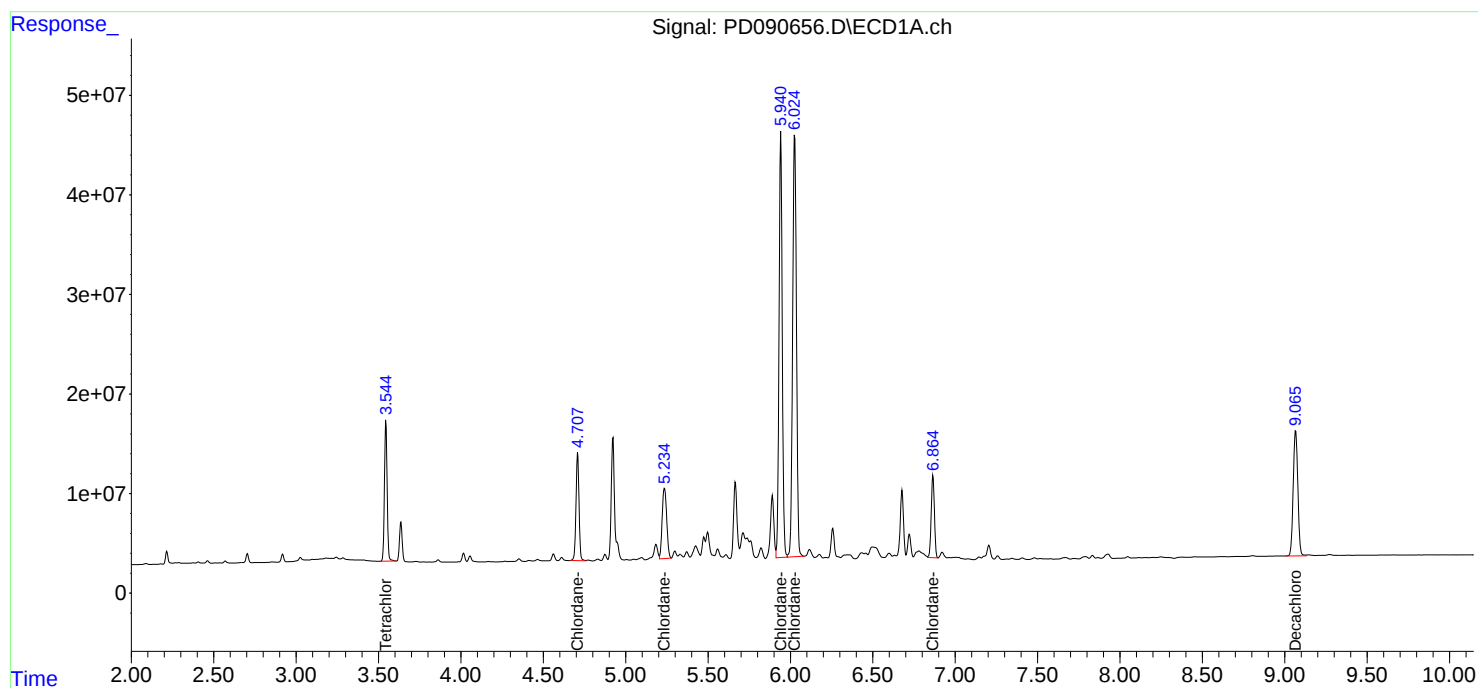


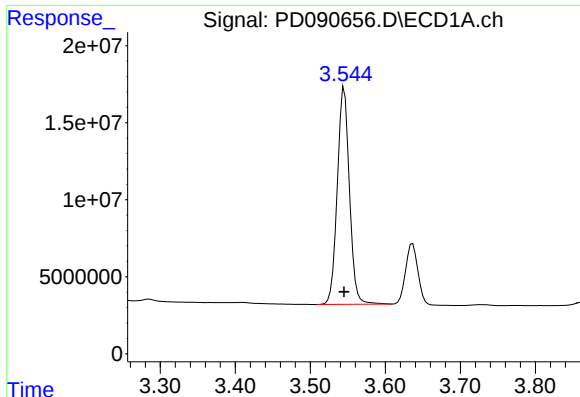

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: 0.000 min
Response: 158902957
Conc: 74.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

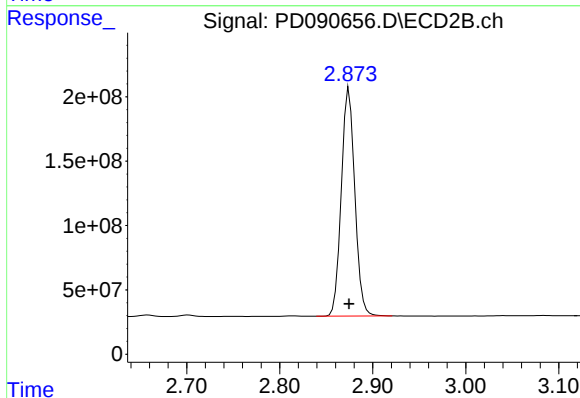


#1 Tetrachloro-m-xylene

R.T.: 2.875 min
Delta R.T.: 0.000 min
Response: 1788068574
Conc: 74.68 ng/ml

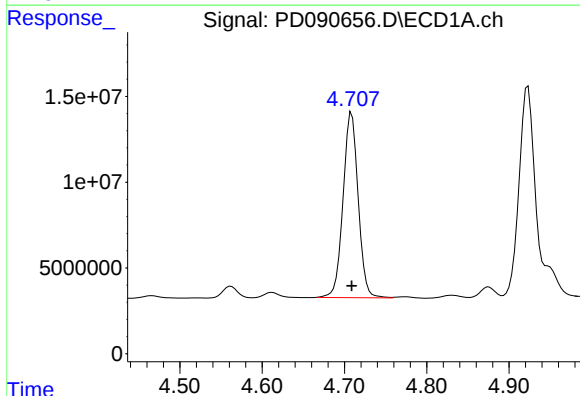


#23 Chlordane-1

R.T.: 4.709 min
Delta R.T.: 0.000 min
Response: 138244348
Conc: 747.86 ng/ml

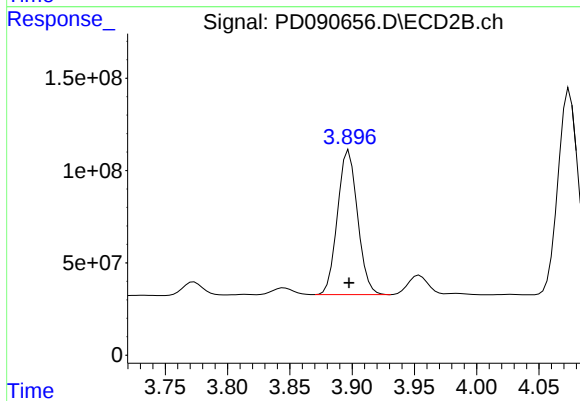

#23 Chlordane-1


R.T.: 3.897 min
Delta R.T.: 0.000 min
Response: 879169122
Conc: 745.31 ng/ml

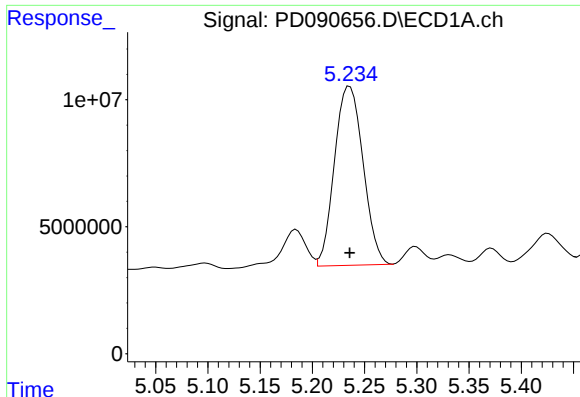

#24 Chlordane-2


R.T.: 5.236 min
Delta R.T.: 0.000 min
Response: 134175913
Conc: 743.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

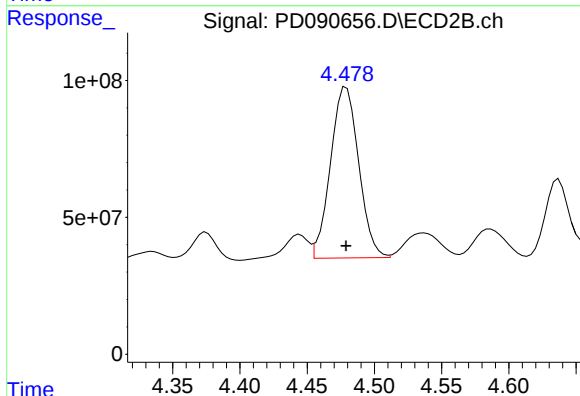


#24 Chlordane-2

R.T.: 4.479 min
Delta R.T.: 0.000 min
Response: 909154809
Conc: 745.84 ng/ml

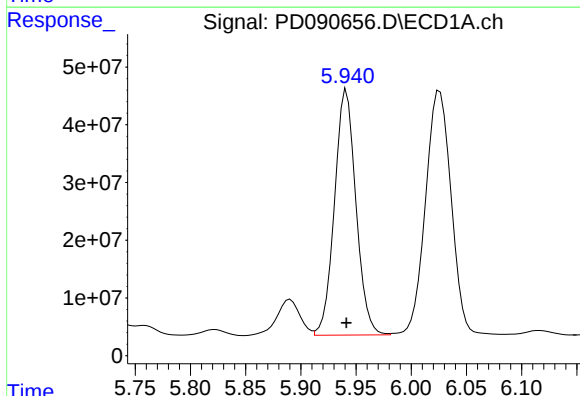


#25 Chlordane-3

R.T.: 5.941 min
Delta R.T.: 0.000 min
Response: 574850335
Conc: 749.59 ng/ml

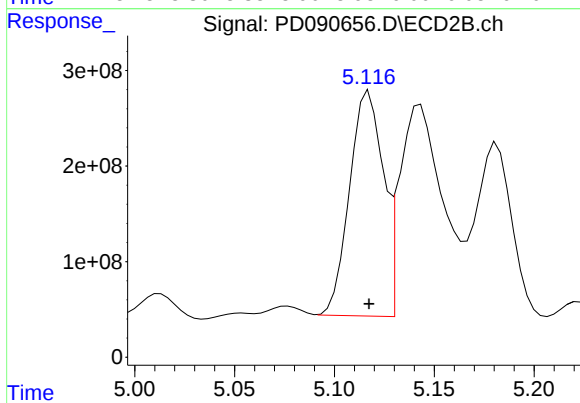

#25 Chlordane-3


R.T.: 5.117 min
Delta R.T.: 0.000 min
Response: 2751649433
Conc: 747.25 ng/ml

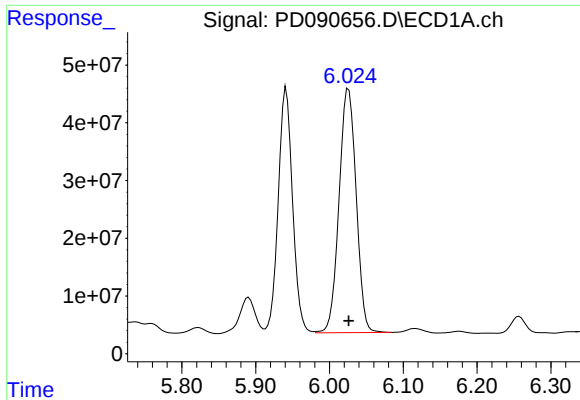

#26 Chlordane-4


R.T.: 6.026 min
Delta R.T.: 0.000 min
Response: 680883845
Conc: 743.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

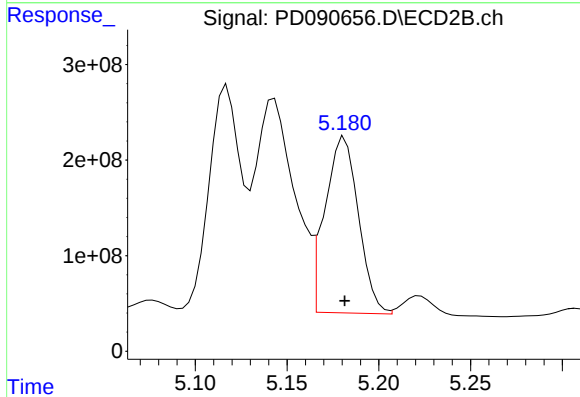


#26 Chlordane-4

R.T.: 5.181 min
Delta R.T.: 0.000 min
Response: 2339569404
Conc: 741.43 ng/ml

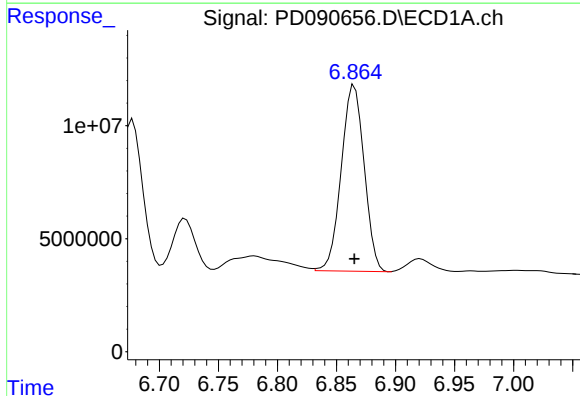


#27 Chlordane-5

R.T.: 6.865 min
Delta R.T.: 0.000 min
Response: 111140532
Conc: 746.24 ng/ml

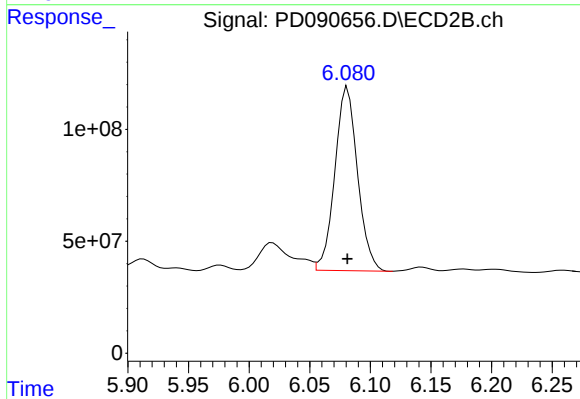

#27 Chlordane-5


R.T.: 6.081 min
Delta R.T.: 0.000 min
Response: 1068355791
Conc: 747.20 ng/ml

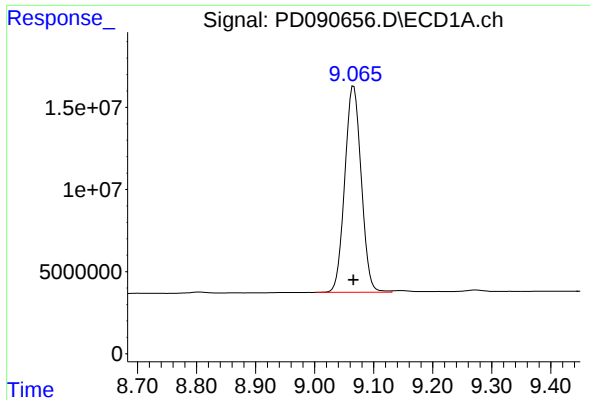

#28 Decachlorobiphenyl

R.T.: 9.066 min
Delta R.T.: 0.000 min
Response: 243436096
Conc: 74.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

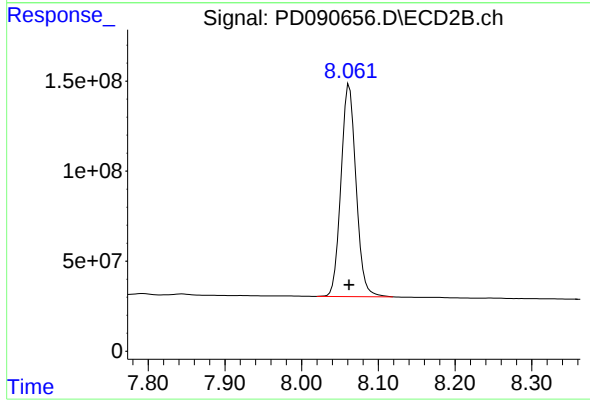

#28 Decachlorobiphenyl

R.T.: 8.062 min
Delta R.T.: 0.000 min
Response: 1612337739
Conc: 74.50 ng/ml