

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101725\
 Data File : PD090658.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2025 13:23
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 13:57:33 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 17 13:48:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.874	55880183	613.3E6	25.889	25.458
28)	SA Decachlor...	9.065	8.061	87506337	565.1E6	26.348	25.825
Target Compounds							
23)	Chlordane-1	4.708	3.897	45856223	311.2E6	248.547	260.251
24)	Chlordane-2	5.234	4.479	48161739	326.7E6	262.482	263.278
25)	Chlordane-3	5.940	5.116	182.5E6	963.4E6	240.827	258.615
26)	Chlordane-4	6.025	5.181	226.4E6	833.0E6	248.036	260.333
27)	Chlordane-5	6.864	6.080	36611884	367.7E6	246.855	255.323



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101725\
Data File : PD090658.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2025 13:23
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 13:57:33 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
Quant Title : GC Extractables
QLast Update : Fri Oct 17 13:48:57 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

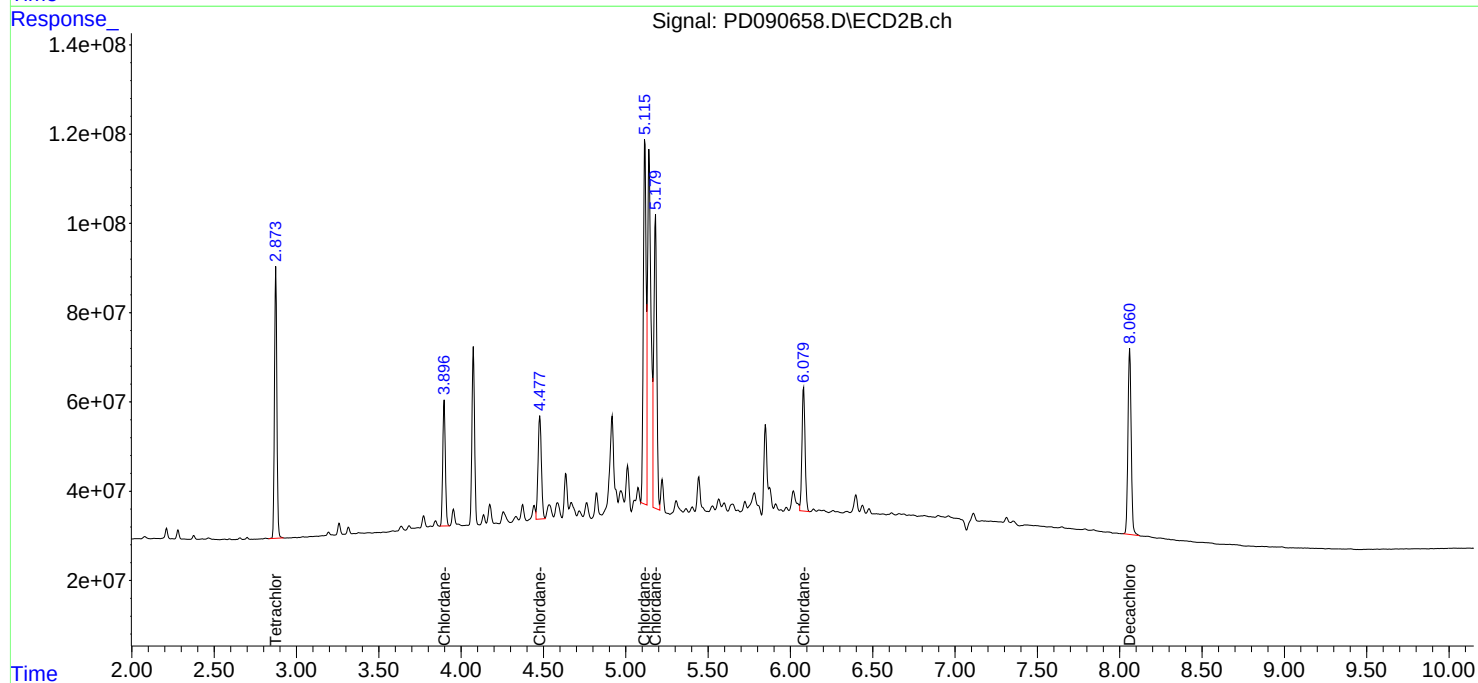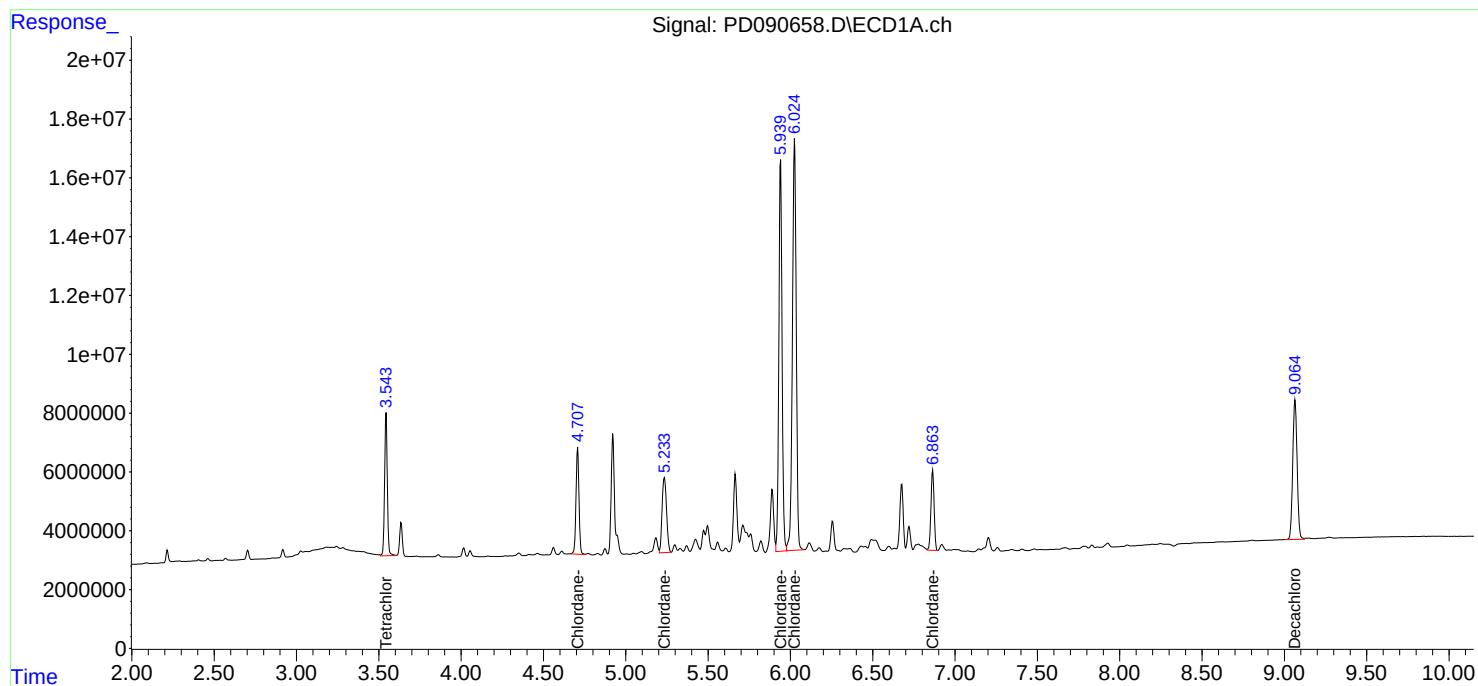


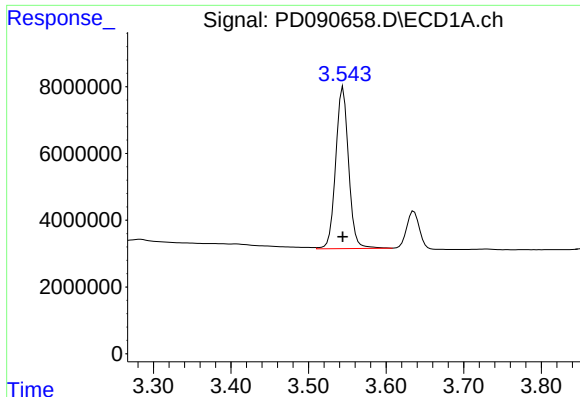

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 55880183
Conc: 25.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

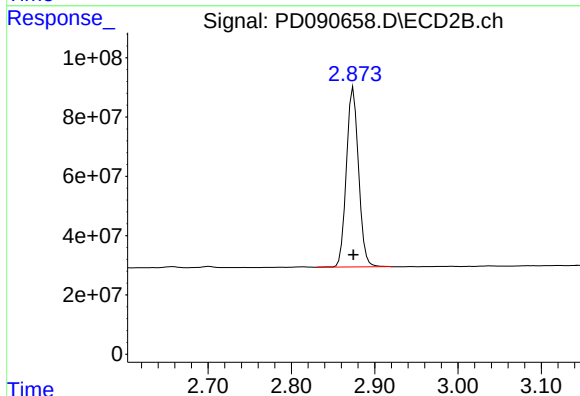


#1 Tetrachloro-m-xylene

R.T.: 2.874 min
Delta R.T.: 0.000 min
Response: 613336657
Conc: 25.46 ng/ml

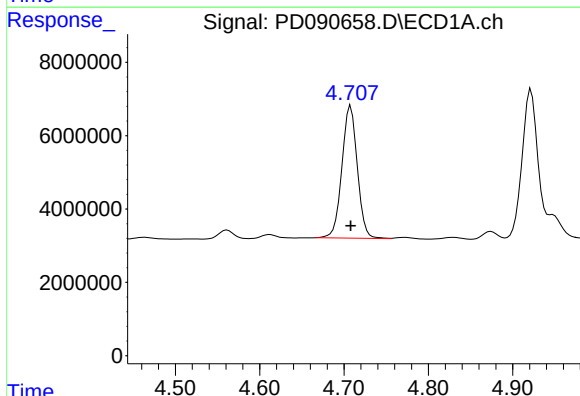


#23 Chlordane-1

R.T.: 4.708 min
Delta R.T.: 0.000 min
Response: 45856223
Conc: 248.55 ng/ml

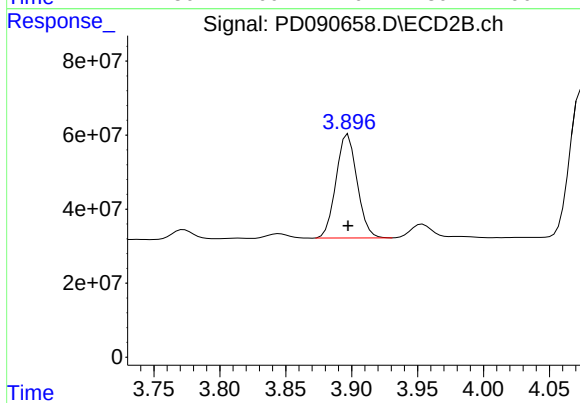

#23 Chlordane-1


R.T.: 3.897 min
Delta R.T.: 0.000 min
Response: 311245113
Conc: 260.25 ng/ml

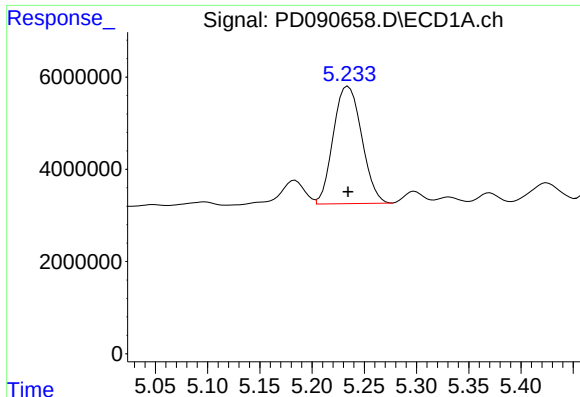

#24 Chlordane-2


R.T.: 5.234 min
Delta R.T.: 0.000 min
Response: 48161739
Conc: 262.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

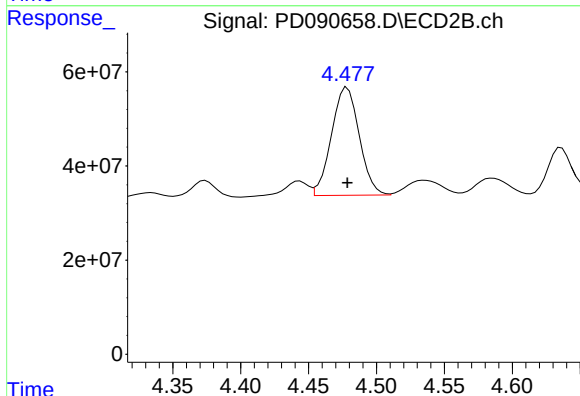


#24 Chlordane-2

R.T.: 4.479 min
Delta R.T.: 0.000 min
Response: 326711450
Conc: 263.28 ng/ml

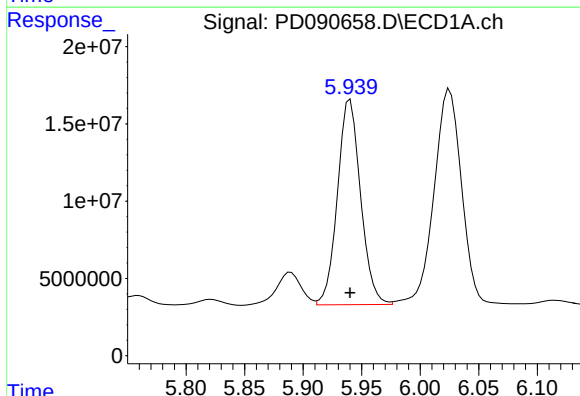


#25 Chlordane-3

R.T.: 5.940 min
Delta R.T.: 0.000 min
Response: 182455425
Conc: 240.83 ng/ml

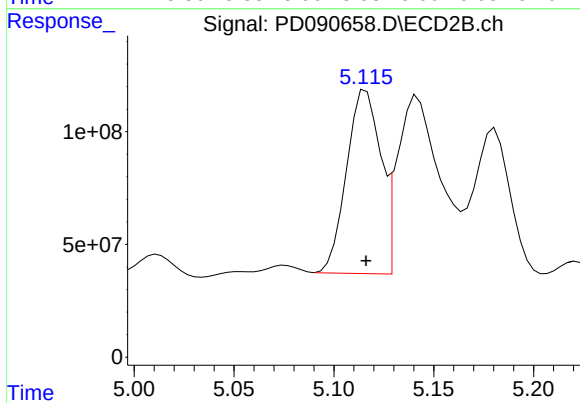

#25 Chlordane-3


R.T.: 5.116 min
Delta R.T.: 0.000 min
Response: 963385892
Conc: 258.62 ng/ml

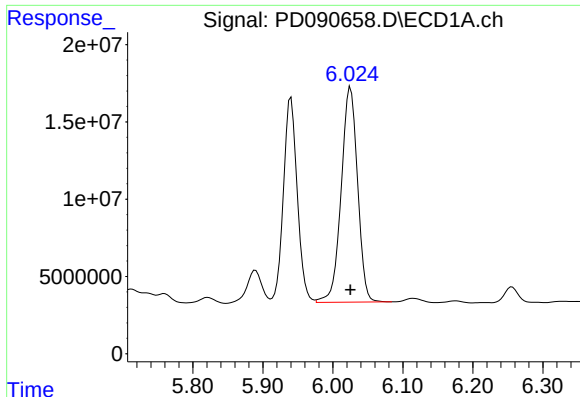

#26 Chlordane-4


R.T.: 6.025 min
Delta R.T.: 0.000 min
Response: 226409772
Conc: 248.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

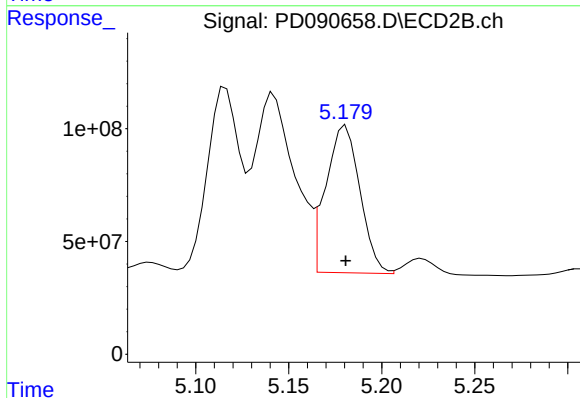


#26 Chlordane-4

R.T.: 5.181 min
Delta R.T.: 0.000 min
Response: 832950676
Conc: 260.33 ng/ml

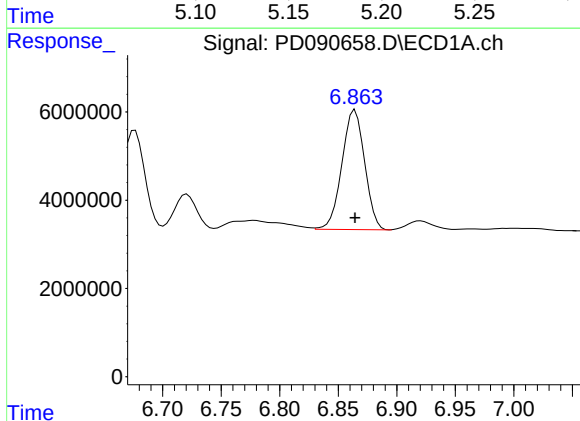


#27 Chlordane-5

R.T.: 6.864 min
Delta R.T.: 0.000 min
Response: 36611884
Conc: 246.86 ng/ml

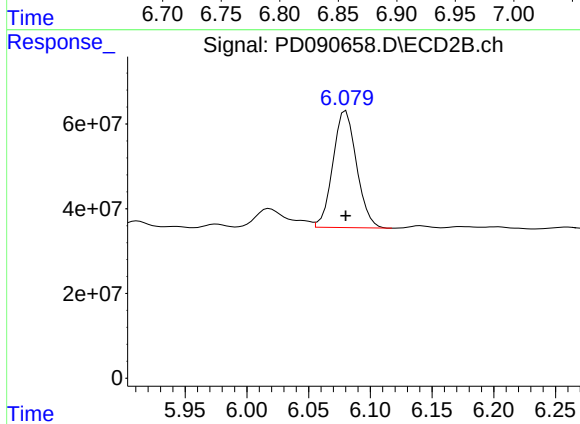

#27 Chlordane-5


R.T.: 6.080 min
Delta R.T.: 0.000 min
Response: 367672701
Conc: 255.32 ng/ml

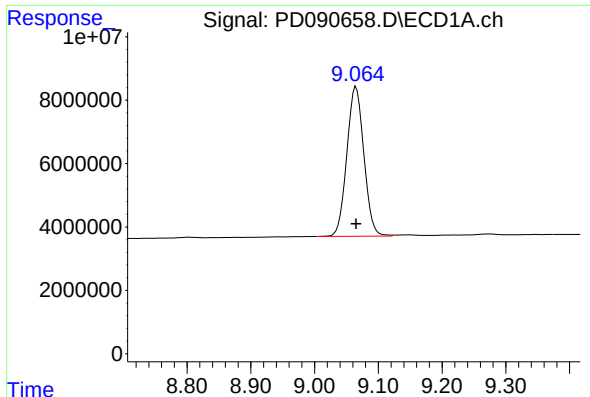

#28 Decachlorobiphenyl

R.T.: 9.065 min
Delta R.T.: 0.000 min
Response: 87506337
Conc: 26.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

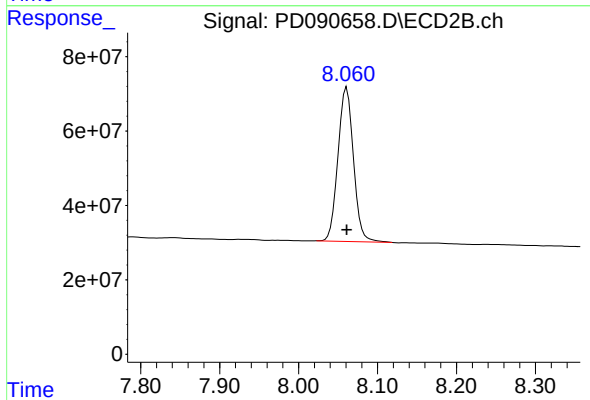

#28 Decachlorobiphenyl

R.T.: 8.061 min
Delta R.T.: 0.000 min
Response: 565109555
Conc: 25.83 ng/ml