

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101818\
 Data File : PD049854.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Oct 2018 16:55
 Operator : AJ\SJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Manual Integrations
 APPROVED

Sohil
 10/19/2018 5:50:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 07:35:55 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101818.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 19 07:31:34 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.225	4.060	46238471	1828.2E6	75.661	75.431
28)	SA Decachlor...	9.006	9.168	43557060	1086.2E6	74.607	74.803
Target Compounds							
23)	Chlordane-1	5.128	5.064	19986653	915.0E6	753.086	752.546
24)	Chlordane-2	5.632	5.534	19397928	809.4E6	746.132	753.117
25)	Chlordane-3	6.207	6.182	65791277	2580.2E6	778.818m	754.605
26)	Chlordane-4	6.267	6.257	53491234	2899.5E6	756.528	754.071
27)	Chlordane-5	7.107	7.065	20073794	518.6E6	754.436	752.713

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101818\
Data File : PD049854.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Oct 2018 16:55
Operator : AJ\SJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
PCHLORICC750


Manual Integrations
APPROVED

Sohil
10/19/2018 5:50:23 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 07:35:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101818.M
Quant Title : GC Extractables
QLast Update : Fri Oct 19 07:31:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

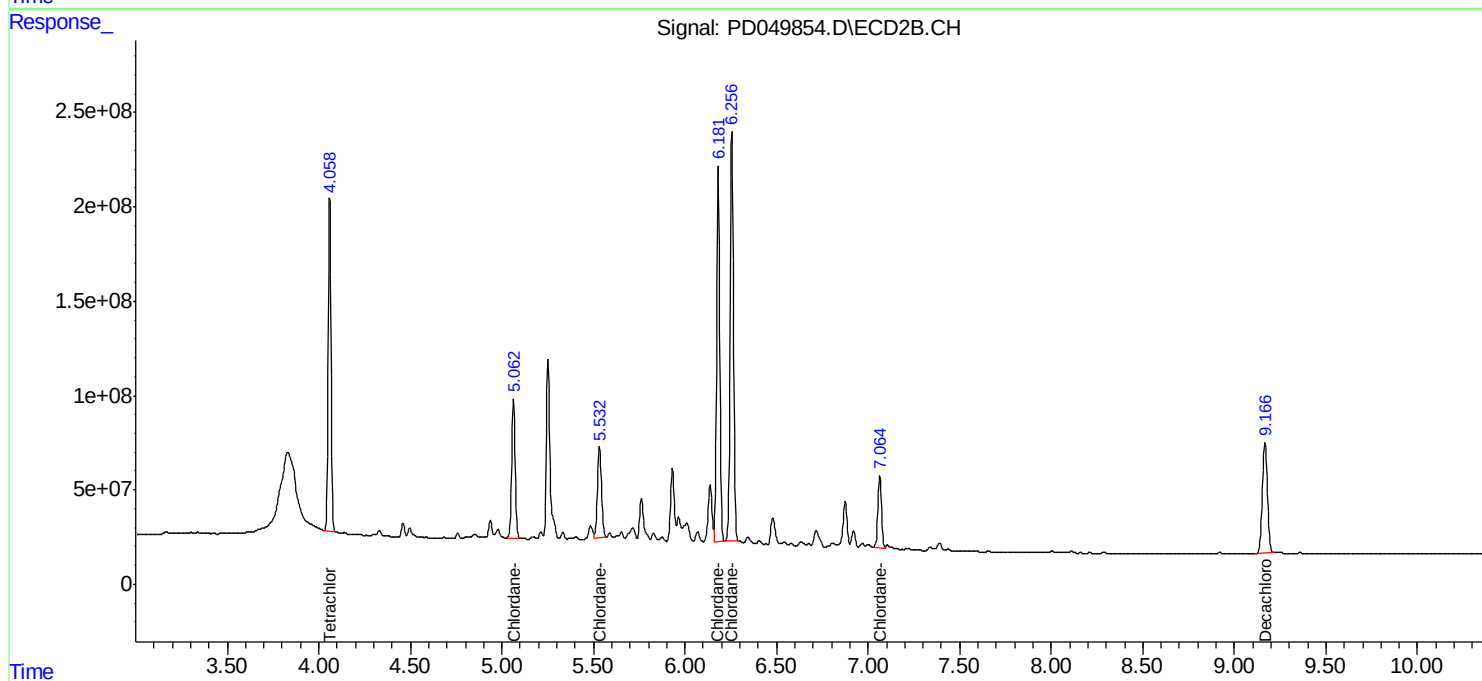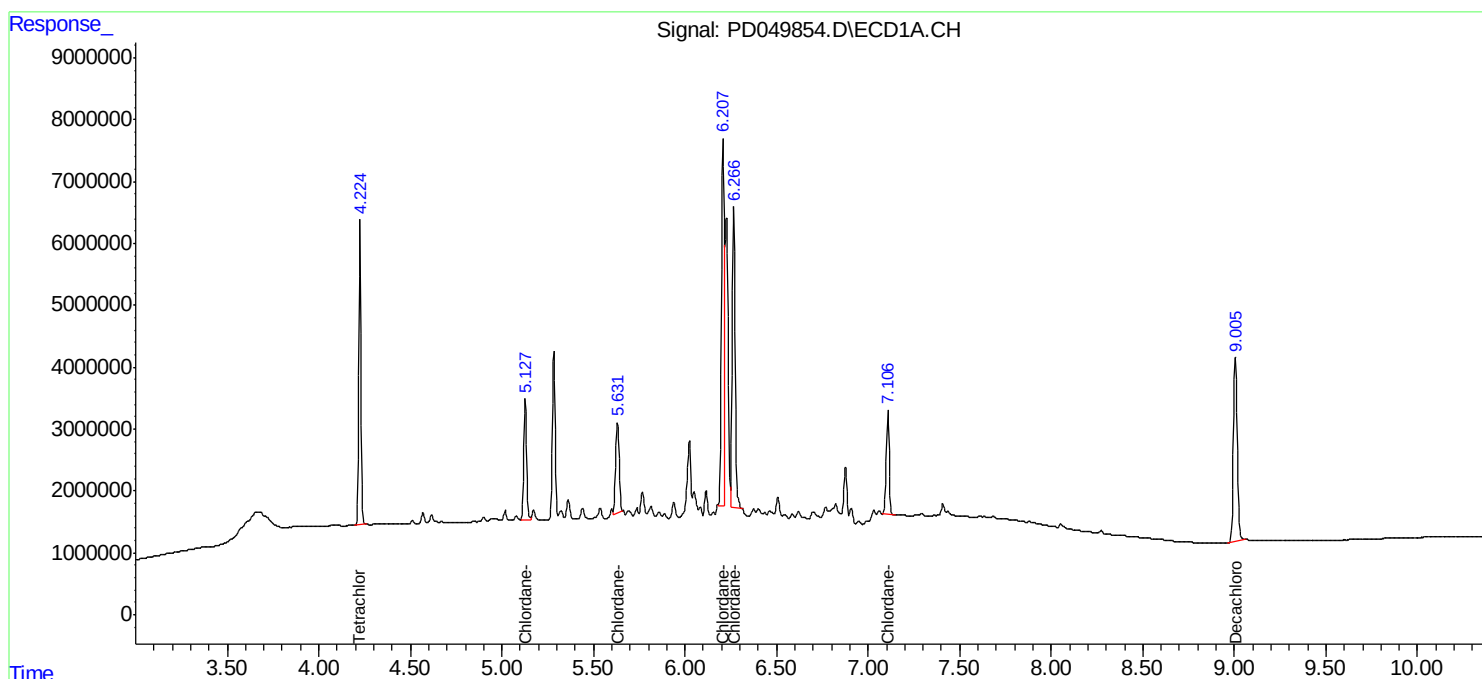

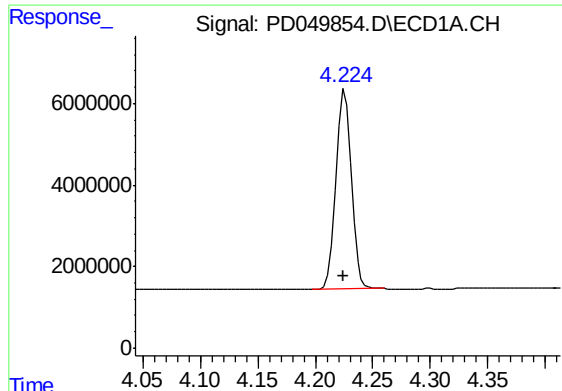


#1 Tetrachloro-m-xylene

R.T.: 4.225 min
Delta R.T.: 0.000 min
Response: 46238471
Conc: 75.66 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750


Manual Integrations
APPROVED

Sohil
10/19/2018 5:50:23 PM

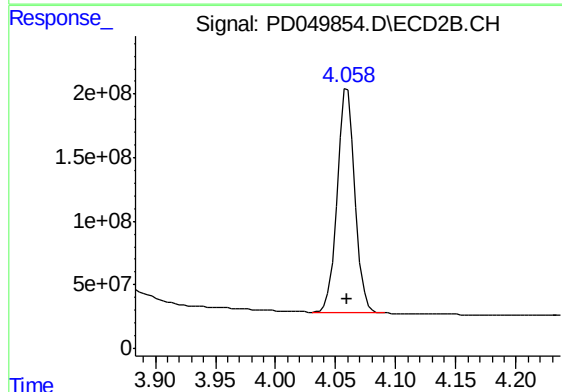


#1 Tetrachloro-m-xylene

R.T.: 4.060 min
Delta R.T.: 0.000 min
Response: 1828165605
Conc: 75.43 ng/ml

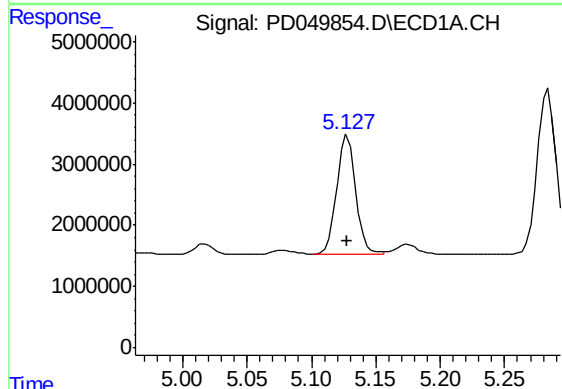


#23 Chlordane-1

R.T.: 5.128 min
Delta R.T.: 0.000 min
Response: 19986653
Conc: 753.09 ng/ml

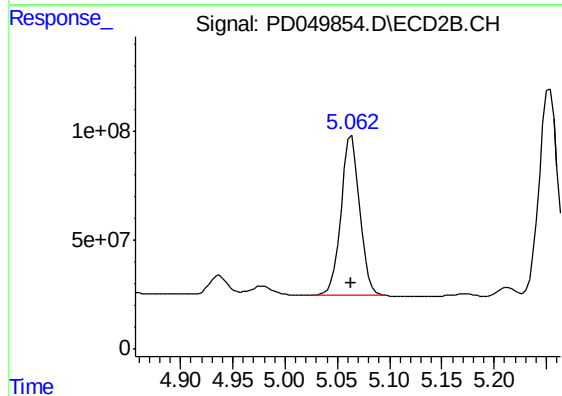

#23 Chlordane-1

R.T.: 5.064 min
Delta R.T.: 0.000 min
Response: 914977709
Conc: 752.55 ng/ml

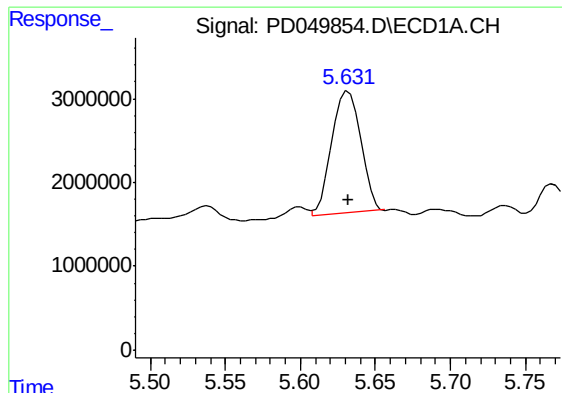


#24 Chlordane-2

R.T.: 5.632 min
Delta R.T.: 0.000 min
Response: 19397928
Conc: 746.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750


Manual Integrations
APPROVED

Sohil
10/19/2018 5:50:23 PM

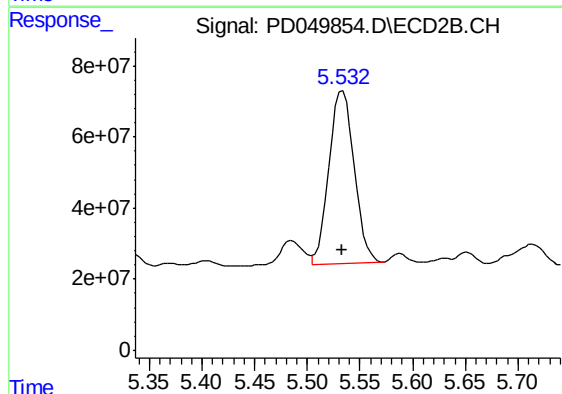


#24 Chlordane-2

R.T.: 5.534 min
Delta R.T.: 0.000 min
Response: 809425456
Conc: 753.12 ng/ml

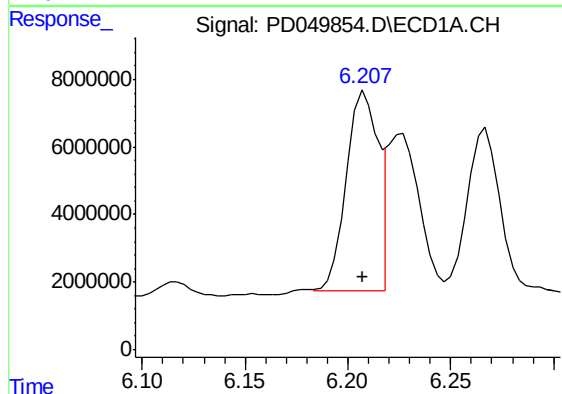


#25 Chlordane-3

R.T.: 6.207 min
Delta R.T.: 0.000 min
Response: 65791277
Conc: 778.82 ng/ml m

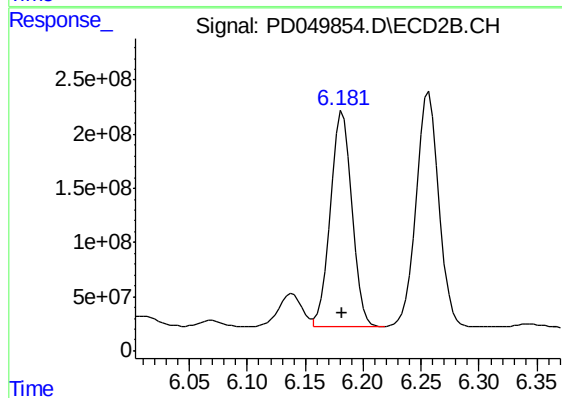

#25 Chlordane-3

R.T.: 6.182 min
Delta R.T.: 0.000 min
Response: 2580160961
Conc: 754.61 ng/ml

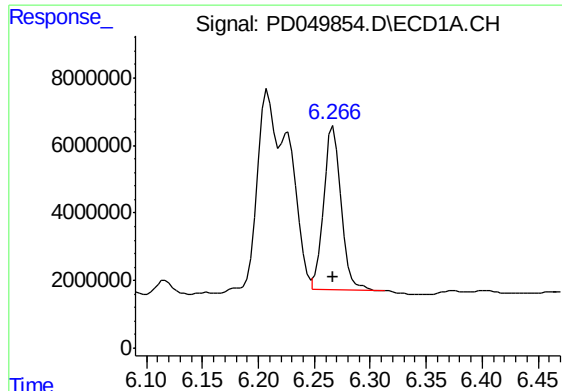


#26 Chlordane-4

R.T.: 6.267 min
Delta R.T.: 0.000 min
Response: 53491234
Conc: 756.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750


Manual Integrations
APPROVED

Sohil
10/19/2018 5:50:23 PM

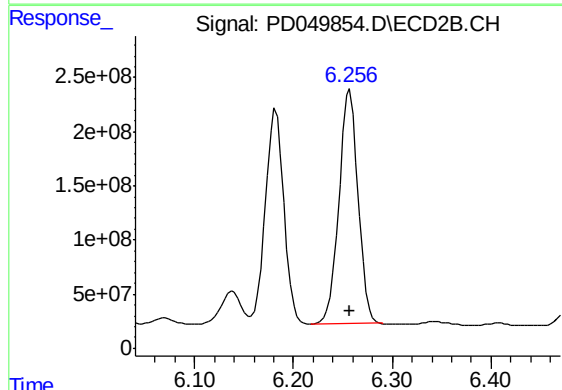


#26 Chlordane-4

R.T.: 6.257 min
Delta R.T.: 0.000 min
Response: 2899504654
Conc: 754.07 ng/ml

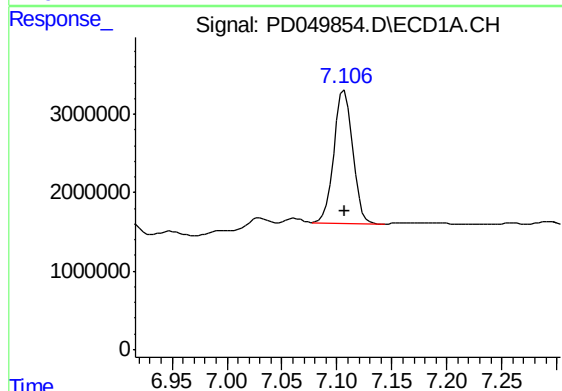


#27 Chlordane-5

R.T.: 7.107 min
Delta R.T.: 0.000 min
Response: 20073794
Conc: 754.44 ng/ml

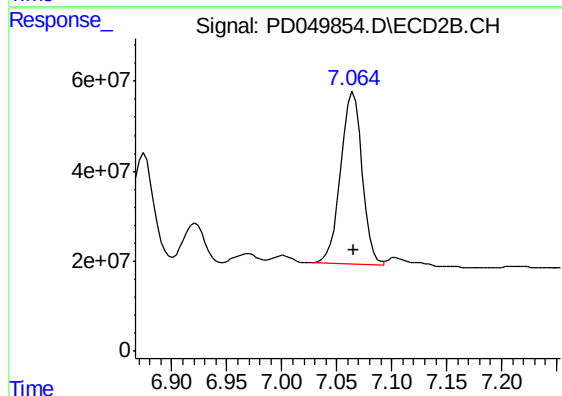

#27 Chlordane-5

R.T.: 7.065 min
Delta R.T.: 0.000 min
Response: 518608704
Conc: 752.71 ng/ml

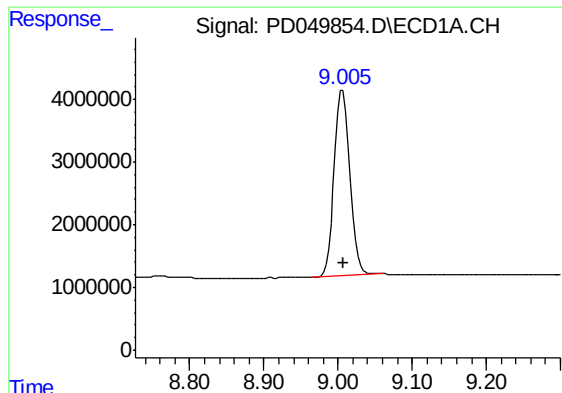


#28 Decachlorobiphenyl

R.T.: 9.006 min
Delta R.T.: 0.000 min
Response: 43557060
Conc: 74.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Manual Integrations
APPROVED

Sohil
10/19/2018 5:50:23 PM

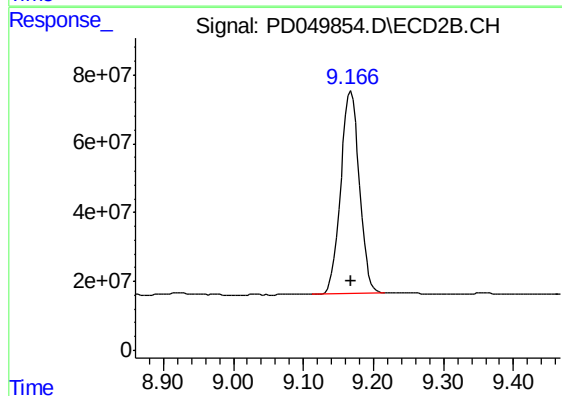

#28 Decachlorobiphenyl

R.T.: 9.168 min
Delta R.T.: 0.000 min
Response: 1086249894
Conc: 74.80 ng/ml