

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101818\
 Data File : PD049864.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Oct 2018 19:15
 Operator : AJ\SJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD101818CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 07:41:22 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101818.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 19 07:31:34 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.226	4.060	30428402	1281.4E6	49.535	49.894
28)	SA Decachlor...	9.008	9.168	29494199	767.2E6	48.391	48.389
Target Compounds							
23)	Chlordane-1	5.129	5.064	13322596	644.7E6	500.997	495.408
24)	Chlordane-2	5.632	5.534	13327235	576.1E6	491.877	489.896
25)	Chlordane-3	6.210	6.183	43532108	1798.9E6	488.851	496.467
26)	Chlordane-4	6.268	6.257	35102025	2023.7E6	489.495	493.932
27)	Chlordane-5	7.108	7.065	13310060	363.4E6	483.383	511.747



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101818\
Data File : PD049864.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Oct 2018 19:15
Operator : AJ\SJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD101818CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 07:41:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101818.M
Quant Title : GC Extractables
QLast Update : Fri Oct 19 07:31:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

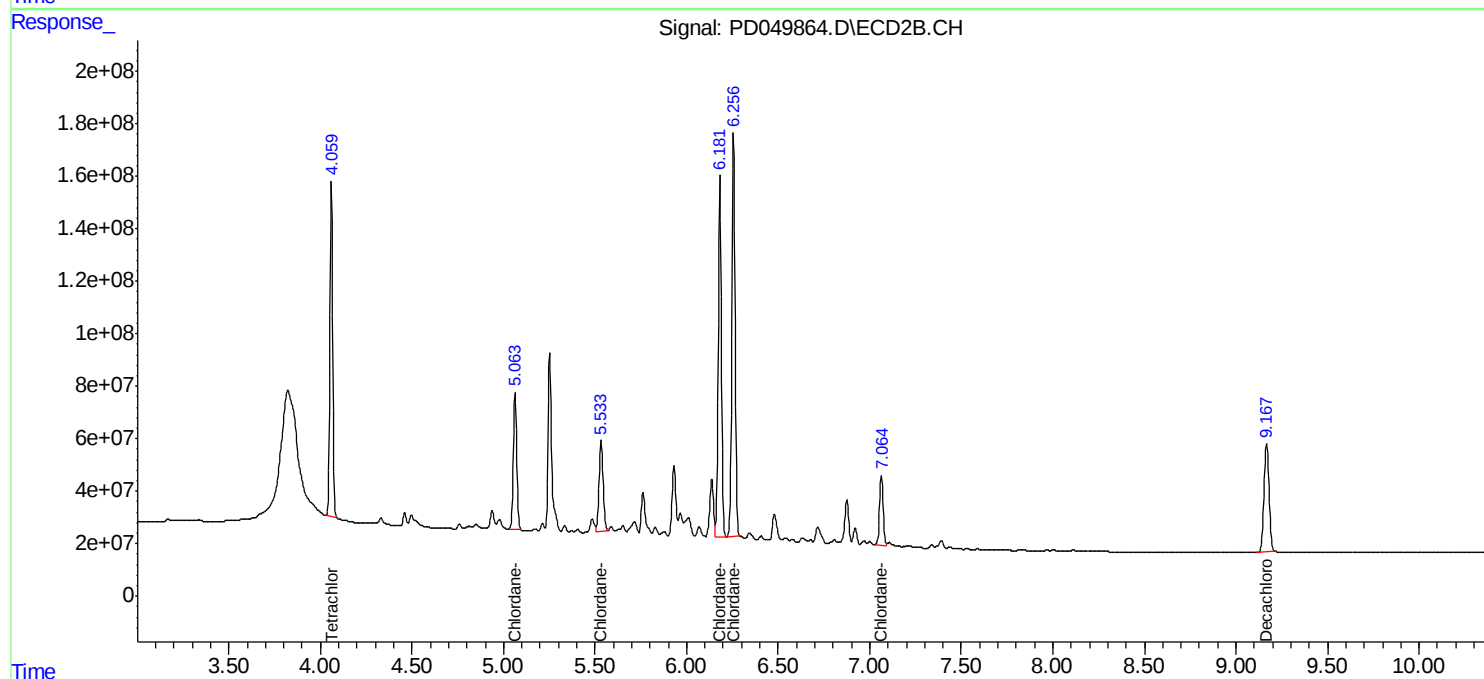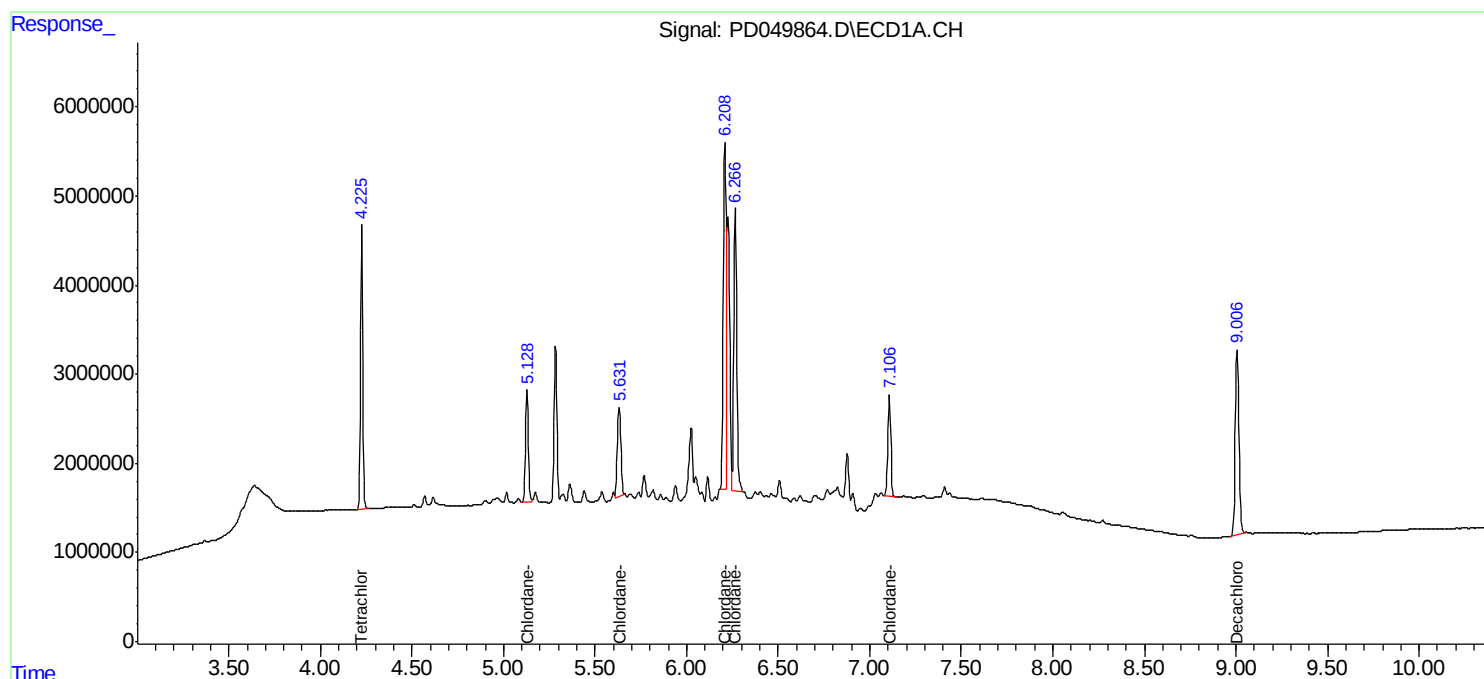


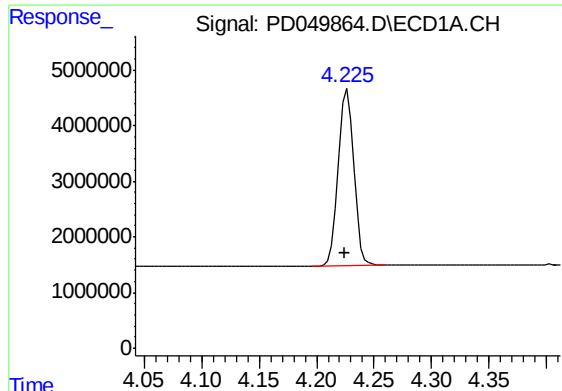

#1 Tetrachloro-m-xylene


R.T.: 4.226 min
Delta R.T.: 0.001 min
Response: 30428402
Conc: 49.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD101818CHLOR

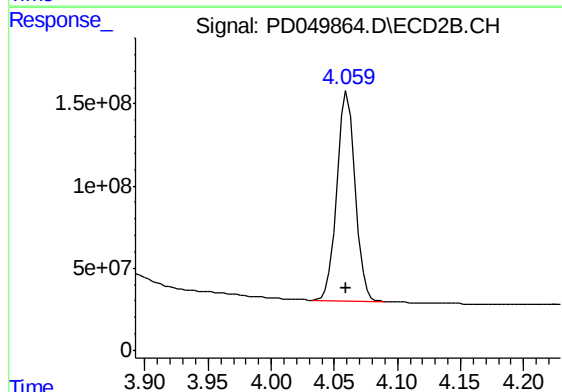


#1 Tetrachloro-m-xylene

R.T.: 4.060 min
Delta R.T.: 0.000 min
Response: 1281444730
Conc: 49.89 ng/ml

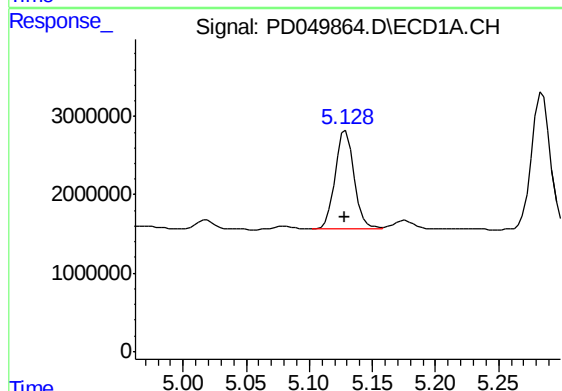


#23 Chlordane-1

R.T.: 5.129 min
Delta R.T.: 0.001 min
Response: 13322596
Conc: 501.00 ng/ml

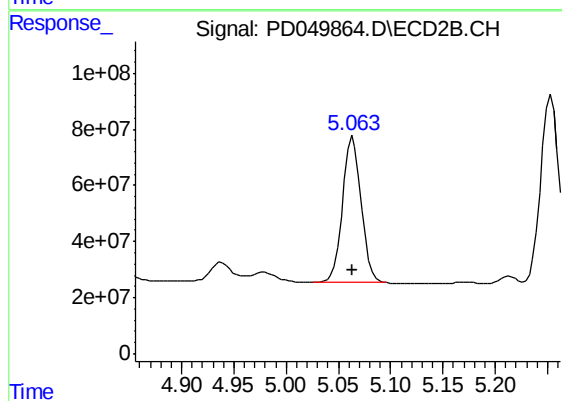

#23 Chlordane-1


R.T.: 5.064 min
Delta R.T.: 0.000 min
Response: 644663716
Conc: 495.41 ng/ml

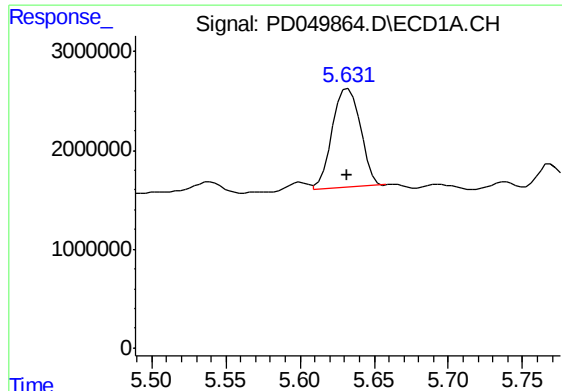

#24 Chlordane-2


R.T.: 5.632 min
Delta R.T.: 0.000 min
Response: 13327235
Conc: 491.88 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD101818CHLOR

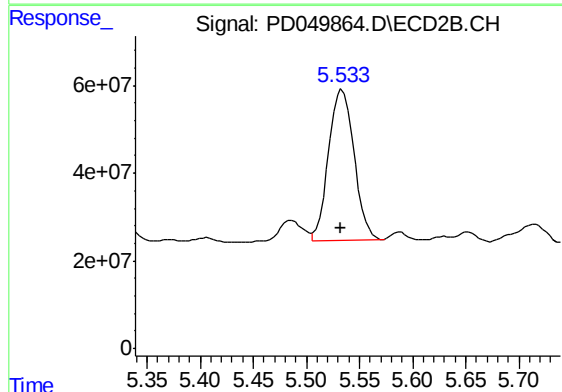


#24 Chlordane-2

R.T.: 5.534 min
Delta R.T.: 0.002 min
Response: 576129591
Conc: 489.90 ng/ml

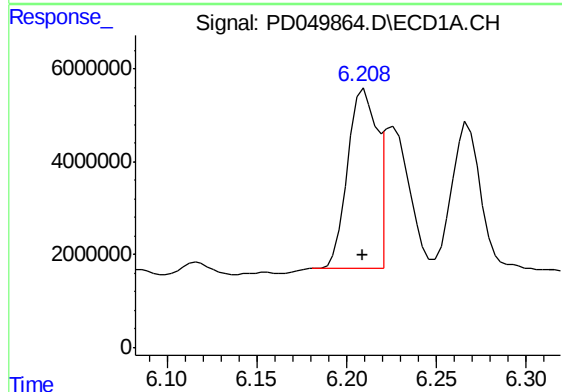


#25 Chlordane-3

R.T.: 6.210 min
Delta R.T.: 0.001 min
Response: 43532108
Conc: 488.85 ng/ml

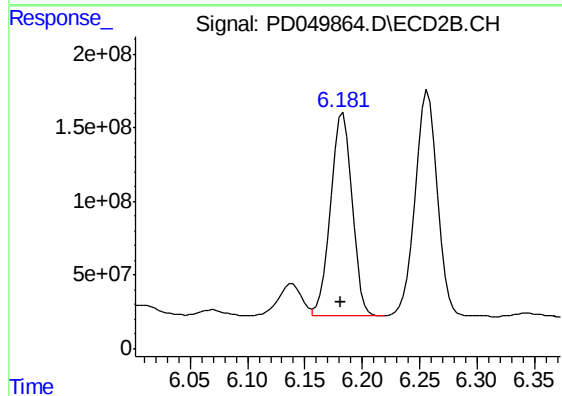

#25 Chlordane-3


R.T.: 6.183 min
Delta R.T.: 0.000 min
Response: 1798903435
Conc: 496.47 ng/ml

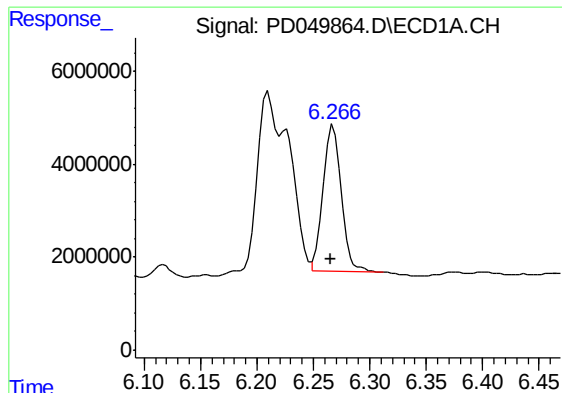

#26 Chlordane-4


R.T.: 6.268 min
Delta R.T.: 0.002 min
Response: 35102025
Conc: 489.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD101818CHLOR

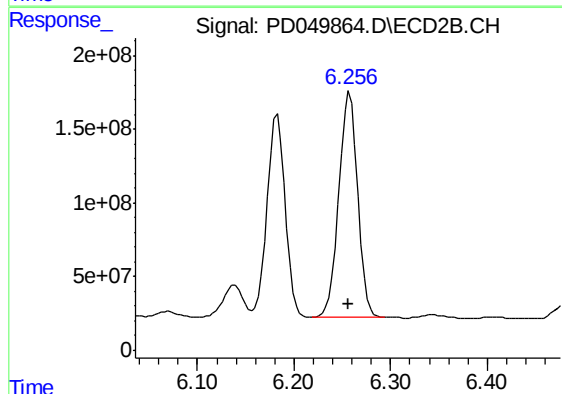


#26 Chlordane-4

R.T.: 6.257 min
Delta R.T.: 0.000 min
Response: 2023745921
Conc: 493.93 ng/ml

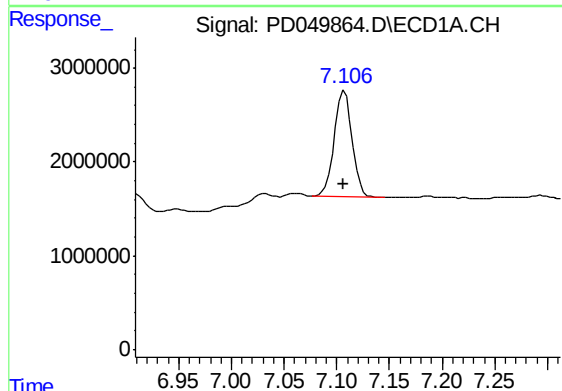


#27 Chlordane-5

R.T.: 7.108 min
Delta R.T.: 0.001 min
Response: 13310060
Conc: 483.38 ng/ml

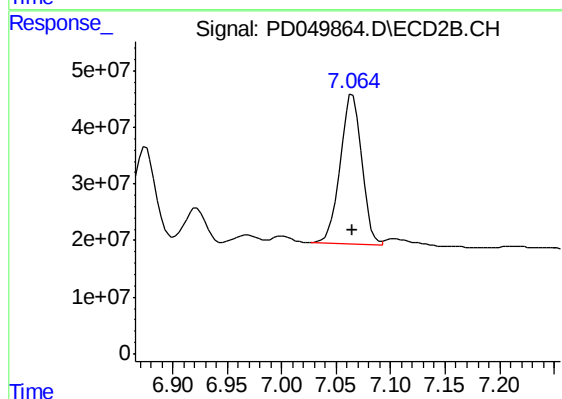

#27 Chlordane-5


R.T.: 7.065 min
Delta R.T.: 0.000 min
Response: 363385556
Conc: 511.75 ng/ml

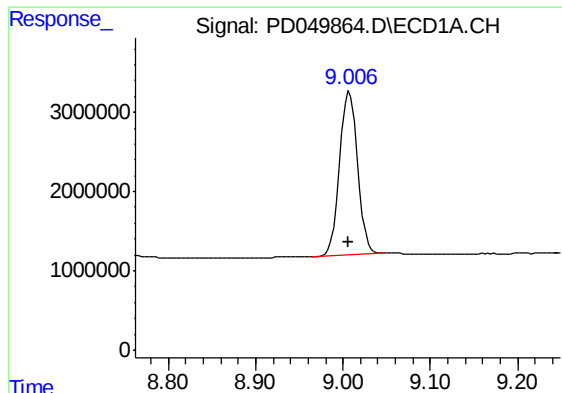

#28 Decachlorobiphenyl

R.T.: 9.008 min
Delta R.T.: 0.000 min
Response: 29494199
Conc: 48.39 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD101818CHLOR

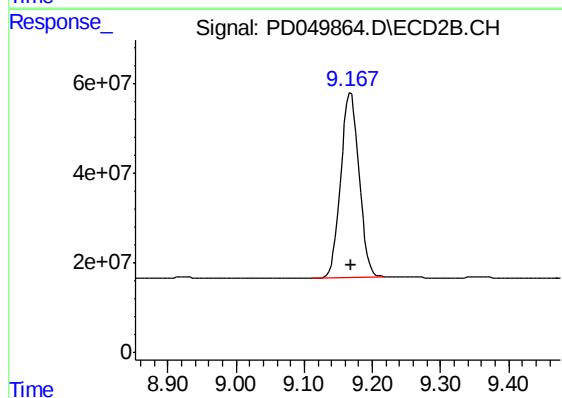

#28 Decachlorobiphenyl

R.T.: 9.168 min
Delta R.T.: 0.000 min
Response: 767213188
Conc: 48.39 ng/ml