

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101819\
 Data File : PD055376.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2019 10:28
 Operator : SG\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA101

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 12:00:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 11:58:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.290	3.963	4489821	6973149	5.019	5.164
27)	SA Decachlor...	7.969	8.999	9708076	13629341	10.605	10.362
Target Compounds							
2)	A alpha-BHC	3.717	4.349	5855842	9436093	4.675	4.872
3)	MA gamma-BHC...	3.993	4.632	5777479	8938537	4.910	4.846
4)	MA Heptachlor	4.279	5.139	4390755	9333729	4.846	5.028
9)	A Endosulfan I	5.286	6.181	4673316	8297605	4.863	5.055
13)	MA Dieldrin	5.526	6.437	10481147	17587053	9.448	9.704
14)	MA Endrin	5.780	6.654	8601675	13653658	9.563	9.784
16)	A 4,4'-DDD	5.914	6.776	7590069	13857746	9.084	9.657
17)	MA 4,4'-DDT	6.150	7.074	5304732	12155045	7.677	8.884
20)	A Methoxychlor	6.699	7.530	17771698	39528303	48.077	50.572


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101819\
Data File : PD055376.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2019 10:28
Operator : SG\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 12:00:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 11:58:59 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

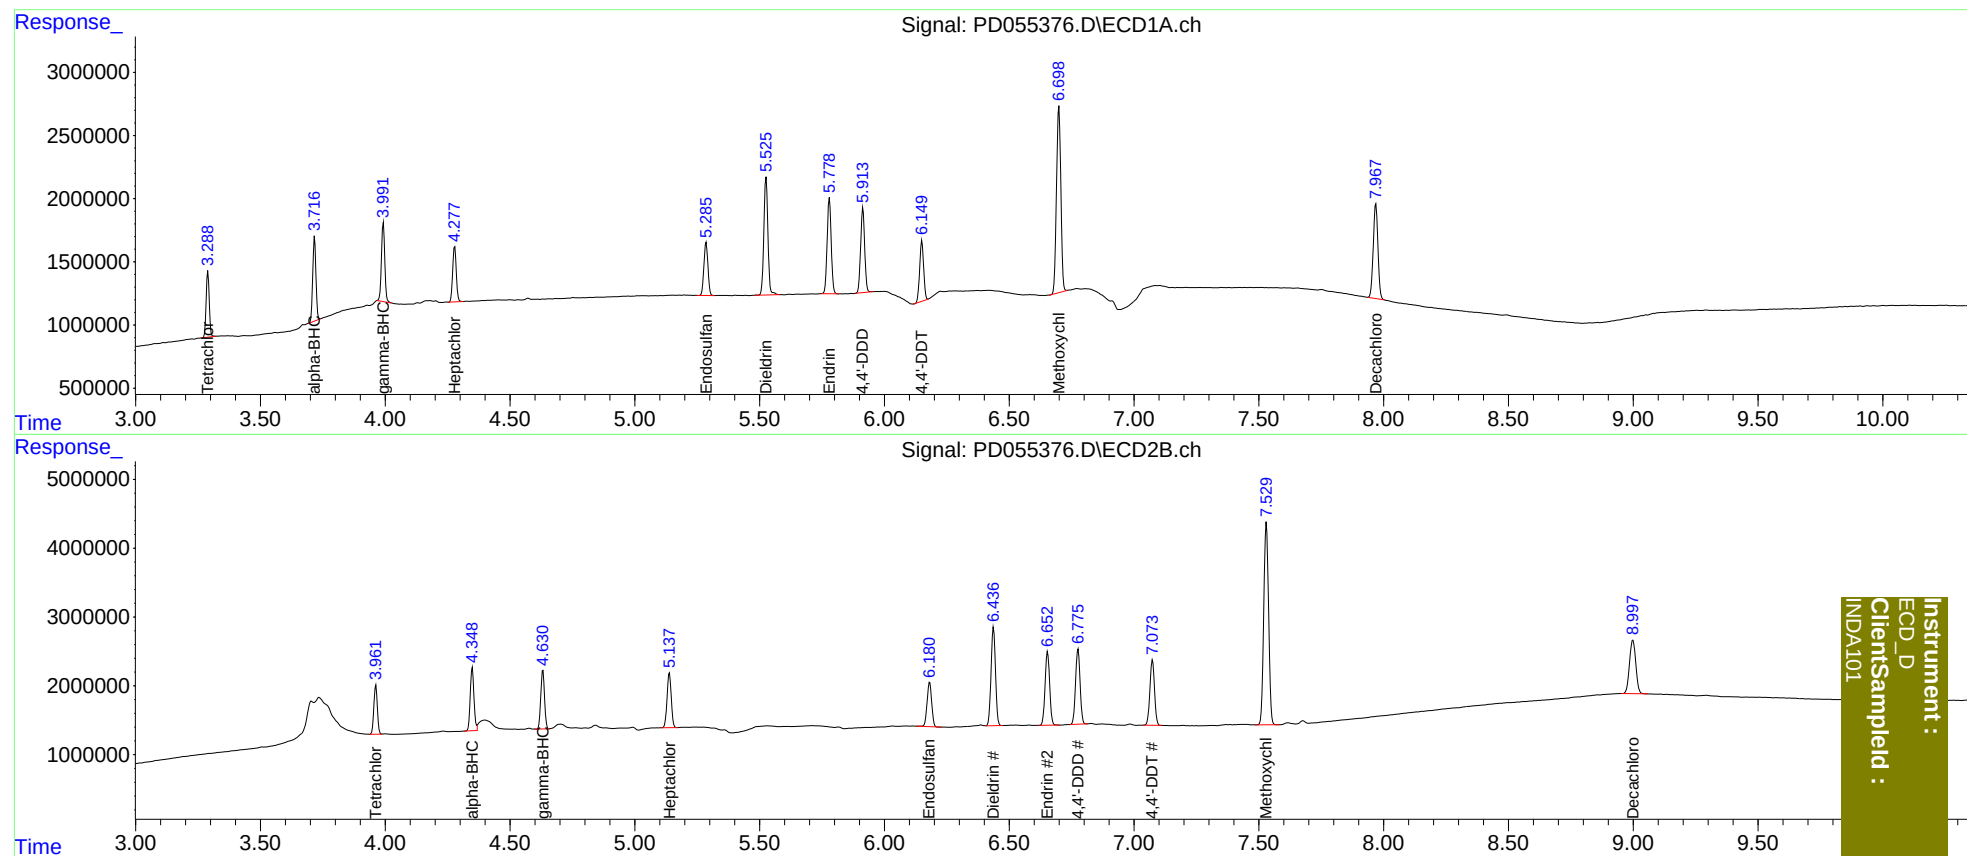


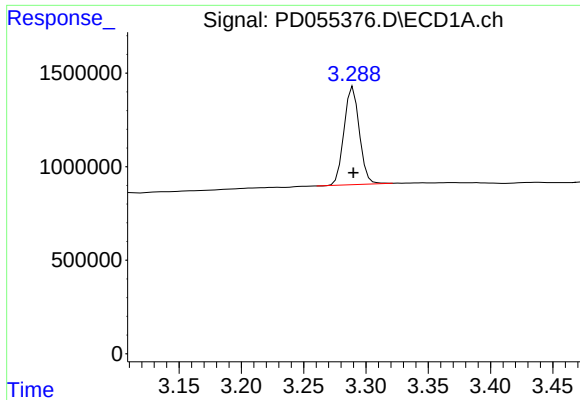

#1 Tetrachloro-m-xylene


R.T.: 3.290 min
Delta R.T.: 0.000 min
Response: 4489821
Conc: 5.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA101

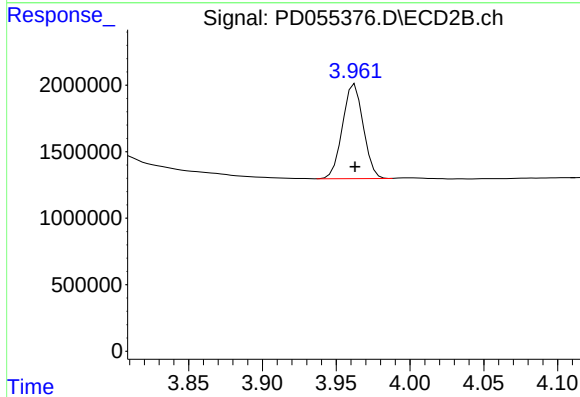


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: 0.000 min
Response: 6973149
Conc: 5.16 ng/ml

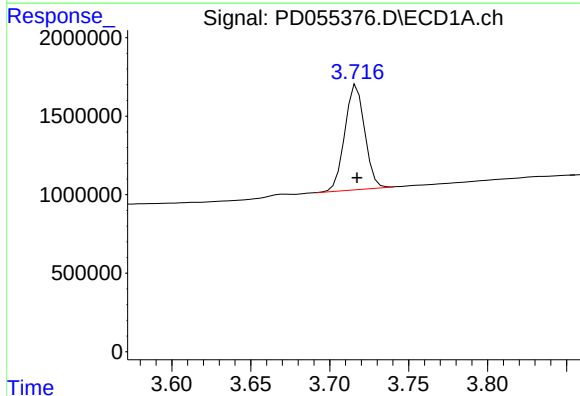


#2 alpha-BHC

R.T.: 3.717 min
Delta R.T.: 0.000 min
Response: 5855842
Conc: 4.67 ng/ml

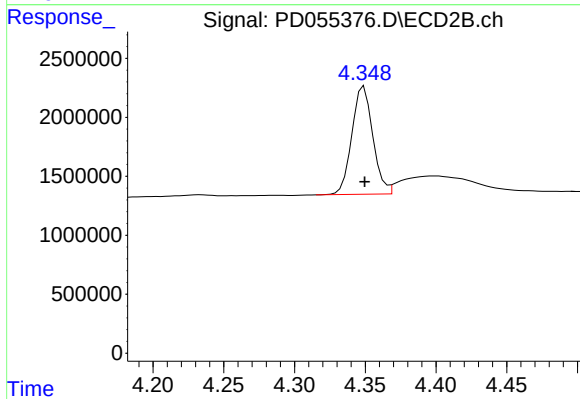

#2 alpha-BHC


R.T.: 4.349 min
Delta R.T.: 0.000 min
Response: 9436093
Conc: 4.87 ng/ml

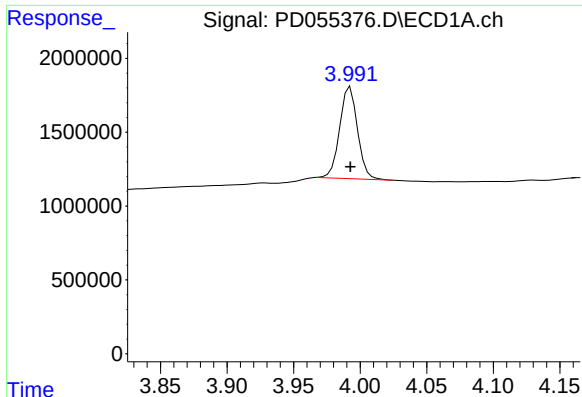

#3 gamma-BHC (Lindane)


R.T.: 3.993 min
Delta R.T.: 0.000 min
Response: 5777479
Conc: 4.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA101

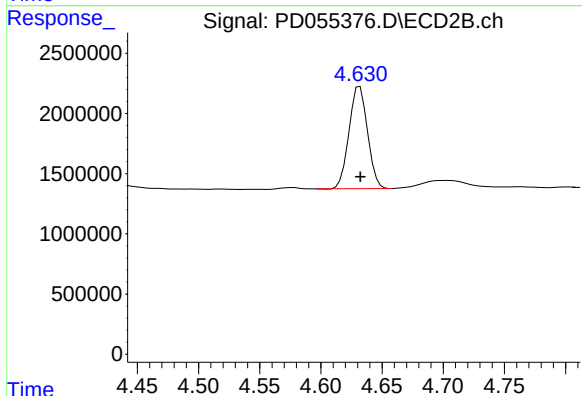


#3 gamma-BHC (Lindane)

R.T.: 4.632 min
Delta R.T.: 0.000 min
Response: 8938537
Conc: 4.85 ng/ml

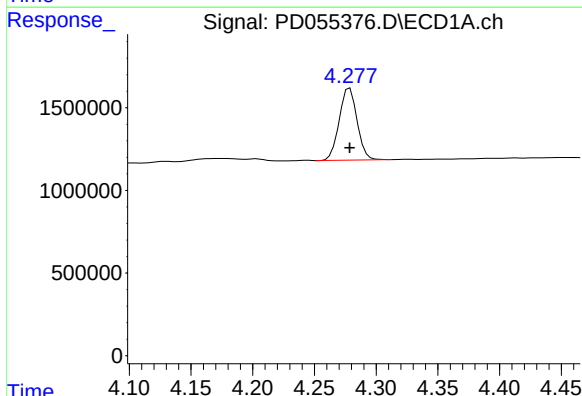


#4 Heptachlor

R.T.: 4.279 min
Delta R.T.: 0.000 min
Response: 4390755
Conc: 4.85 ng/ml

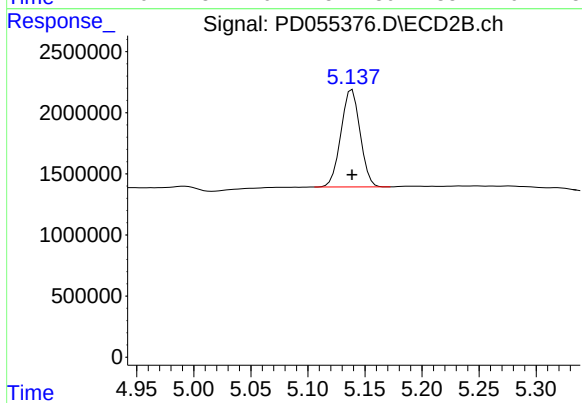

#4 Heptachlor


R.T.: 5.139 min
Delta R.T.: 0.000 min
Response: 9333729
Conc: 5.03 ng/ml

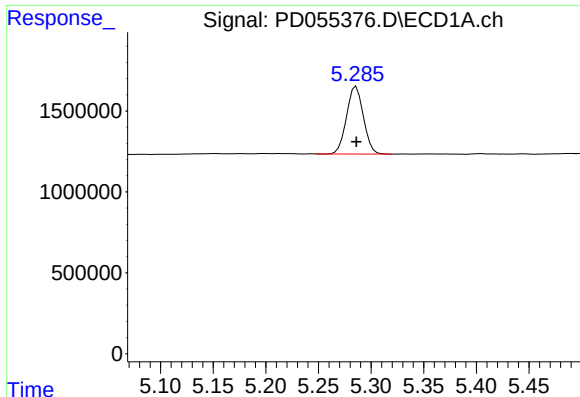

#9 Endosulfan I


R.T.: 5.286 min
Delta R.T.: 0.000 min
Response: 4673316
Conc: 4.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA101

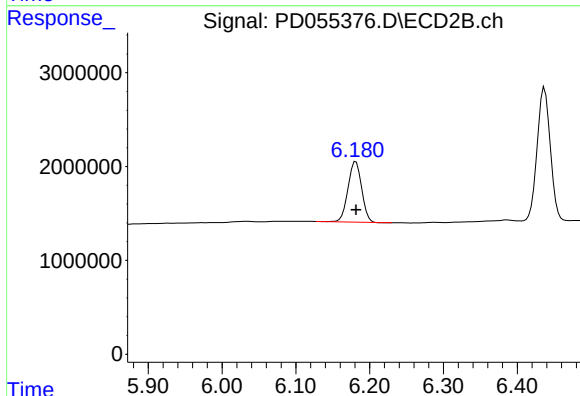


#9 Endosulfan I

R.T.: 6.181 min
Delta R.T.: 0.000 min
Response: 8297605
Conc: 5.06 ng/ml

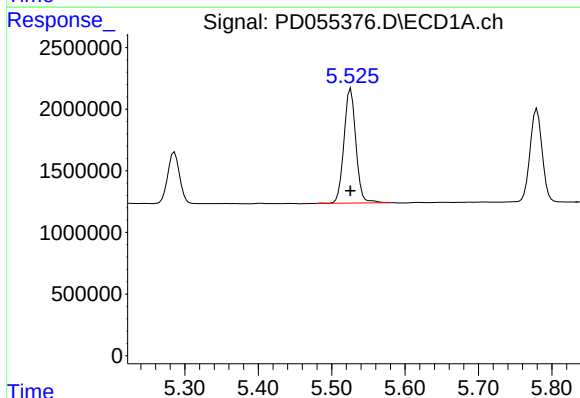


#13 Dieldrin

R.T.: 5.526 min
Delta R.T.: 0.000 min
Response: 10481147
Conc: 9.45 ng/ml

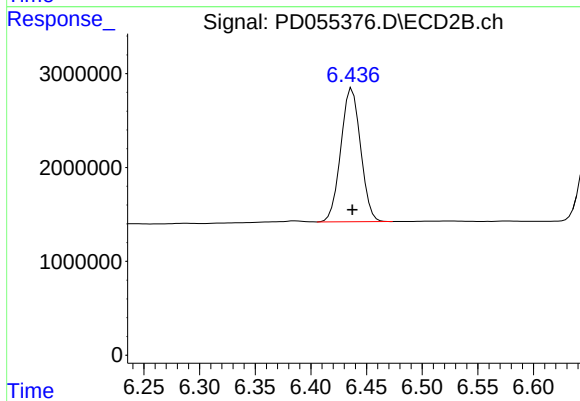

#13 Dieldrin


R.T.: 6.437 min
Delta R.T.: 0.000 min
Response: 17587053
Conc: 9.70 ng/ml

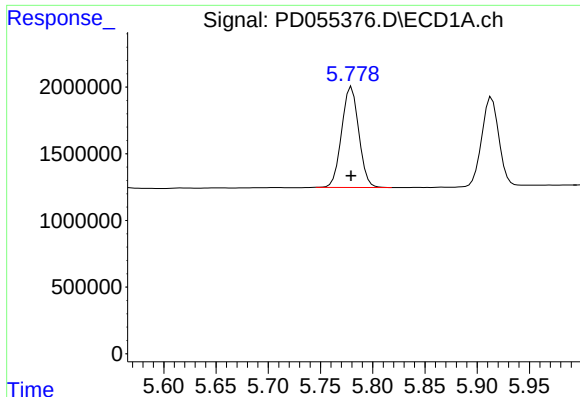

#14 Endrin


R.T.: 5.780 min
Delta R.T.: 0.000 min
Response: 8601675
Conc: 9.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA101

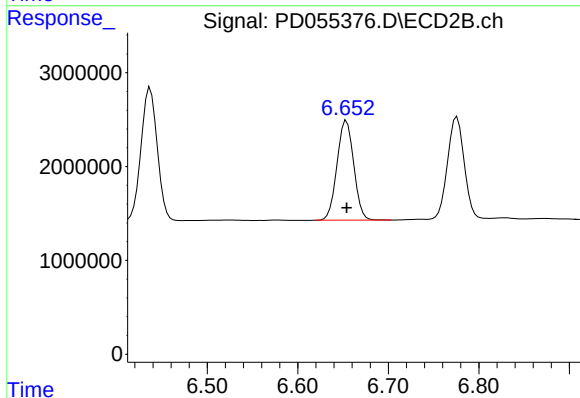


#14 Endrin

R.T.: 6.654 min
Delta R.T.: 0.000 min
Response: 13653658
Conc: 9.78 ng/ml

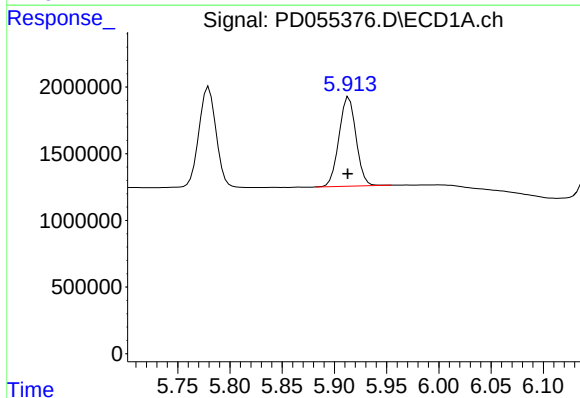


#16 4,4'-DDD

R.T.: 5.914 min
Delta R.T.: 0.001 min
Response: 7590069
Conc: 9.08 ng/ml

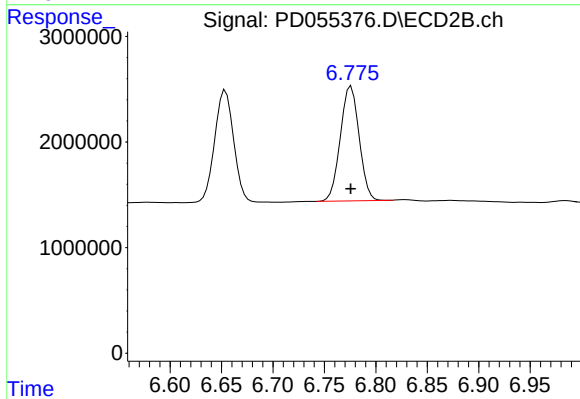

#16 4,4'-DDD


R.T.: 6.776 min
Delta R.T.: 0.000 min
Response: 13857746
Conc: 9.66 ng/ml

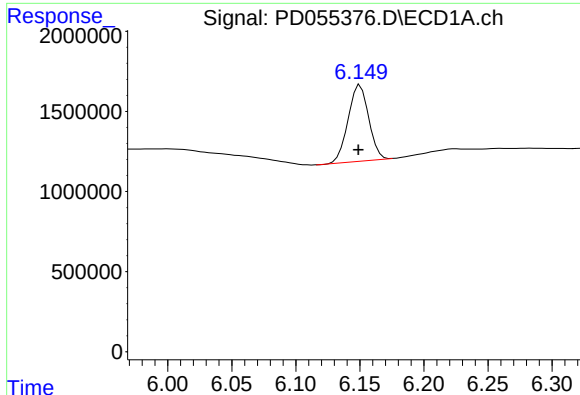

#17 4,4'-DDT


R.T.: 6.150 min
Delta R.T.: 0.001 min
Response: 5304732
Conc: 7.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA101

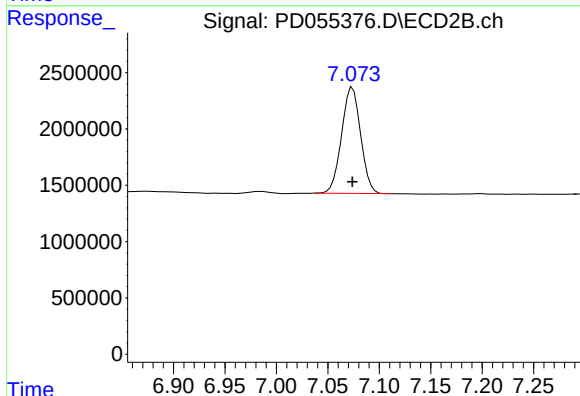


#17 4,4'-DDT

R.T.: 7.074 min
Delta R.T.: 0.000 min
Response: 12155045
Conc: 8.88 ng/ml

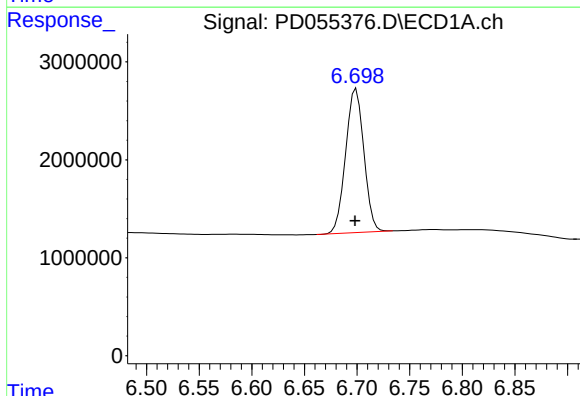


#20 Methoxychlor

R.T.: 6.699 min
Delta R.T.: 0.001 min
Response: 17771698
Conc: 48.08 ng/ml

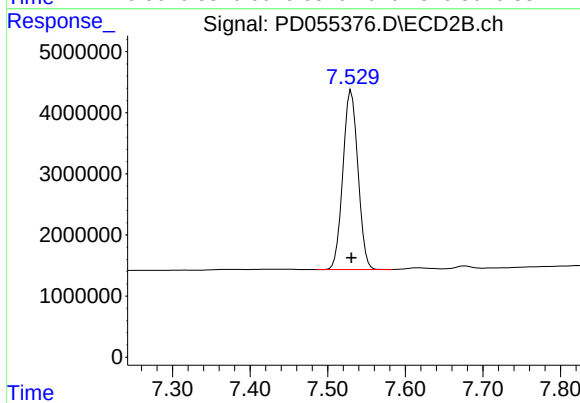

#20 Methoxychlor


R.T.: 7.530 min
Delta R.T.: 0.000 min
Response: 39528303
Conc: 50.57 ng/ml

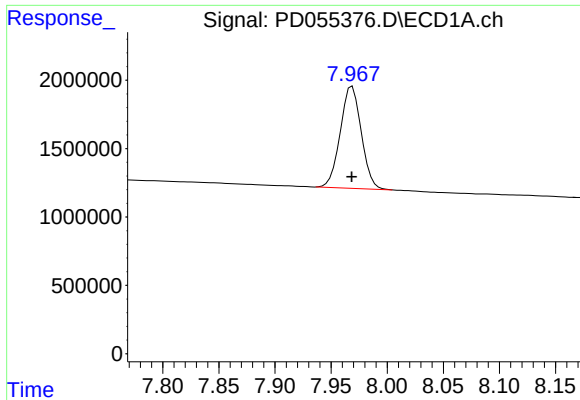

#27 Decachlorobiphenyl

R.T.: 7.969 min
Delta R.T.: 0.000 min
Response: 9708076
Conc: 10.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA101

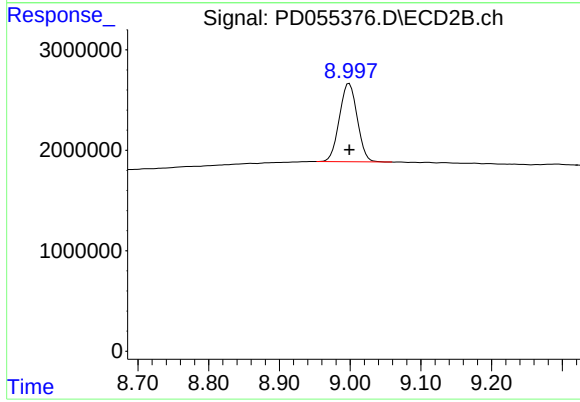

#27 Decachlorobiphenyl

R.T.: 8.999 min
Delta R.T.: 0.000 min
Response: 13629341
Conc: 10.36 ng/ml