

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101819\
 Data File : PD055382.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2019 11:52
 Operator : SG\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA401

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 12:05:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 12:01:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.290	3.963	35636589	53442427	39.534	38.931
27)	SA Decachlor...	7.968	8.999	71183297	102.1E6	75.140	75.684
Target Compounds							
2)	A alpha-BHC	3.717	4.350	52467333	80102646	43.172	41.897
3)	MA gamma-BHC...	3.992	4.632	48476742	75617516	41.456	41.545
4)	MA Heptachlor	4.278	5.138	37164856	75275678	41.302	40.341
9)	A Endosulfan I	5.286	6.181	39146941	65563748	41.010	39.559
13)	MA Dieldrin	5.526	6.437	91930221	148.3E6	84.801	82.744
14)	MA Endrin	5.779	6.653	73549638	113.9E6	83.173	82.103
16)	A 4,4'-DDD	5.913	6.776	66602941	117.2E6	83.584	82.705
17)	MA 4,4'-DDT	6.150	7.074	60562910	115.3E6	98.277	88.811
20)	A Methoxychlor	6.698	7.530	148.5E6	305.9E6	406.409	386.485


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101819\
Data File : PD055382.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2019 11:52
Operator : SG\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 12:05:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 12:01:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

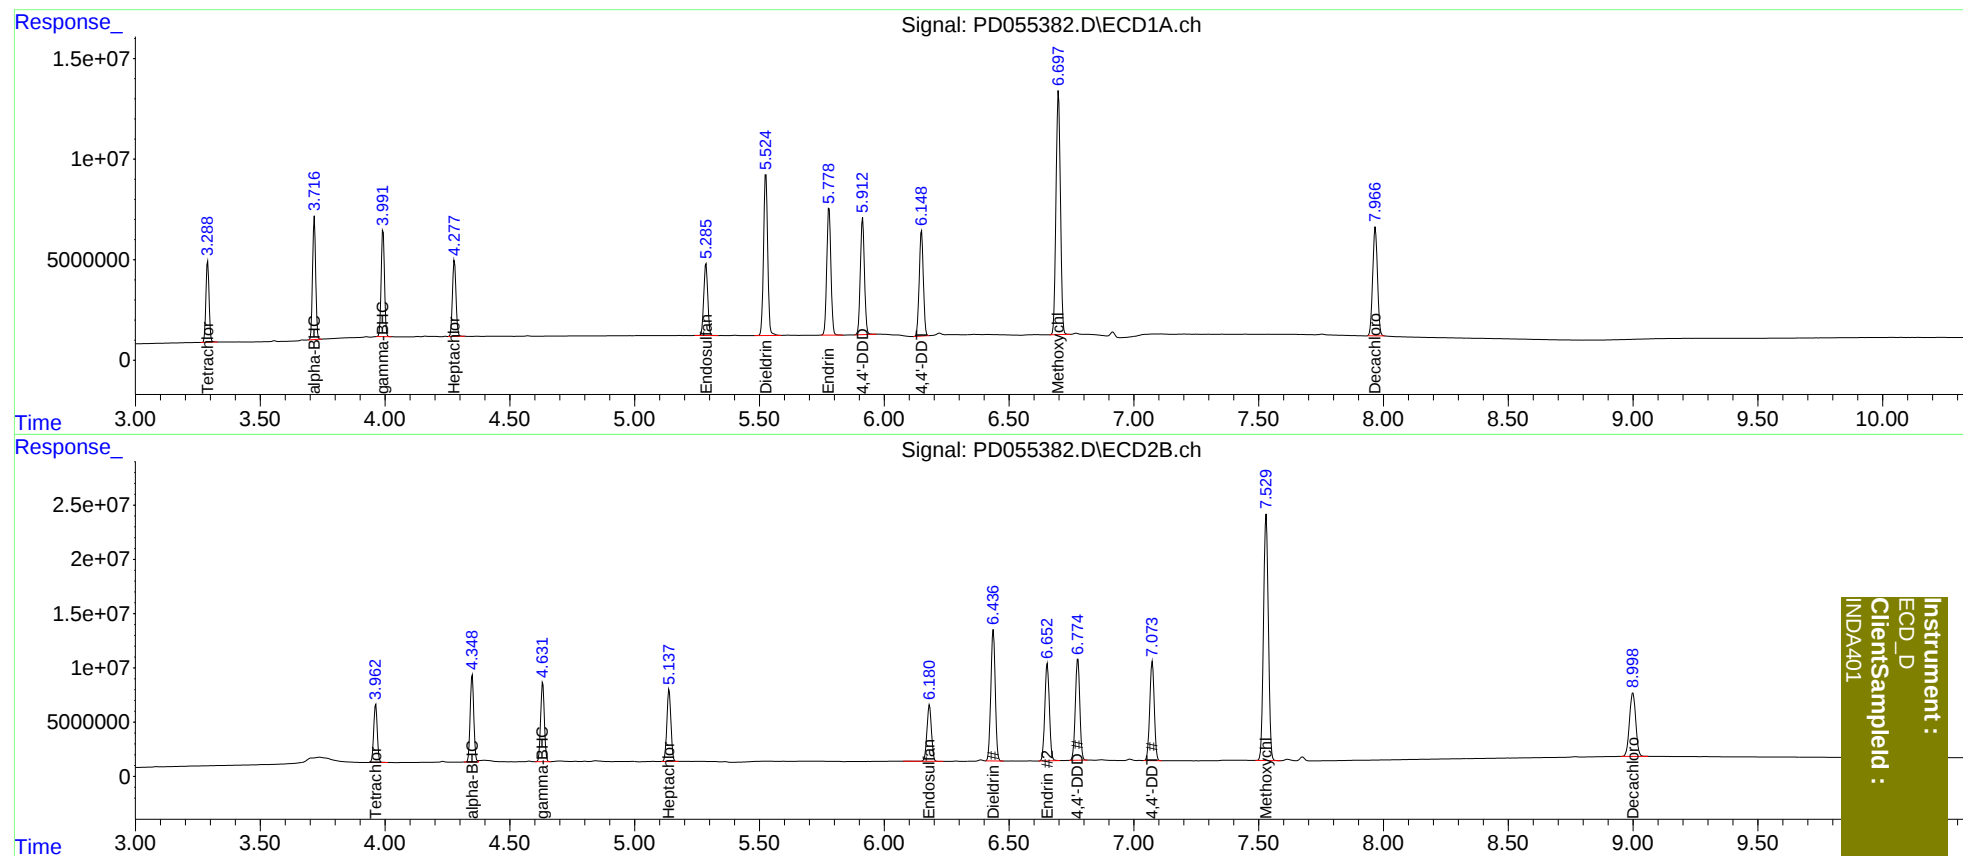


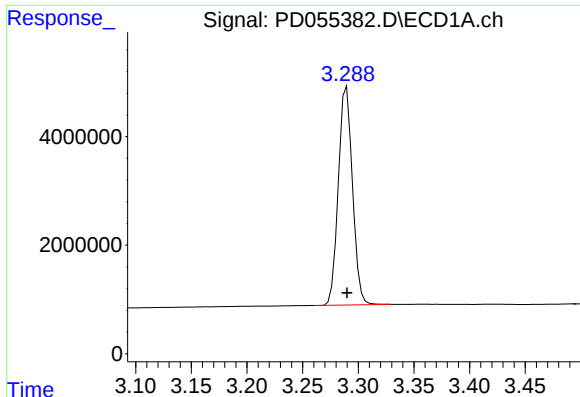

#1 Tetrachloro-m-xylene


R.T.: 3.290 min
Delta R.T.: 0.000 min
Response: 35636589
Conc: 39.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

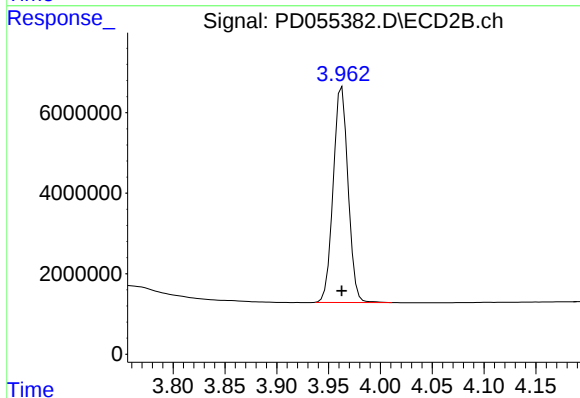


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: 0.000 min
Response: 53442427
Conc: 38.93 ng/ml

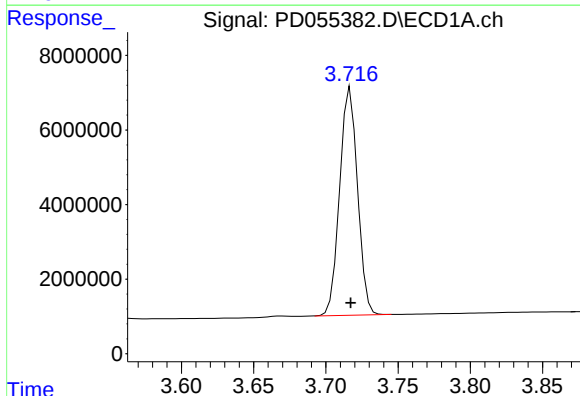


#2 alpha-BHC

R.T.: 3.717 min
Delta R.T.: 0.000 min
Response: 52467333
Conc: 43.17 ng/ml

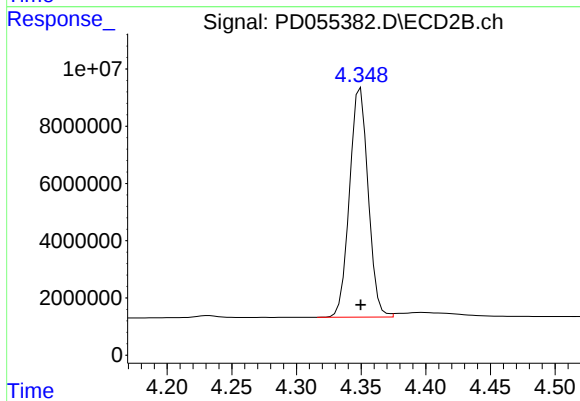

#2 alpha-BHC


R.T.: 4.350 min
Delta R.T.: 0.000 min
Response: 80102646
Conc: 41.90 ng/ml

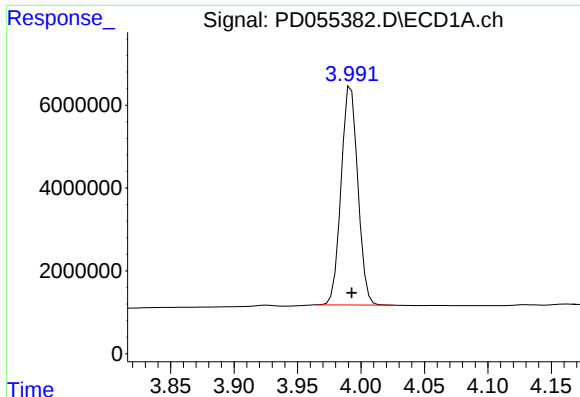

#3 gamma-BHC (Lindane)


R.T.: 3.992 min
Delta R.T.: 0.000 min
Response: 48476742
Conc: 41.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

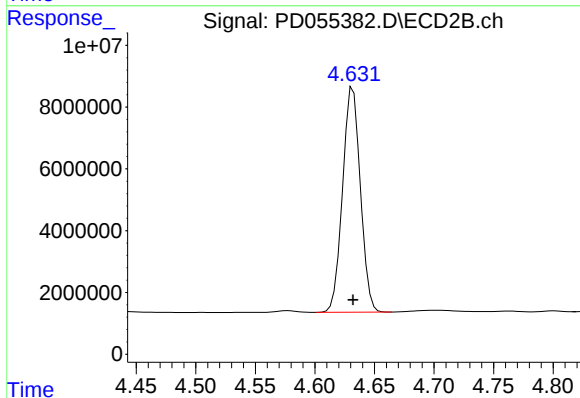


#3 gamma-BHC (Lindane)

R.T.: 4.632 min
Delta R.T.: 0.000 min
Response: 75617516
Conc: 41.55 ng/ml

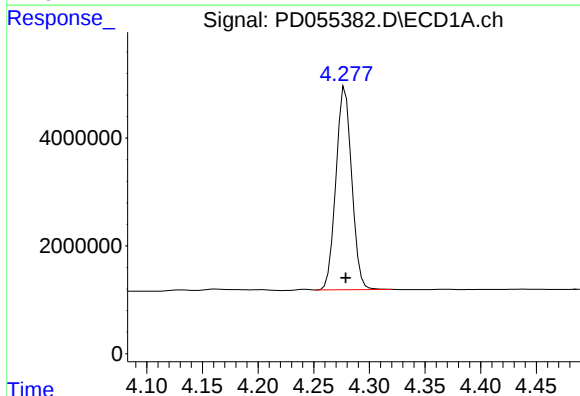


#4 Heptachlor

R.T.: 4.278 min
Delta R.T.: 0.000 min
Response: 37164856
Conc: 41.30 ng/ml

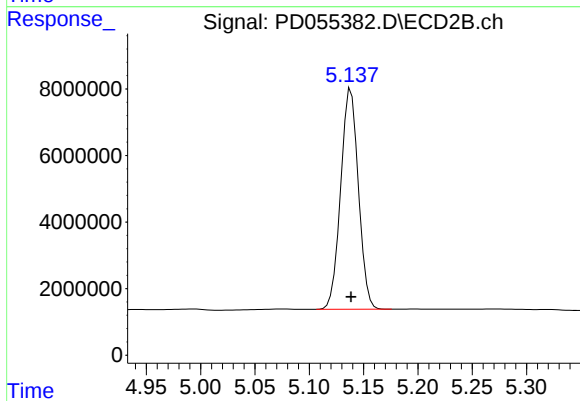

#4 Heptachlor


R.T.: 5.138 min
Delta R.T.: 0.000 min
Response: 75275678
Conc: 40.34 ng/ml

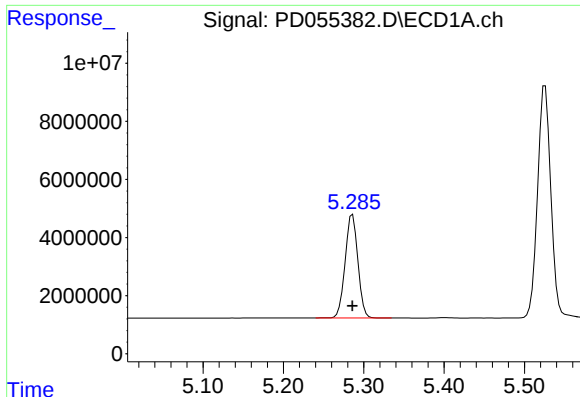

#9 Endosulfan I


R.T.: 5.286 min
Delta R.T.: 0.000 min
Response: 39146941
Conc: 41.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

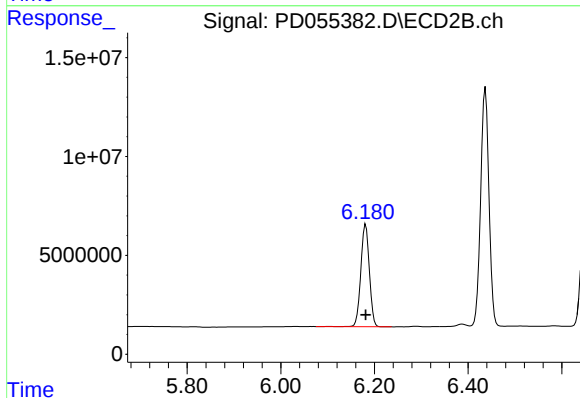


#9 Endosulfan I

R.T.: 6.181 min
Delta R.T.: 0.000 min
Response: 65563748
Conc: 39.56 ng/ml

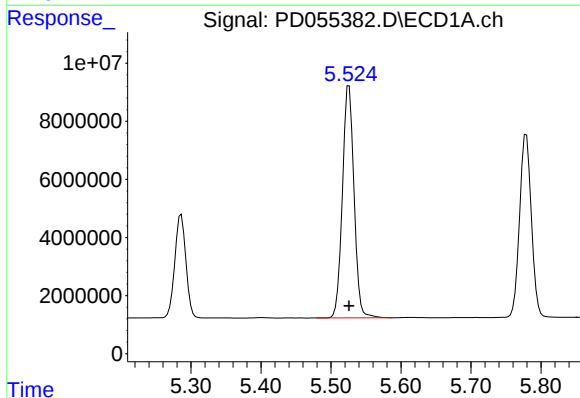


#13 Dieldrin

R.T.: 5.526 min
Delta R.T.: 0.000 min
Response: 91930221
Conc: 84.80 ng/ml

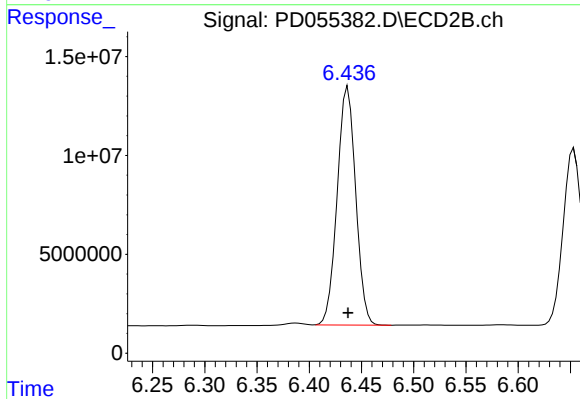

#13 Dieldrin


R.T.: 6.437 min
Delta R.T.: 0.000 min
Response: 148311228
Conc: 82.74 ng/ml

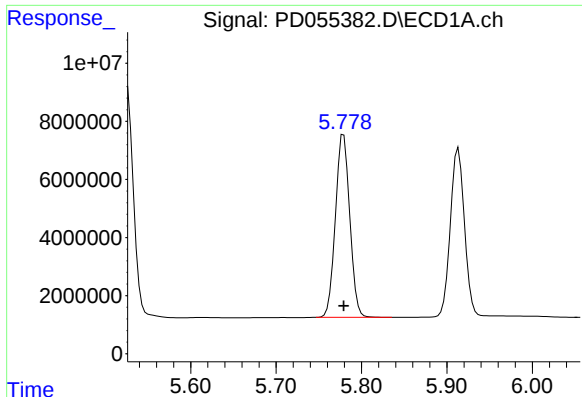

#14 Endrin


R.T.: 5.779 min
Delta R.T.: 0.000 min
Response: 73549638
Conc: 83.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

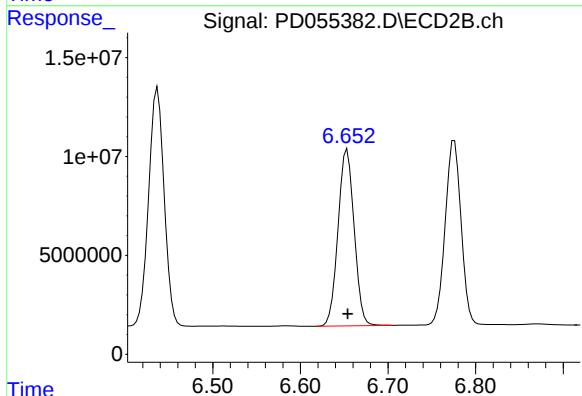


#14 Endrin

R.T.: 6.653 min
Delta R.T.: 0.000 min
Response: 113919255
Conc: 82.10 ng/ml

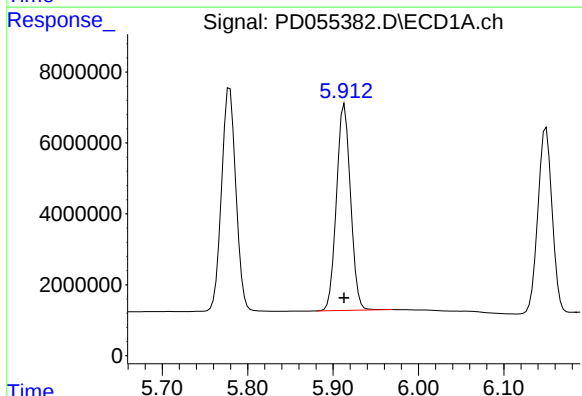


#16 4,4'-DDD

R.T.: 5.913 min
Delta R.T.: 0.000 min
Response: 66602941
Conc: 83.58 ng/ml

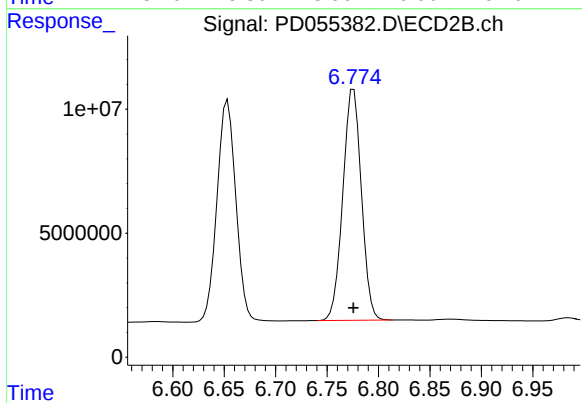

#16 4,4'-DDD


R.T.: 6.776 min
Delta R.T.: 0.000 min
Response: 117236356
Conc: 82.71 ng/ml

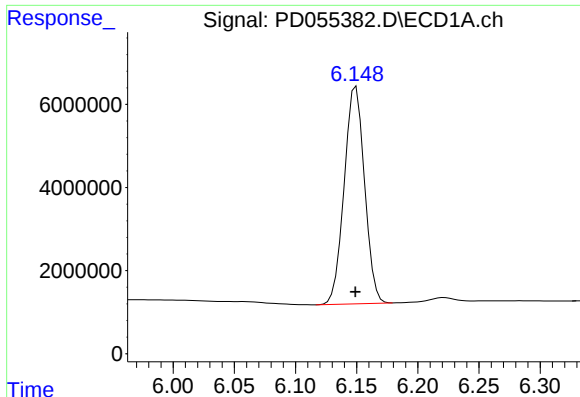

#17 4,4'-DDT


R.T.: 6.150 min
Delta R.T.: 0.000 min
Response: 60562910
Conc: 98.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

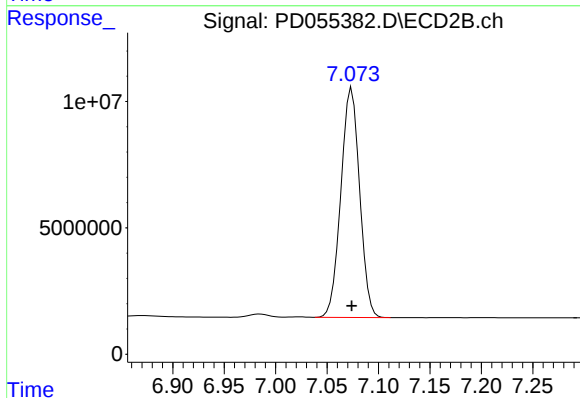


#17 4,4'-DDT

R.T.: 7.074 min
Delta R.T.: 0.000 min
Response: 115269496
Conc: 88.81 ng/ml

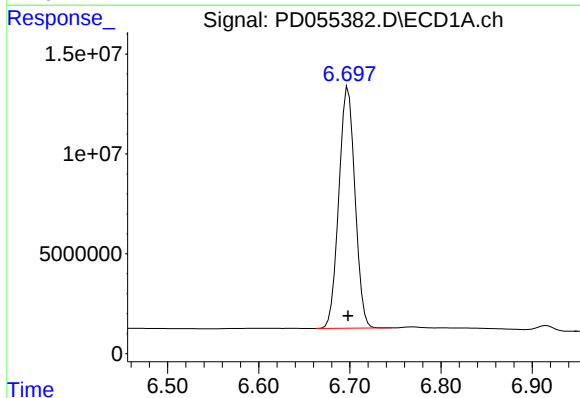


#20 Methoxychlor

R.T.: 6.698 min
Delta R.T.: 0.000 min
Response: 148509535
Conc: 406.41 ng/ml

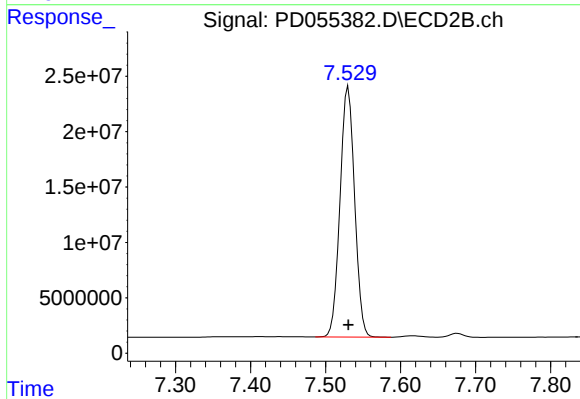

#20 Methoxychlor


R.T.: 7.530 min
Delta R.T.: 0.000 min
Response: 305850571
Conc: 386.49 ng/ml

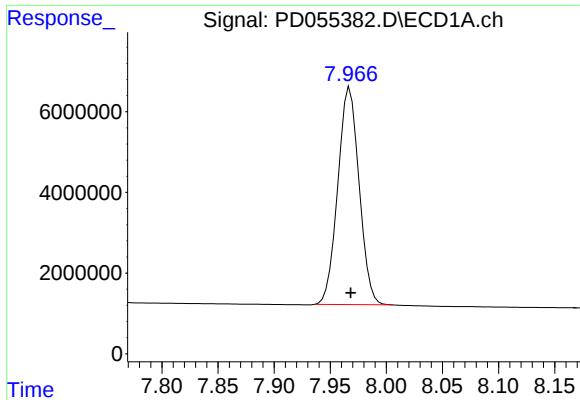

#27 Decachlorobiphenyl

R.T.: 7.968 min
Delta R.T.: 0.000 min
Response: 71183297
Conc: 75.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

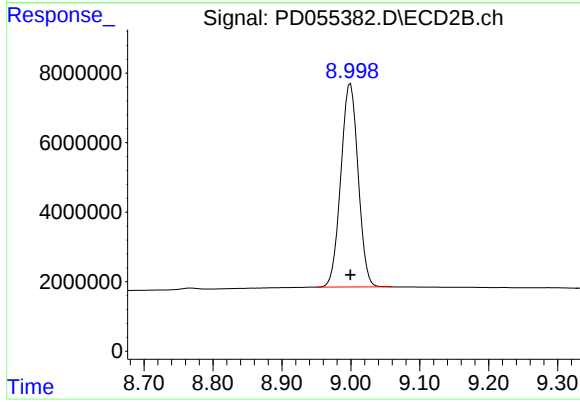

#27 Decachlorobiphenyl

R.T.: 8.999 min
Delta R.T.: 0.000 min
Response: 102143155
Conc: 75.68 ng/ml