

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101819\
 Data File : PD055384.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2019 12:20
 Operator : SG\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA501

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 12:31:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 12:06:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.290	3.963	69019145	102.2E6	76.791	74.946
27)	SA Decachlor...	7.967	8.998	135.4E6	191.7E6	145.184	144.015
Target Compounds							
2)	A alpha-BHC	3.717	4.349	105.7E6	159.1E6	85.305	82.247
3)	MA gamma-BHC...	3.992	4.632	96405329	149.5E6	81.700	81.359
4)	MA Heptachlor	4.278	5.139	73693293	147.5E6	81.236	78.906
9)	A Endosulfan I	5.286	6.181	77084774	126.7E6	80.247	76.665
13)	MA Dieldrin	5.526	6.437	182.4E6	290.9E6	165.748	160.910
14)	MA Endrin	5.779	6.654	145.0E6	223.6E6	162.369	160.088
16)	A 4,4'-DDD	5.913	6.776	132.7E6	229.6E6	164.676	160.624
17)	MA 4,4'-DDT	6.149	7.074	125.5E6	230.8E6	192.602	173.057
20)	A Methoxychlor	6.698	7.531	284.7E6	572.7E6	775.869	729.908


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101819\
Data File : PD055384.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2019 12:20
Operator : SG\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 12:31:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 12:06:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

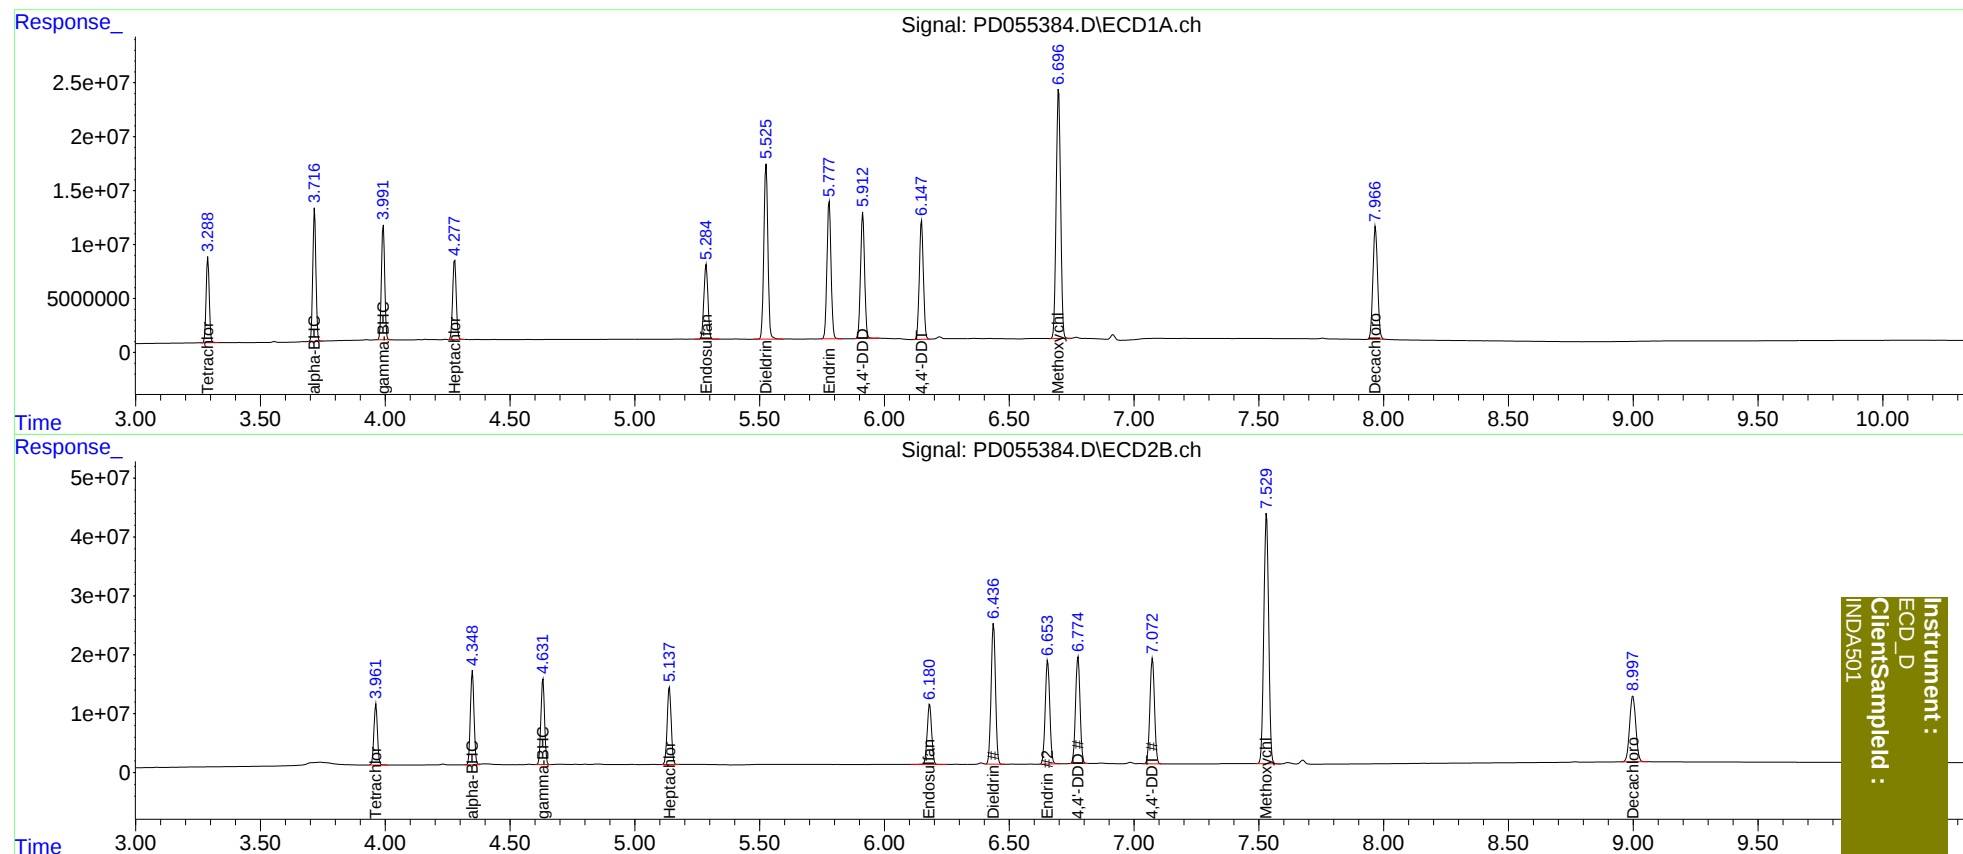


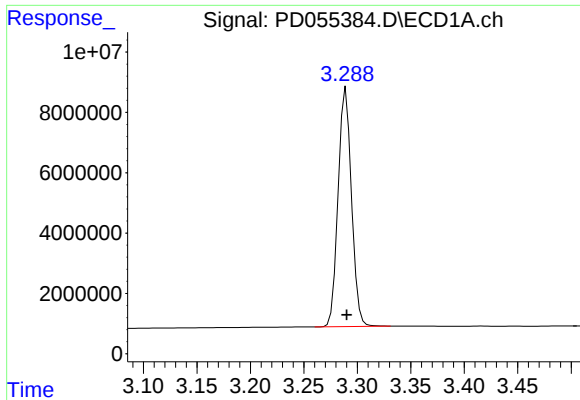

#1 Tetrachloro-m-xylene


R.T.: 3.290 min
Delta R.T.: 0.000 min
Response: 69019145
Conc: 76.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

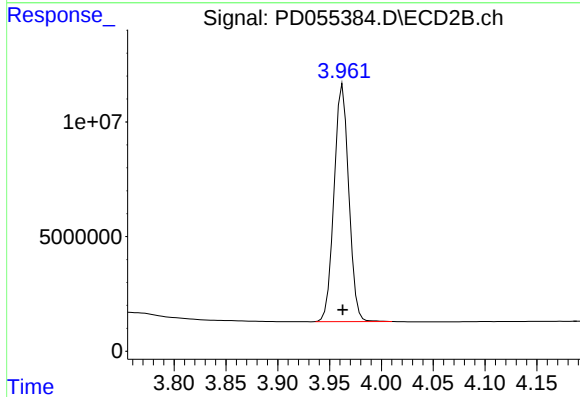


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: 0.000 min
Response: 102194954
Conc: 74.95 ng/ml

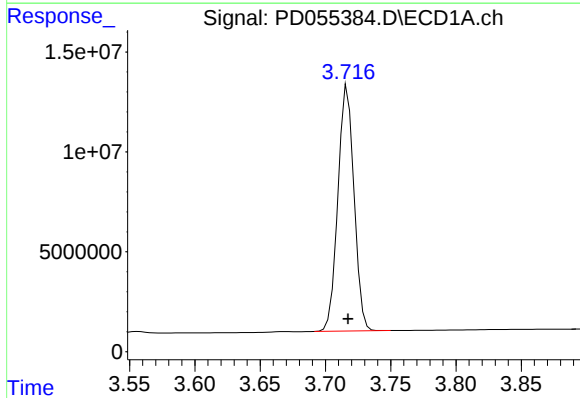


#2 alpha-BHC

R.T.: 3.717 min
Delta R.T.: 0.000 min
Response: 105727669
Conc: 85.31 ng/ml

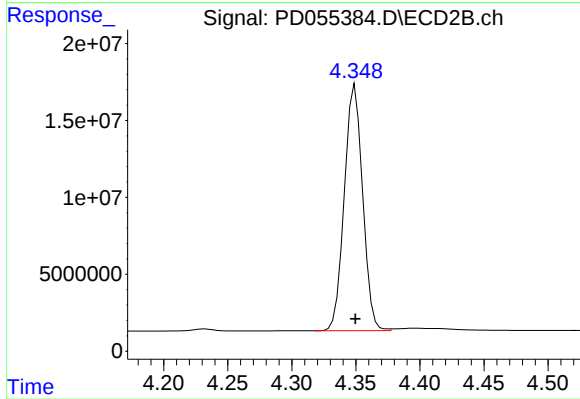

#2 alpha-BHC

R.T.: 4.349 min
Delta R.T.: 0.000 min
Response: 159113782
Conc: 82.25 ng/ml

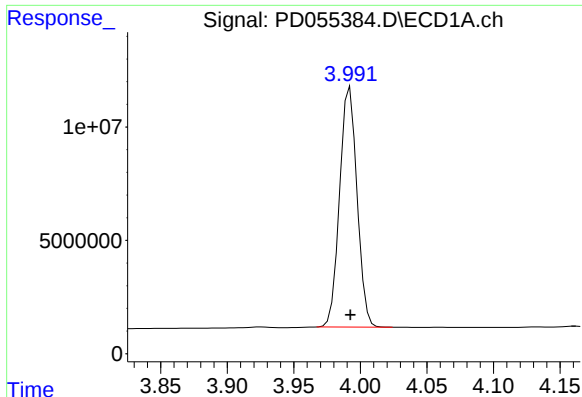

#3 gamma-BHC (Lindane)


R.T.: 3.992 min

Delta R.T.: 0.000 min

Response: 96405329

Conc: 81.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

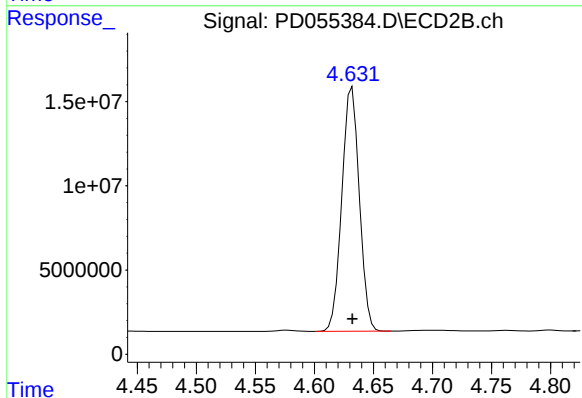


#3 gamma-BHC (Lindane)

R.T.: 4.632 min

Delta R.T.: 0.000 min

Response: 149512997

Conc: 81.36 ng/ml

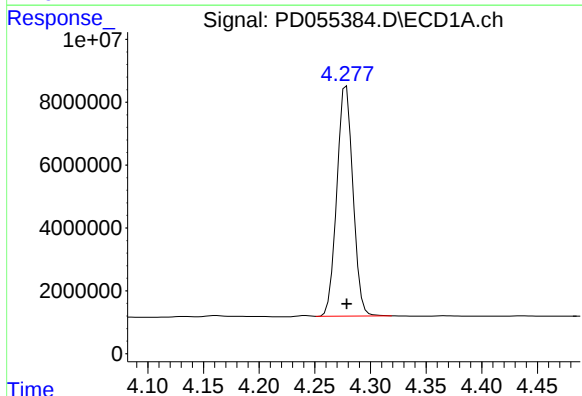


#4 Heptachlor

R.T.: 4.278 min

Delta R.T.: 0.000 min

Response: 73693293

Conc: 81.24 ng/ml

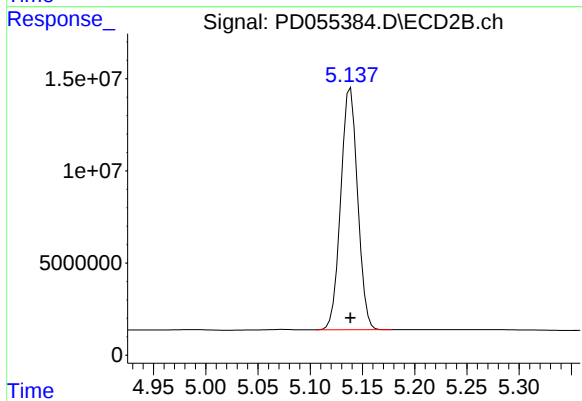


#4 Heptachlor

R.T.: 5.139 min

Delta R.T.: 0.000 min

Response: 147549295


Conc: 78.91 ng/ml

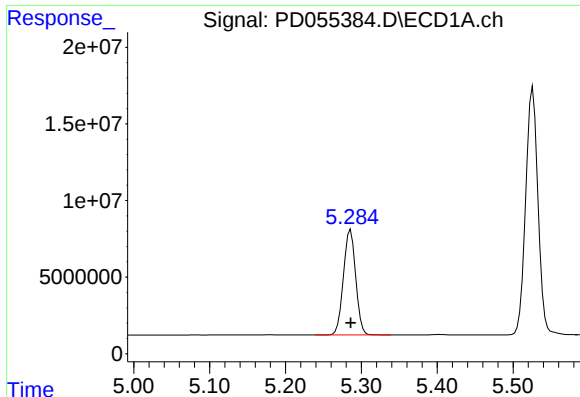

#9 Endosulfan I


R.T.: 5.286 min
Delta R.T.: 0.000 min
Response: 77084774
Conc: 80.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

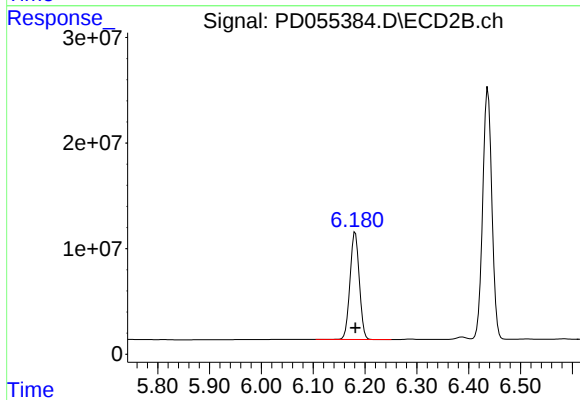


#9 Endosulfan I

R.T.: 6.181 min
Delta R.T.: 0.000 min
Response: 126712067
Conc: 76.66 ng/ml

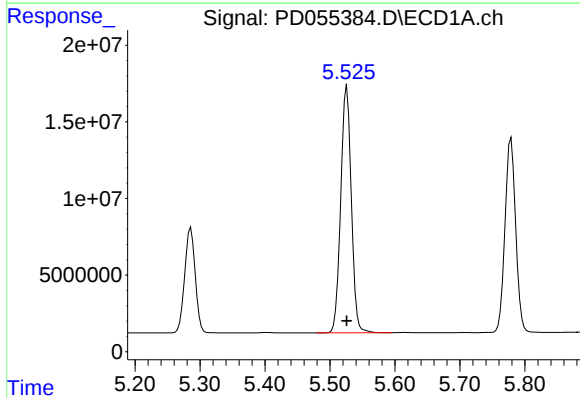


#13 Dieldrin

R.T.: 5.526 min
Delta R.T.: 0.000 min
Response: 182378679
Conc: 165.75 ng/ml

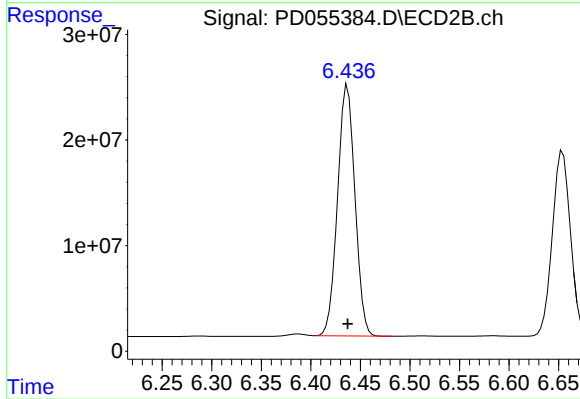

#13 Dieldrin


R.T.: 6.437 min
Delta R.T.: 0.000 min
Response: 290889608
Conc: 160.91 ng/ml

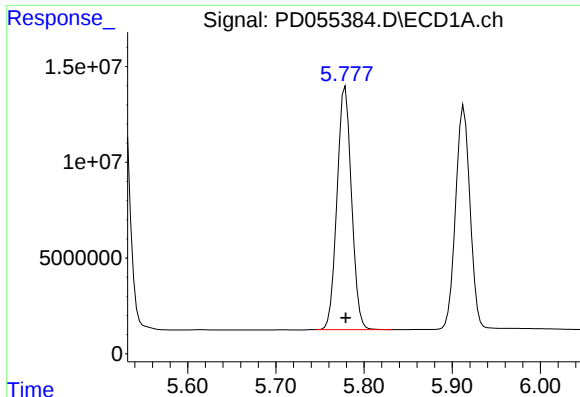

#14 Endrin


R.T.: 5.779 min
Delta R.T.: 0.000 min
Response: 145006299
Conc: 162.37 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

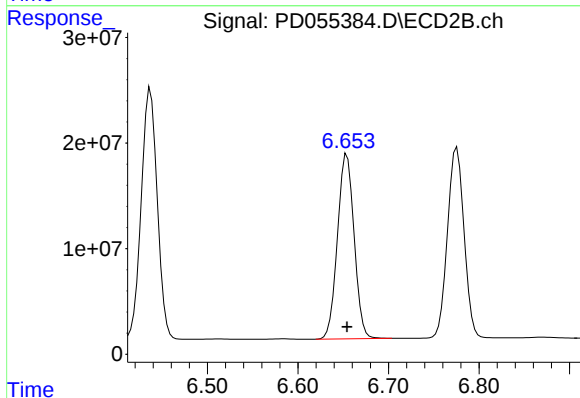


#14 Endrin

R.T.: 6.654 min
Delta R.T.: 0.000 min
Response: 223583786
Conc: 160.09 ng/ml

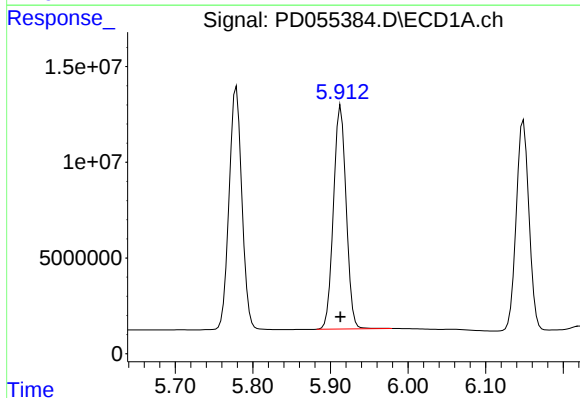


#16 4,4'-DDD

R.T.: 5.913 min
Delta R.T.: 0.000 min
Response: 132689678
Conc: 164.68 ng/ml

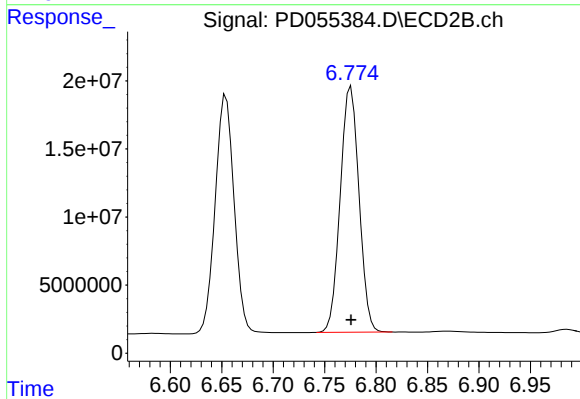

#16 4,4'-DDD


R.T.: 6.776 min
Delta R.T.: 0.000 min
Response: 229612096
Conc: 160.62 ng/ml

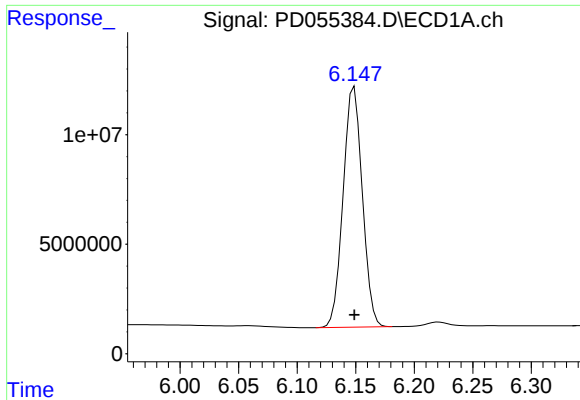

#17 4,4'-DDT


R.T.: 6.149 min
Delta R.T.: 0.000 min
Response: 125469324
Conc: 192.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

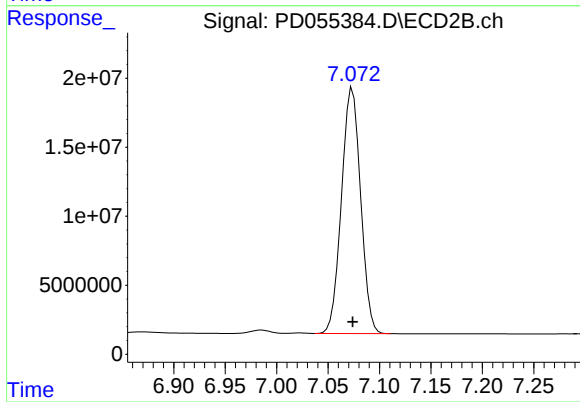


#17 4,4'-DDT

R.T.: 7.074 min
Delta R.T.: 0.000 min
Response: 230797460
Conc: 173.06 ng/ml

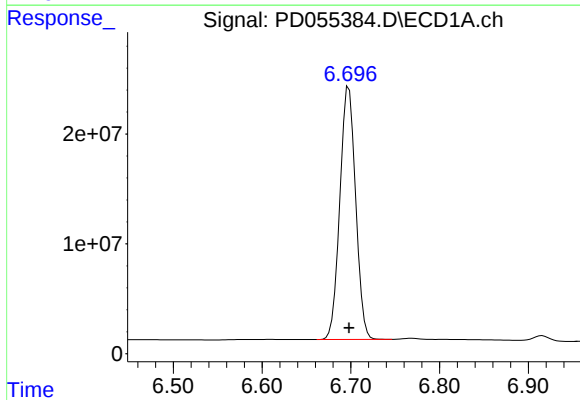


#20 Methoxychlor

R.T.: 6.698 min
Delta R.T.: 0.000 min
Response: 284652862
Conc: 775.87 ng/ml

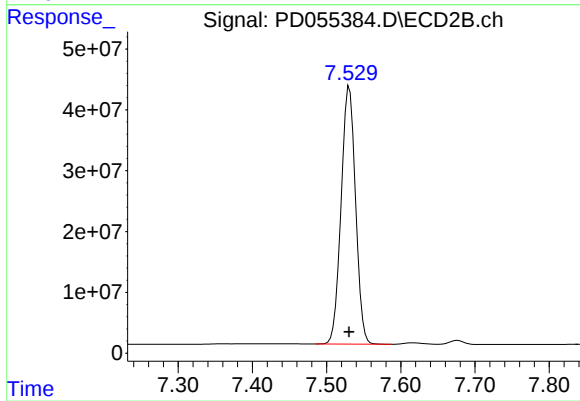

#20 Methoxychlor


R.T.: 7.531 min
Delta R.T.: 0.000 min
Response: 572744137
Conc: 729.91 ng/ml

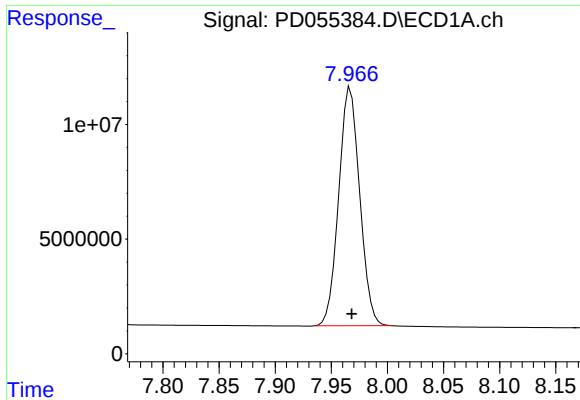

#27 Decachlorobiphenyl

R.T.: 7.967 min
Delta R.T.: -0.001 min
Response: 135449574
Conc: 145.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

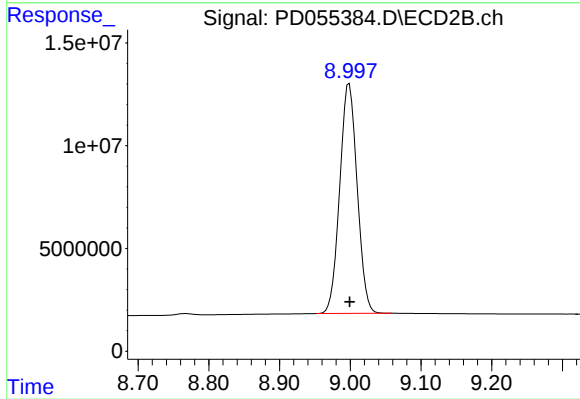

#27 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: 0.000 min
Response: 191741027
Conc: 144.01 ng/ml