

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101819\
 Data File : PD055408.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2019 18:28
 Operator : SG\AJ
 Sample : K5426-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 JLNK0

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 01:03:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 19 00:42:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.290	3.963	17222244	25058642	19.317	18.612
27)	SA Decachlor...	7.968	8.999	28739632	40932493	31.386	31.371
Target Compounds							
15)	B Endosulfa...	0.000	6.877	0	1835759	N.D.	1.181


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101819\
Data File : PD055408.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2019 18:28
Operator : SG\AJ
Sample : K5426-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
JLNK0

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 01:03:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
Quant Title : GC Extractables
QLast Update : Sat Oct 19 00:42:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

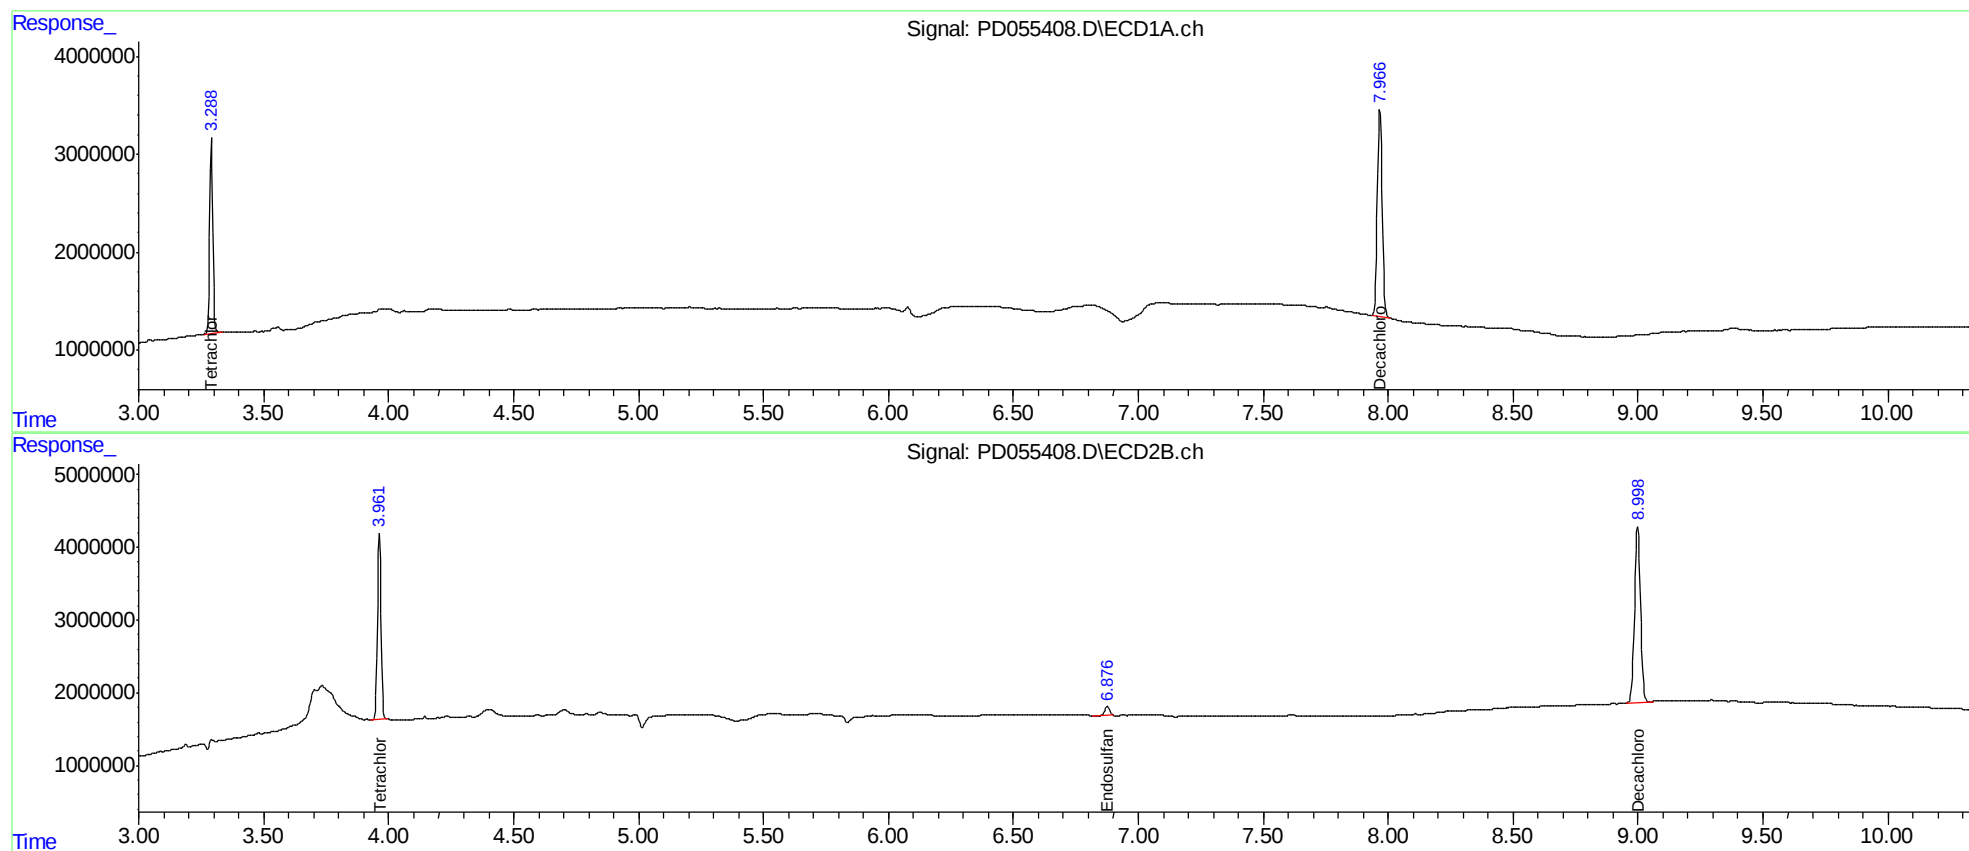


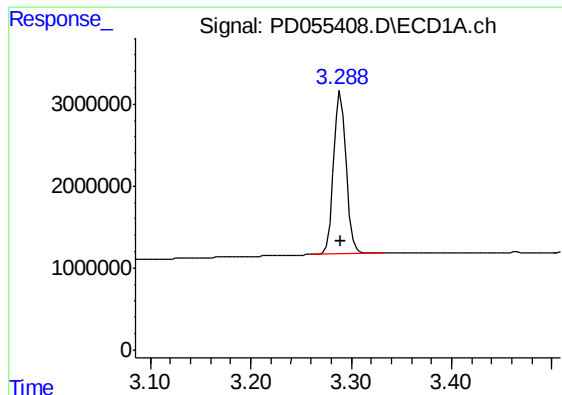

#1 Tetrachloro-m-xylene


R.T.: 3.290 min
Delta R.T.: 0.000 min
Response: 17222244
Conc: 19.32 ng/ml

Instrument :
ECD_D
ClientSampleId :
JLNK0

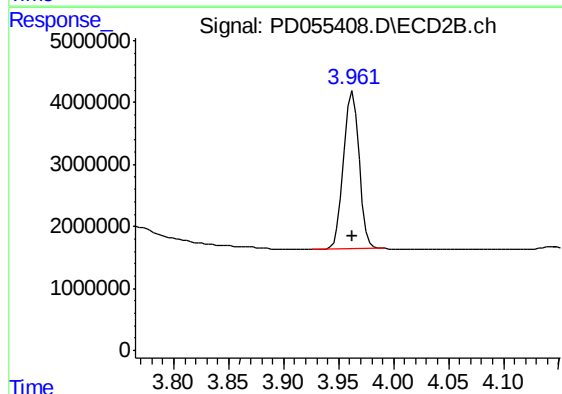


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: 0.000 min
Response: 25058642
Conc: 18.61 ng/ml

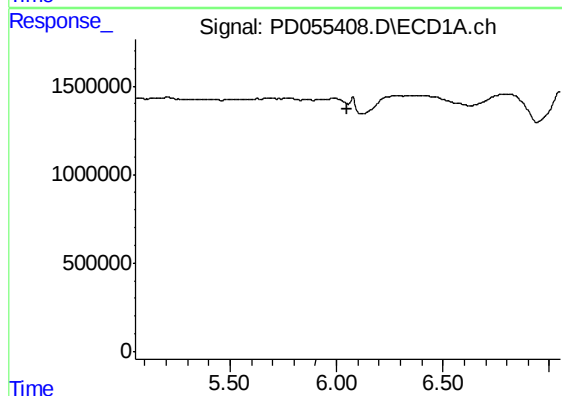


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.053 min
Response: 0
Conc: N.D.

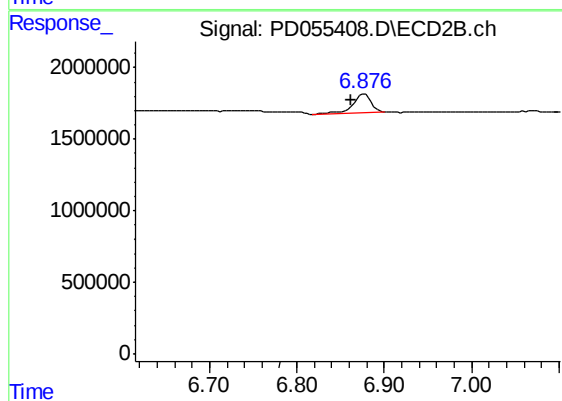

#15 Endosulfan II


R.T.: 6.877 min
Delta R.T.: 0.016 min
Response: 1835759
Conc: 1.18 ng/ml

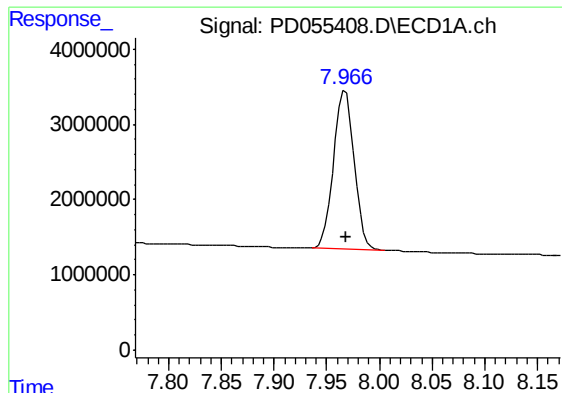

#27 Decachlorobiphenyl

R.T.: 7.968 min
Delta R.T.: -0.001 min
Response: 28739632
Conc: 31.39 ng/ml

Instrument :
ECD_D
ClientSampleId :
JLNK0

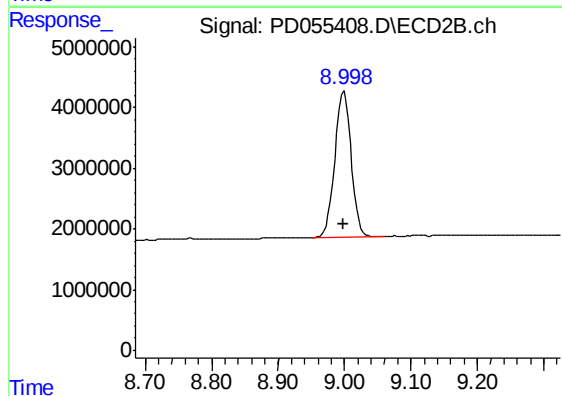

#27 Decachlorobiphenyl

R.T.: 8.999 min
Delta R.T.: 0.000 min
Response: 40932493
Conc: 31.37 ng/ml