

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101819\
 Data File : PD055423.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2019 21:59
 Operator : SG\AJ
 Sample : K5426-17
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 JLNJ6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 01:06:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 19 00:42:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.290	3.963	16798936	24096150	18.842	17.897
27) SA	Decachlor...	7.967	8.999	26482852	38038701	28.922	29.153
Target Compounds							
8) B	Heptachlo...	0.000	5.769f	0	3637924	N.D.	2.130


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101819\
Data File : PD055423.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2019 21:59
Operator : SG\AJ
Sample : K5426-17
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
JLNJ6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 01:06:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
Quant Title : GC Extractables
QLast Update : Sat Oct 19 00:42:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

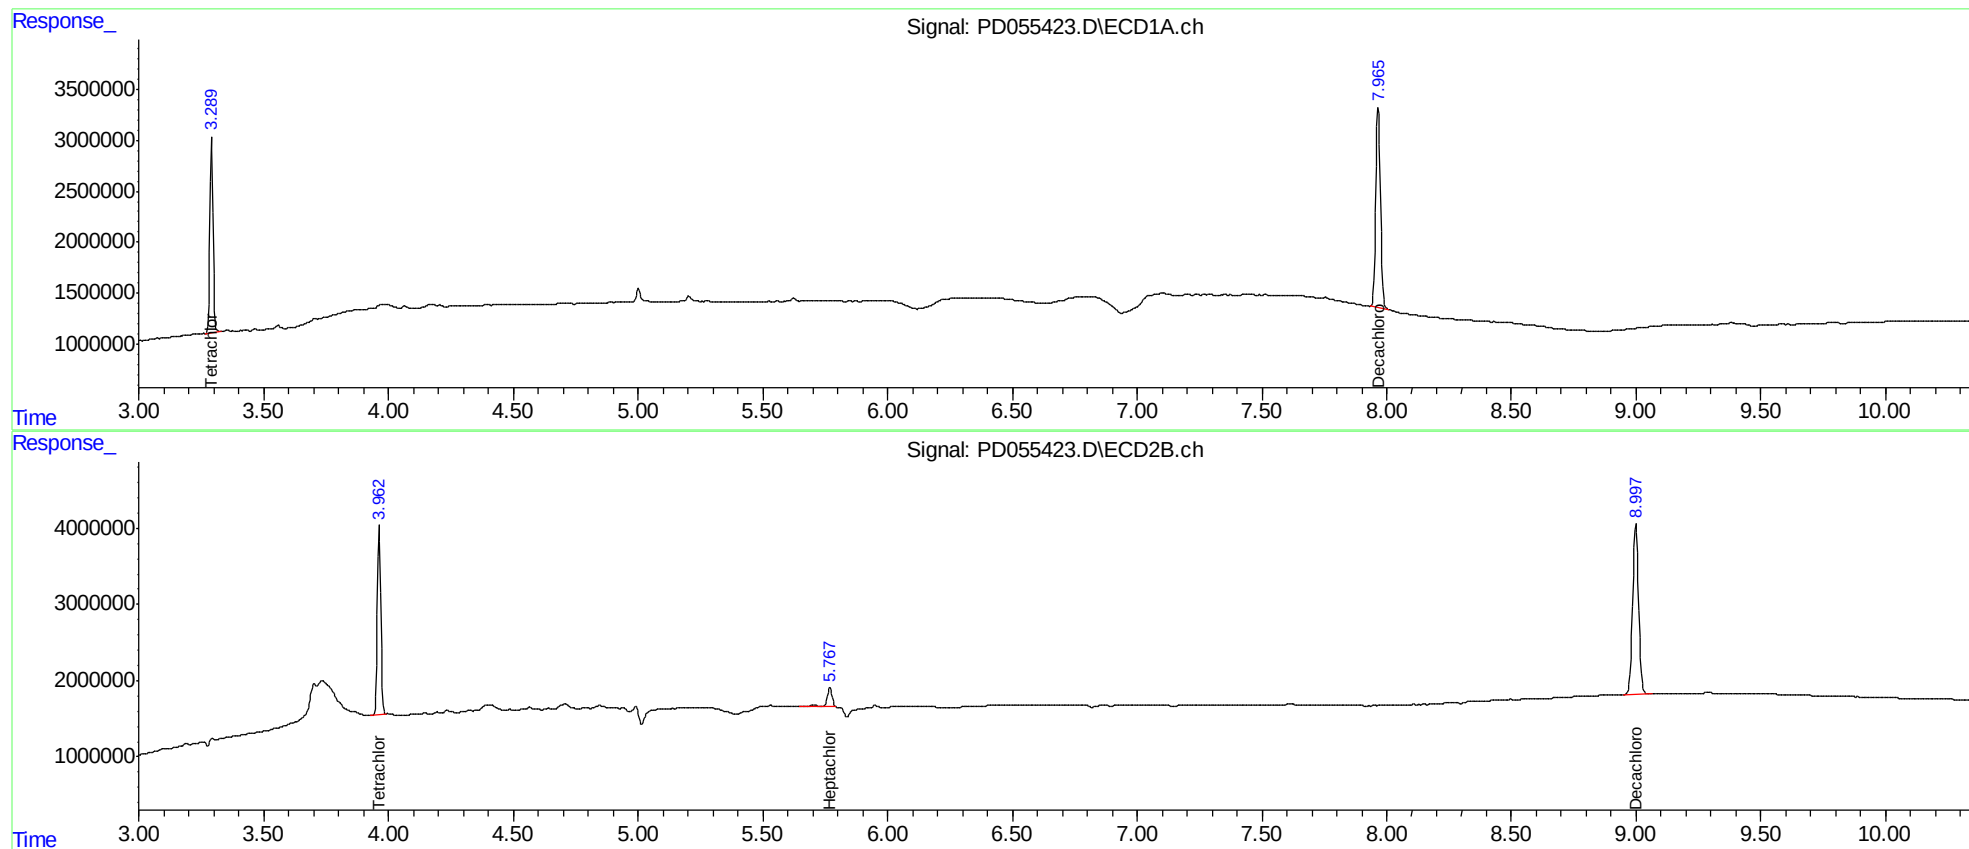


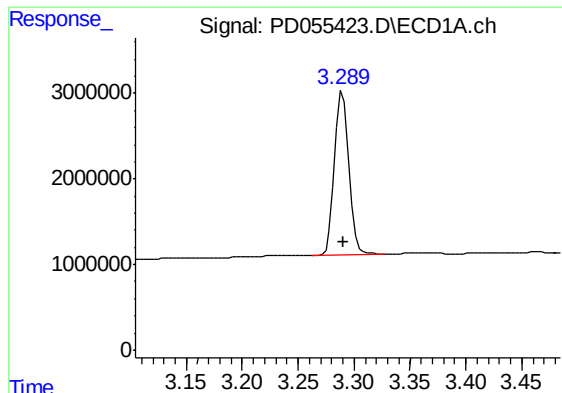

#1 Tetrachloro-m-xylene


R.T.: 3.290 min
Delta R.T.: 0.000 min
Response: 16798936
Conc: 18.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
JLNJ6

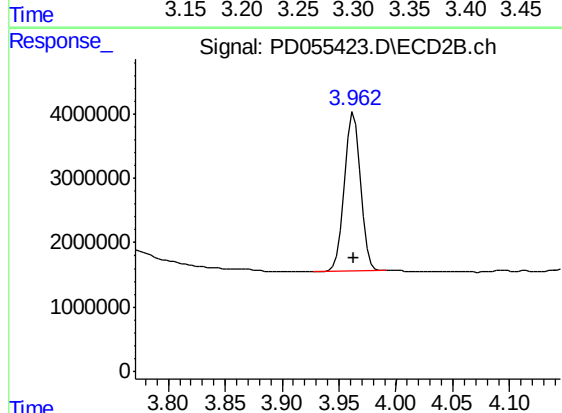


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: 0.000 min
Response: 24096150
Conc: 17.90 ng/ml

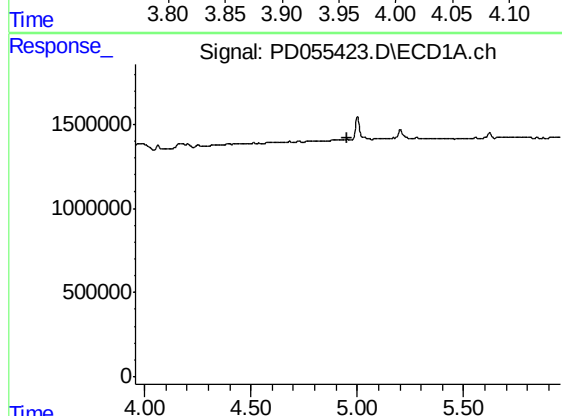


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.955 min
Response: 0
Conc: N.D.

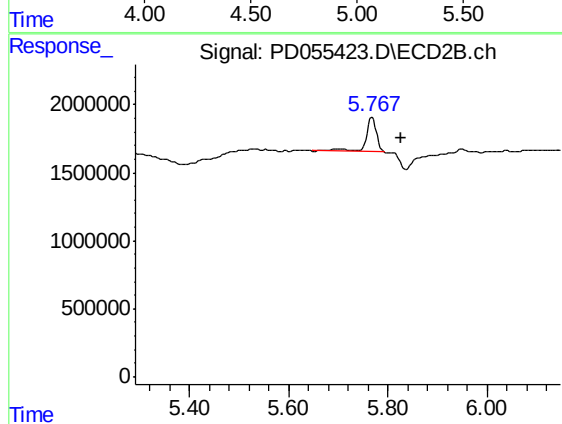

#8 Heptachlor epoxide


R.T.: 5.769 min
Delta R.T.: -0.057 min
Response: 3637924
Conc: 2.13 ng/ml

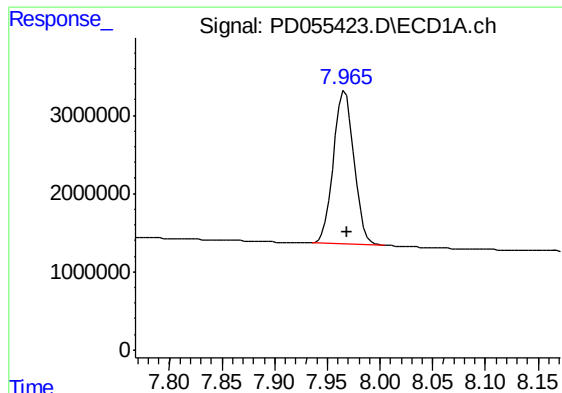

#27 Decachlorobiphenyl

R.T.: 7.967 min
Delta R.T.: -0.002 min
Response: 26482852
Conc: 28.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
JLNJ6

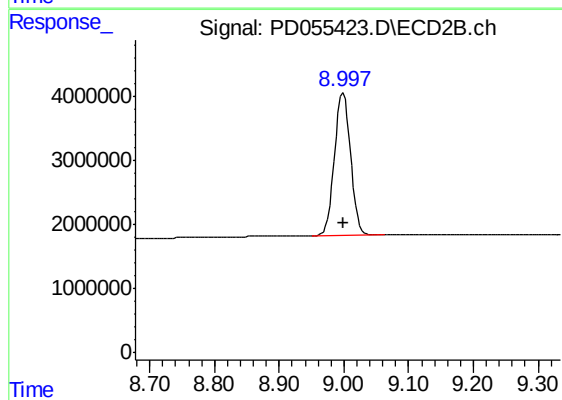

#27 Decachlorobiphenyl

R.T.: 8.999 min
Delta R.T.: 0.000 min
Response: 38038701
Conc: 29.15 ng/ml