

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101819\
 Data File : PD055369.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2019 08:50
 Operator : SG\AJ
 Sample : RESC08
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC08

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 00:56:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 19 00:42:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.290	3.962	16454483	24749720	18.455	18.383
2)	SA Decachlor...	7.967	9.000	33834038	48392635	36.950	37.088
Target Compounds							
2)	A alpha-BHC	3.717	4.349	10629356	16613251	8.464	8.540
3)	MA gamma-BHC...	3.992	4.632	10167618	15737857	8.580	8.535
4)	MA Heptachlor	4.279	5.138	7402217	15670367	8.135	8.403
5)	MB Aldrin	4.518	5.442	10074371	16543715	9.471	9.514
6)	B beta-BHC	4.242	4.800	5229742	8876493	9.838	10.039
7)	B delta-BHC	4.438	5.015	11462438	17551272	9.358	9.250
8)	B Heptachlo...	4.955	5.826	9669433	16437324	9.585	9.626
9)	A Endosulfan I	5.286	6.181	8439346	14729573	8.780	8.987
10)	B trans-Chl...	5.177	6.059	9922619	17105163	9.597	9.712
11)	B cis-Chlor...	5.234	6.132	9641880	17051712	9.597	9.918
12)	B 4,4'-DDE	5.403	6.287	19204346	31962391	18.842	18.956
13)	MA Dieldrin	5.526	6.437	18389547	31091225	16.593	17.179
14)	MA Endrin	5.779	6.653	15136222	24097407	16.899	17.252
15)	B Endosulfa...	6.052	6.861	18297074	30128318	19.113	19.379
16)	A 4,4'-DDD	5.913	6.775	13054919	24458898	16.108	17.097
17)	MA 4,4'-DDT	6.149	7.074	10016080	22202487	14.773	16.381
18)	B Endrin al...	6.221	6.984	15878540	26141690	19.569	19.749
19)	B Endosulfa...	6.431	7.207	17076006	29034238	19.156	19.475
20)	A Methoxychlor	6.698	7.530	29205484	67739913	80.088	87.868
21)	B Endrin ke...	6.916	7.676	19607139	32223284	20.061	20.119

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101819\
Data File : PD055369.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2019 08:50
Operator : SG\AJ
Sample : RESC08
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 00:56:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
Quant Title : GC Extractables
QLast Update : Sat Oct 19 00:42:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

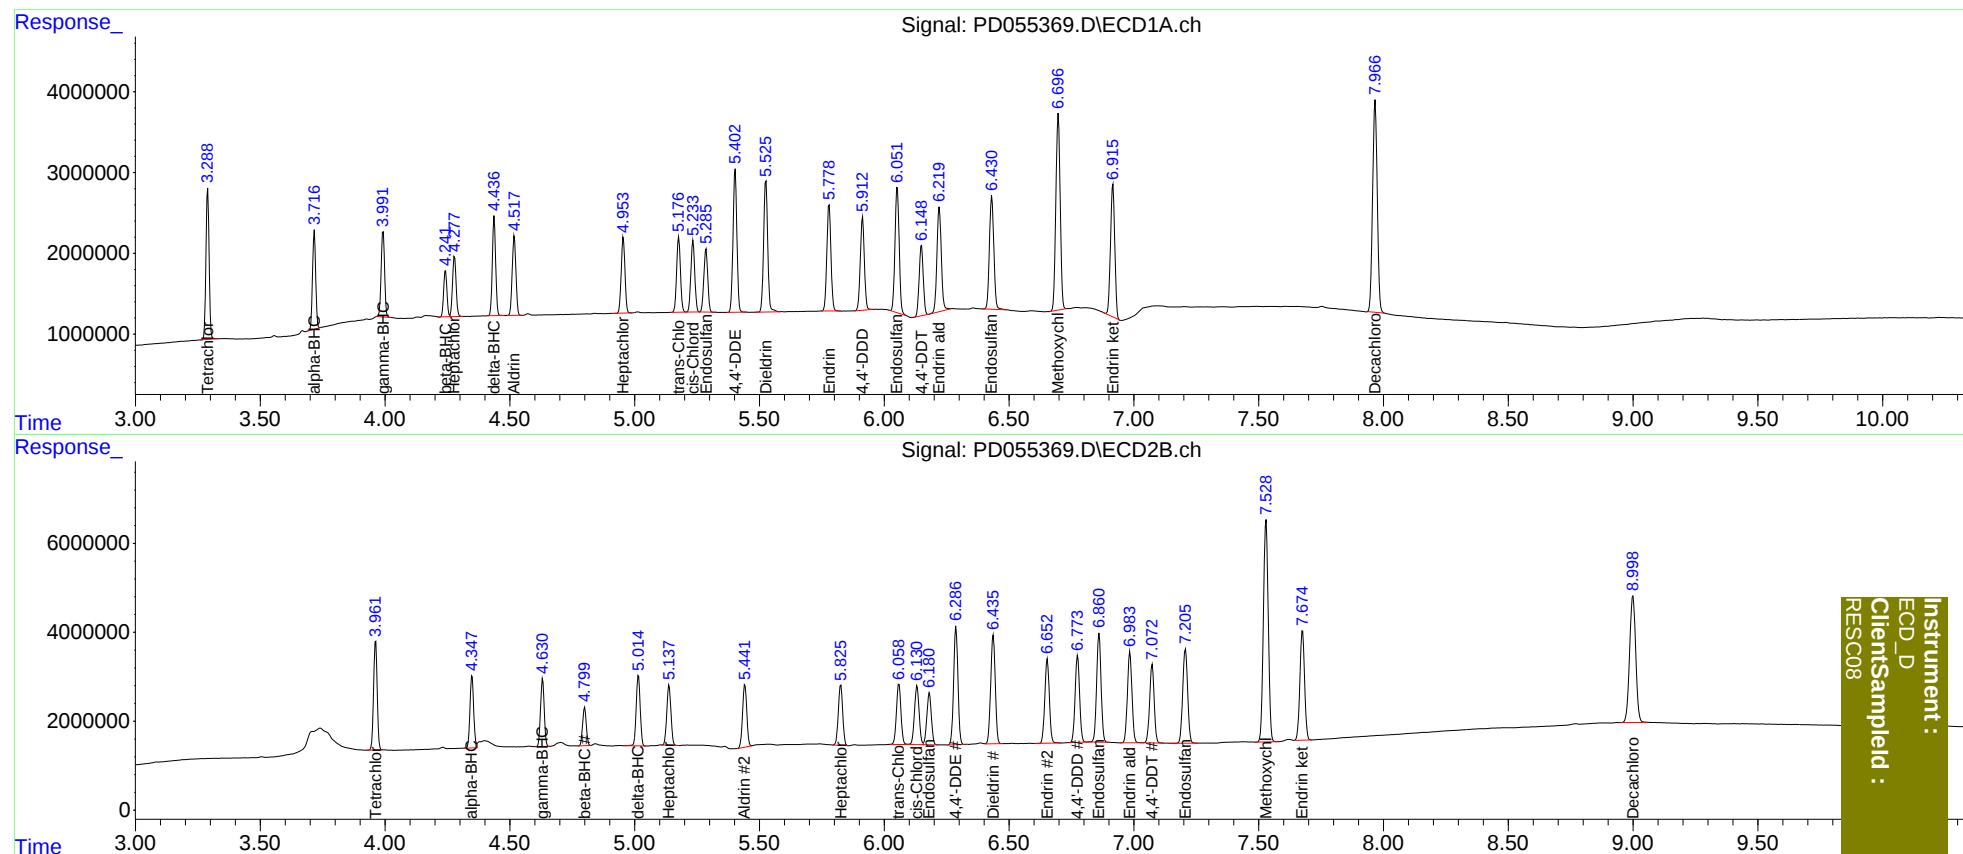

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101819\
Data File : PD055369.D
Acq On : 18 Oct 2019 08:50
Operator : SG\AJ
Sample : RESC08
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC08

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
Title : GC Extractables
Last Update : Sat Oct 19 00:42:03 2019
Integrator: ChemStation

RT#1	RT#2	Resolution
3.290	3.717	100.00%
3.717	3.992	100.00%
3.992	4.242	100.00%
4.242	4.279	95.67%
4.279	4.438	100.00%
4.438	4.518	100.00%
4.518	4.955	100.00%
4.955	5.177	100.00%
5.177	5.234	100.00%
5.234	5.286	100.00%
5.286	5.403	100.00%
5.403	5.526	100.00%
5.526	5.779	100.00%
5.779	5.913	100.00%
5.913	6.052	100.00%
6.052	6.149	100.00%
6.149	6.221	100.00%
6.221	6.431	100.00%
6.431	6.698	100.00%
6.698	6.916	100.00%
6.916	7.967	100.00%

Signal #2


3.962	4.349	100.00%
4.349	4.632	100.00%
4.632	4.800	100.00%
4.800	5.015	100.00%
5.015	5.138	100.00%
5.138	5.442	100.00%
5.442	5.826	100.00%
5.826	6.059	100.00%
6.059	6.132	100.00%
6.132	6.181	97.43%
6.181	6.288	100.00%
6.288	6.437	100.00%
6.437	6.653	100.00%
6.653	6.775	100.00%
6.775	6.861	100.00%
6.861	6.984	100.00%
6.984	7.074	100.00%
7.074	7.207	100.00%
7.207	7.530	100.00%
7.530	7.676	100.00%
7.676	9.000	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101819\
Data File : PD055369.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2019 08:50
Operator : SG\AJ
Sample : RESC08
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC08

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 00:56:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
Quant Title : GC Extractables
QLast Update : Sat Oct 19 00:42:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

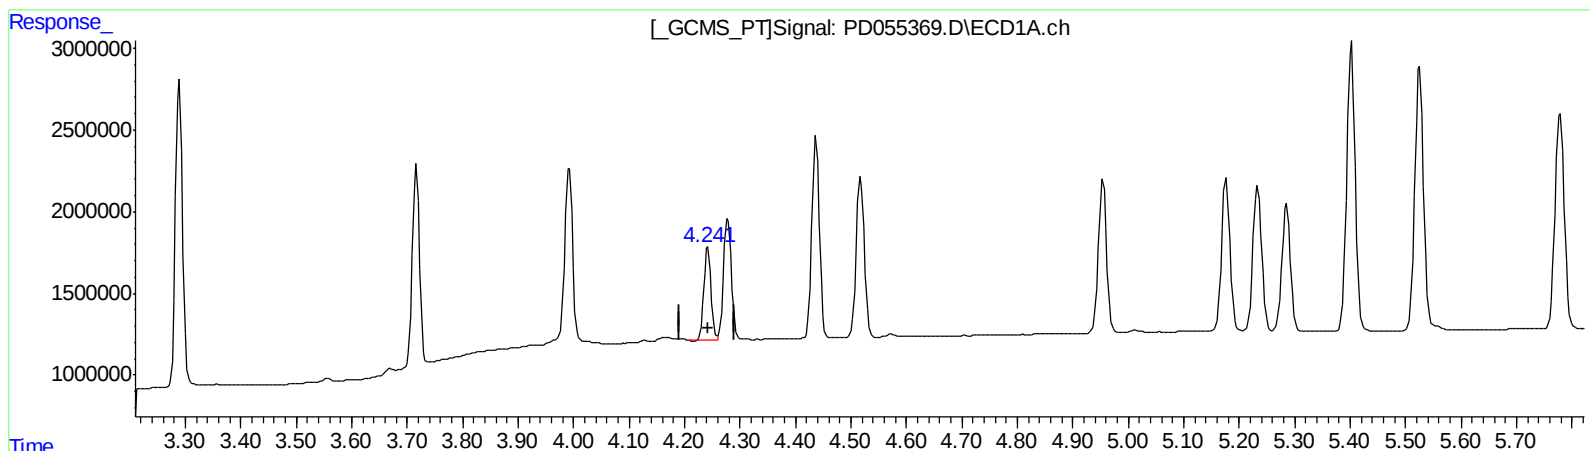

(6) beta-BHC (B)

4.242min 9.838 ng/ml

response 5229742

(6) beta-BHC #2 (B)

4.800min 10.039 ng/ml


response 8876493

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101819\
Data File : PD055369.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2019 08:50
Operator : SG\AJ
Sample : RESC08
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC08

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 00:56:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
Quant Title : GC Extractables
QLast Update : Sat Oct 19 00:42:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

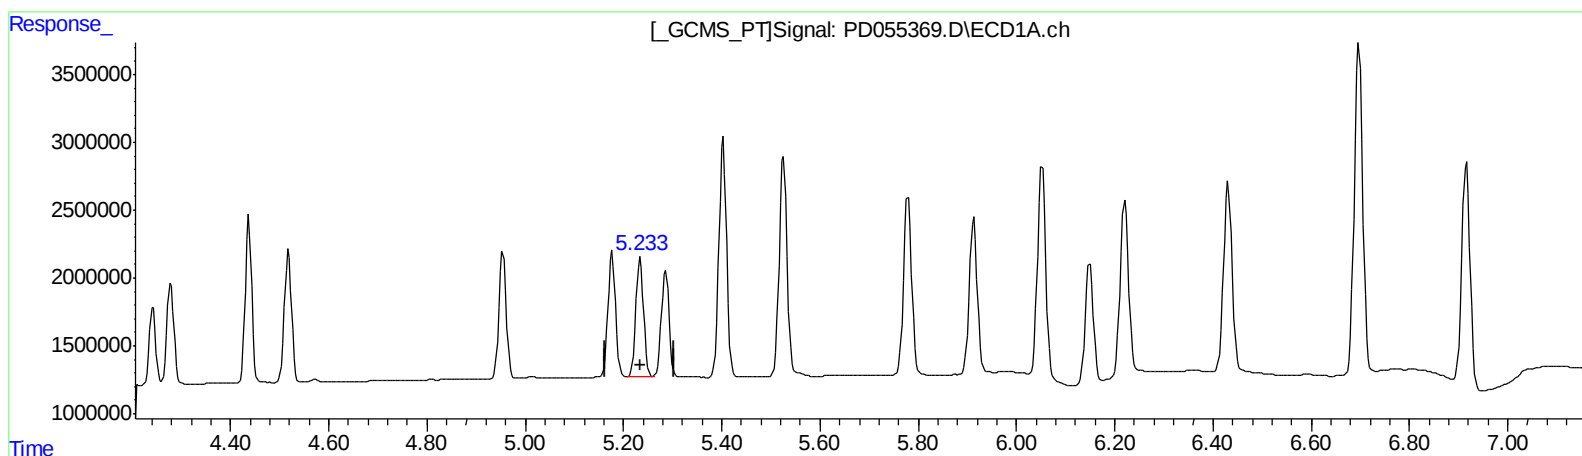

(11) cis-Chlordane (B)

5.234min 9.597 ng/ml

response 9641880

(11) cis-Chlordane #2 (B)

6.132min 9.918 ng/ml

response 17051712