

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101822\
 Data File : PD072496.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2022 14:16
 Operator : AR\AJ
 Sample : PIBLK643
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 01:44:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 18 06:21:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.712	3.464	53715611	862.2E6	21.067	22.956
27)	SA Decachlor...	7.852	8.929	85240983	406.2E6	42.586	45.120
Target Compounds							
2)	A alpha-BHC	3.199	0.000	174318	0	<MDL	N.D. #
5)	MB Aldrin	4.179	0.000	252359	0	<MDL	N.D. #
8)	B Heptachlo...	0.000	5.603	0 40091086		N.D.	2.060
9)	A Endosulfan I	4.963f	0.000	218247	0	<MDL	N.D. #
10)	B trans-Chl...	4.909	0.000	89705	0	<MDL	N.D. #
11)	B cis-Chlor...	4.963	0.000	218247	0	<MDL	N.D. #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101822\
Data File : PD072496.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2022 14:16
Operator : AR\AJ
Sample : PIBLK643
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 01:44:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 18 06:21:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

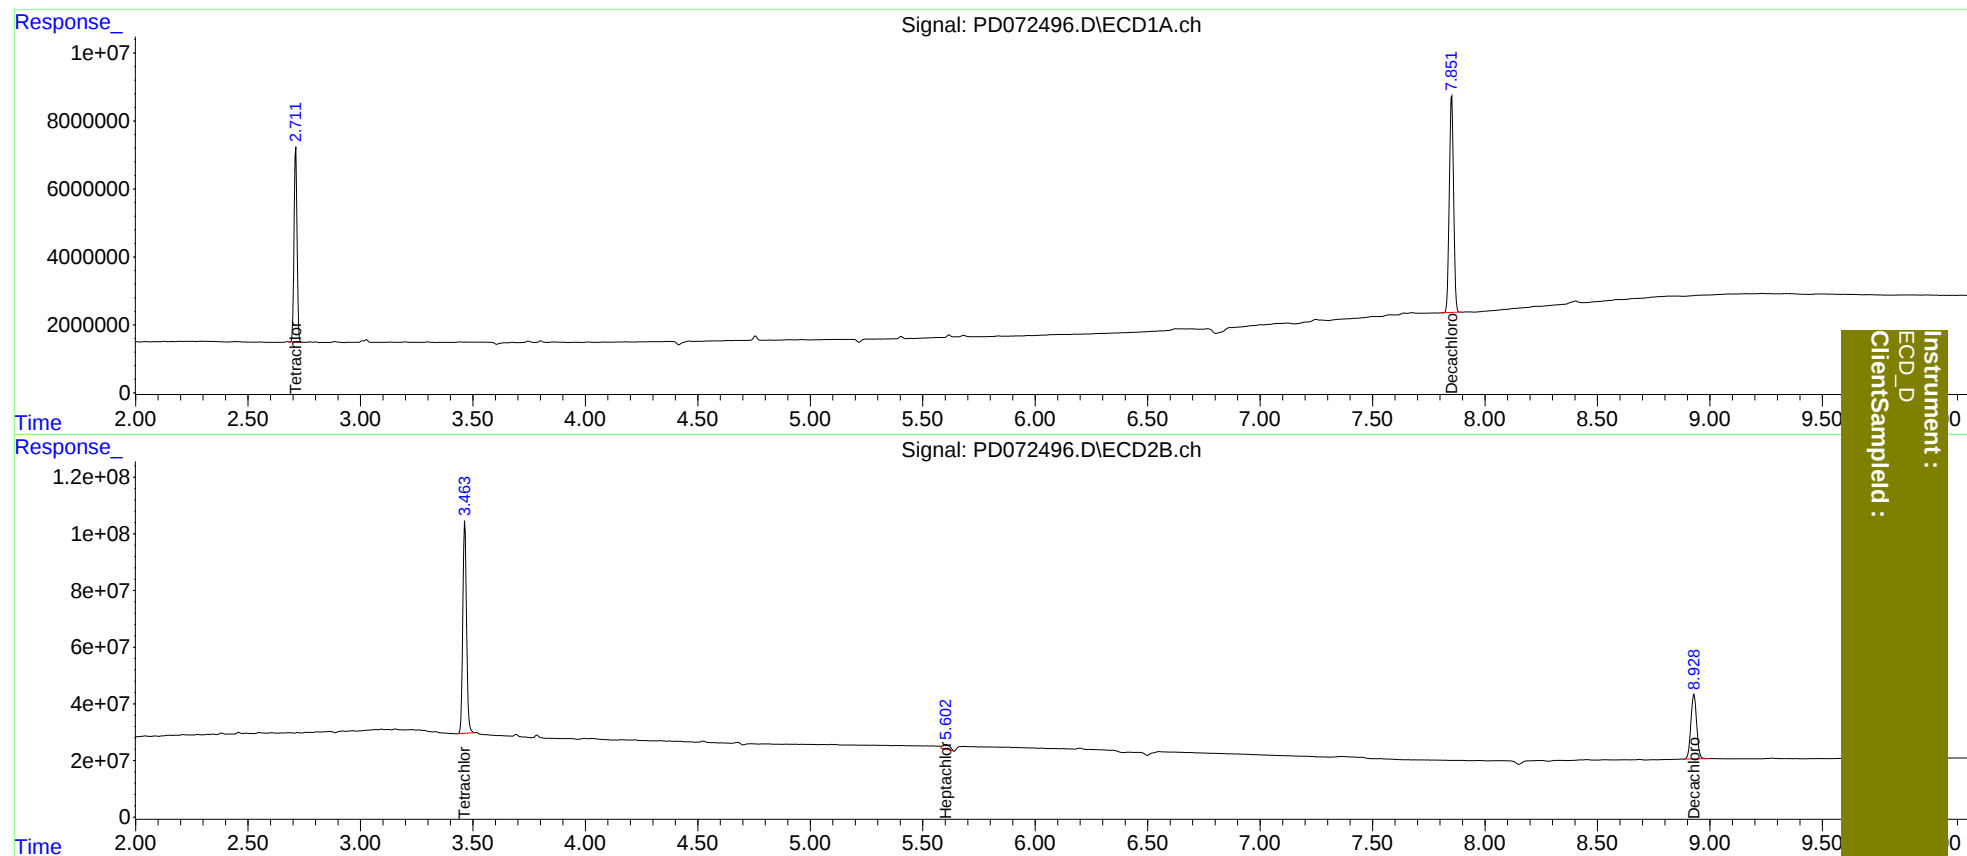


Instrument :
ECD_D
ClientSampled : 0

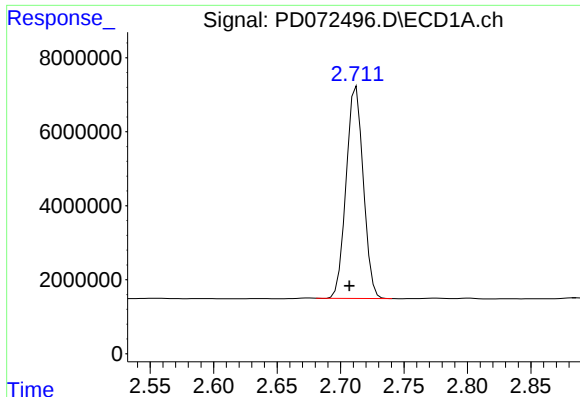

#1 Tetrachloro-m-xylene


R.T.: 2.712 min
Delta R.T.: 0.006 min
Response: 53715611
Conc: 21.07 ng/ml

Instrument :
ECD_D
ClientSampleId :

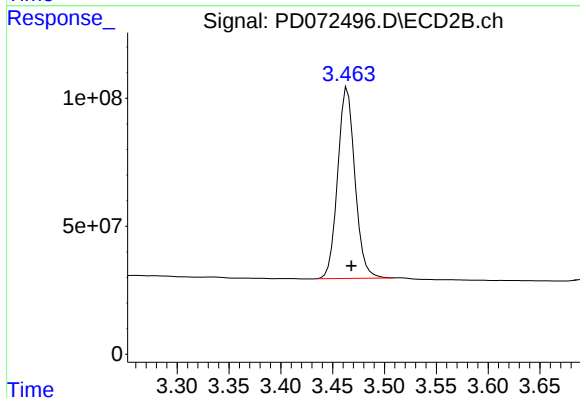


#1 Tetrachloro-m-xylene

R.T.: 3.464 min
Delta R.T.: -0.004 min
Response: 862212688
Conc: 22.96 ng/ml

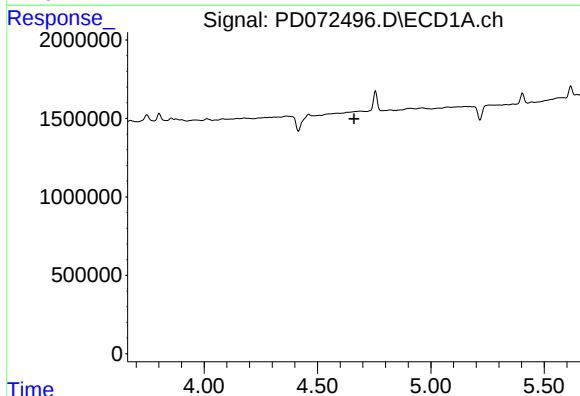


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.661 min
Response: 0
Conc: N.D.

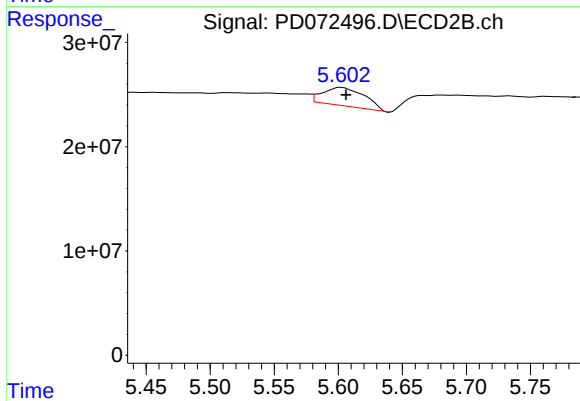

#8 Heptachlor epoxide


R.T.: 5.603 min
Delta R.T.: -0.003 min
Response: 40091086
Conc: 2.06 ng/ml

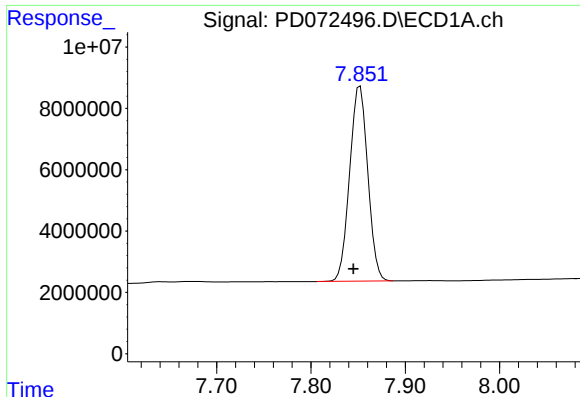

#27 Decachlorobiphenyl

R.T.: 7.852 min
Delta R.T.: 0.007 min
Response: 85240983
Conc: 42.59 ng/ml

Instrument :
ECD_D
ClientSampleId :

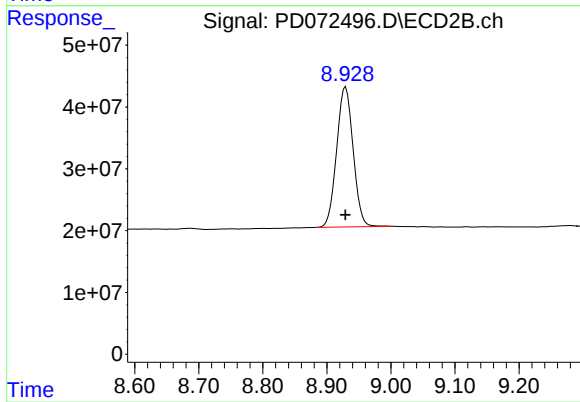

#27 Decachlorobiphenyl

R.T.: 8.929 min
Delta R.T.: 0.000 min
Response: 406173559
Conc: 45.12 ng/ml