

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101822\
 Data File : PD072491.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2022 12:28
 Operator : AR\AJ
 Sample : PB148404BS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS404

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/19/2022
 Supervised By :Ankita Jodhani 10/20/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 01:41:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 18 06:21:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.707	3.467	47698724	731.9E6	18.707	19.487
27)	SA Decachlor...	7.846	8.930	80989794	381.6E6	40.462	42.385
Target Compounds							
2)	A alpha-BHC	3.213	3.932	16184903	258.8E6	4.324	5.259
3)	MA gamma-BHC...	3.544	4.267	15517839	218.3E6	4.714	5.237
4)	MA Heptachlor	3.875	4.834	15233311	158.2E6	4.407m	5.496
5)	MB Aldrin	4.156	5.173	15699476	131.6E6	4.634	5.469
6)	B beta-BHC	3.845	4.482	7571028	84899179	4.736m	5.100
7)	B delta-BHC	4.076	4.726	15203664	169.4E6	4.287	5.318
8)	B Heptachlo...	4.662	5.606	14474056	105.2E6	4.772	5.405
9)	A Endosulfan I	5.032	5.989	13245355	91101056	4.927	5.671m
10)	B trans-Chl...	4.911	5.859	13974892	95756611	4.496	5.118
11)	B cis-Chlor...	4.974	5.935	14209001	92093235	4.705	5.147
12)	B 4,4'-DDE	5.163	6.109	25121266	166.2E6	8.624	10.160
13)	MA Dieldrin	5.298	6.268	27214405	178.5E6	9.292	10.934
14)	MA Endrin	5.575	6.500	23625019	145.9E6	9.228	10.612
15)	B Endosulfa...	5.873	6.729	23244268	143.1E6	9.650	11.220
16)	A 4,4'-DDD	5.722	6.634	19910665	140.0E6	8.765	11.293 #
17)	MA 4,4'-DDT	5.971	6.942	18878184	126.4E6	8.541	10.508
18)	B Endrin al...	6.057	6.861	19710257	115.1E6	9.645	10.702
19)	B Endosulfa...	6.280	7.094	22474448	121.7E6	9.311	10.196
20)	A Methoxychlor	6.556	7.422	57285107	302.4E6	47.997	55.081
21)	B Endrin ke...	6.791	7.585	27138412	142.4E6	9.523	11.107

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101822\
Data File : PD072491.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2022 12:28
Operator : AR\AJ
Sample : PB148404BS
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 01:41:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 18 06:21:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

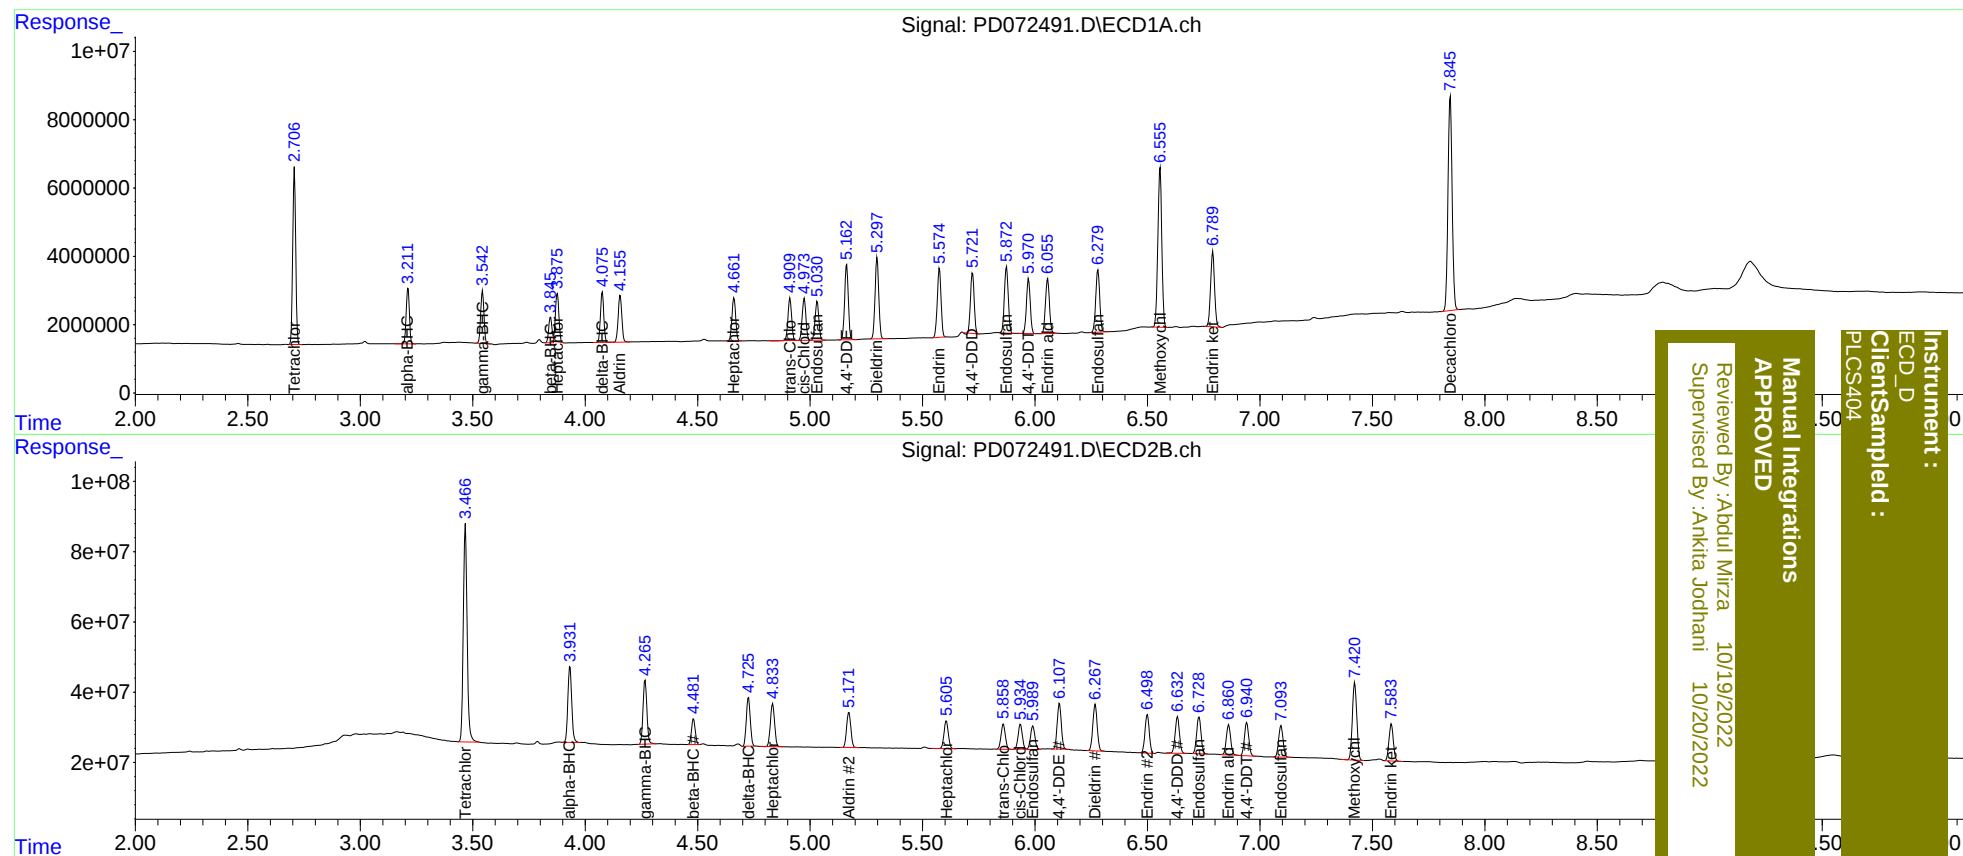

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 10/19/2022
Supervised By: Ankita Jodhani 10/20/2022

Instrument :
ECD_D
Client Sampled :
PLCS404