

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101823\
 Data File : PD078952.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2023 16:43
 Operator : AR\AJ
 Sample : PB156344TB 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 22:13:00 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101623CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 05:35:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.807	29326205	40860546	19.056	19.109
27)	SA Decachlor...	9.117	7.957	38461186	48632259	21.064	21.484
Target Compounds							
2)	A alpha-BHC	4.047	3.298	155514	94484	<MDL	<MDL #
4)	MA Heptachlor	0.000	3.976	0	20731	N.D.	<MDL
5)	MB Aldrin	0.000	4.286	0	55040	N.D.	<MDL
6)	B beta-BHC	0.000	3.976f	0	20731	N.D.	<MDL
7)	B delta-BHC	4.798	4.191f	3661227	134653	1.355	<MDL #
8)	B Heptachlo...	0.000	4.768	0	49987	N.D.	<MDL
9)	A Endosulfan I	6.139	0.000	340657	0	0.161	N.D. #
12)	B 4,4'-DDE	0.000	5.225f	0	247658	N.D.	<MDL
13)	MA Dieldrin	6.393	0.000	291154	0	0.128	N.D. #
15)	B Endosulfa...	0.000	5.906f	0	419436	N.D.	0.178
19)	B Endosulfa...	0.000	6.370	0	170512	N.D.	<MDL
20)	A Methoxychlor	0.000	6.667	0	101854	N.D.	<MDL
21)	B Endrin ke...	7.712	0.000	74428	0	<MDL	N.D. #
24)	Toxaphene-3	0.000	6.626	0	84210	N.D.	1.629


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101823\
Data File : PD078952.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2023 16:43
Operator : AR\AJ
Sample : PB156344TB 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 22:13:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101623CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 05:35:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

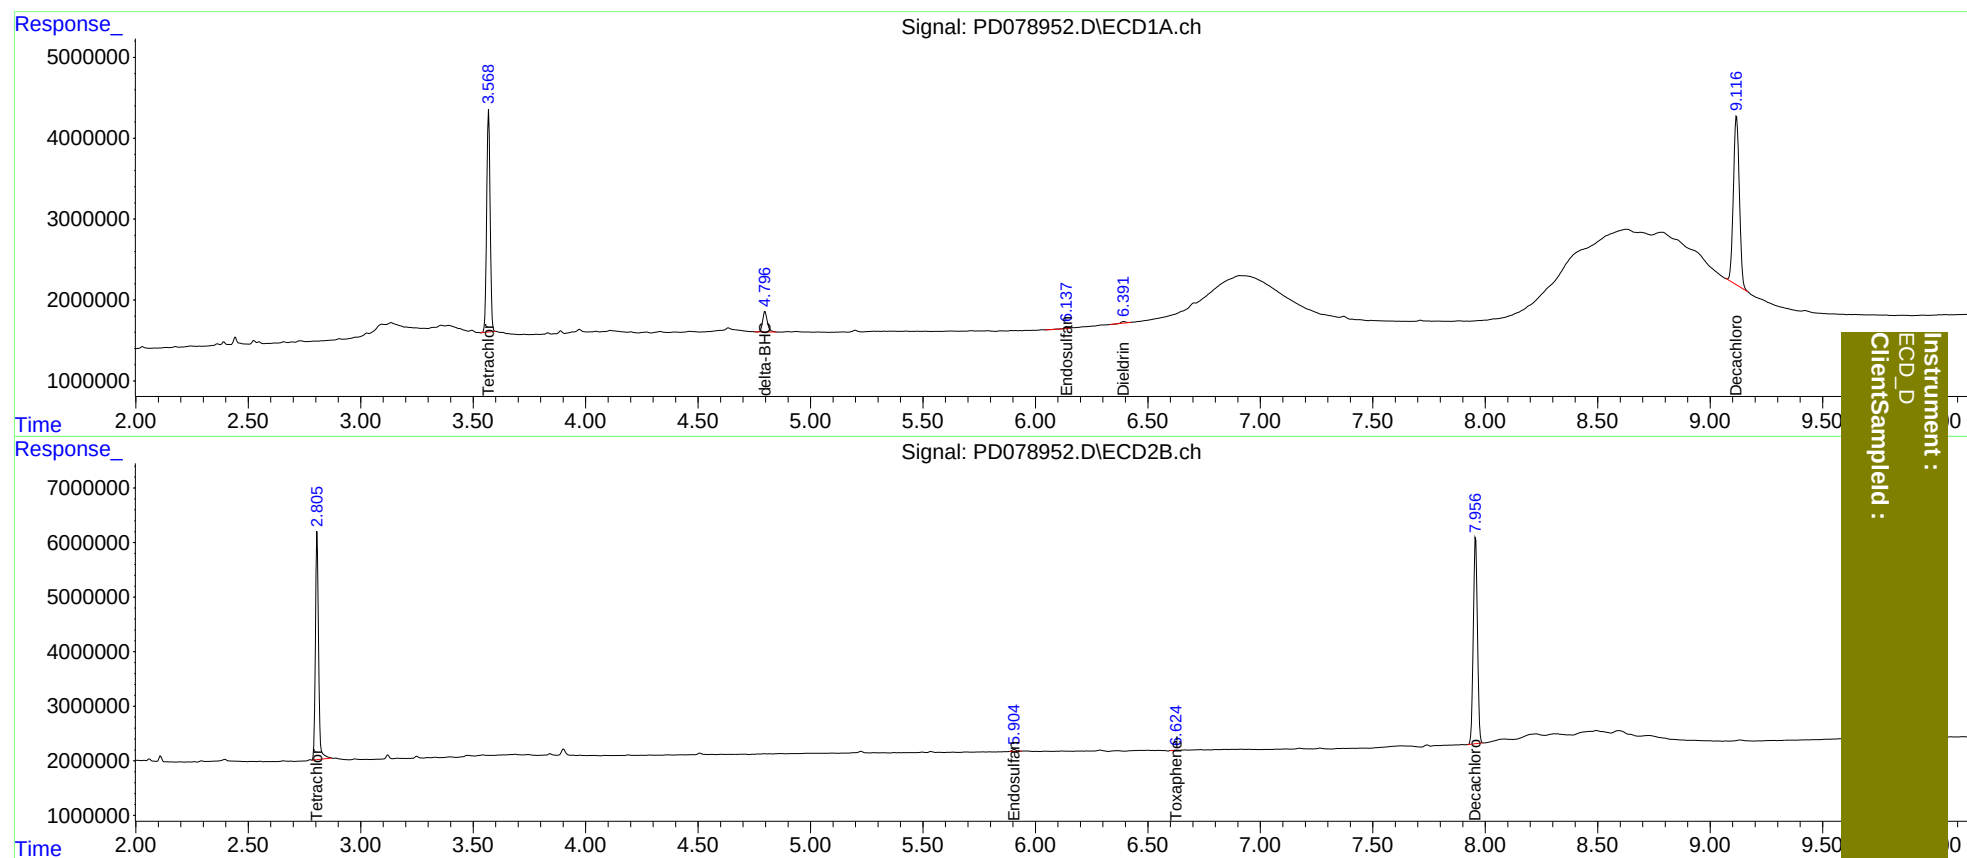


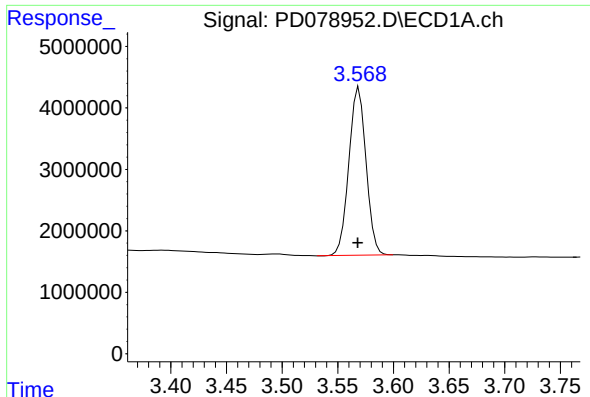

#1 Tetrachloro-m-xylene


R.T.: 3.569 min
Delta R.T.: 0.001 min
Response: 29326205
Conc: 19.06 ng/ml

Instrument :
ECD_D
ClientSampleId :

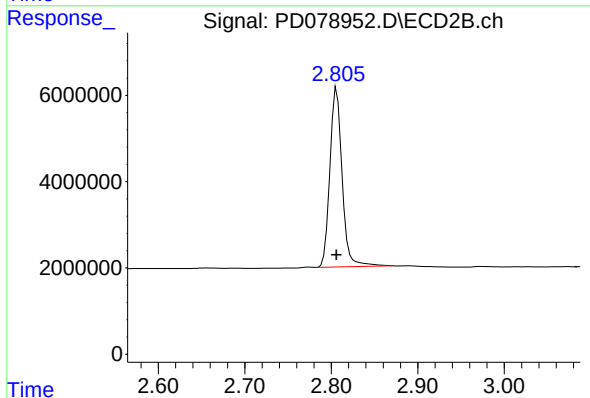


#1 Tetrachloro-m-xylene

R.T.: 2.807 min
Delta R.T.: 0.000 min
Response: 40860546
Conc: 19.11 ng/ml

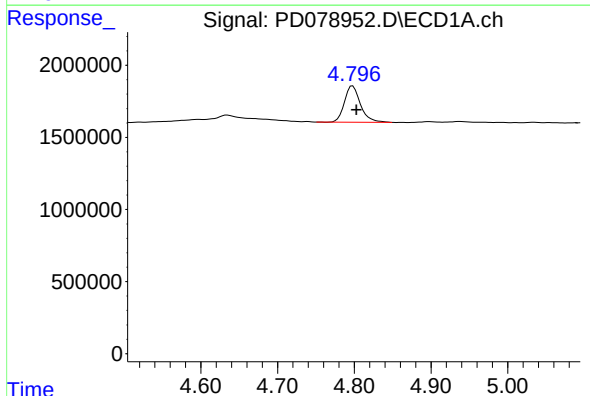


#7 delta-BHC

R.T.: 4.798 min
Delta R.T.: -0.005 min
Response: 3661227
Conc: 1.35 ng/ml

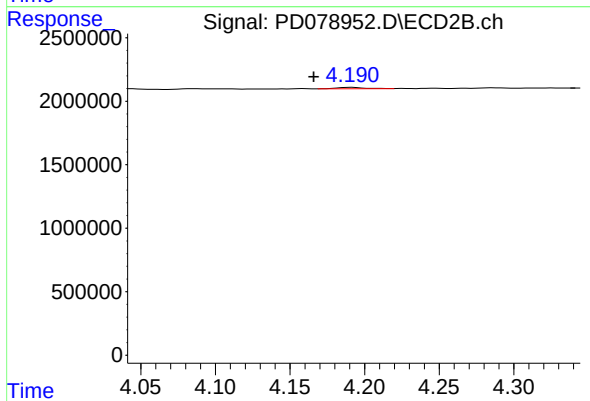

#7 delta-BHC


R.T.: 4.191 min
Delta R.T.: 0.025 min
Response: 134653
Conc: N.D.

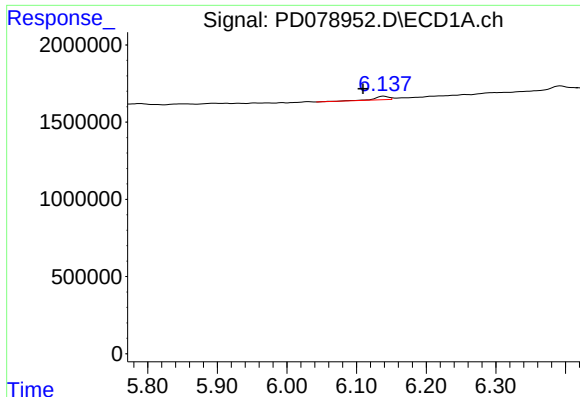

#9 Endosulfan I


R.T.: 6.139 min
Delta R.T.: 0.030 min
Response: 340657
Conc: 0.16 ng/ml

Instrument :
ECD_D
ClientSampleId :

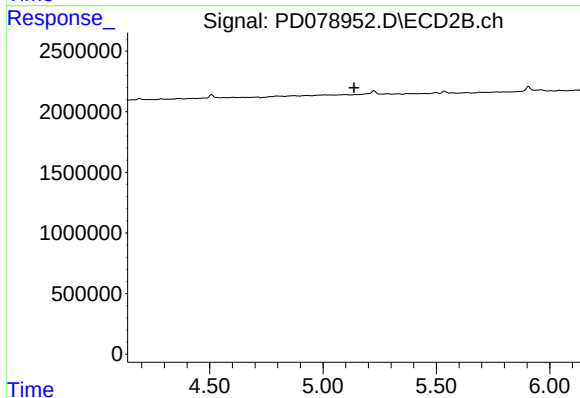


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.138 min
Response: 0
Conc: N.D.

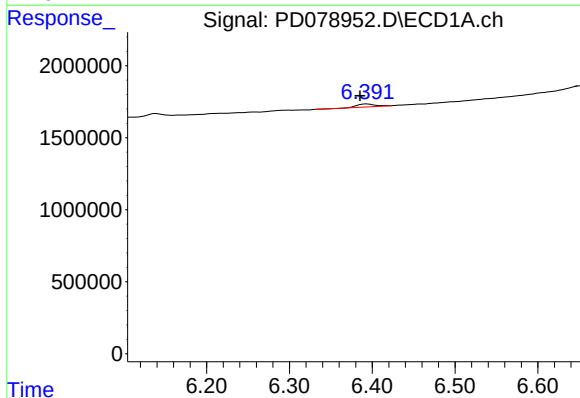


#13 Dieldrin

R.T.: 6.393 min
Delta R.T.: 0.008 min
Response: 291154
Conc: 0.13 ng/ml

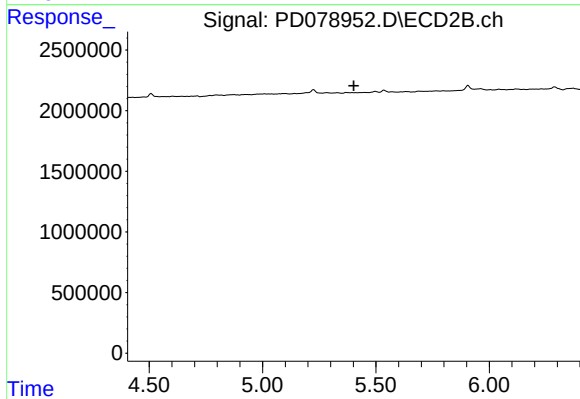

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 5.402 min
Response: 0
Conc: N.D.

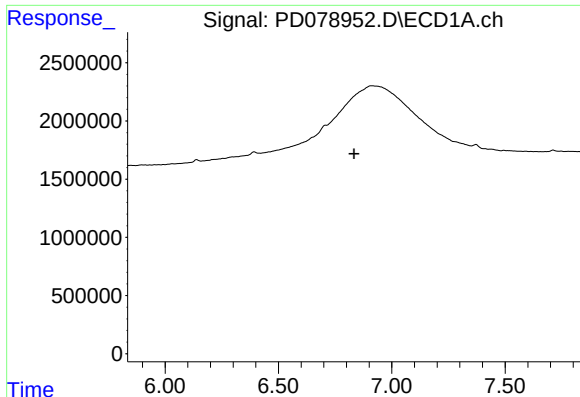

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.834 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

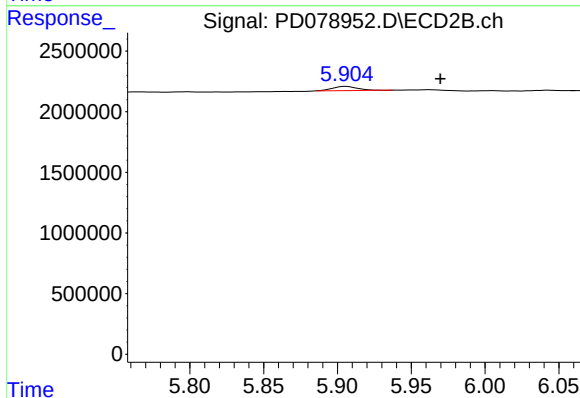


#15 Endosulfan II

R.T.: 5.906 min
Delta R.T.: -0.064 min
Response: 419436
Conc: 0.18 ng/ml

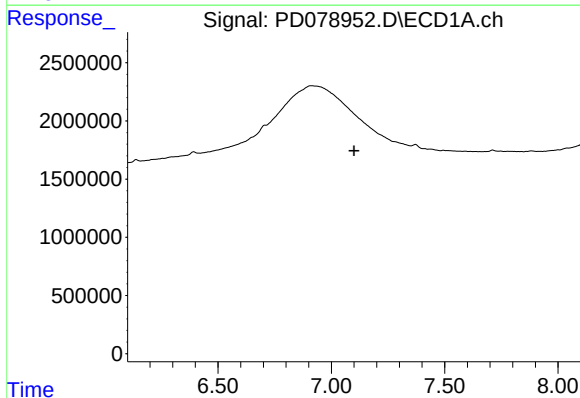


#24 Toxaphene-3

R.T.: 0.000 min
Exp R.T.: 7.100 min
Response: 0
Conc: N.D.

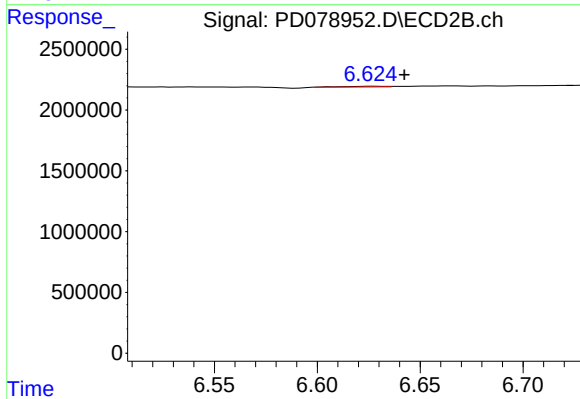

#24 Toxaphene-3


R.T.: 6.626 min
Delta R.T.: -0.016 min
Response: 84210
Conc: 1.63 ng/ml

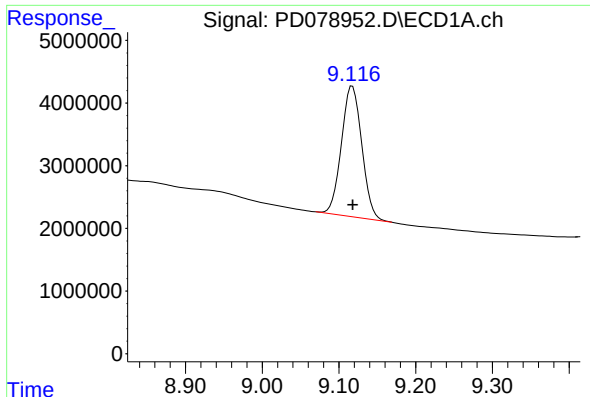

#27 Decachlorobiphenyl

R.T.: 9.117 min
Delta R.T.: 0.000 min
Response: 38461186
Conc: 21.06 ng/ml

Instrument :
ECD_D
ClientSampleId :

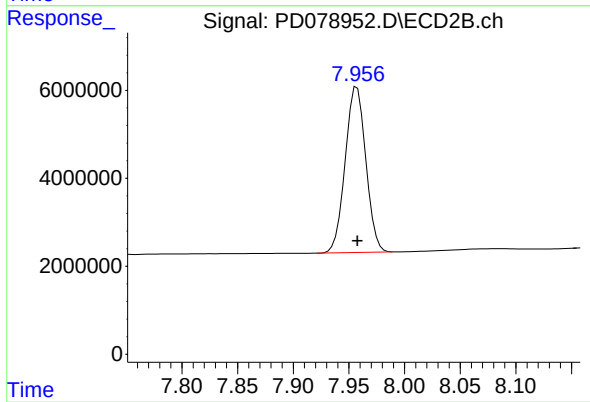

#27 Decachlorobiphenyl

R.T.: 7.957 min
Delta R.T.: 0.000 min
Response: 48632259
Conc: 21.48 ng/ml