

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101823\
 Data File : PD078950.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2023 16:16
 Operator : AR\AJ
 Sample : 04824-03MS 10X (Sig #1); 04824-01MS 10X (Sig #2)
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 JYCA4MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 22:12:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101623CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 05:35:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.806	33254605	40996260	21.608	19.173
2)	SA Decachlor...	9.118	7.956	44840026	52310540	24.557	23.109
Target Compounds							
2)	A alpha-BHC	4.026	3.310	139.5E6	176.2E6	52.403	52.783
3)	MA gamma-BHC...	4.360	3.640	125.1E6	157.3E6	49.320	50.496
4)	MA Heptachlor	4.953	3.984	138.6E6	154.6E6	51.222	51.839
5)	MB Aldrin	5.296	4.265	129.6E6	159.9E6	52.376	52.380
6)	B beta-BHC	4.553	3.934	54696708	66825020	48.482	46.759
7)	B delta-BHC	4.802	4.166	99171326	117.3E6	36.695	35.916
8)	B Heptachlo...	5.723	4.767	117.4E6	147.4E6	51.120	51.661
9)	A Endosulfan I	6.109	5.137	110.7E6	136.8E6	52.406	53.953
10)	B trans-Chl...	5.979	5.017	114.6E6	144.1E6	51.702	52.181
11)	B cis-Chlor...	6.059	5.082	115.2E6	145.9E6	51.148	51.242
12)	B 4,4'-DDE	6.229	5.271	222.4E6	282.2E6	107.171	107.915
13)	MA Dieldrin	6.385	5.402	240.5E6	306.7E6	105.704	107.068
14)	MA Endrin	6.616	5.677	203.2E6	270.0E6	107.898	108.341
15)	B Endosulfa...	6.833	5.969	203.9E6	255.8E6	104.880	108.315
16)	A 4,4'-DDD	6.746	5.824	179.5E6	232.8E6	106.398	106.335
17)	MA 4,4'-DDT	7.062	6.076	197.2E6	243.2E6	109.294	108.399
18)	B Endrin al...	6.963	6.148	142.7E6	178.5E6	95.170	97.933
19)	B Endosulfa...	7.198	6.371	186.9E6	226.5E6	98.587	100.225
20)	A Methoxychlor	7.537	6.651	497.4E6	601.1E6	521.697	512.860
21)	B Endrin ke...	7.685	6.877	211.2E6	277.1E6	102.591	106.458

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101823\
Data File : PD078950.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2023 16:16
Operator : AR\AJ
Sample : 04824-03MS 10X (Sig #1); 04824-01MS 10X (Sig #2)
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 22:12:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101623CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 05:35:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

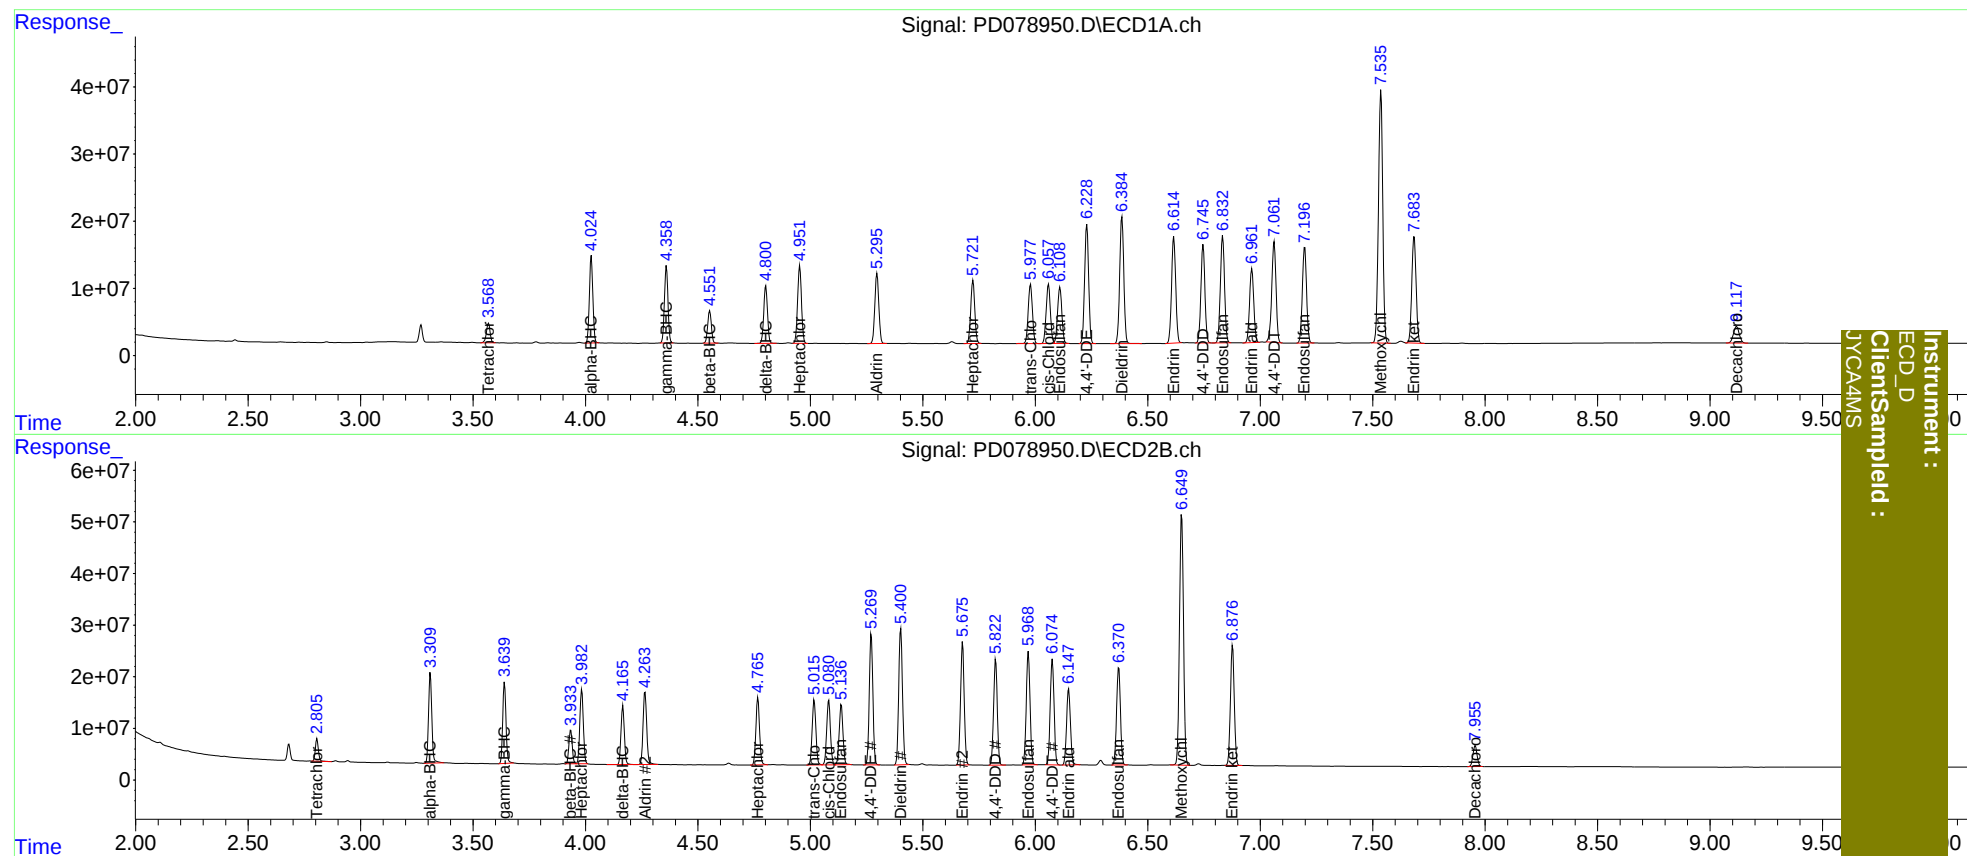

Instrument :
ECD_D
ClientSampled :
JYCA4AMS