

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101823\
 Data File : PD078960.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2023 18:29
 Operator : AR\AJ
 Sample : 04885-06MSD 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 COM28MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 22:15:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101623CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 05:35:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.568	2.806	32961902	40536110	21.418	18.958
2)	SA Decachlor...	9.117	7.956	44379574	51533333	24.305	22.765
Target Compounds							
2)	A alpha-BHC	4.026	3.310	143.1E6	180.8E6	53.753	54.168
3)	MA gamma-BHC...	4.359	3.640	127.7E6	161.6E6	50.321	51.874
4)	MA Heptachlor	4.952	3.983	126.1E6	147.3E6	46.600	49.369
5)	MB Aldrin	5.296	4.265	117.8E6	146.7E6	47.639	48.042
6)	B beta-BHC	4.552	3.934	54705822	69005107	48.491	48.284
7)	B delta-BHC	4.802	4.166	96699562	118.8E6	35.780	36.386
8)	B Heptachlo...	5.723	4.766	119.2E6	151.9E6	51.870	53.236
9)	A Endosulfan I	6.110	5.137	112.9E6	140.4E6	53.452	55.389
10)	B trans-Chl...	5.978	5.017	114.1E6	144.2E6	51.463	52.224
11)	B cis-Chlor...	6.059	5.081	115.0E6	146.5E6	51.039	51.453
12)	B 4,4'-DDE	6.229	5.270	222.6E6	284.1E6	107.245	108.650
13)	MA Dieldrin	6.385	5.402	244.9E6	314.5E6	107.650	109.780
14)	MA Endrin	6.615	5.676	206.5E6	275.1E6	109.671	110.370
15)	B Endosulfa...	6.833	5.969	208.0E6	262.5E6	107.006	111.146
16)	A 4,4'-DDD	6.746	5.824	182.1E6	237.3E6	107.913	108.357
17)	MA 4,4'-DDT	7.062	6.076	195.2E6	242.4E6	108.188	108.059
18)	B Endrin al...	6.963	6.148	150.1E6	189.2E6	100.083	103.803
19)	B Endosulfa...	7.197	6.370	190.2E6	230.9E6	100.329	102.167
20)	A Methoxychlor	7.535	6.651	502.2E6	606.9E6	526.678	517.829
21)	B Endrin ke...	7.684	6.877	217.9E6	283.4E6	105.854	108.876

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101823\
Data File : PD078960.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2023 18:29
Operator : AR\AJ
Sample : 04885-06MSD 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 22:15:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101623CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 05:35:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

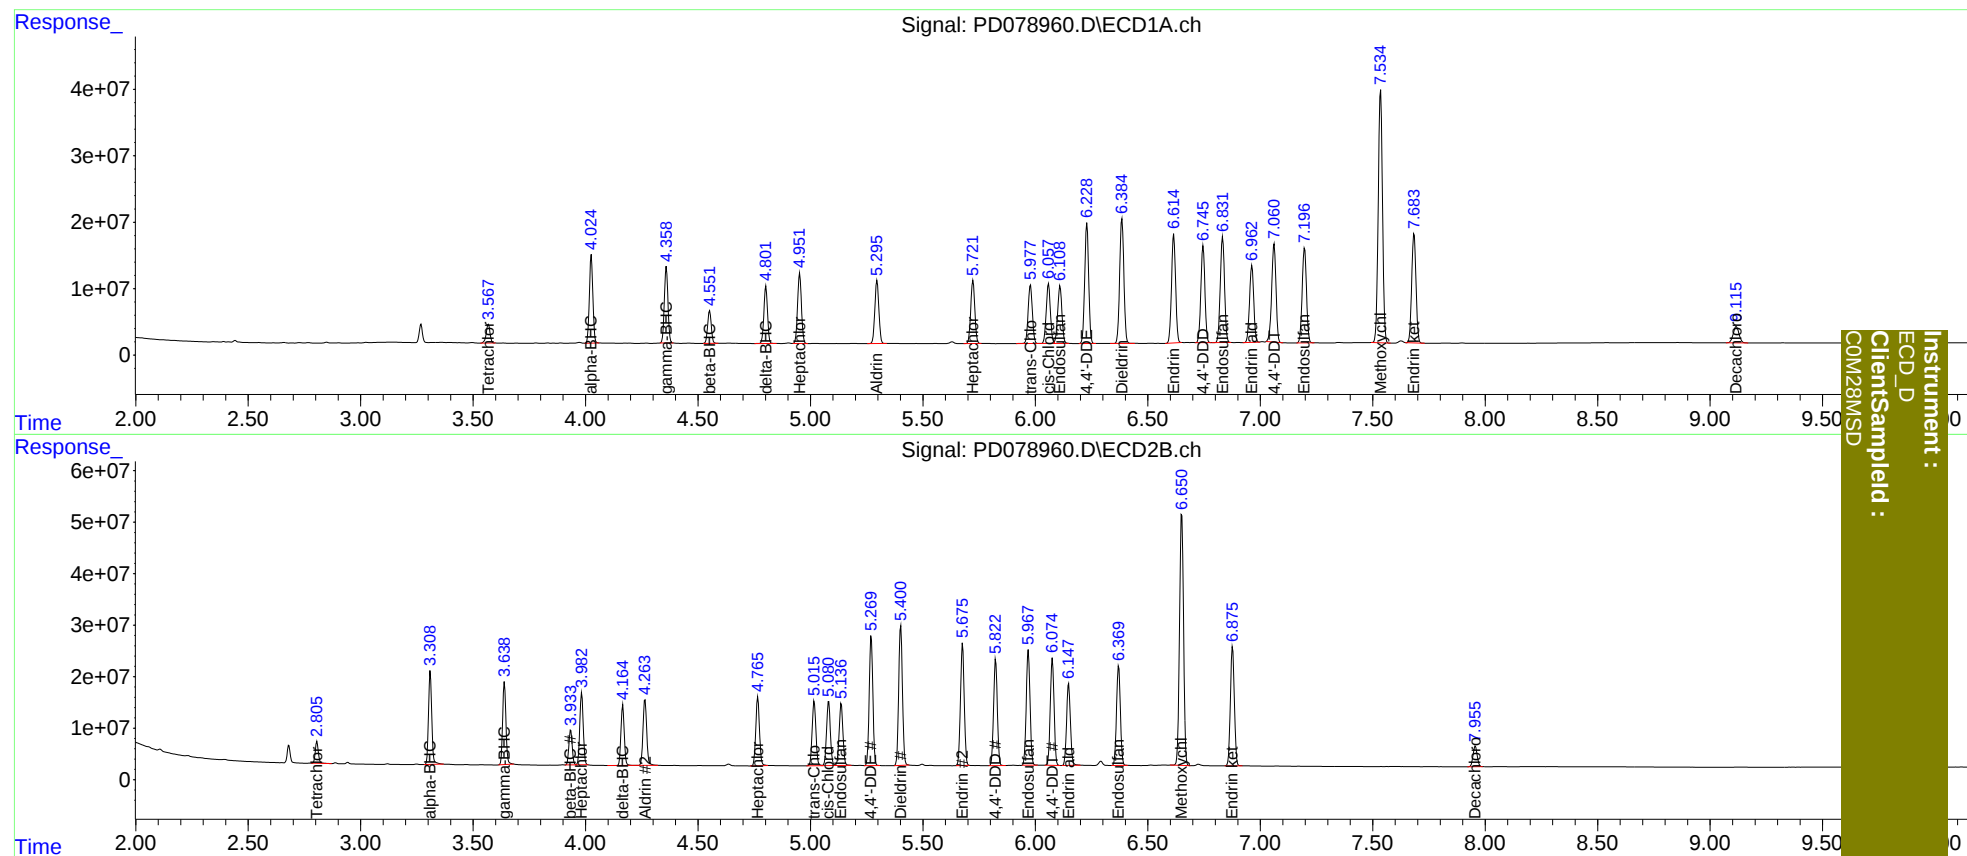

Instrument :
ECD_D
ClientSampled :
COM28MSD