


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101918\
Data File : PD049867.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Oct 2018 19:57
Operator : AJ\SJ
Sample : RESC30
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 05:14:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101918CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 19 05:13:06 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

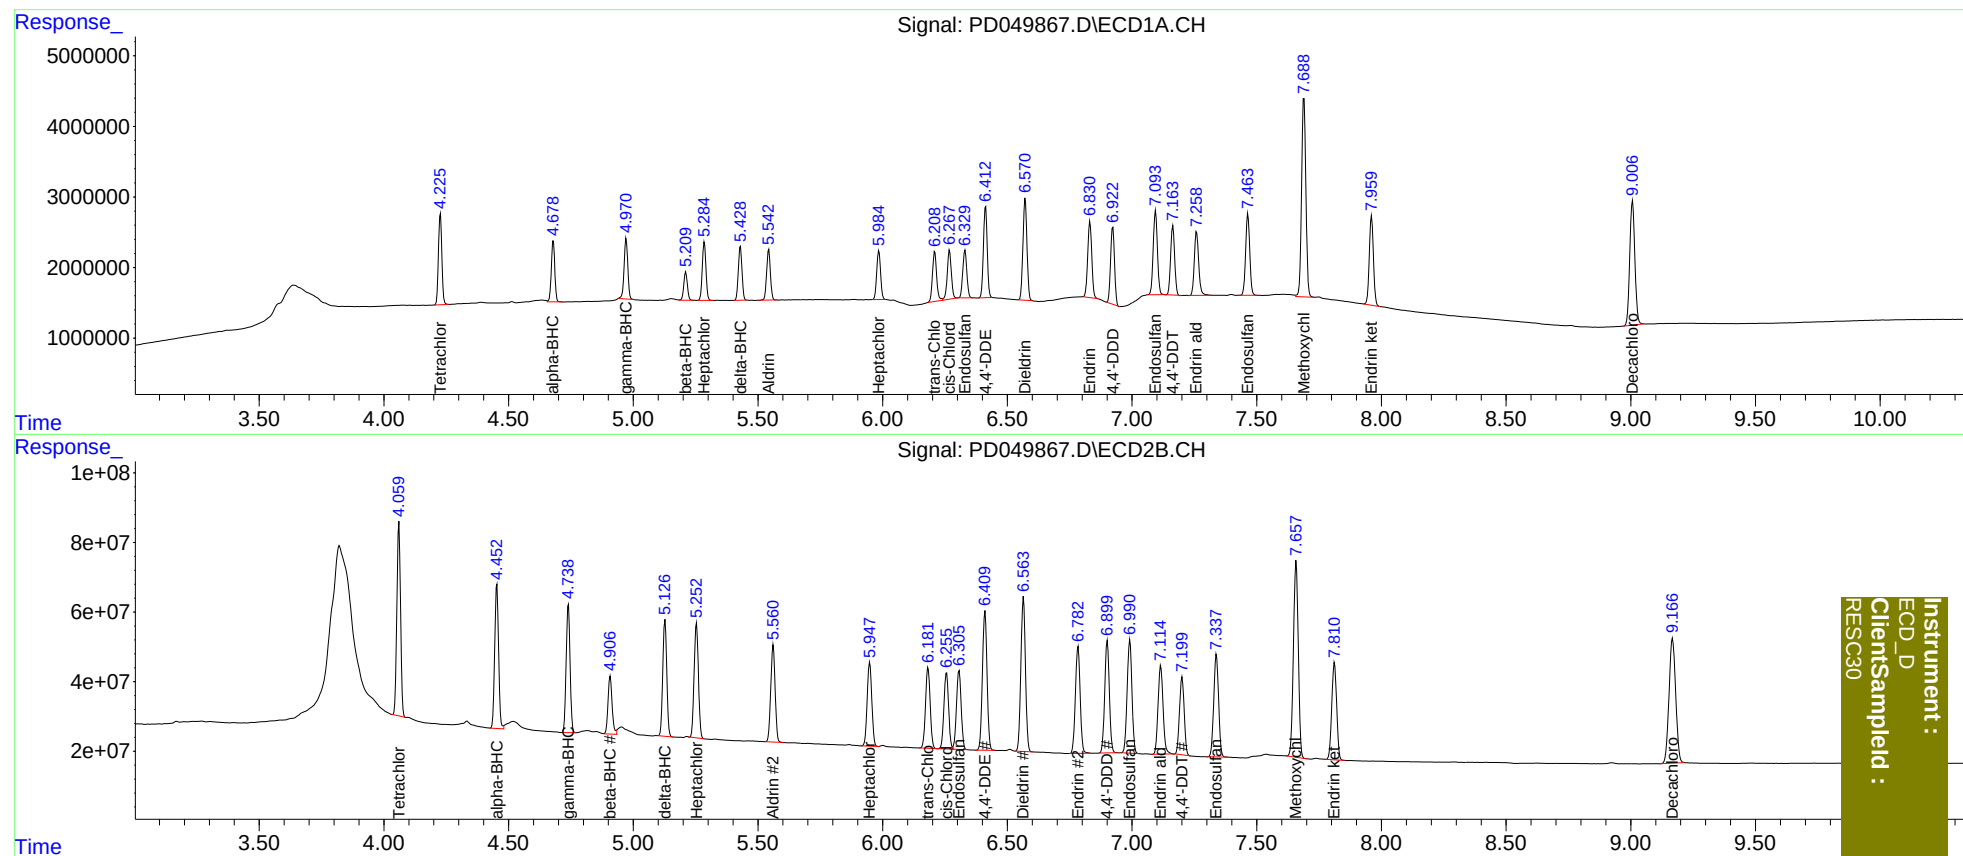

Instrument :
ECD_D
ClientSampled :
RESC30

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101918\
 Data File : PD049867.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Oct 2018 19:57
 Operator : AJ\SJ
 Sample : RESC30
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC30

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 05:14:03 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101918CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 19 05:13:06 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.226	4.060	12411611	567.2E6	18.764	18.753
27)	SA Decachlor...	9.007	9.168	25254052	665.4E6	37.798	37.446
Target Compounds							
2)	A alpha-BHC	4.679	4.453	8433372	445.5E6	9.392	9.927
3)	MA gamma-BHC...	4.972	4.740	8873771	402.3E6	9.626	9.985
4)	MA Heptachlor	5.285	5.254	8452353	392.3E6	9.693	9.974
5)	MB Aldrin	5.543	5.561	7597946	340.9E6	9.448	9.888
6)	B beta-BHC	5.211	4.908	4080959	188.0E6	10.053	10.155
7)	B delta-BHC	5.430	5.127	7733074	374.1E6	9.234	9.772
8)	B Heptachlo...	5.985	5.948	7524186	309.2E6	9.691	9.955
9)	A Endosulfan I	6.330	6.307	7678583	296.7E6	9.913	10.300
10)	B trans-Chl...	6.209	6.182	8239948	301.6E6	9.823	9.882
11)	B cis-Chlor...	6.268	6.256	8031563	285.9E6	9.818	9.894
12)	B 4,4'-DDE	6.413	6.411	13800124	518.0E6	18.587	19.545
13)	MA Dieldrin	6.572	6.565	16269085	568.5E6	18.861	19.764
14)	MA Endrin	6.831	6.784	12310511	410.9E6	19.601	20.308
15)	B Endosulfa...	7.094	6.991	13975236	438.1E6	19.119	19.798
16)	A 4,4'-DDD	6.923	6.901	11896409	416.3E6	18.645	19.758
17)	MA 4,4'-DDT	7.164	7.201	10898502	290.2E6	18.247	18.506
18)	B Endrin al...	7.259	7.115	11069100	354.6E6	20.194	20.718
19)	B Endosulfa...	7.465	7.338	13224448	399.8E6	19.349	19.802
20)	A Methoxychlor	7.689	7.658	33792744	761.2E6	97.004	96.049
21)	B Endrin ke...	7.961	7.812	14563207	378.7E6	20.628	20.735

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.