

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101920\
 Data File : PD059818.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2020 16:24
 Operator : DD\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 06:58:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101920.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 20 06:57:35 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.507	4.024	180.4E6	245.7E6	99.125	99.321
28)	SA Decachlor...	8.307	9.107	153.0E6	176.0E6	98.167	97.016
Target Compounds							
23)	Chlordane-1	4.389	5.023	56087759	92263070	965.187	979.406
24)	Chlordane-2	4.896	5.491	57685358	91782721	954.699	946.448
25)	Chlordane-3	5.472	6.139	193.2E6	378.5E6	1006.501	1001.730
26)	Chlordane-4	5.530	6.214	154.5E6	444.0E6	995.292	991.959
27)	Chlordane-5	6.373	7.020	66260474	82575349	975.027	993.712



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101920\
Data File : PD059818.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2020 16:24
Operator : DD\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 06:58:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101920.M
Quant Title : GC Extractables
QLast Update : Tue Oct 20 06:57:35 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

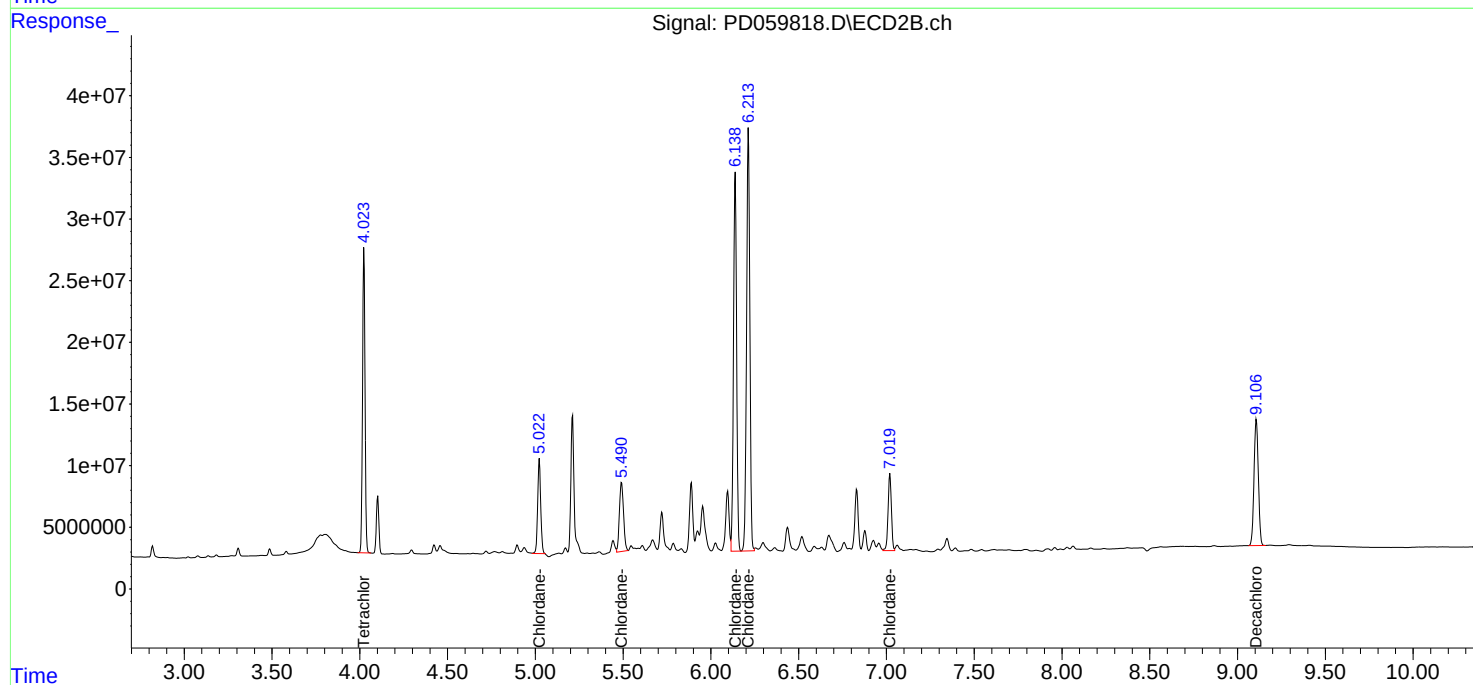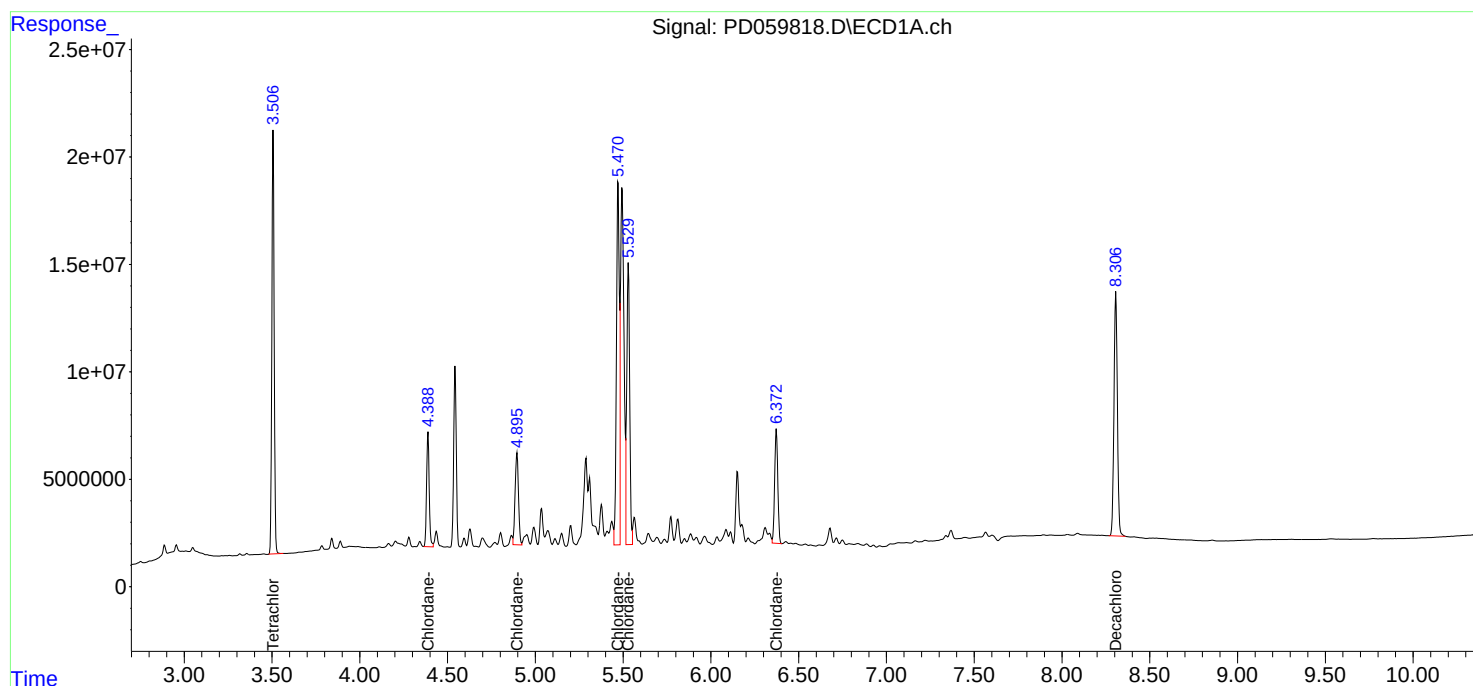


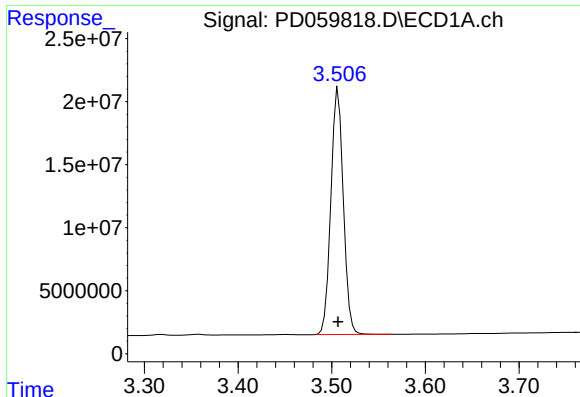

#1 Tetrachloro-m-xylene


R.T.: 3.507 min
Delta R.T.: 0.000 min
Response: 180436534
Conc: 99.13 ng/ml

Instrument :
ECD_D
ClientSampleId :

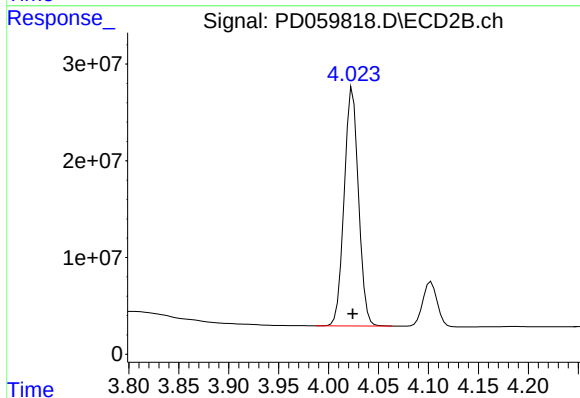


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 245728744
Conc: 99.32 ng/ml

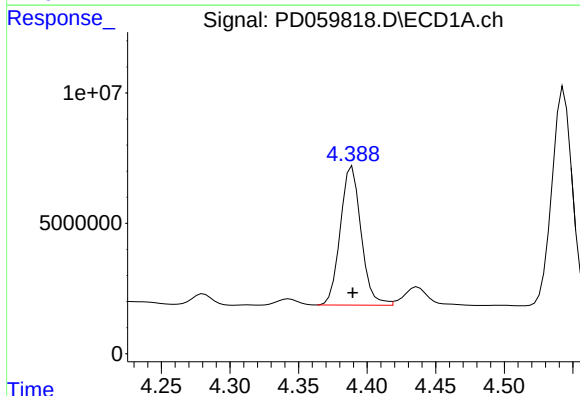


#23 Chlordane-1

R.T.: 4.389 min
Delta R.T.: 0.000 min
Response: 56087759
Conc: 965.19 ng/ml

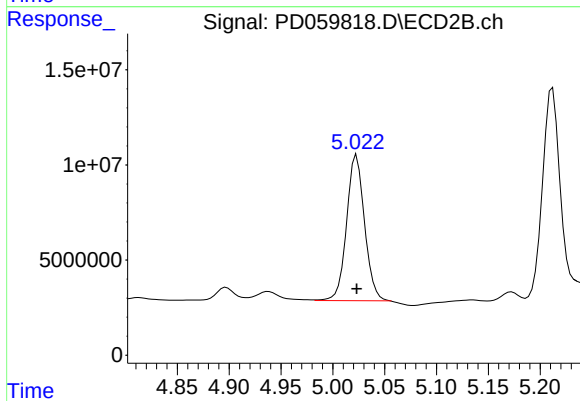

#23 Chlordane-1


R.T.: 5.023 min
Delta R.T.: 0.000 min
Response: 92263070
Conc: 979.41 ng/ml

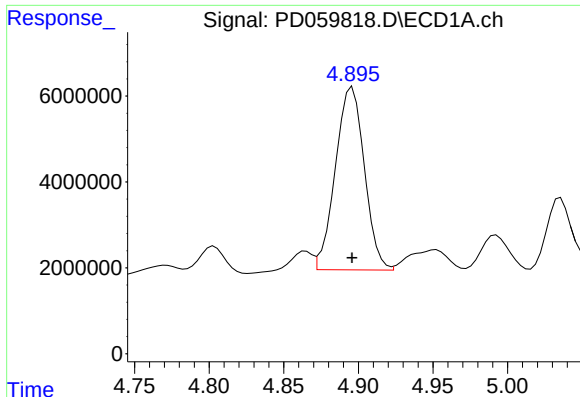

#24 Chlordane-2


R.T.: 4.896 min
Delta R.T.: 0.000 min
Response: 57685358
Conc: 954.70 ng/ml

Instrument :
ECD_D
ClientSampleId :

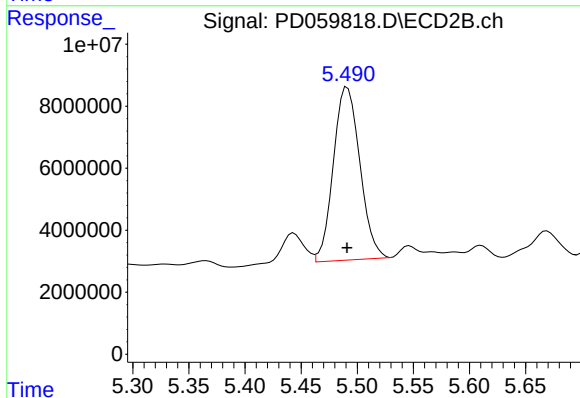


#24 Chlordane-2

R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 91782721
Conc: 946.45 ng/ml

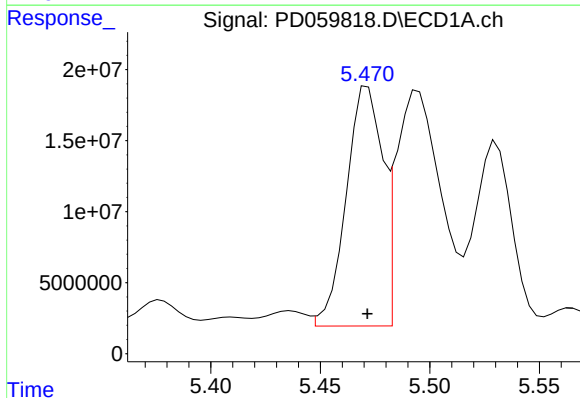


#25 Chlordane-3

R.T.: 5.472 min
Delta R.T.: 0.000 min
Response: 193153517
Conc: 1006.50 ng/ml

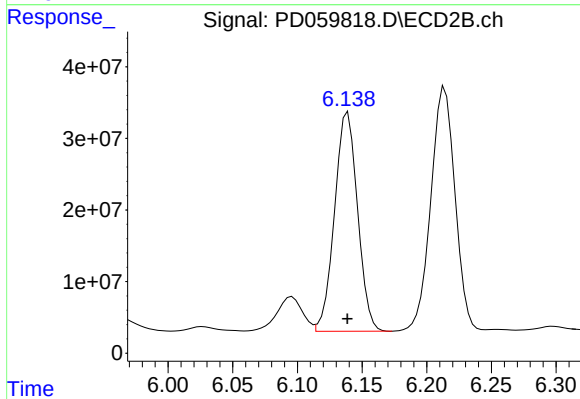

#25 Chlordane-3


R.T.: 6.139 min
Delta R.T.: 0.000 min
Response: 378538229
Conc: 1001.73 ng/ml

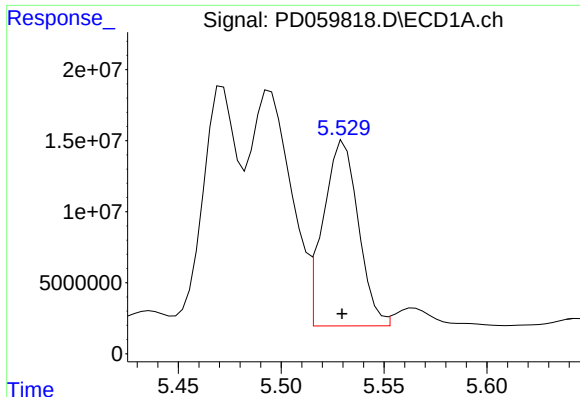

#26 Chlordane-4


R.T.: 5.530 min
Delta R.T.: 0.000 min
Response: 154521012
Conc: 995.29 ng/ml

Instrument :
ECD_D
ClientSampleId :

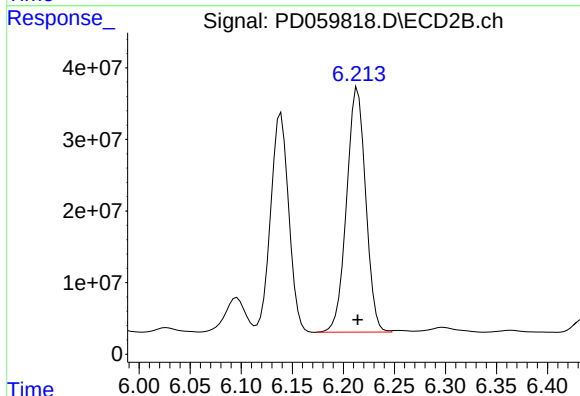


#26 Chlordane-4

R.T.: 6.214 min
Delta R.T.: 0.000 min
Response: 443972700
Conc: 991.96 ng/ml

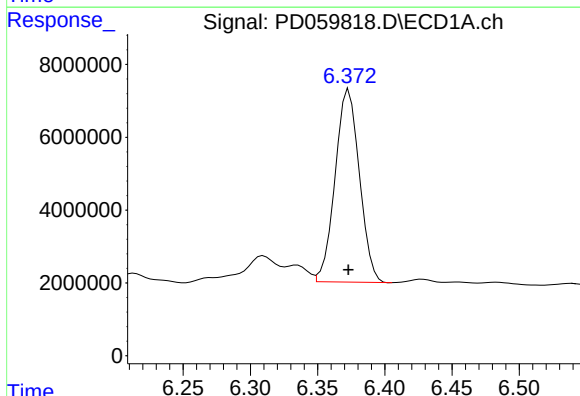


#27 Chlordane-5

R.T.: 6.373 min
Delta R.T.: 0.000 min
Response: 66260474
Conc: 975.03 ng/ml

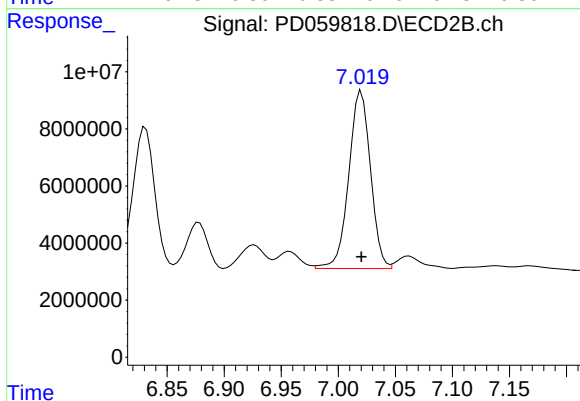

#27 Chlordane-5


R.T.: 7.020 min
Delta R.T.: 0.000 min
Response: 82575349
Conc: 993.71 ng/ml

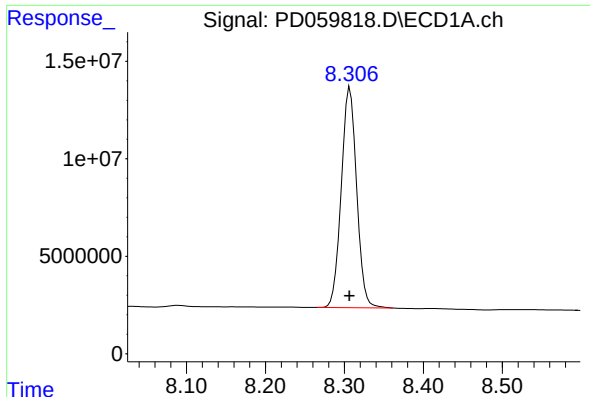

#28 Decachlorobiphenyl

R.T.: 8.307 min
Delta R.T.: 0.000 min
Response: 152974272
Conc: 98.17 ng/ml

Instrument :
ECD_D
ClientSampleId :

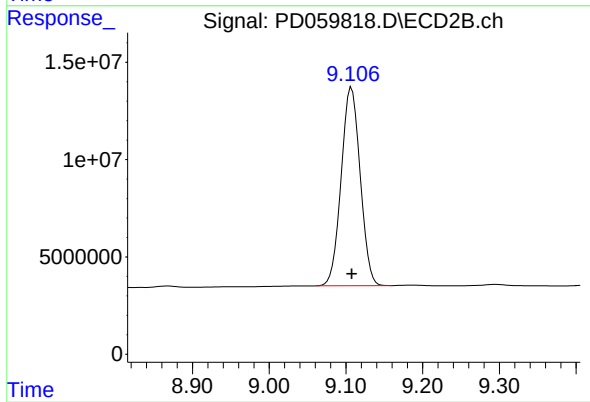

#28 Decachlorobiphenyl

R.T.: 9.107 min
Delta R.T.: 0.000 min
Response: 176047789
Conc: 97.02 ng/ml