

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101920\
 Data File : PD059821.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2020 17:06
 Operator : DD\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 06:58:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101920.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 20 06:57:35 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.507	4.024	43998807	60659540	24.171	24.518
28)	SA Decachlor...	8.306	9.108	39500136	45995854	25.348	25.347
Target Compounds							
23)	Chlordane-1	4.389	5.023	14748304	23591632	253.797	250.434
24)	Chlordane-2	4.895	5.491	15295447	25087322	253.141	258.696
25)	Chlordane-3	5.471	6.139	45914045	91353591	239.253	241.750
26)	Chlordane-4	5.530	6.214	37964403	109.0E6	244.534	243.529
27)	Chlordane-5	6.373	7.020	17437891	20125206	256.600	242.187



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101920\
Data File : PD059821.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2020 17:06
Operator : DD\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 06:58:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101920.M
Quant Title : GC Extractables
QLast Update : Tue Oct 20 06:57:35 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

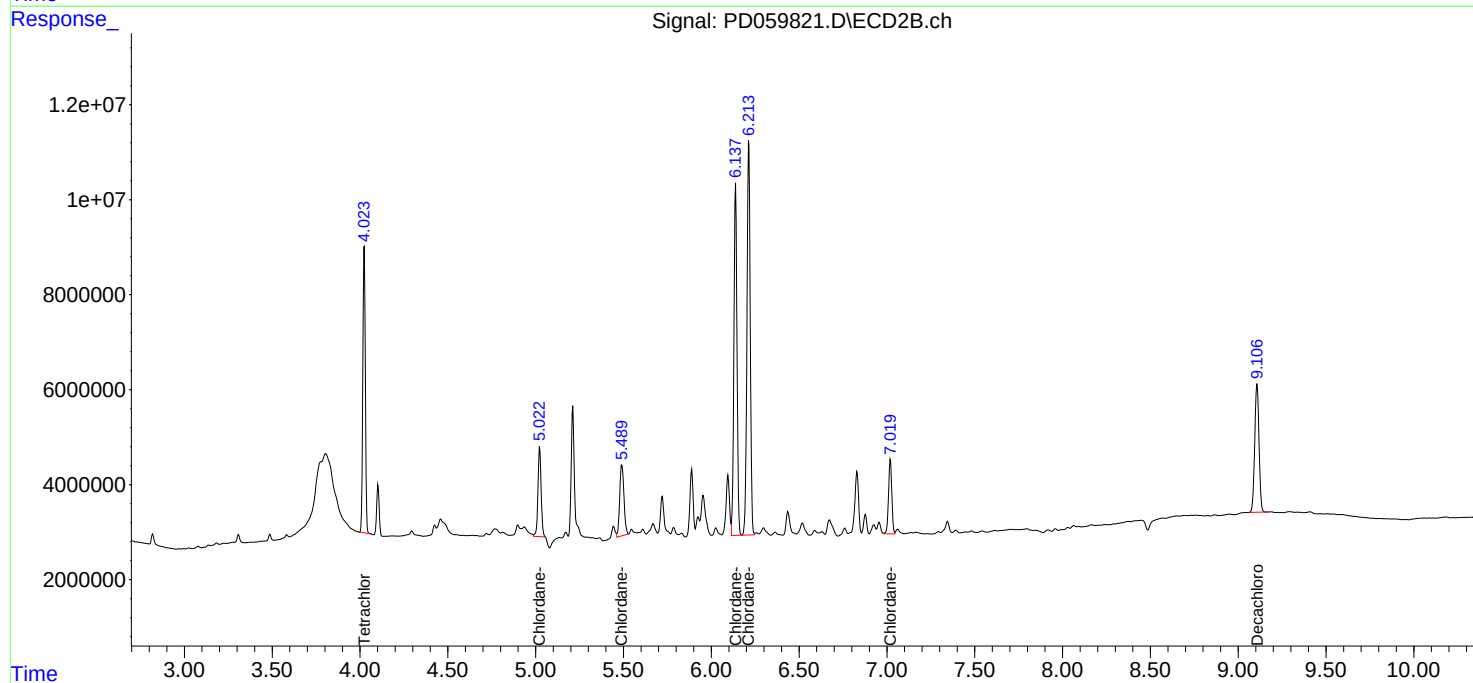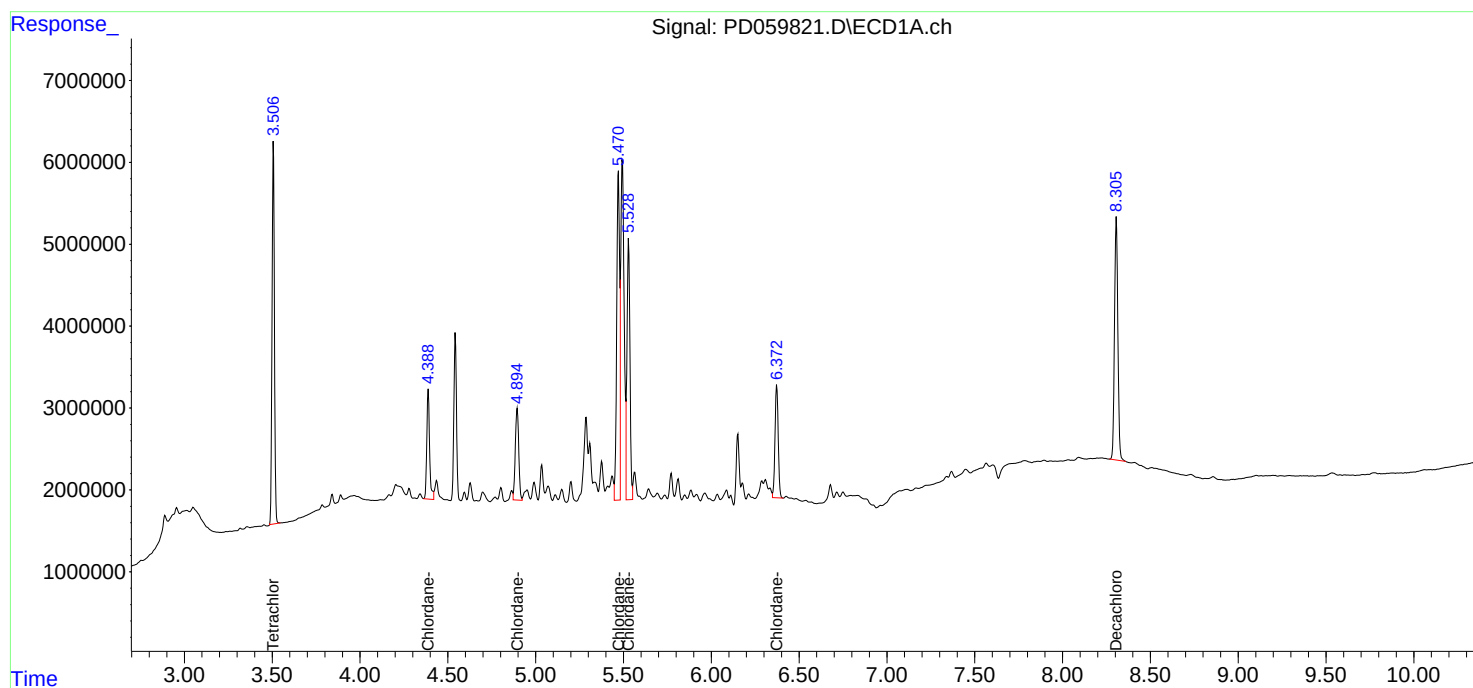


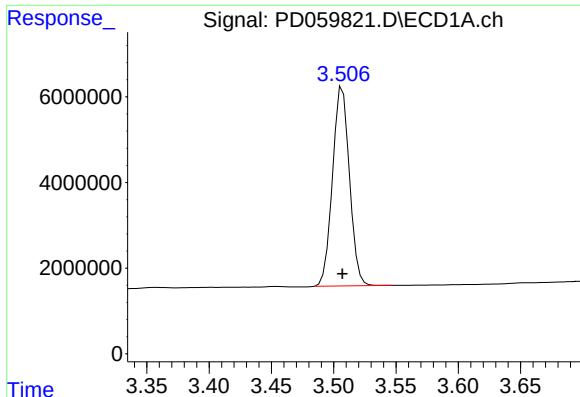

#1 Tetrachloro-m-xylene


R.T.: 3.507 min
Delta R.T.: 0.000 min
Response: 43998807
Conc: 24.17 ng/ml

Instrument :
ECD_D
ClientSampleId :

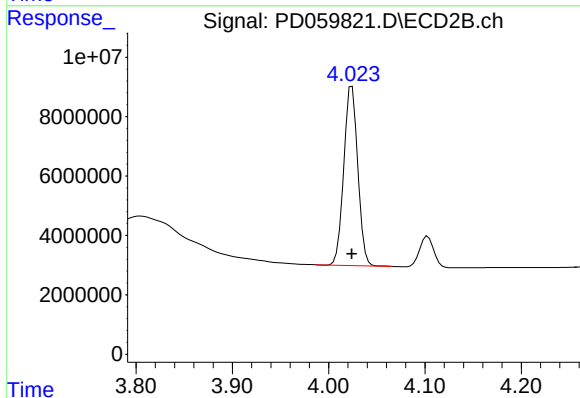


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 60659540
Conc: 24.52 ng/ml

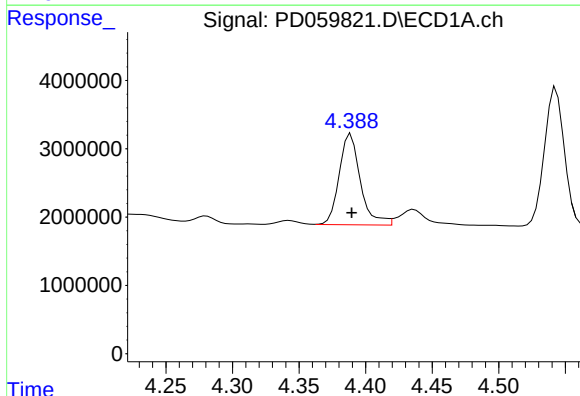


#23 Chlordane-1

R.T.: 4.389 min
Delta R.T.: 0.000 min
Response: 14748304
Conc: 253.80 ng/ml

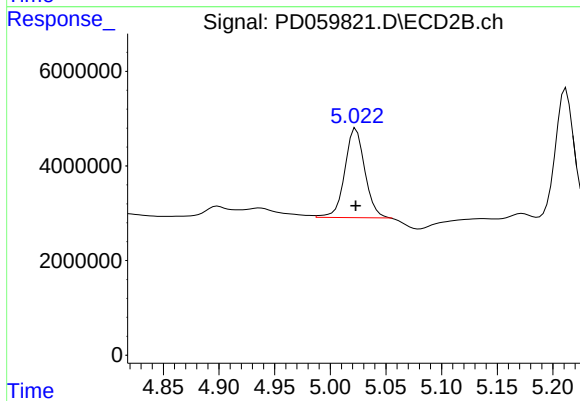

#23 Chlordane-1


R.T.: 5.023 min
Delta R.T.: 0.000 min
Response: 23591632
Conc: 250.43 ng/ml

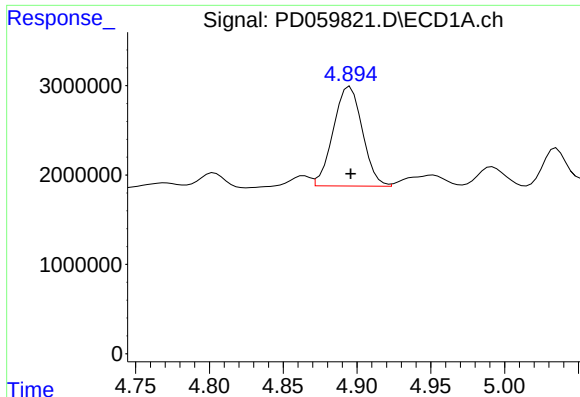

#24 Chlordane-2


R.T.: 4.895 min
Delta R.T.: 0.000 min
Response: 15295447
Conc: 253.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

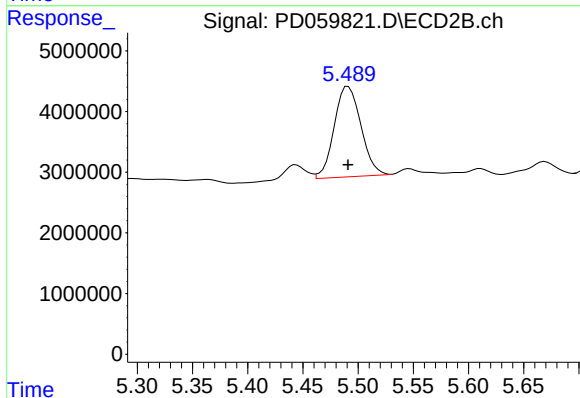


#24 Chlordane-2

R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 25087322
Conc: 258.70 ng/ml

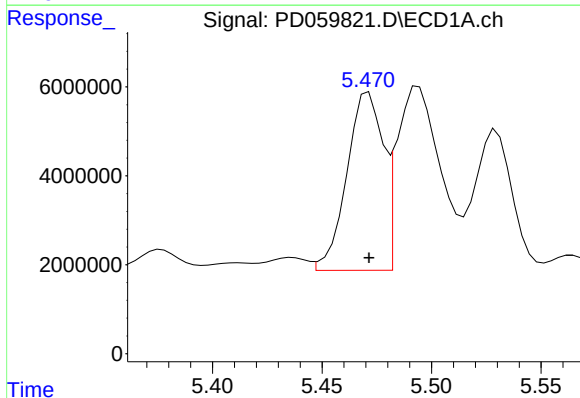


#25 Chlordane-3

R.T.: 5.471 min
Delta R.T.: 0.000 min
Response: 45914045
Conc: 239.25 ng/ml

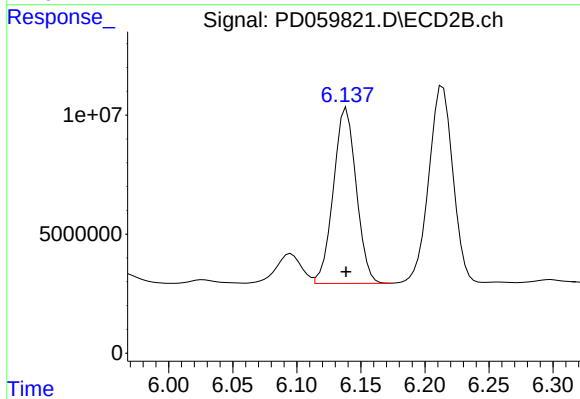

#25 Chlordane-3


R.T.: 6.139 min
Delta R.T.: 0.000 min
Response: 91353591
Conc: 241.75 ng/ml

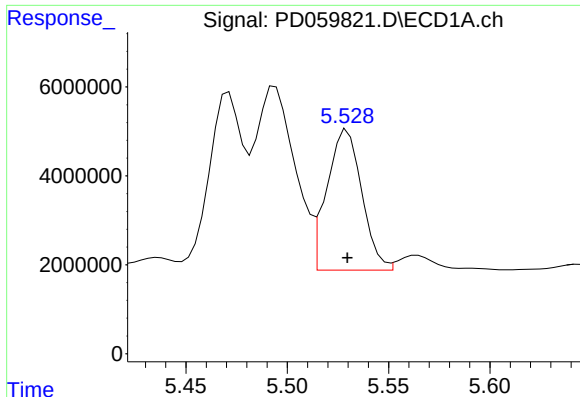

#26 Chlordane-4


R.T.: 5.530 min
Delta R.T.: 0.000 min
Response: 37964403
Conc: 244.53 ng/ml

Instrument :
ECD_D
ClientSampleId :

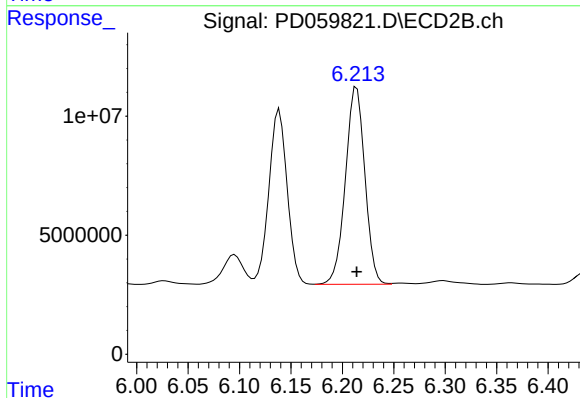


#26 Chlordane-4

R.T.: 6.214 min
Delta R.T.: 0.000 min
Response: 108996492
Conc: 243.53 ng/ml

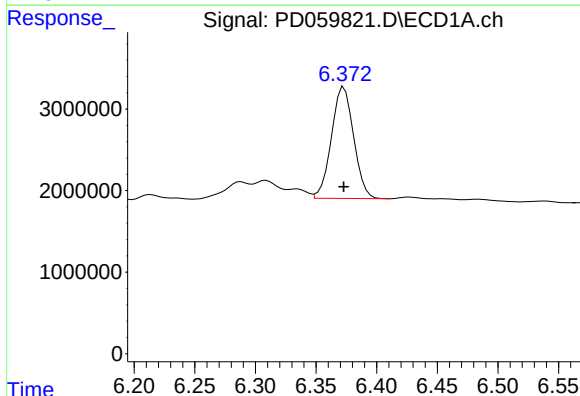


#27 Chlordane-5

R.T.: 6.373 min
Delta R.T.: 0.000 min
Response: 17437891
Conc: 256.60 ng/ml

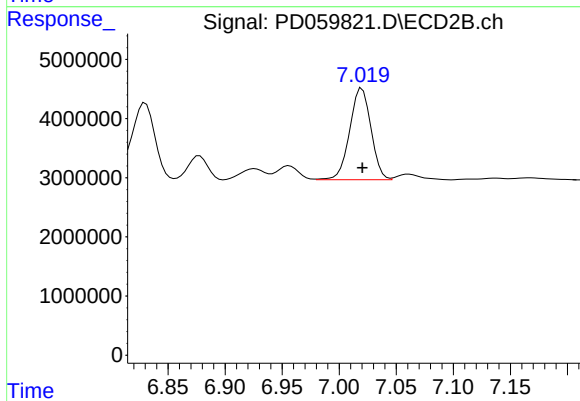

#27 Chlordane-5


R.T.: 7.020 min
Delta R.T.: 0.000 min
Response: 20125206
Conc: 242.19 ng/ml

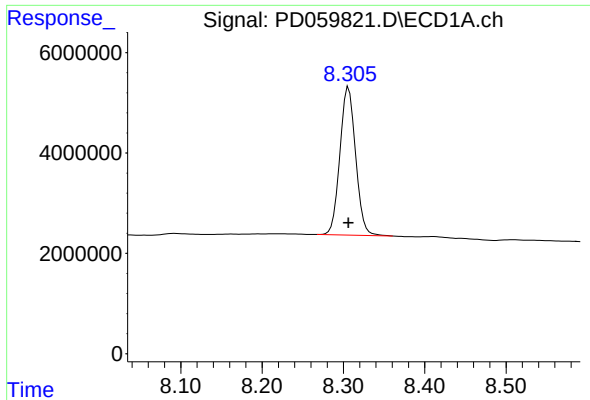

#28 Decachlorobiphenyl

R.T.: 8.306 min
Delta R.T.: 0.000 min
Response: 39500136
Conc: 25.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

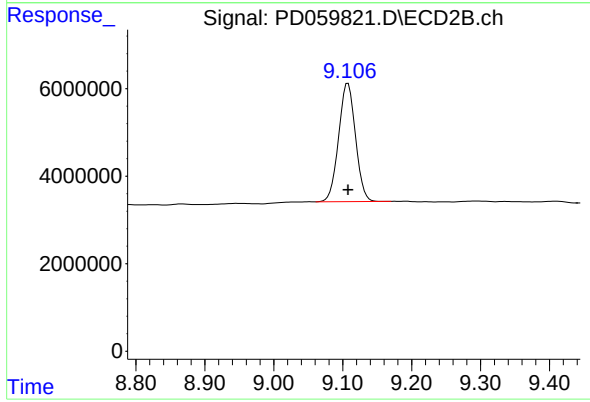

#28 Decachlorobiphenyl

R.T.: 9.108 min
Delta R.T.: 0.000 min
Response: 45995854
Conc: 25.35 ng/ml