

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101920\
 Data File : PD059812.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2020 14:59
 Operator : DD\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 07:15:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101920.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 20 07:13:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.508	4.024	40051271	66447390	26.973	27.072
28)	SA Decachlor...	8.307	9.107	41445712	47804025	26.806	26.398
Target Compounds							
9)	A Endosulfan I	5.583	6.262	24194838	34156075	12.774	12.794
10)	B gamma-Chl...	5.471	6.138	26174321	35928313	12.689	12.292
12)	B 4,4'-DDE	5.695	6.367	52548059	69357895	25.929	25.289
13)	MA Dieldrin	5.830	6.520	52795662	73477055	25.695	25.594
19)	B Endosulfa...	6.746	7.292	40260612	57060905	24.904	24.808
20)	A Methoxychlor	7.006	7.613	117.4E6	153.3E6	123.976	120.395
21)	B Endrin ke...	7.241	7.765	47217347	62543057	25.184	25.169



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101920\
Data File : PD059812.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2020 14:59
Operator : DD\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleID :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 07:15:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101920.M
Quant Title : GC Extractables
QLast Update : Tue Oct 20 07:13:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

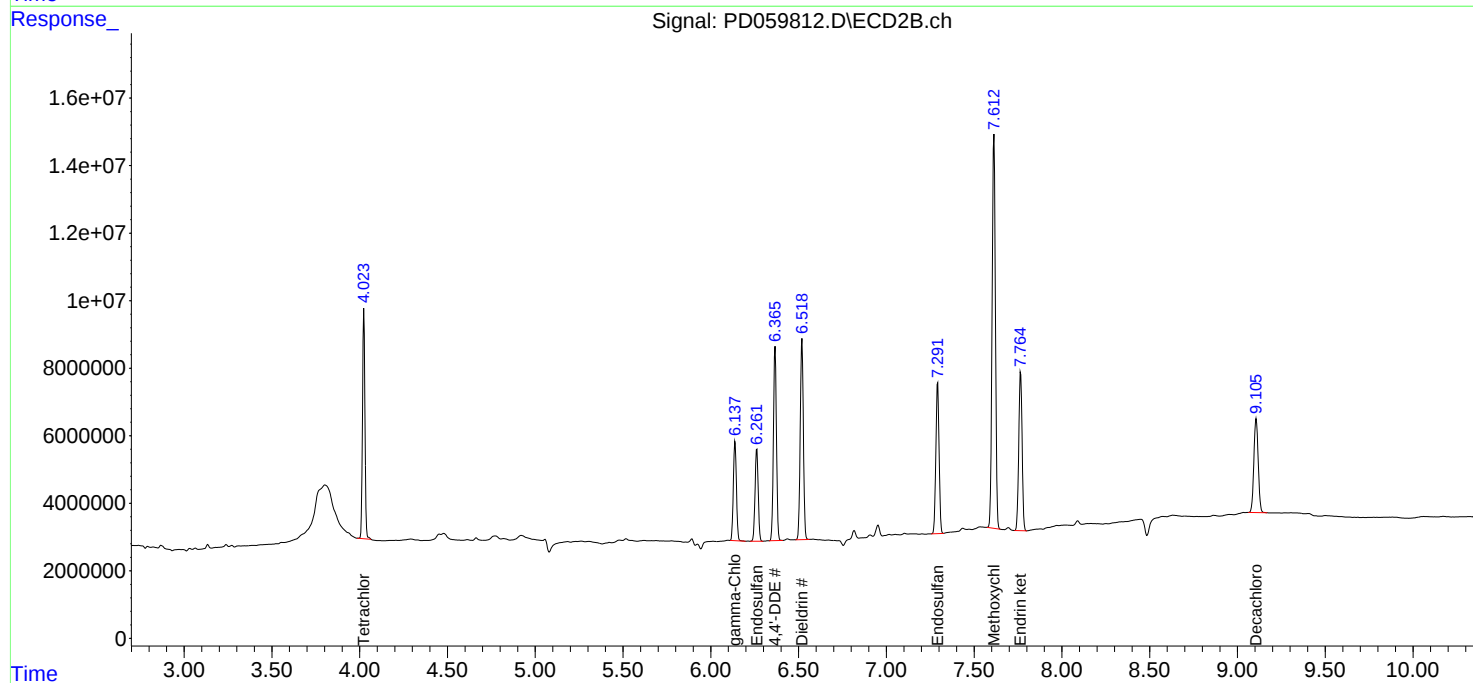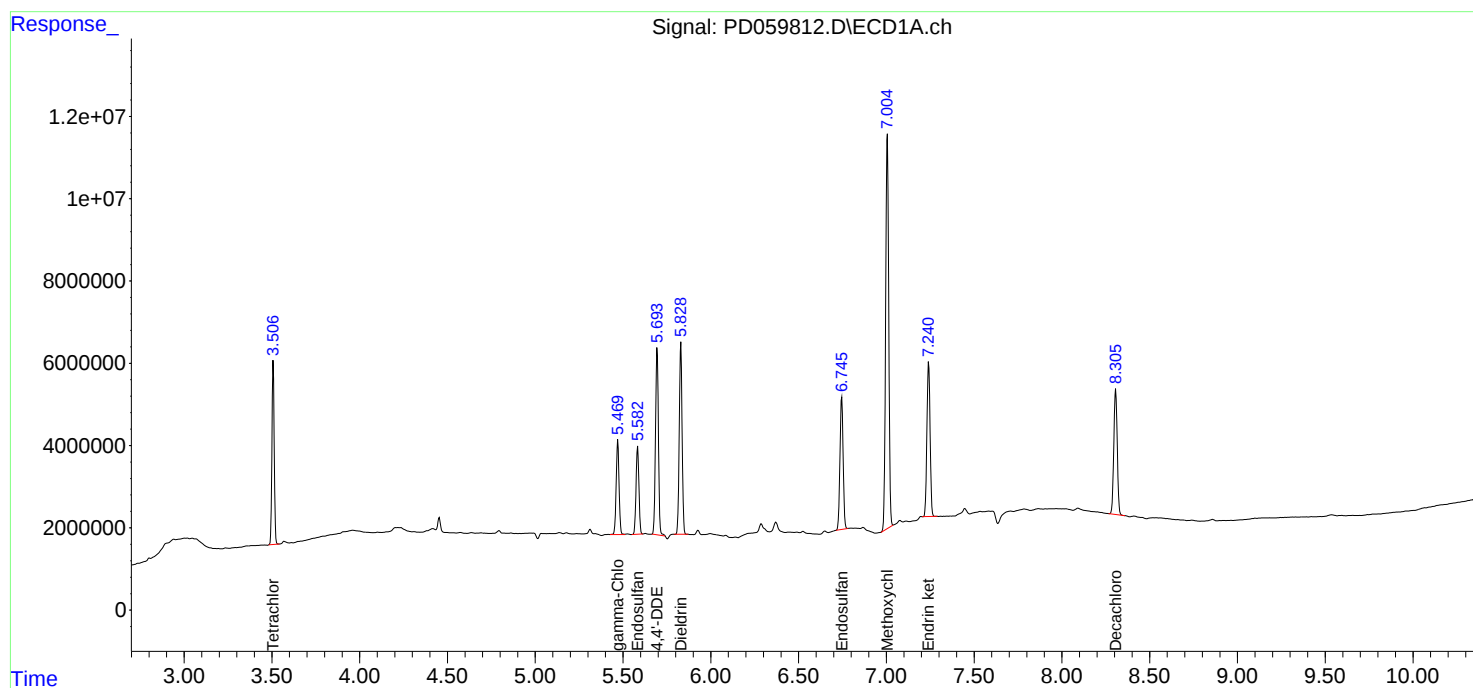


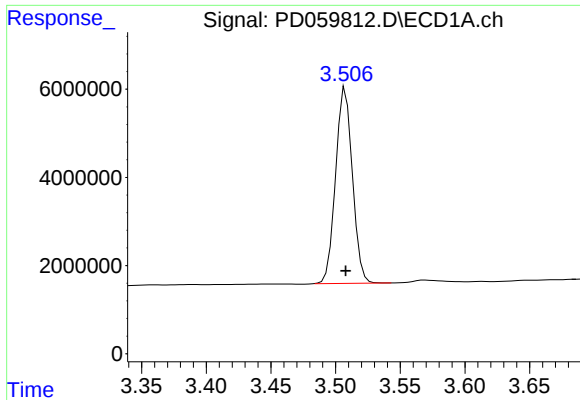

#1 Tetrachloro-m-xylene


R.T.: 3.508 min
Delta R.T.: 0.000 min
Response: 40051271
Conc: 26.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

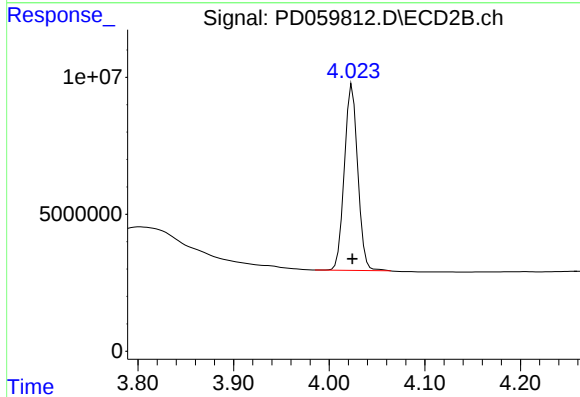


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 66447390
Conc: 27.07 ng/ml

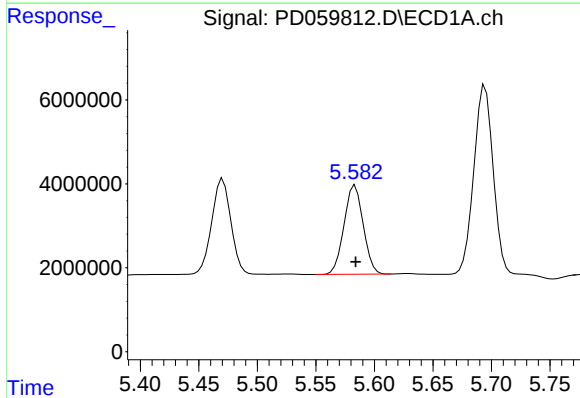


#9 Endosulfan I

R.T.: 5.583 min
Delta R.T.: 0.000 min
Response: 24194838
Conc: 12.77 ng/ml

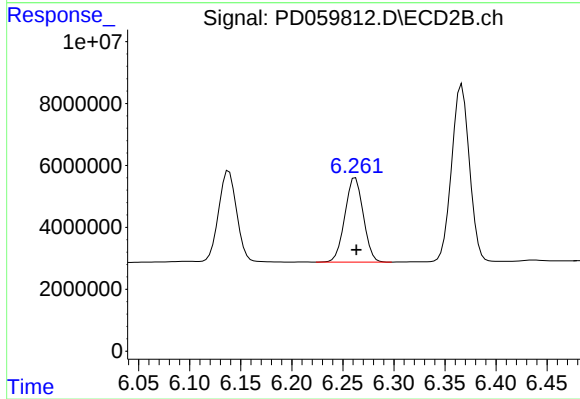

#9 Endosulfan I


R.T.: 6.262 min
Delta R.T.: 0.000 min
Response: 34156075
Conc: 12.79 ng/ml

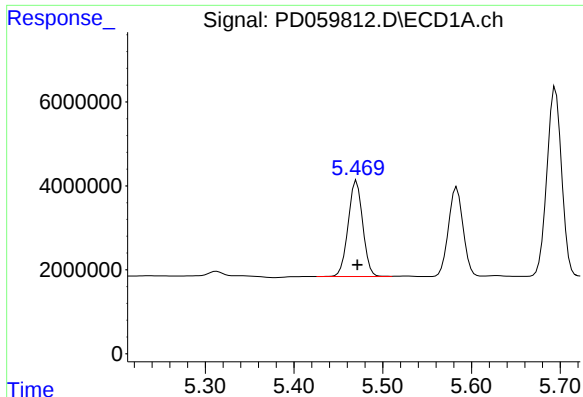

#10 gamma-Chlordane


R.T.: 5.471 min
Delta R.T.: 0.000 min
Response: 26174321
Conc: 12.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

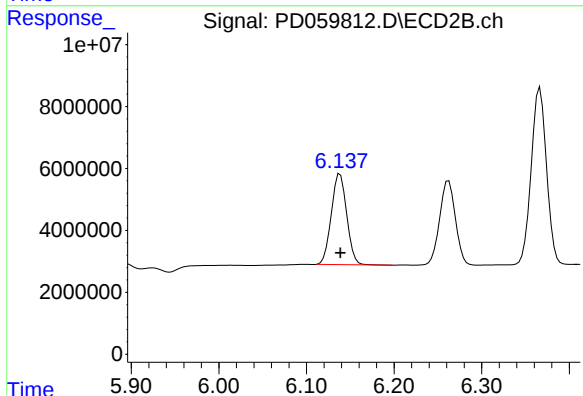


#10 gamma-Chlordane

R.T.: 6.138 min
Delta R.T.: 0.000 min
Response: 35928313
Conc: 12.29 ng/ml

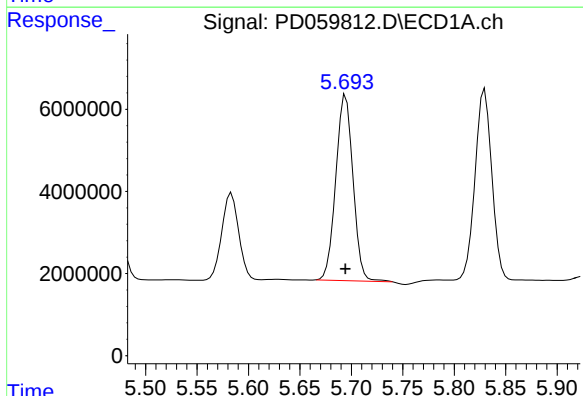


#12 4,4'-DDE

R.T.: 5.695 min
Delta R.T.: 0.000 min
Response: 52548059
Conc: 25.93 ng/ml

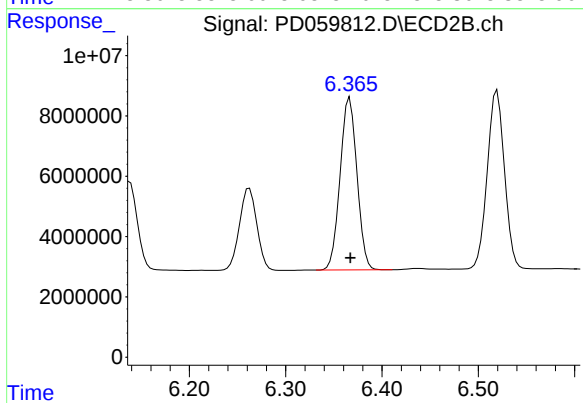

#12 4,4'-DDE


R.T.: 6.367 min
Delta R.T.: 0.000 min
Response: 69357895
Conc: 25.29 ng/ml

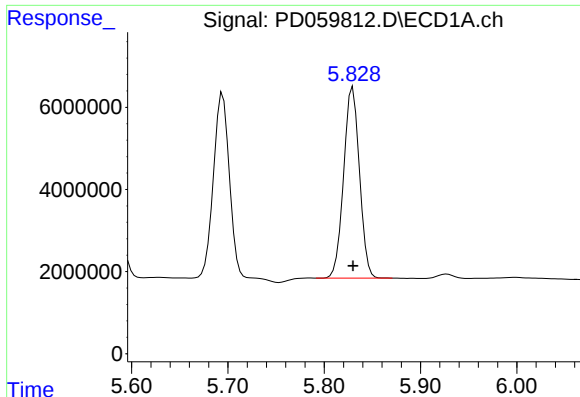

#13 Dieldrin


R.T.: 5.830 min
Delta R.T.: 0.000 min
Response: 52795662
Conc: 25.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

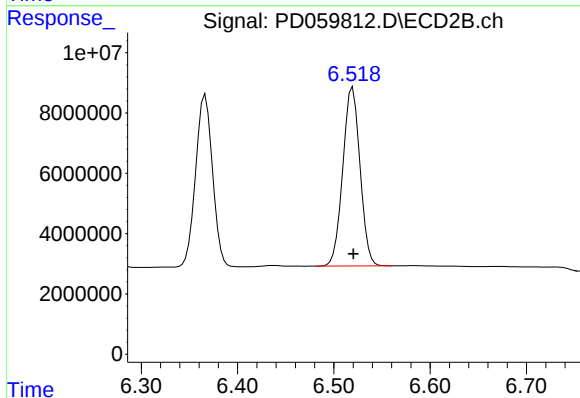


#13 Dieldrin

R.T.: 6.520 min
Delta R.T.: 0.000 min
Response: 73477055
Conc: 25.59 ng/ml

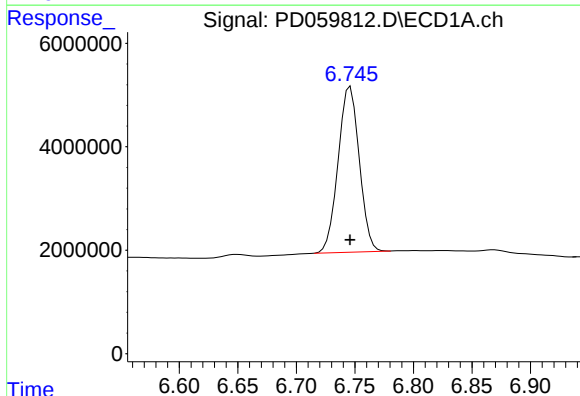


#19 Endosulfan Sulfate

R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 40260612
Conc: 24.90 ng/ml

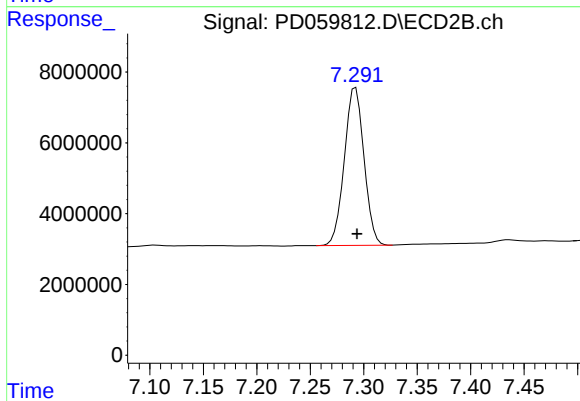

#19 Endosulfan Sulfate


R.T.: 7.292 min
Delta R.T.: -0.001 min
Response: 57060905
Conc: 24.81 ng/ml

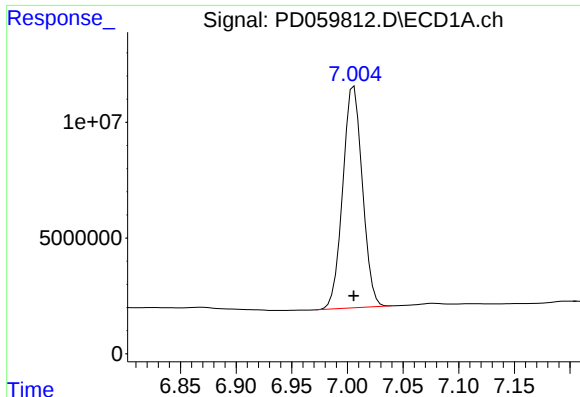

#20 Methoxychlor


R.T.: 7.006 min
Delta R.T.: 0.000 min
Response: 117441328
Conc: 123.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

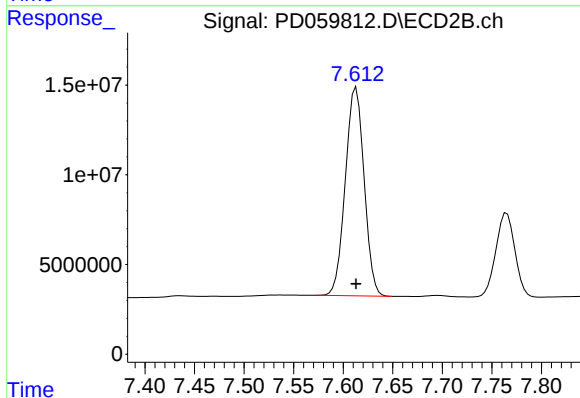


#20 Methoxychlor

R.T.: 7.613 min
Delta R.T.: 0.000 min
Response: 153252439
Conc: 120.40 ng/ml

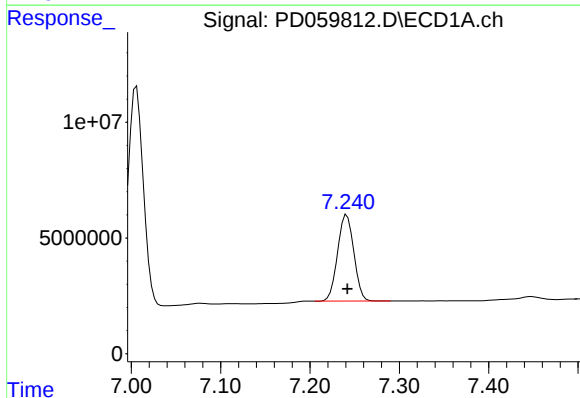


#21 Endrin ketone

R.T.: 7.241 min
Delta R.T.: 0.000 min
Response: 47217347
Conc: 25.18 ng/ml

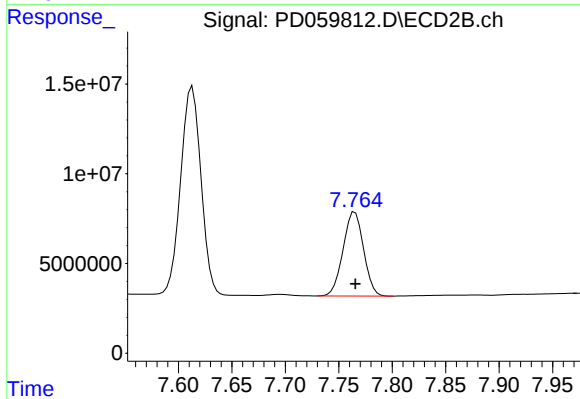

#21 Endrin ketone


R.T.: 7.765 min
Delta R.T.: 0.000 min
Response: 62543057
Conc: 25.17 ng/ml

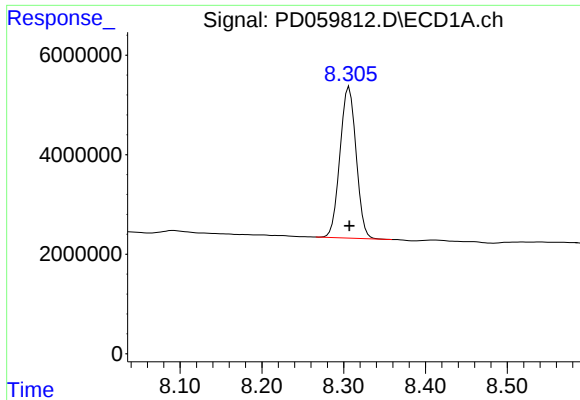

#28 Decachlorobiphenyl

R.T.: 8.307 min
Delta R.T.: 0.000 min
Response: 41445712
Conc: 26.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

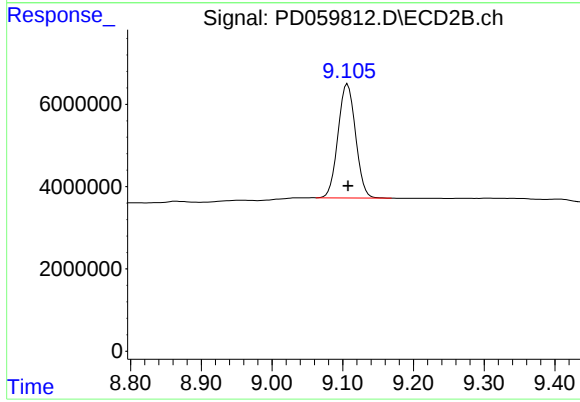

#28 Decachlorobiphenyl

R.T.: 9.107 min
Delta R.T.: -0.001 min
Response: 47804025
Conc: 26.40 ng/ml