

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101920\
 Data File : PD059819.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2020 16:38
 Operator : DD\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 07:05:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101920.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 20 06:57:35 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.507	4.024	134.6E6	184.3E6	73.928	74.507
28)	SA Decachlor...	8.307	9.107	115.1E6	133.6E6	73.861	73.611
Target Compounds							
23)	Chlordane-1	4.389	5.023	42350847	70294257	728.795	746.199
24)	Chlordane-2	4.895	5.490	44076401	70035478	729.469	722.194
25)	Chlordane-3	5.471	6.138	142.7E6	283.1E6	743.680	749.066
26)	Chlordane-4	5.530	6.214	115.3E6	333.3E6	742.739	744.675
27)	Chlordane-5	6.374	7.020	50035715	61803874	736.279	743.748



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101920\
Data File : PD059819.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2020 16:38
Operator : DD\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 07:05:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101920.M
Quant Title : GC Extractables
QLast Update : Tue Oct 20 06:57:35 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

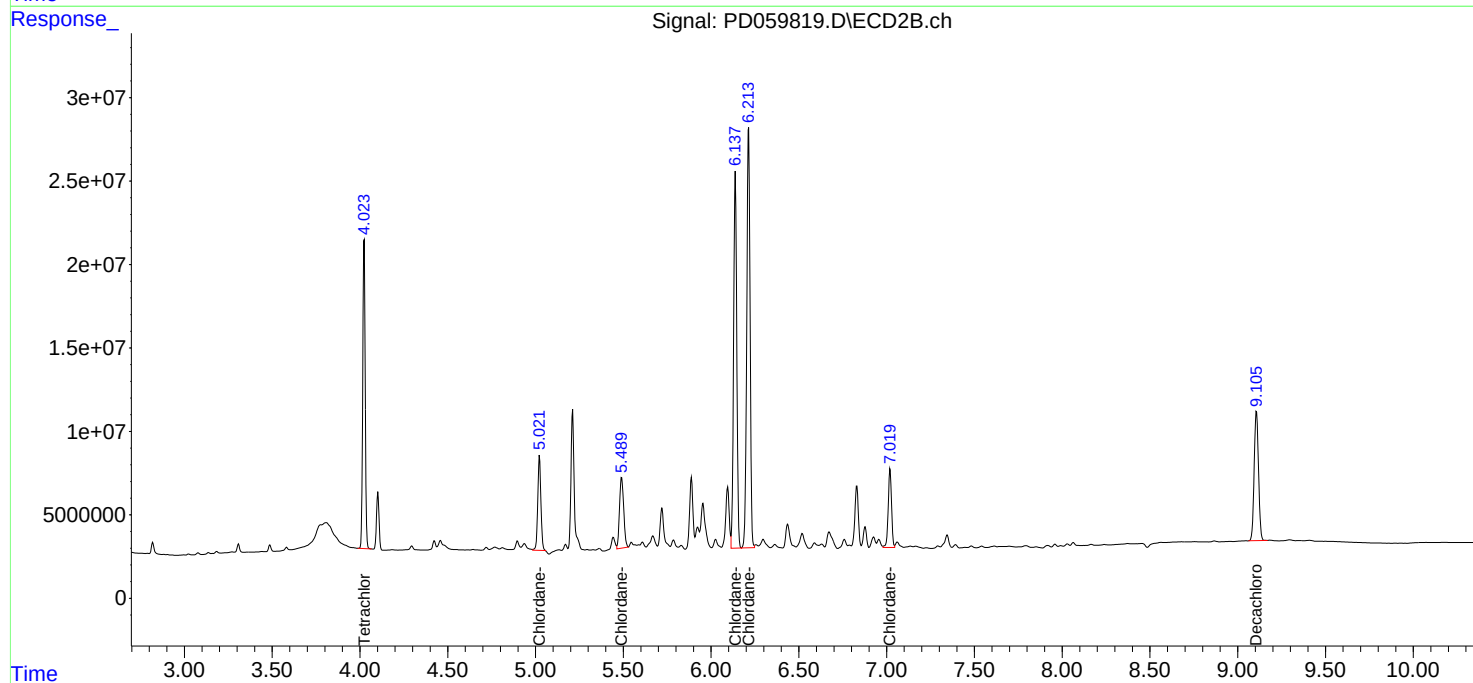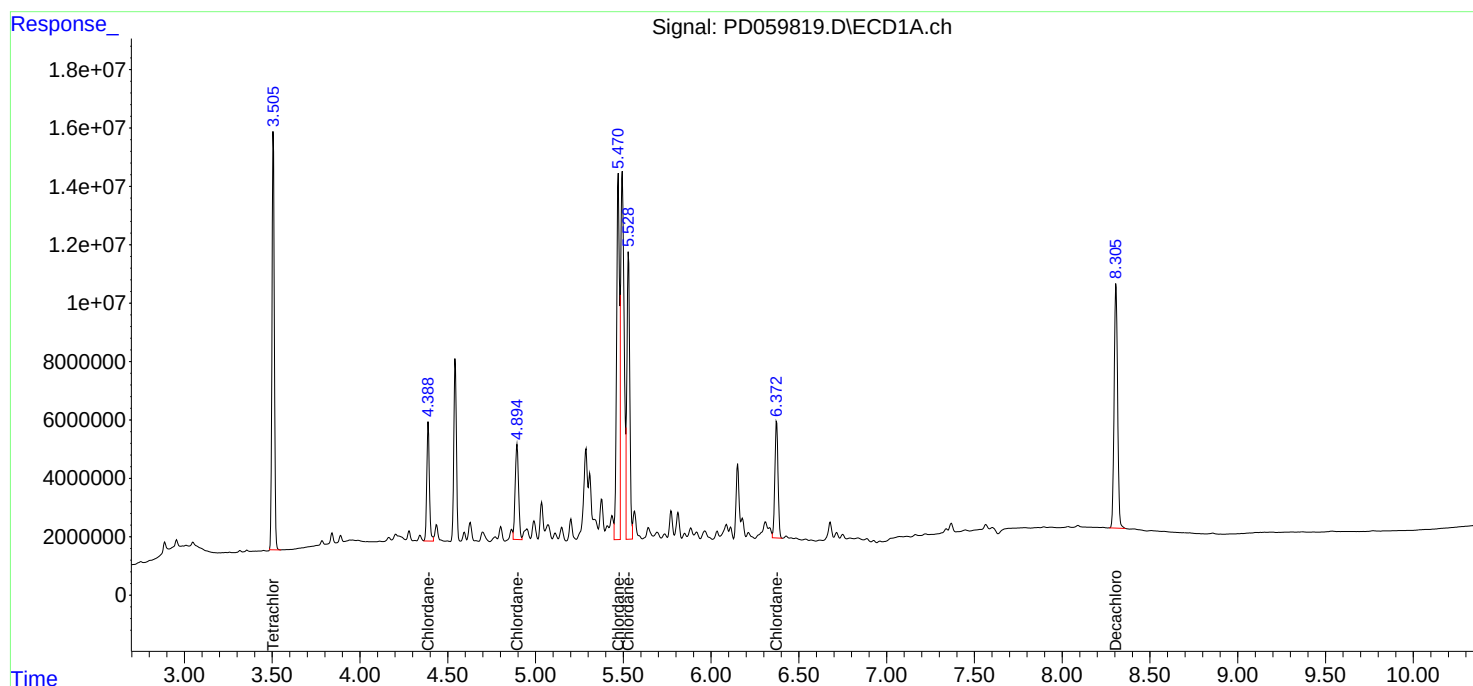


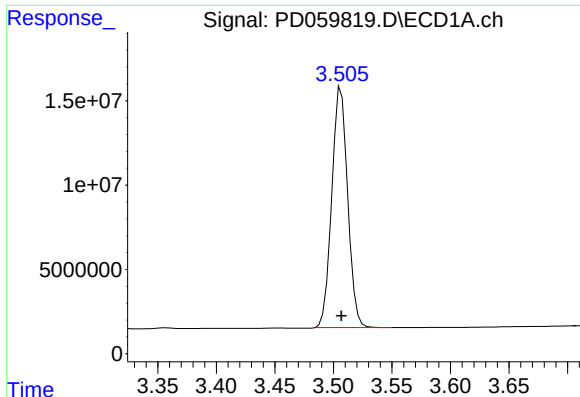

#1 Tetrachloro-m-xylene


R.T.: 3.507 min
Delta R.T.: 0.000 min
Response: 134570715
Conc: 73.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

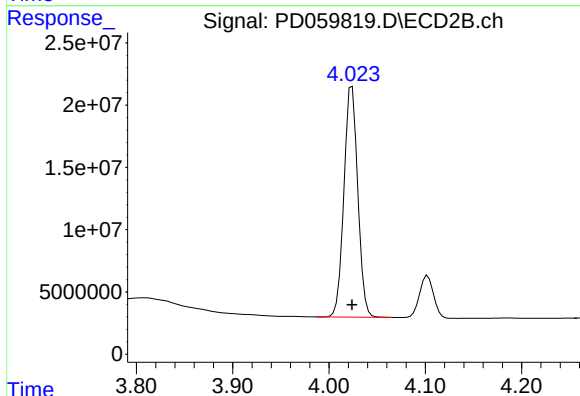


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 184336920
Conc: 74.51 ng/ml

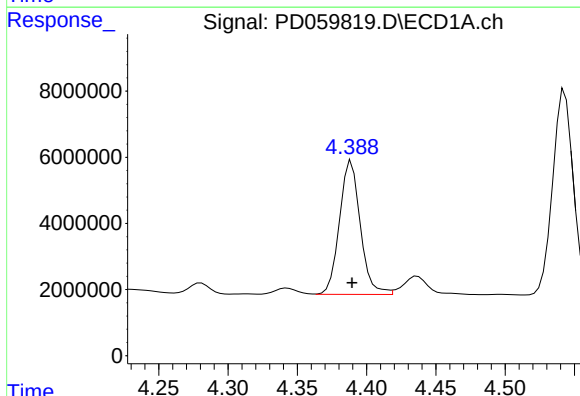


#23 Chlordane-1

R.T.: 4.389 min
Delta R.T.: 0.000 min
Response: 42350847
Conc: 728.80 ng/ml

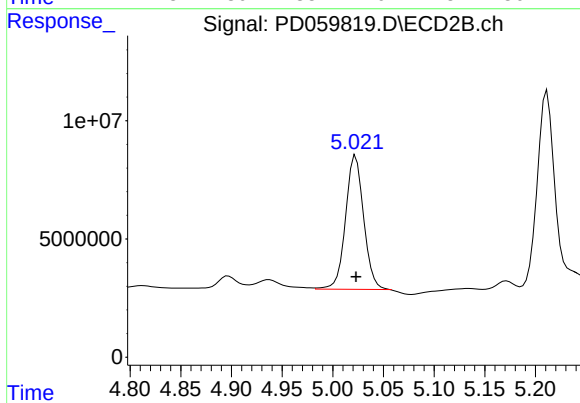

#23 Chlordane-1


R.T.: 5.023 min
Delta R.T.: 0.000 min
Response: 70294257
Conc: 746.20 ng/ml

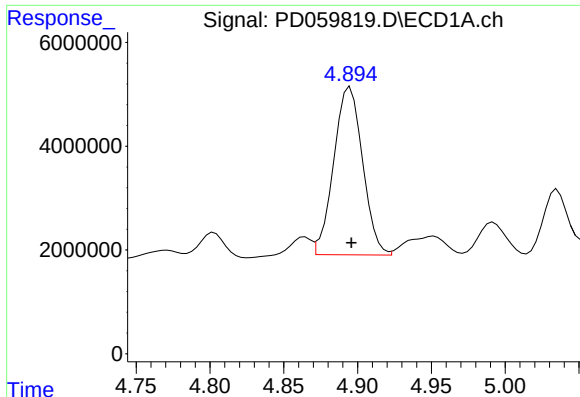

#24 Chlordane-2


R.T.: 4.895 min
Delta R.T.: 0.000 min
Response: 44076401
Conc: 729.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

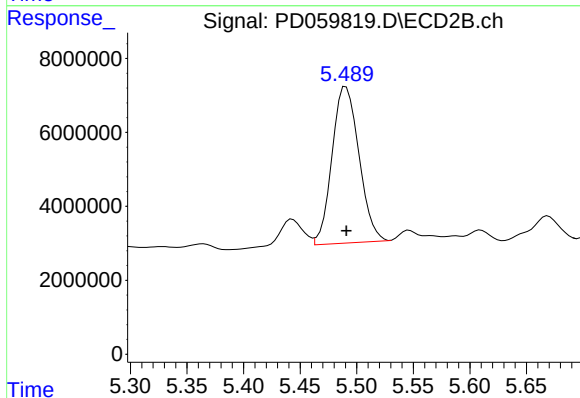


#24 Chlordane-2

R.T.: 5.490 min
Delta R.T.: 0.000 min
Response: 70035478
Conc: 722.19 ng/ml

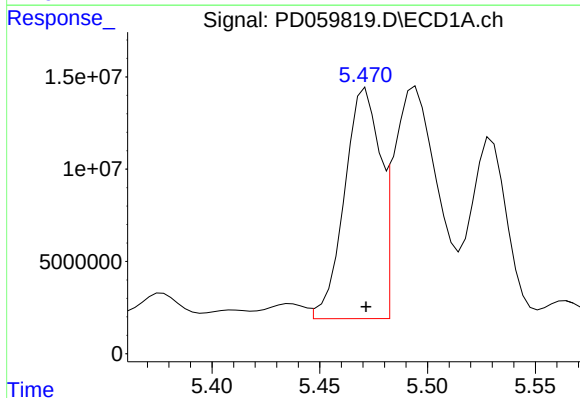


#25 Chlordane-3

R.T.: 5.471 min
Delta R.T.: 0.000 min
Response: 142716697
Conc: 743.68 ng/ml

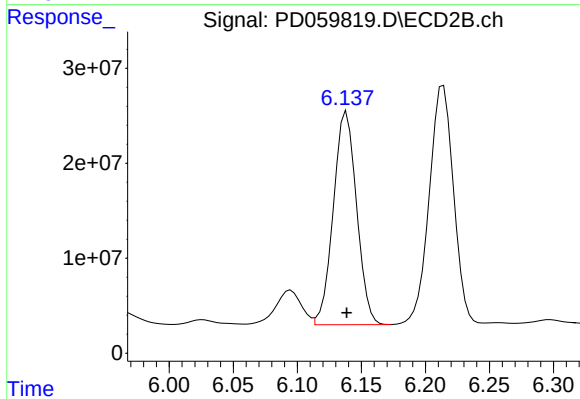

#25 Chlordane-3


R.T.: 6.138 min
Delta R.T.: 0.000 min
Response: 283060290
Conc: 749.07 ng/ml

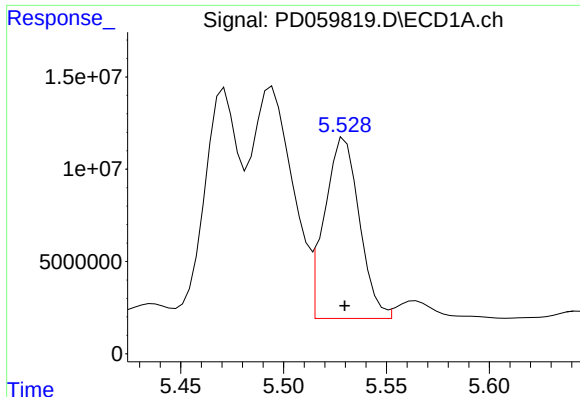

#26 Chlordane-4


R.T.: 5.530 min
Delta R.T.: 0.000 min
Response: 115311707
Conc: 742.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

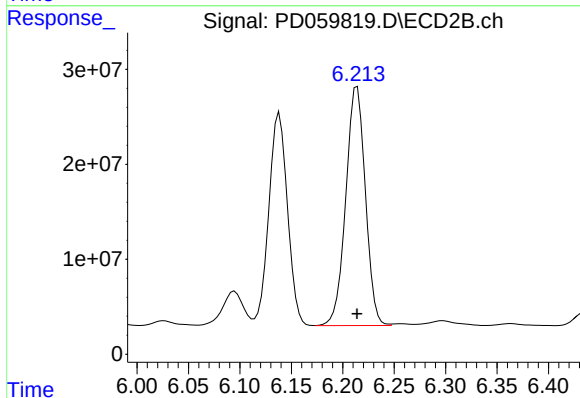


#26 Chlordane-4

R.T.: 6.214 min
Delta R.T.: 0.000 min
Response: 333295374
Conc: 744.67 ng/ml

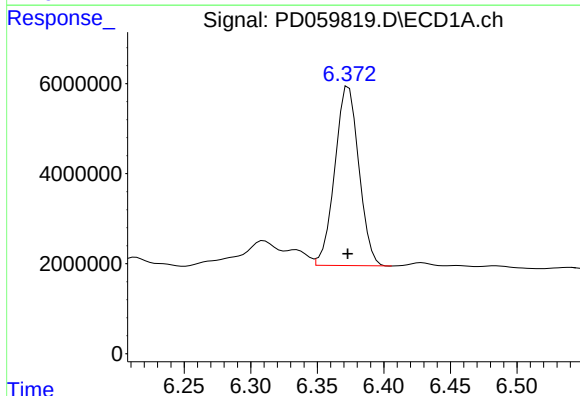


#27 Chlordane-5

R.T.: 6.374 min
Delta R.T.: 0.000 min
Response: 50035715
Conc: 736.28 ng/ml

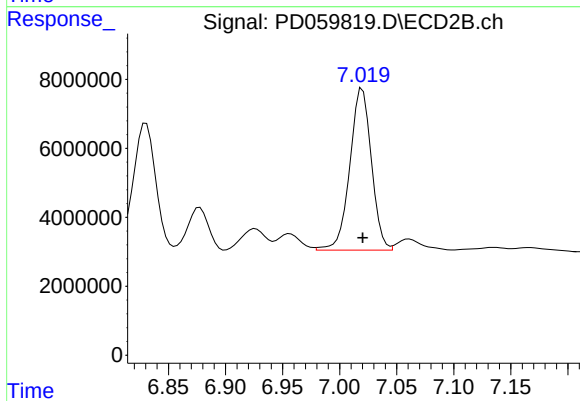

#27 Chlordane-5


R.T.: 7.020 min
Delta R.T.: 0.000 min
Response: 61803874
Conc: 743.75 ng/ml

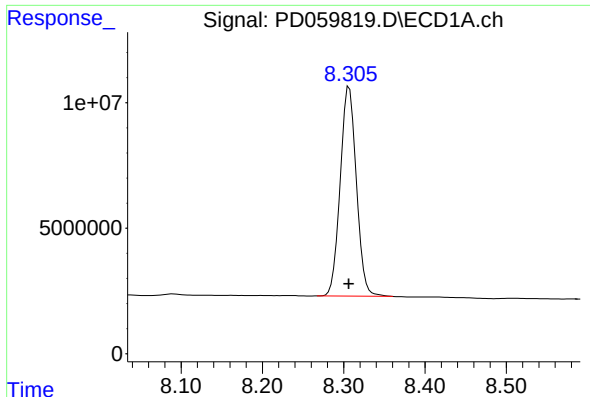

#28 Decachlorobiphenyl

R.T.: 8.307 min
Delta R.T.: 0.000 min
Response: 115098052
Conc: 73.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

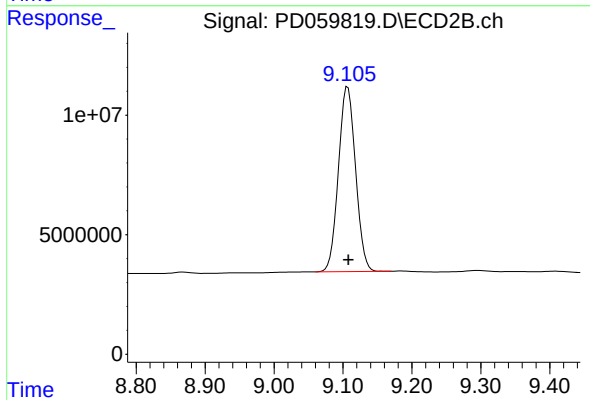

#28 Decachlorobiphenyl

R.T.: 9.107 min
Delta R.T.: 0.000 min
Response: 133576626
Conc: 73.61 ng/ml